




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050929.D
 Acq On : 23 Sep 2022 19:05
 Operator : JC/MD
 Sample : N4747-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45B1

Manual IntegrationsAPPROVED

Quant Time: Sep 24 00:26:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 24 00:22:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/26/2022
 Supervised By :Mahesh Dadoda 09/26/2022

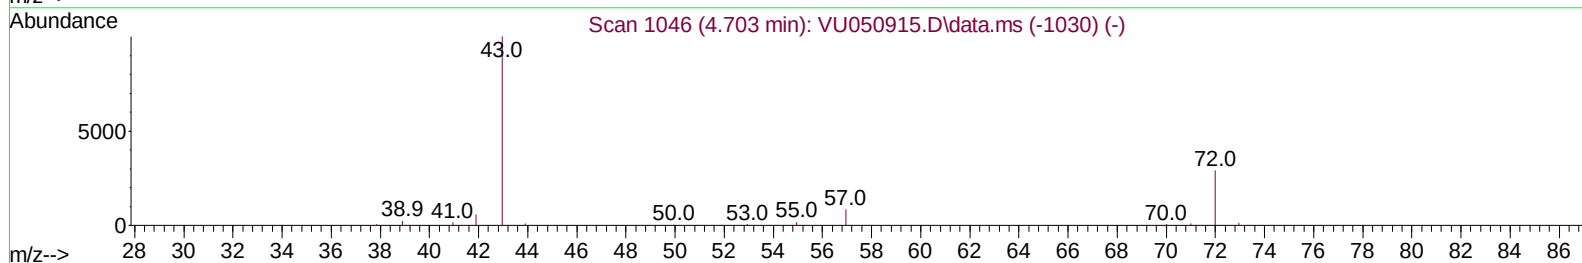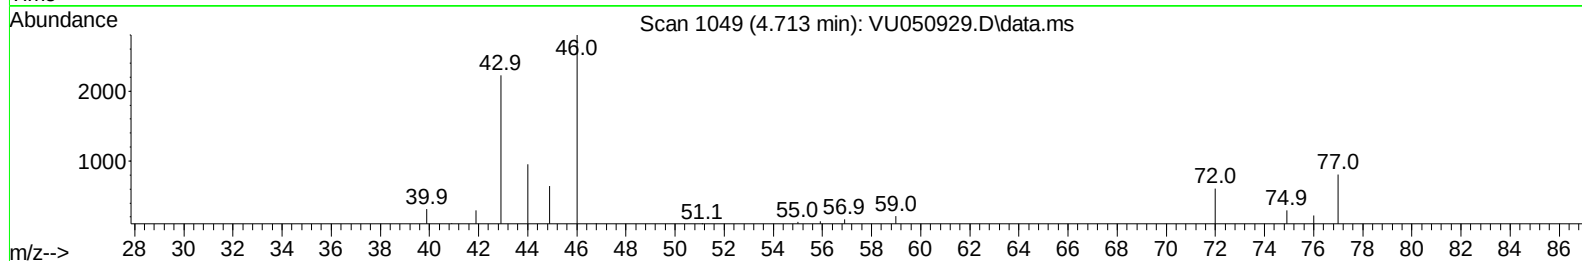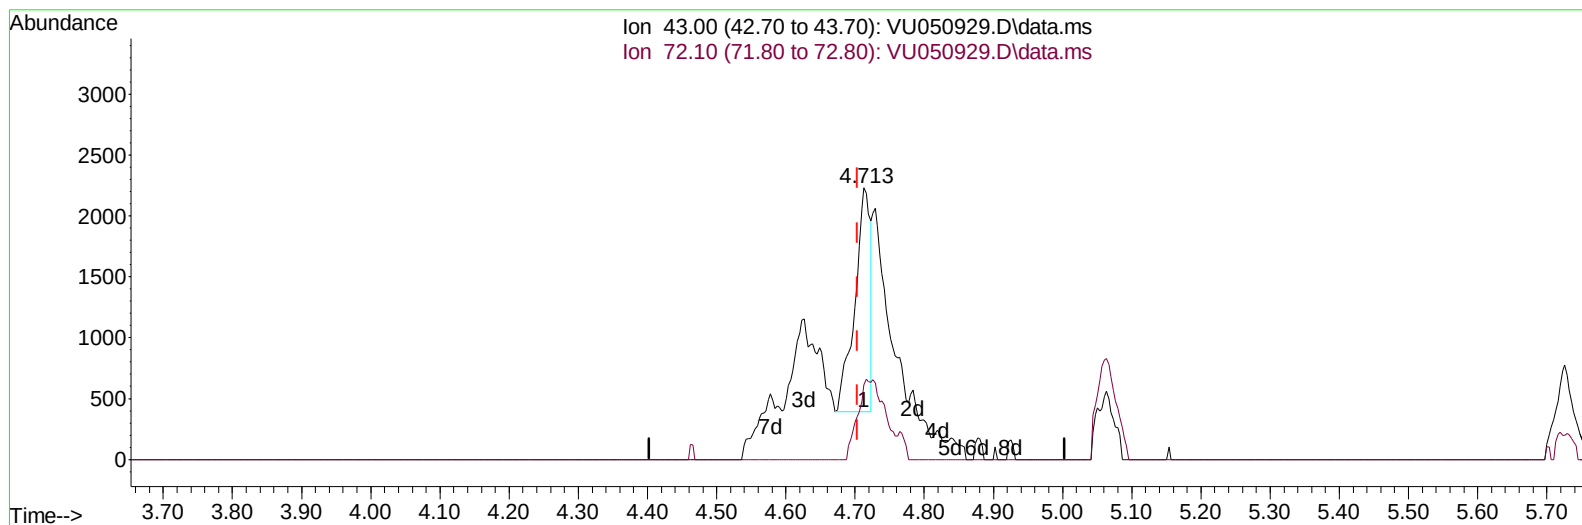

TIC: VU050929.D\data.ms

(22) 2-Butanone (T)

4.713min (+ 0.010) 0.96 ug/L

response 2843

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.50	31.13
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050929.D
 Acq On : 23 Sep 2022 19:05
 Operator : JC/MD
 Sample : N4747-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45B1

Manual IntegrationsAPPROVED

Quant Time: Sep 24 00:26:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 24 00:22:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/26/2022
 Supervised By :Mahesh Dadoda 09/26/2022

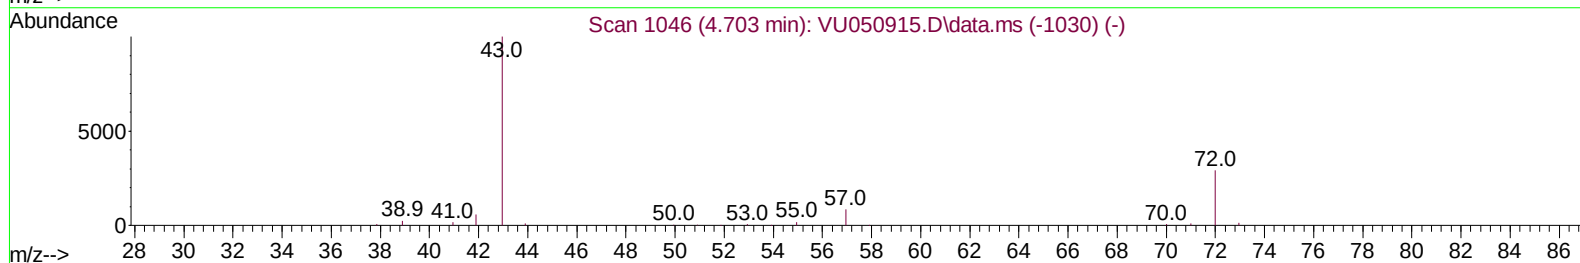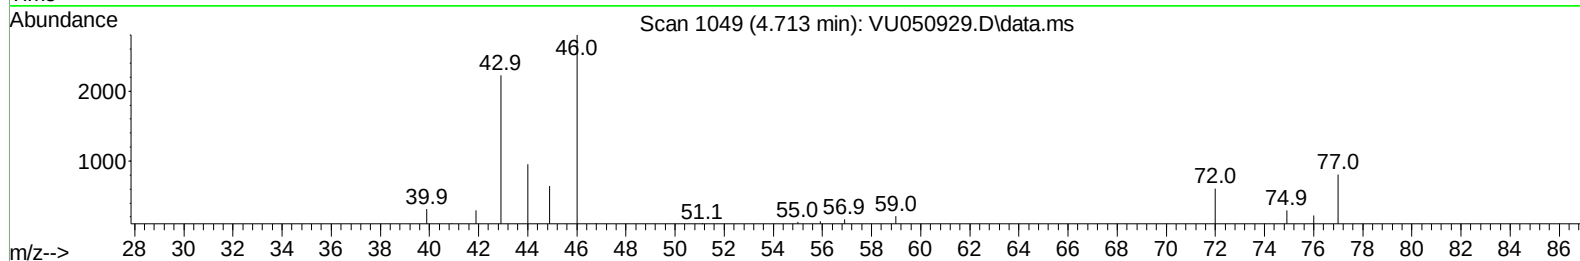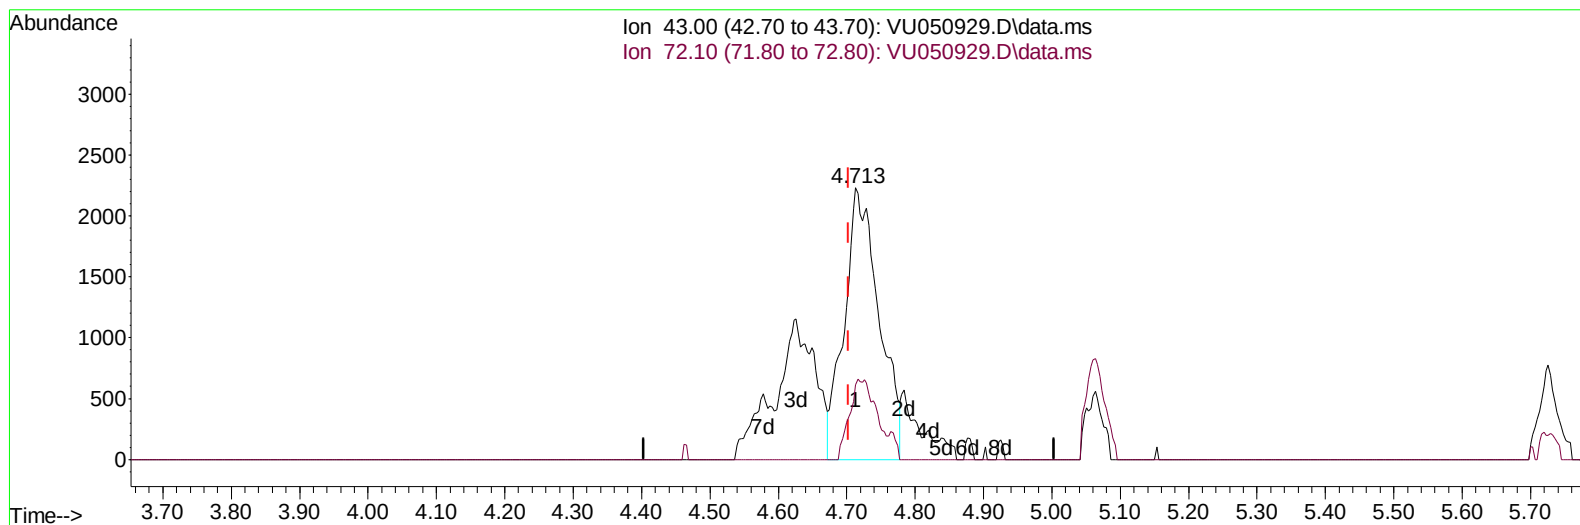

TIC: VU050929.D\data.ms

(22) 2-Butanone (T)

4.713min (+ 0.010) 2.65 ug/L m

response 7855

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.50	11.27#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050929.D
 Acq On : 23 Sep 2022 19:05
 Operator : JC/MD
 Sample : N4747-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45B1

Manual IntegrationsAPPROVED

Quant Time: Sep 24 00:26:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 24 00:22:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/26/2022
 Supervised By :Mahesh Dadoda 09/26/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	396464	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	389617	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	142138	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	165432	40.274	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.540%		
7) Chloroethane-d5	1.912	69	140387	47.989	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.980%		
11) 1,1-Dichloroethene-d2	2.565	63	206094	32.245	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	64.480%		
21) 2-Butanone-d5	4.626	46	308620	116.378	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	116.380%		
24) Chloroform-d	5.060	84	297500	46.216	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.440%		
26) 1,2-Dichloroethane-d4	5.700	65	193766	48.843	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.680%		
32) Benzene-d6	5.726	84	585109	45.593	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.180%		
36) 1,2-Dichloropropane-d6	6.690	67	205318	47.398	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.800%		
41) Toluene-d8	7.896	98	477150	42.535	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.080%		
43) trans-1,3-Dichloroprop...	8.179	79	81321	43.154	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.300%		
47) 2-Hexanone-d5	8.632	63	165026	92.445	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.450%		
56) 1,1,2,2-Tetrachloroeth...	10.755	84	308902	46.773	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.540%		
66) 1,2-Dichlorobenzene-d4	12.192	152	157771	53.014	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.020%		
Target Compounds						
						Qvalue
13) Acetone	2.642	43	45558	20.289	ug/L	98
14) Carbon disulfide	2.793	76	10052	1.043	ug/L	95
22) 2-Butanone	4.713	43	7855m	2.654	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050929.D
Acq On : 23 Sep 2022 19:05
Operator : JC/MD
Sample : N4747-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45B1

Manual IntegrationsAPPROVED

Quant Time: Sep 24 00:26:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 24 00:22:43 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/26/2022
Supervised By :Mahesh Dadoda 09/26/2022

