

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050918.D
 Acq On : 23 Sep 2022 14:31
 Operator : JC/MD
 Sample : VIBLK137
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	99	rVB	197979	237084	13.28%	1.852%
2	1.909	168	177	194	rVB	173258	232193	13.01%	1.813%
3	2.565	369	381	398	rBV	323837	534471	29.95%	4.174%
4	2.784	446	449	453	rBV5	700	685	0.04%	0.005%
5	2.951	498	501	504	rBV	382	347	0.02%	0.003%
6	3.044	521	530	541	rBV3	5263	8723	0.49%	0.068%
7	3.179	558	572	592	rVB	7206	16983	0.95%	0.133%
8	3.292	602	607	613	rVB3	426	351	0.02%	0.003%
9	3.346	622	624	631	rVB4	423	415	0.02%	0.003%
10	3.501	668	672	676	rBV3	331	319	0.02%	0.002%
11	3.658	716	721	729	rBV2	474	583	0.03%	0.005%
12	3.838	773	777	779	rBV2	458	327	0.02%	0.003%
13	3.870	784	787	792	rVB2	687	635	0.04%	0.005%
14	3.977	814	820	823	rBV2	254	295	0.02%	0.002%
15	4.327	924	929	931	rBV2	408	360	0.02%	0.003%
16	4.449	963	967	972	rVB2	384	379	0.02%	0.003%
17	4.491	977	980	985	rBV	336	344	0.02%	0.003%
18	4.620	1007	1020	1057	rBV	212220	558361	31.29%	4.361%
19	4.899	1104	1107	1111	rBV2	533	501	0.03%	0.004%
20	4.957	1121	1125	1128	rVB2	468	289	0.02%	0.002%
21	5.063	1140	1158	1185	rBV	322527	716651	40.16%	5.597%
22	5.243	1210	1214	1220	rBV5	578	524	0.03%	0.004%
23	5.279	1220	1225	1227	rBV2	1196	969	0.05%	0.008%
24	5.372	1248	1254	1257	rBV4	661	674	0.04%	0.005%
25	5.404	1262	1264	1269	rVB2	472	297	0.02%	0.002%
26	5.597	1321	1324	1329	rVB2	380	318	0.02%	0.002%
27	5.639	1331	1337	1338	rBV	510	298	0.02%	0.002%
28	5.722	1341	1363	1389	rBV2	650335	1784677	100.00%	13.937%
29	5.890	1412	1415	1417	rBV4	794	586	0.03%	0.005%
30	6.038	1458	1461	1463	rBV3	616	434	0.02%	0.003%
31	6.163	1494	1500	1503	rBV3	364	281	0.02%	0.002%
32	6.247	1513	1526	1551	rBV	457861	873211	48.93%	6.819%
33	6.529	1601	1614	1626	rVB2	14827	27212	1.52%	0.213%
34	6.690	1649	1664	1686	rBV	432647	842181	47.19%	6.577%
35	6.951	1742	1745	1752	rVB3	366	282	0.02%	0.002%
36	7.050	1771	1776	1783	rBV	580	624	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050918.D
 Acq On : 23 Sep 2022 14:31
 Operator : JC/MD
 Sample : VIBLK137
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.185	1811	1818	1826	rBV4	2122	3555	0.20%	0.028%
38	7.565	1922	1936	1958	rBV2	208941	372543	20.87%	2.909%
39	7.687	1970	1974	1975	rBV3	1058	714	0.04%	0.006%
40	7.783	2001	2004	2012	rVB3	563	573	0.03%	0.004%
41	7.896	2025	2039	2056	rBV	720143	1245141	69.77%	9.724%
42	8.076	2093	2095	2098	rVB	642	388	0.02%	0.003%
43	8.179	2112	2127	2146	rBV	150345	261361	14.64%	2.041%
44	8.330	2171	2174	2183	rVB4	784	881	0.05%	0.007%
45	8.558	2241	2245	2248	rVB2	494	362	0.02%	0.003%
46	8.632	2254	2268	2297	rBV2	564196	1140502	63.91%	8.907%
47	8.838	2329	2332	2335	rVB3	808	543	0.03%	0.004%
48	8.864	2335	2340	2342	rBV3	685	493	0.03%	0.004%
49	8.912	2353	2355	2361	rVB3	888	716	0.04%	0.006%
50	8.938	2361	2363	2366	rBV3	558	318	0.02%	0.002%
51	8.999	2379	2382	2385	rVB2	447	299	0.02%	0.002%
52	9.063	2399	2402	2405	rVB2	473	317	0.02%	0.002%
53	9.172	2432	2436	2441	rBV3	353	330	0.02%	0.003%
54	9.201	2442	2445	2450	rVB2	367	279	0.02%	0.002%
55	9.272	2462	2467	2473	rBV3	387	426	0.02%	0.003%
56	9.414	2497	2511	2530	rBV	664551	1096248	61.43%	8.561%
57	9.558	2550	2556	2558	rBV4	449	478	0.03%	0.004%
58	9.697	2592	2599	2602	rVV5	947	1148	0.06%	0.009%
59	9.815	2635	2636	2643	rVB2	313	290	0.02%	0.002%
60	9.938	2670	2674	2677	rBV2	344	306	0.02%	0.002%
61	10.073	2714	2716	2721	rVB2	438	312	0.02%	0.002%
62	10.275	2770	2779	2781	rBV	443	526	0.03%	0.004%
63	10.487	2842	2845	2848	rBV2	417	326	0.02%	0.003%
64	10.600	2876	2880	2883	rBV2	334	325	0.02%	0.003%
65	10.664	2896	2900	2902	rBV4	1249	970	0.05%	0.008%
66	10.754	2915	2928	2955	rBV	630695	1022704	57.30%	7.987%
67	10.857	2958	2960	2964	rBV3	424	328	0.02%	0.003%
68	10.886	2966	2969	2972	rBV2	617	549	0.03%	0.004%
69	10.996	2995	3003	3004	rBV2	357	333	0.02%	0.003%
70	11.089	3029	3032	3036	rVV2	574	565	0.03%	0.004%
71	11.114	3036	3040	3049	rVB6	1004	1288	0.07%	0.010%
72	11.372	3115	3120	3125	rVB2	699	409	0.02%	0.003%
73	11.446	3139	3143	3145	rBV3	888	654	0.04%	0.005%
74	11.465	3145	3149	3155	rVB3	945	1027	0.06%	0.008%
75	11.696	3215	3221	3224	rBV2	637	586	0.03%	0.005%
76	11.751	3230	3238	3243	rBV4	850	1109	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050918.D
 Acq On : 23 Sep 2022 14:31
 Operator : JC/MD
 Sample : VIBLK137
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.809	3243	3256	3274	rBV	501280	789651	44.25%	6.167%
78	12.028	3320	3324	3329	rBV2	743	816	0.05%	0.006%
79	12.073	3335	3338	3341	rBV2	522	443	0.02%	0.003%
80	12.192	3361	3375	3395	rBV	609436	995623	55.79%	7.775%
81	12.478	3458	3464	3471	rBV6	3022	4486	0.25%	0.035%
82	12.619	3506	3508	3514	rVB3	621	440	0.02%	0.003%
83	12.712	3533	3537	3541	rBV3	1105	1180	0.07%	0.009%
84	12.876	3584	3588	3592	rBV2	457	437	0.02%	0.003%
85	13.005	3626	3628	3636	rVB3	515	451	0.03%	0.004%
86	13.240	3697	3701	3704	rBV2	627	478	0.03%	0.004%
87	13.600	3808	3813	3817	rVB2	607	570	0.03%	0.004%
88	13.667	3829	3834	3838	rBV3	828	816	0.05%	0.006%
89	13.687	3838	3840	3849	rVB2	695	835	0.05%	0.007%
90	13.729	3849	3853	3854	rBV2	412	291	0.02%	0.002%
91	14.002	3936	3938	3943	rBV2	388	423	0.02%	0.003%
92	14.204	3998	4001	4005	rBV2	624	479	0.03%	0.004%
93	14.237	4008	4011	4012	rBV2	452	288	0.02%	0.002%
94	14.632	4130	4134	4136	rBV3	562	449	0.03%	0.004%
95	14.745	4165	4169	4170	rBV	751	508	0.03%	0.004%
96	14.867	4205	4207	4210	rBV2	624	354	0.02%	0.003%
97	15.314	4344	4346	4353	rBV3	732	673	0.04%	0.005%
98	15.349	4353	4357	4359	rBV2	968	746	0.04%	0.006%
99	15.426	4378	4381	4383	rBV2	801	493	0.03%	0.004%
100	15.642	4444	4448	4450	rBV3	904	842	0.05%	0.007%




Sum of corrected areas: 12804858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050918.D
Acq On : 23 Sep 2022 14:31
Operator : JC/MD
Sample : VIBLK137
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK137

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

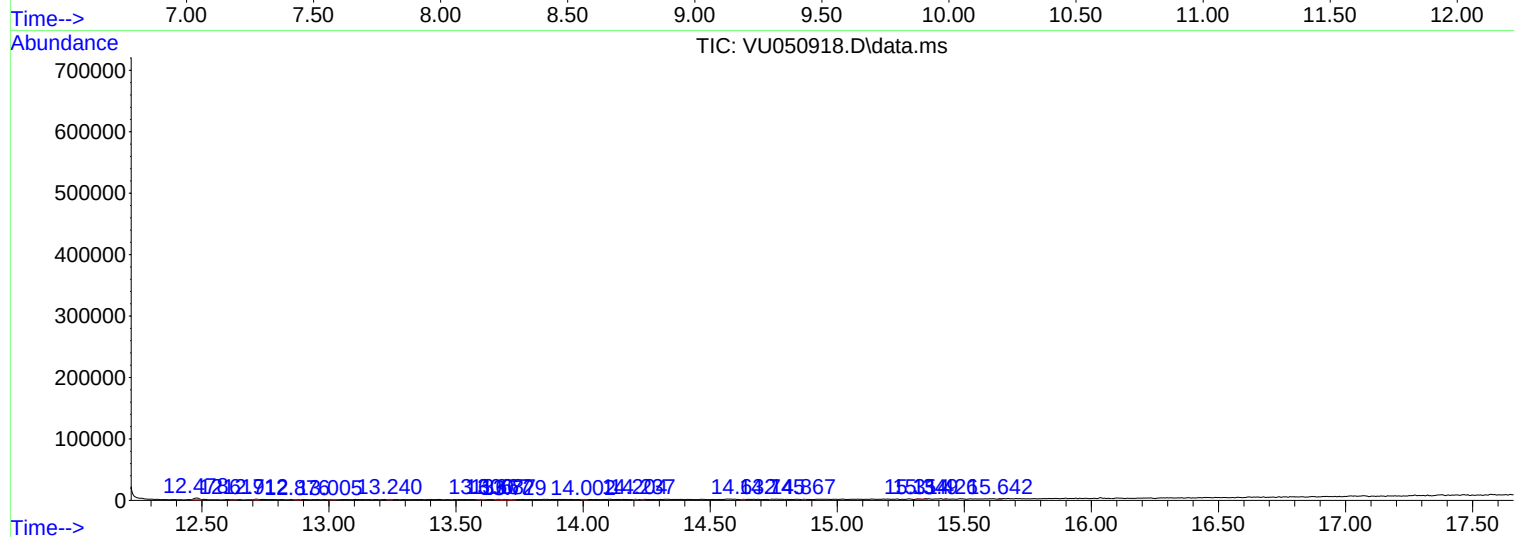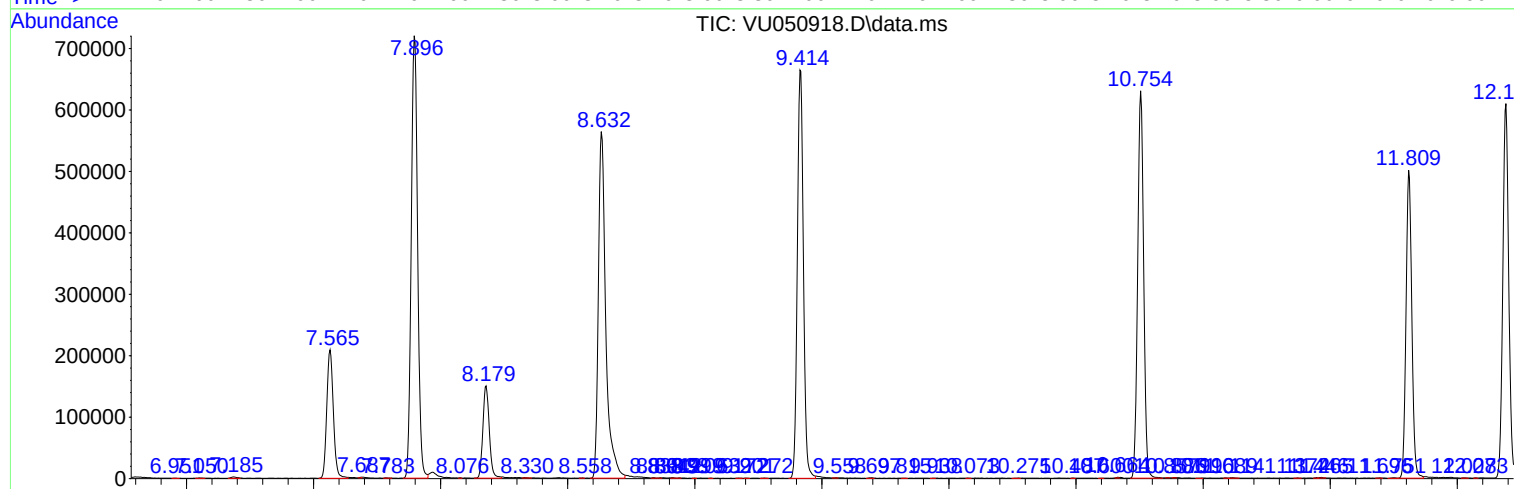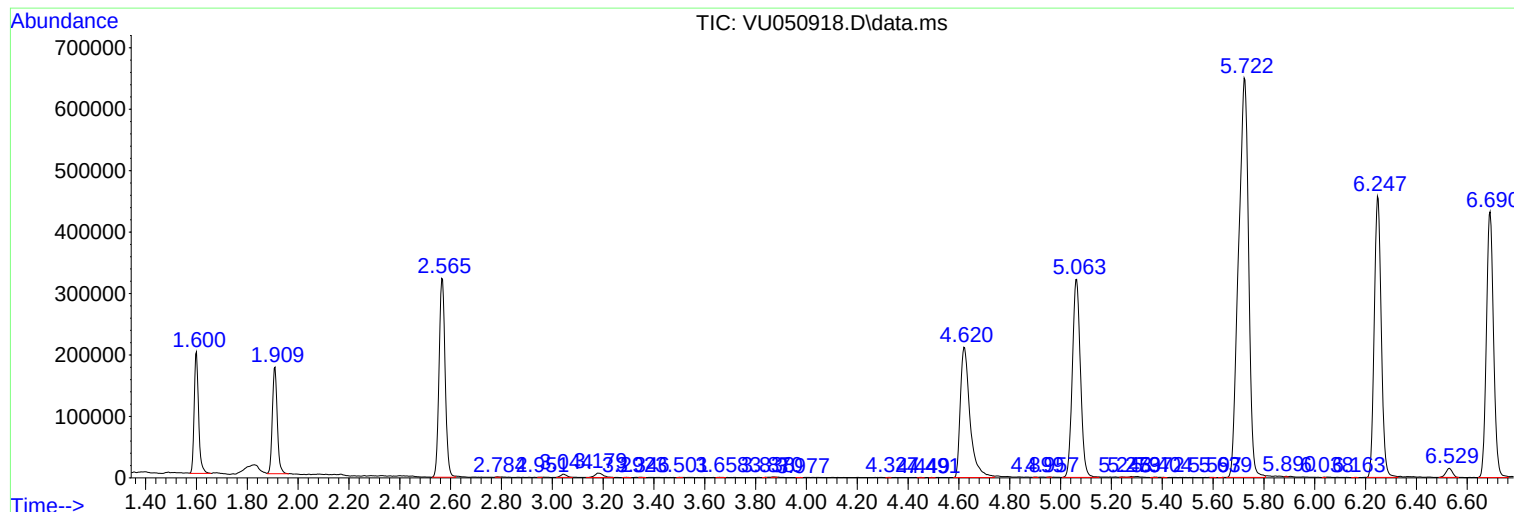

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050918.D
Acq On : 23 Sep 2022 14:31
Operator : JC/MD
Sample : VIBLK137
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK137

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050918.D
Acq On : 23 Sep 2022 14:31
Operator : JC/MD
Sample : VIBLK137
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK137

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
