

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050921.D
 Acq On : 23 Sep 2022 15:43
 Operator : JC/MD
 Sample : N4650-01DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYZ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	104	rVB2	272897	344705	18.61%	2.389%
2	1.906	168	176	180	rBV	192701	249504	13.47%	1.729%
3	2.565	369	381	401	rBV	372416	620003	33.47%	4.297%
4	2.706	422	425	428	rBV2	564	330	0.02%	0.002%
5	2.790	444	451	453	rBV3	1093	1222	0.07%	0.008%
6	2.915	483	490	493	rBV3	572	595	0.03%	0.004%
7	2.960	501	504	507	rVB3	590	359	0.02%	0.002%
8	3.044	520	530	540	rBV4	6770	12929	0.70%	0.090%
9	3.186	562	574	587	rBV2	4528	10636	0.57%	0.074%
10	3.350	616	625	639	rVB3	8774	17493	0.94%	0.121%
11	3.488	664	668	671	rVB	364	290	0.02%	0.002%
12	3.520	671	678	681	rBV2	319	284	0.02%	0.002%
13	3.542	681	685	689	rVB3	354	283	0.02%	0.002%
14	3.658	715	721	724	rBV2	283	300	0.02%	0.002%
15	3.806	761	767	768	rBV2	472	372	0.02%	0.003%
16	3.867	769	786	812	rVV	273663	645374	34.84%	4.472%
17	3.989	821	824	828	rVB4	540	372	0.02%	0.003%
18	4.031	833	837	839	rBV2	402	275	0.01%	0.002%
19	4.083	849	853	856	rBV2	366	273	0.01%	0.002%
20	4.214	892	894	897	rVB2	464	272	0.01%	0.002%
21	4.311	919	924	928	rVB2	420	345	0.02%	0.002%
22	4.337	928	932	934	rBV2	426	276	0.01%	0.002%
23	4.362	935	940	943	rBV3	409	372	0.02%	0.003%
24	4.623	1007	1021	1026	rBV	216883	438400	23.67%	3.038%
25	5.063	1141	1158	1186	rVV	335501	738952	39.89%	5.121%
26	5.314	1220	1236	1255	rBV	109118	249700	13.48%	1.730%
27	5.456	1277	1280	1284	rVB3	494	358	0.02%	0.002%
28	5.488	1284	1290	1294	rBV3	368	465	0.03%	0.003%
29	5.510	1295	1297	1301	rVB2	425	280	0.02%	0.002%
30	5.722	1340	1363	1382	rBV2	680583	1852349	100.00%	12.837%
31	5.970	1438	1440	1444	rBV2	451	271	0.01%	0.002%
32	6.073	1470	1472	1475	rVB3	509	319	0.02%	0.002%
33	6.108	1475	1483	1485	rBV3	642	588	0.03%	0.004%
34	6.247	1512	1526	1551	rBV	523603	992358	53.57%	6.877%
35	6.410	1575	1577	1581	rVB2	641	357	0.02%	0.002%
36	6.536	1603	1616	1631	rVB7	23116	51693	2.79%	0.358%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050921.D
 Acq On : 23 Sep 2022 15:43
 Operator : JC/MD
 Sample : N4650-01DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYZ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1685	rBV	441129	862447	46.56%	5.977%
38	6.983	1747	1755	1766	rBV5	2177	4462	0.24%	0.031%
39	7.060	1773	1779	1784	rVB4	512	594	0.03%	0.004%
40	7.099	1788	1791	1795	rBV2	462	311	0.02%	0.002%
41	7.189	1812	1819	1833	rVV5	2869	5213	0.28%	0.036%
42	7.243	1833	1836	1841	rVB3	461	320	0.02%	0.002%
43	7.304	1850	1855	1857	rBV2	324	325	0.02%	0.002%
44	7.433	1890	1895	1900	rBV2	450	391	0.02%	0.003%
45	7.565	1922	1936	1953	rBV	219704	384692	20.77%	2.666%
46	7.896	2025	2039	2055	rBV	787425	1347170	72.73%	9.336%
47	8.179	2114	2127	2141	rBV	152168	259964	14.03%	1.802%
48	8.304	2164	2166	2169	rBV3	542	294	0.02%	0.002%
49	8.472	2210	2218	2225	rBV5	1477	2569	0.14%	0.018%
50	8.549	2235	2242	2252	rVB4	7988	13098	0.71%	0.091%
51	8.632	2255	2268	2306	rBV2	562337	1128922	60.95%	7.823%
52	9.095	2408	2412	2417	rVB	363	372	0.02%	0.003%
53	9.150	2424	2429	2433	rVB	418	426	0.02%	0.003%
54	9.240	2453	2457	2462	rBV2	363	348	0.02%	0.002%
55	9.417	2497	2512	2538	rBV	709929	1184564	63.95%	8.209%
56	9.568	2555	2559	2570	rVB6	2318	3280	0.18%	0.023%
57	9.616	2570	2574	2578	rVB4	551	489	0.03%	0.003%
58	9.655	2582	2586	2591	rVB3	512	511	0.03%	0.004%
59	9.690	2591	2597	2606	rBV6	1558	2289	0.12%	0.016%
60	9.835	2640	2642	2647	rVV2	399	307	0.02%	0.002%
61	9.928	2667	2671	2674	rBV	526	474	0.03%	0.003%
62	10.031	2698	2703	2708	rVB3	336	437	0.02%	0.003%
63	10.095	2716	2723	2726	rBV4	734	836	0.05%	0.006%
64	10.439	2823	2830	2835	rBV	362	525	0.03%	0.004%
65	10.478	2838	2842	2850	rVB4	591	842	0.05%	0.006%
66	10.590	2871	2877	2879	rBV	455	351	0.02%	0.002%
67	10.648	2891	2895	2896	rBV2	579	344	0.02%	0.002%
68	10.668	2896	2901	2910	rVB4	2295	3263	0.18%	0.023%
69	10.754	2914	2928	2949	rBV	618737	999565	53.96%	6.927%
70	10.880	2964	2967	2968	rBV2	866	469	0.03%	0.003%
71	11.086	3028	3031	3034	rBV3	553	412	0.02%	0.003%
72	11.118	3037	3041	3047	rVB3	1094	1089	0.06%	0.008%
73	11.195	3061	3065	3069	rVB2	333	272	0.01%	0.002%
74	11.221	3069	3073	3075	rBV	426	369	0.02%	0.003%
75	11.291	3091	3095	3098	rBV2	881	725	0.04%	0.005%
76	11.340	3108	3110	3116	rVB2	359	295	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050921.D
 Acq On : 23 Sep 2022 15:43
 Operator : JC/MD
 Sample : N4650-01DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYZ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.372	3117	3120	3124	rBV2	315	291	0.02%	0.002%
78	11.414	3130	3133	3136	rVV3	771	460	0.02%	0.003%
79	11.465	3141	3149	3159	rVB6	3398	5598	0.30%	0.039%
80	11.574	3177	3183	3186	rBV4	518	610	0.03%	0.004%
81	11.690	3216	3219	3221	rBV3	584	383	0.02%	0.003%
82	11.751	3230	3238	3241	rBV3	662	822	0.04%	0.006%
83	11.809	3243	3256	3276	rBV	550238	877479	47.37%	6.081%
84	11.950	3297	3300	3301	rBV3	753	409	0.02%	0.003%
85	12.066	3329	3336	3337	rBV4	2271	2217	0.12%	0.015%
86	12.192	3358	3375	3398	rBV	644063	1053813	56.89%	7.303%
87	12.372	3428	3431	3435	rBV	512	334	0.02%	0.002%
88	12.420	3443	3446	3449	rVB2	376	274	0.01%	0.002%
89	12.478	3454	3464	3476	rBV	20977	35376	1.91%	0.245%
90	12.632	3509	3512	3516	rBV2	581	481	0.03%	0.003%
91	12.758	3548	3551	3553	rBV3	522	365	0.02%	0.003%
92	12.938	3601	3607	3609	rVV3	329	380	0.02%	0.003%
93	13.230	3695	3698	3705	rBV3	834	820	0.04%	0.006%
94	13.330	3726	3729	3734	rVB3	546	461	0.02%	0.003%
95	13.439	3760	3763	3766	rBV2	452	311	0.02%	0.002%
96	13.690	3836	3841	3844	rBV2	624	557	0.03%	0.004%
97	13.757	3859	3862	3866	rVV3	431	386	0.02%	0.003%
98	14.089	3960	3965	3967	rBV3	847	822	0.04%	0.006%
99	14.327	4037	4039	4042	rBV4	512	395	0.02%	0.003%
100	14.764	4172	4175	4178	rBV2	504	486	0.03%	0.003%


Sum of corrected areas: 14430110

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050921.D
Acq On : 23 Sep 2022 15:43
Operator : JC/MD
Sample : N4650-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
XYZZ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

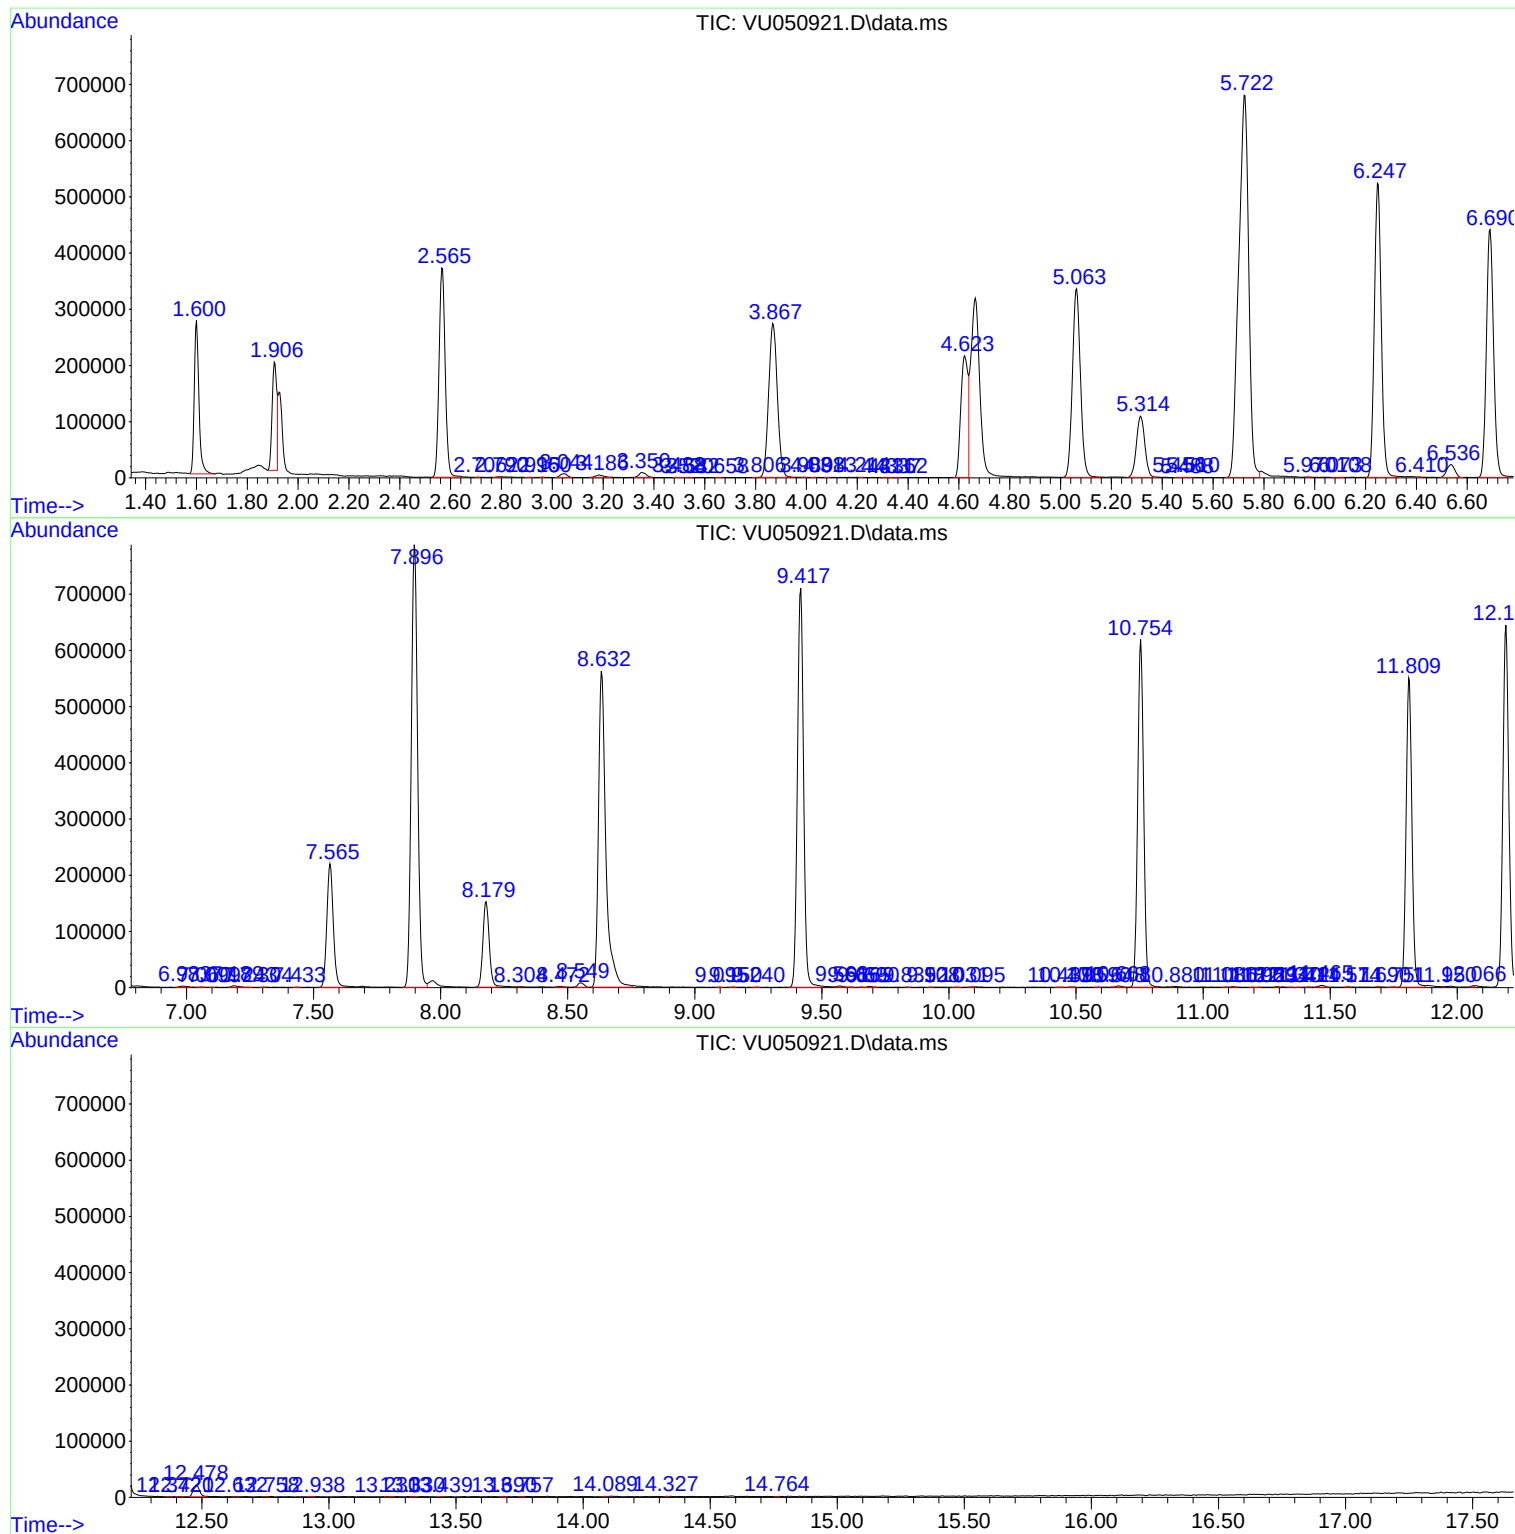

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050921.D
Acq On : 23 Sep 2022 15:43
Operator : JC/MD
Sample : N4650-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYZ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050921.D
Acq On : 23 Sep 2022 15:43
Operator : JC/MD
Sample : N4650-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYZ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------