

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050922.D
 Acq On : 23 Sep 2022 16:07
 Operator : JC/MD
 Sample : N4650-04DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rVB2	245694	308582	17.11%	2.170%
2	1.909	168	177	179	rBV	191738	220342	12.22%	1.549%
3	2.565	368	381	397	rBV	361075	598082	33.17%	4.205%
4	2.704	422	424	431	rVB5	408	360	0.02%	0.003%
5	2.781	446	448	450	rBV2	668	411	0.02%	0.003%
6	2.929	491	494	498	rBV2	298	263	0.01%	0.002%
7	3.048	519	531	542	rBV3	7521	14709	0.82%	0.103%
8	3.186	562	574	590	rVB2	3774	8765	0.49%	0.062%
9	3.356	616	627	637	rVV6	4060	8397	0.47%	0.059%
10	3.552	685	688	692	rBV2	360	271	0.02%	0.002%
11	3.867	769	786	813	rBV	194418	459271	25.47%	3.229%
12	4.112	860	862	867	rVV3	360	297	0.02%	0.002%
13	4.167	876	879	886	rVB4	522	643	0.04%	0.005%
14	4.202	886	890	894	rBV4	445	446	0.02%	0.003%
15	4.298	915	920	924	rBV3	319	317	0.02%	0.002%
16	4.623	1008	1021	1027	rBV	210936	453251	25.14%	3.187%
17	5.060	1141	1157	1180	rBV	329202	717127	39.77%	5.042%
18	5.163	1187	1189	1196	rVB4	462	364	0.02%	0.003%
19	5.314	1220	1236	1255	rBV2	153204	339975	18.85%	2.391%
20	5.462	1280	1282	1287	rVB2	489	396	0.02%	0.003%
21	5.491	1287	1291	1294	rBV3	504	500	0.03%	0.004%
22	5.520	1296	1300	1304	rVV3	506	419	0.02%	0.003%
23	5.617	1324	1330	1333	rBV3	285	302	0.02%	0.002%
24	5.723	1341	1363	1400	rBV2	658945	1803219	100.00%	12.679%
25	5.964	1436	1438	1440	rBV	368	233	0.01%	0.002%
26	6.067	1467	1470	1475	rVB2	602	481	0.03%	0.003%
27	6.247	1511	1526	1555	rBV	513033	974969	54.07%	6.856%
28	6.530	1603	1614	1628	rVB4	17273	34949	1.94%	0.246%
29	6.591	1630	1633	1635	rBV2	597	339	0.02%	0.002%
30	6.691	1649	1664	1682	rBV	426539	834832	46.30%	5.870%
31	7.041	1769	1773	1776	rBV3	517	467	0.03%	0.003%
32	7.102	1788	1792	1798	rBV2	289	268	0.01%	0.002%
33	7.179	1810	1816	1818	rBV4	2043	2009	0.11%	0.014%
34	7.414	1882	1889	1891	rBV2	350	266	0.01%	0.002%
35	7.565	1920	1936	1954	rBV	208869	371074	20.58%	2.609%
36	7.690	1971	1975	1990	rVB4	2070	3723	0.21%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050922.D
 Acq On : 23 Sep 2022 16:07
 Operator : JC/MD
 Sample : N4650-04DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.748	1990	1993	1999	rBV4	410	453	0.03%	0.003%
38	7.793	2004	2007	2010	rBV3	568	456	0.03%	0.003%
39	7.896	2023	2039	2053	rBV	749557	1286842	71.36%	9.048%
40	7.967	2053	2061	2079	rVB2	71104	127111	7.05%	0.894%
41	8.179	2114	2127	2142	rBV2	147414	252758	14.02%	1.777%
42	8.411	2196	2199	2205	rVB2	611	631	0.03%	0.004%
43	8.440	2205	2208	2210	rBV2	449	310	0.02%	0.002%
44	8.552	2233	2243	2253	rVB3	12879	21448	1.19%	0.151%
45	8.633	2253	2268	2307	rBV3	556200	1124320	62.35%	7.906%
46	8.861	2335	2339	2342	rVB3	515	446	0.02%	0.003%
47	8.906	2347	2353	2354	rBV	613	452	0.03%	0.003%
48	8.919	2355	2357	2360	rVB	477	244	0.01%	0.002%
49	9.034	2388	2393	2395	rBV3	429	389	0.02%	0.003%
50	9.205	2442	2446	2451	rBV3	430	363	0.02%	0.003%
51	9.314	2478	2480	2484	rVB2	529	292	0.02%	0.002%
52	9.414	2498	2511	2534	rBV	701607	1178850	65.37%	8.289%
53	9.571	2551	2560	2574	rVB2	11667	19549	1.08%	0.137%
54	9.626	2574	2577	2585	rVB3	587	730	0.04%	0.005%
55	9.690	2586	2597	2612	rBV2	19857	33534	1.86%	0.236%
56	9.861	2647	2650	2654	rVB	403	251	0.01%	0.002%
57	10.099	2710	2724	2737	rBV	14308	23566	1.31%	0.166%
58	10.231	2761	2765	2771	rBV2	451	455	0.03%	0.003%
59	10.481	2837	2843	2854	rBV4	1153	1760	0.10%	0.012%
60	10.555	2863	2866	2872	rVB2	428	299	0.02%	0.002%
61	10.639	2887	2892	2893	rBV2	337	270	0.01%	0.002%
62	10.665	2893	2900	2911	rVB3	1943	3017	0.17%	0.021%
63	10.755	2915	2928	2946	rBV	608182	979842	54.34%	6.890%
64	10.858	2955	2960	2963	rBV2	487	448	0.02%	0.003%
65	10.899	2968	2973	2985	rVB4	2895	4408	0.24%	0.031%
66	10.996	2995	3003	3009	rBV5	6131	9885	0.55%	0.070%
67	11.089	3023	3032	3047	rVB5	3786	6935	0.38%	0.049%
68	11.208	3065	3069	3071	rBV2	472	414	0.02%	0.003%
69	11.231	3073	3076	3078	rBV3	490	342	0.02%	0.002%
70	11.288	3086	3094	3106	rVB2	7438	10810	0.60%	0.076%
71	11.366	3115	3118	3123	rVB	422	386	0.02%	0.003%
72	11.401	3127	3129	3135	rBV4	430	374	0.02%	0.003%
73	11.433	3137	3139	3140	rBV	497	239	0.01%	0.002%
74	11.465	3140	3149	3160	rVV2	18778	29374	1.63%	0.207%
75	11.642	3201	3204	3208	rVB4	734	584	0.03%	0.004%
76	11.690	3216	3219	3222	rVB2	540	295	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050922.D
 Acq On : 23 Sep 2022 16:07
 Operator : JC/MD
 Sample : N4650-04DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

77	11.742	3233	3235	3240	rVB4	867	758	0.04%	0.005%
78	11.809	3243	3256	3274	rBV	542950	867763	48.12%	6.102%
79	11.893	3275	3282	3293	rVB2	12052	19123	1.06%	0.134%
80	12.092	3333	3344	3351	rBV4	5339	8494	0.47%	0.060%
81	12.192	3360	3375	3393	rBV	618005	1026157	56.91%	7.215%
82	12.475	3454	3463	3469	rBV7	2319	3925	0.22%	0.028%
83	12.533	3478	3481	3486	rBV2	670	547	0.03%	0.004%
84	12.571	3486	3493	3501	rVV4	1020	1517	0.08%	0.011%
85	12.671	3520	3524	3525	rBV2	460	277	0.02%	0.002%
86	12.771	3553	3555	3561	rVB2	586	383	0.02%	0.003%
87	12.980	3616	3620	3625	rBV3	951	885	0.05%	0.006%
88	13.021	3630	3633	3634	rBV2	662	381	0.02%	0.003%
89	13.073	3644	3649	3651	rBV3	509	452	0.03%	0.003%
90	13.243	3698	3702	3705	rBV2	462	402	0.02%	0.003%
91	13.449	3759	3766	3771	rBV6	1476	1918	0.11%	0.013%
92	13.665	3830	3833	3835	rBV	470	357	0.02%	0.003%
93	14.002	3936	3938	3941	rVB2	499	254	0.01%	0.002%
94	14.092	3960	3966	3967	rBV3	1304	1075	0.06%	0.008%
95	14.668	4143	4145	4149	rBV2	592	491	0.03%	0.003%
96	14.957	4232	4235	4237	rBV3	693	471	0.03%	0.003%
97	15.153	4293	4296	4298	rBV2	670	436	0.02%	0.003%
98	15.324	4347	4349	4353	rBV4	691	625	0.03%	0.004%
99	15.555	4419	4421	4428	rVB3	1150	1110	0.06%	0.008%
100	15.684	4459	4461	4464	rBV3	874	449	0.02%	0.003%




Sum of corrected areas: 14221701

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050922.D
Acq On : 23 Sep 2022 16:07
Operator : JC/MD
Sample : N4650-04DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

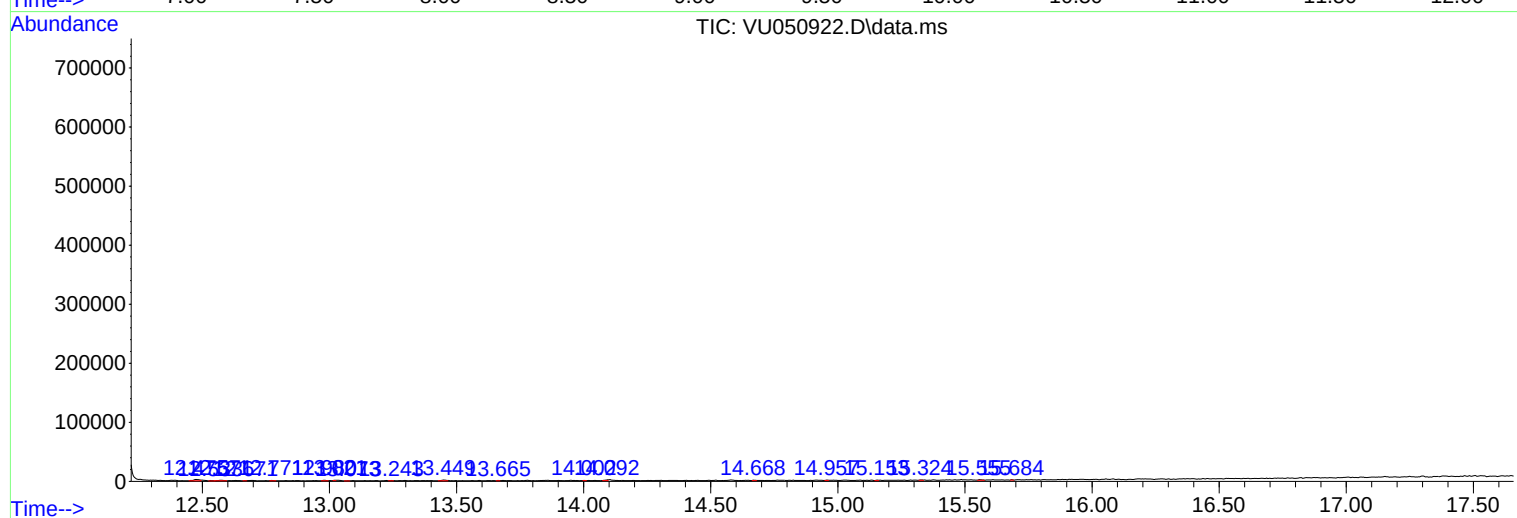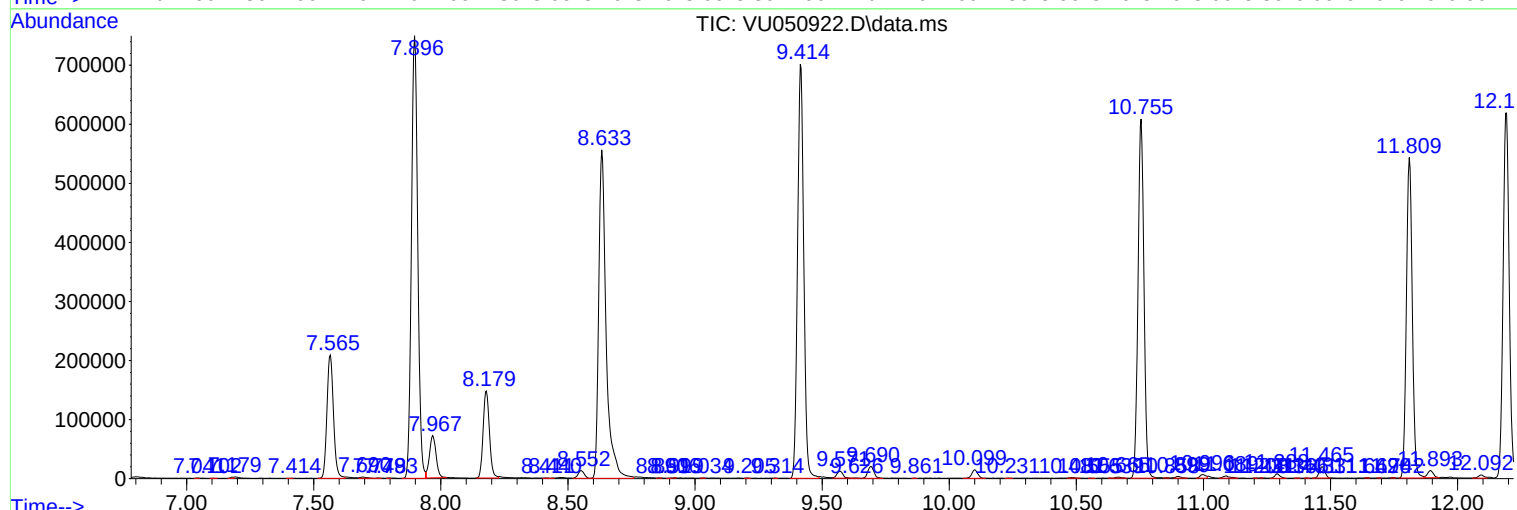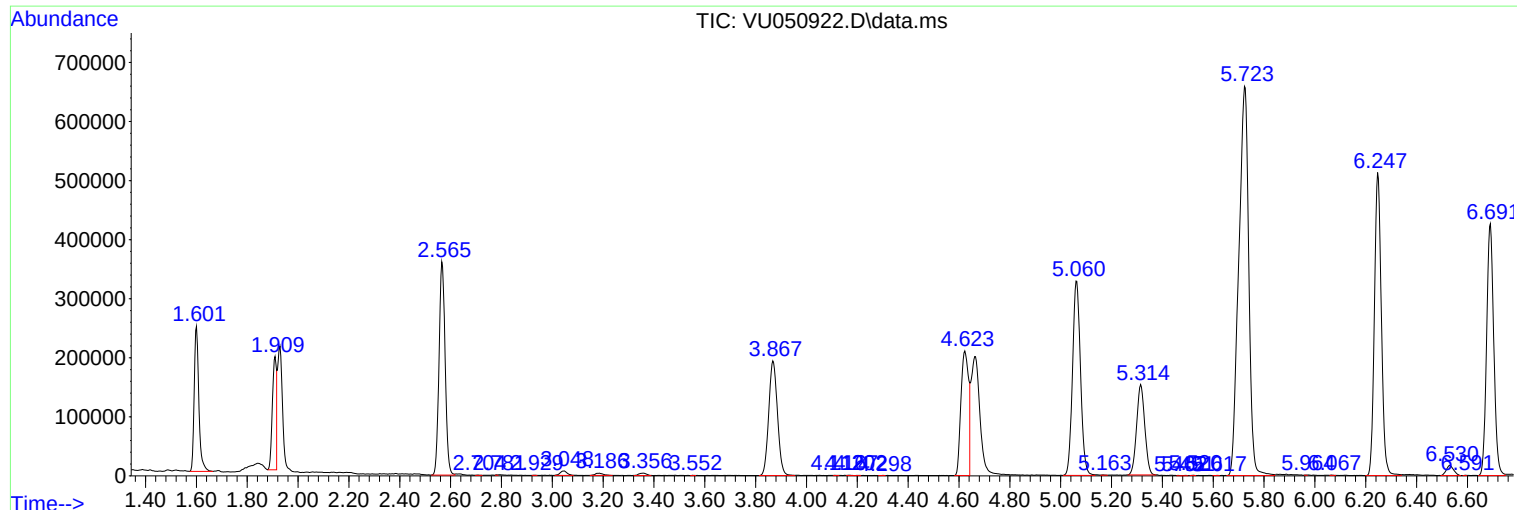

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050922.D
Acq On : 23 Sep 2022 16:07
Operator : JC/MD
Sample : N4650-04DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050922.D
Acq On : 23 Sep 2022 16:07
Operator : JC/MD
Sample : N4650-04DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc