

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050924.D
 Acq On : 23 Sep 2022 16:54
 Operator : JC/MD
 Sample : N4650-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	230592	276954	6.16%	1.155%
2	1.909	170	177	201	rVB	219970	293746	6.54%	1.225%
3	2.080	225	230	237	rBV3	5304	6143	0.14%	0.026%
4	2.465	347	350	353	rBV	660	365	0.01%	0.002%
5	2.568	368	382	399	rBV2	411506	733624	16.32%	3.059%
6	2.736	431	434	437	rVB2	541	331	0.01%	0.001%
7	2.768	440	444	445	rBV2	619	452	0.01%	0.002%
8	2.797	446	453	456	rBV4	3574	4389	0.10%	0.018%
9	2.954	500	502	508	rVB4	503	439	0.01%	0.002%
10	3.044	521	530	539	rBV4	2653	4960	0.11%	0.021%
11	3.141	554	560	563	rBV3	716	710	0.02%	0.003%
12	3.182	563	573	585	rVV3	3275	6760	0.15%	0.028%
13	3.353	614	626	645	rBV2	22798	45109	1.00%	0.188%
14	3.549	685	687	692	rVB3	290	255	0.01%	0.001%
15	3.867	766	786	814	rBV	777760	1842992	41.00%	7.685%
16	4.041	838	840	844	rVB3	498	265	0.01%	0.001%
17	4.102	855	859	861	rBV4	352	338	0.01%	0.001%
18	4.157	874	876	879	rVB	575	263	0.01%	0.001%
19	4.308	921	923	929	rVB3	350	284	0.01%	0.001%
20	4.459	963	970	972	rBV3	391	325	0.01%	0.001%
21	4.504	979	984	987	rBV3	366	328	0.01%	0.001%
22	4.665	1008	1034	1066	rBV2	1781597	4494764	100.00%	18.741%
23	5.063	1142	1158	1180	rVB	339076	755972	16.82%	3.152%
24	5.314	1215	1236	1268	rBV	1772634	3967172	88.26%	16.542%
25	5.723	1342	1363	1394	rBV2	702283	1906387	42.41%	7.949%
26	5.970	1437	1440	1442	rBV3	585	408	0.01%	0.002%
27	6.121	1482	1487	1491	rBV4	581	743	0.02%	0.003%
28	6.247	1512	1526	1556	rBV	524314	988680	22.00%	4.122%
29	6.539	1603	1617	1633	rBV5	47990	99972	2.22%	0.417%
30	6.690	1648	1664	1686	rBV	452480	880445	19.59%	3.671%
31	6.912	1728	1733	1734	rBV2	449	420	0.01%	0.002%
32	6.993	1753	1758	1763	rVB3	324	395	0.01%	0.002%
33	7.041	1770	1773	1778	rBV2	485	455	0.01%	0.002%
34	7.189	1811	1819	1832	rVB8	2763	5590	0.12%	0.023%
35	7.446	1896	1899	1902	rBV2	391	288	0.01%	0.001%
36	7.565	1922	1936	1956	rBV	219999	393048	8.74%	1.639%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050924.D
 Acq On : 23 Sep 2022 16:54
 Operator : JC/MD
 Sample : N4650-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.790	2003	2006	2008	rBV	458	307	0.01%	0.001%
38	7.851	2022	2025	2026	rBV2	399	253	0.01%	0.001%
39	7.896	2026	2039	2055	rBV	789711	1350830	30.05%	5.632%
40	8.176	2112	2126	2144	rBV2	164637	303165	6.74%	1.264%
41	8.398	2189	2195	2205	rVB3	3332	4721	0.11%	0.020%
42	8.468	2205	2217	2231	rBV3	4968	9694	0.22%	0.040%
43	8.552	2231	2243	2256	rBV	108613	181367	4.04%	0.756%
44	8.632	2256	2268	2311	rBV2	599487	1205746	26.83%	5.027%
45	8.857	2337	2338	2343	rVB4	609	408	0.01%	0.002%
46	8.954	2363	2368	2370	rBV2	522	451	0.01%	0.002%
47	8.973	2372	2374	2380	rVB	404	334	0.01%	0.001%
48	9.041	2391	2395	2397	rBV3	348	270	0.01%	0.001%
49	9.156	2428	2431	2437	rVV3	574	491	0.01%	0.002%
50	9.288	2469	2472	2475	rBV	379	258	0.01%	0.001%
51	9.327	2481	2484	2489	rVB2	415	337	0.01%	0.001%
52	9.417	2498	2512	2543	rBV	713438	1186148	26.39%	4.946%
53	9.571	2557	2560	2566	rVB5	812	752	0.02%	0.003%
54	9.687	2589	2596	2601	rBV6	1114	1633	0.04%	0.007%
55	9.755	2613	2617	2620	rVB3	422	425	0.01%	0.002%
56	9.864	2644	2651	2653	rBV2	272	303	0.01%	0.001%
57	9.951	2676	2678	2684	rVB2	487	466	0.01%	0.002%
58	9.983	2684	2688	2690	rBV2	608	432	0.01%	0.002%
59	10.005	2693	2695	2699	rVV	451	393	0.01%	0.002%
60	10.037	2700	2705	2709	rVV2	471	661	0.01%	0.003%
61	10.066	2712	2714	2717	rVV2	426	273	0.01%	0.001%
62	10.092	2719	2722	2723	rVV	424	273	0.01%	0.001%
63	10.105	2723	2726	2728	rVV2	559	398	0.01%	0.002%
64	10.124	2730	2732	2738	rVB2	477	395	0.01%	0.002%
65	10.282	2780	2781	2788	rVB2	459	351	0.01%	0.001%
66	10.484	2840	2844	2848	rBV3	346	280	0.01%	0.001%
67	10.626	2886	2888	2891	rBV2	424	240	0.01%	0.001%
68	10.642	2891	2893	2895	rBV	454	316	0.01%	0.001%
69	10.664	2895	2900	2906	rVV4	1743	2173	0.05%	0.009%
70	10.754	2914	2928	2946	rBV	640925	1030748	22.93%	4.298%
71	10.890	2959	2970	2982	rVB3	8075	13335	0.30%	0.056%
72	11.044	3014	3018	3024	rBV3	427	488	0.01%	0.002%
73	11.111	3033	3039	3047	rVV5	1403	2277	0.05%	0.009%
74	11.272	3085	3089	3091	rBV	365	307	0.01%	0.001%
75	11.301	3096	3098	3104	rVB4	469	436	0.01%	0.002%
76	11.375	3116	3121	3127	rVB4	795	870	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050924.D
 Acq On : 23 Sep 2022 16:54
 Operator : JC/MD
 Sample : N4650-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.414	3128	3133	3139	rBV4	554	623	0.01%	0.003%
78	11.455	3140	3146	3148	rBV3	1341	1420	0.03%	0.006%
79	11.529	3163	3169	3171	rBV2	388	345	0.01%	0.001%
80	11.610	3190	3194	3196	rBV	443	347	0.01%	0.001%
81	11.687	3214	3218	3220	rBV3	839	640	0.01%	0.003%
82	11.809	3243	3256	3278	rBV	550870	873940	19.44%	3.644%
83	11.973	3302	3307	3314	rVB4	1754	1881	0.04%	0.008%
84	12.063	3329	3335	3339	rBV5	3240	4649	0.10%	0.019%
85	12.192	3360	3375	3393	rBV	665549	1072589	23.86%	4.472%
86	12.436	3448	3451	3455	rBV2	389	321	0.01%	0.001%
87	12.462	3455	3459	3461	rVV2	502	349	0.01%	0.001%
88	12.700	3528	3533	3536	rBV	563	485	0.01%	0.002%
89	12.770	3549	3555	3570	rVB5	2104	3165	0.07%	0.013%
90	12.835	3570	3575	3578	rBV3	409	441	0.01%	0.002%
91	13.172	3677	3680	3681	rBV	448	247	0.01%	0.001%
92	13.291	3708	3717	3724	rBV3	892	1592	0.04%	0.007%
93	13.410	3752	3754	3757	rBV2	364	250	0.01%	0.001%
94	13.439	3758	3763	3766	rVV3	524	574	0.01%	0.002%
95	13.533	3789	3792	3798	rVB4	551	515	0.01%	0.002%
96	13.835	3883	3886	3887	rBV	453	264	0.01%	0.001%
97	13.967	3924	3927	3930	rBV4	503	415	0.01%	0.002%
98	14.201	3998	4000	4005	rVB3	638	340	0.01%	0.001%
99	14.700	4153	4155	4159	rVB2	610	268	0.01%	0.001%
100	15.304	4340	4343	4348	rBV4	901	683	0.02%	0.003%




Sum of corrected areas: 23983119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050924.D
Acq On : 23 Sep 2022 16:54
Operator : JC/MD
Sample : N4650-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

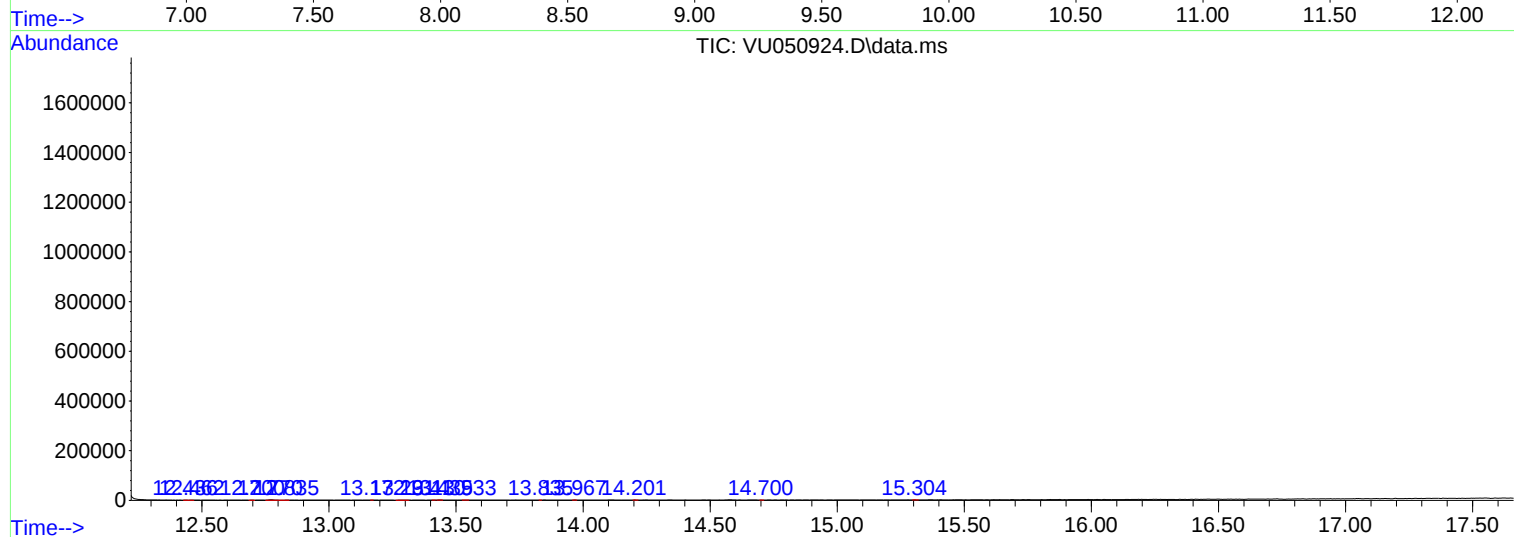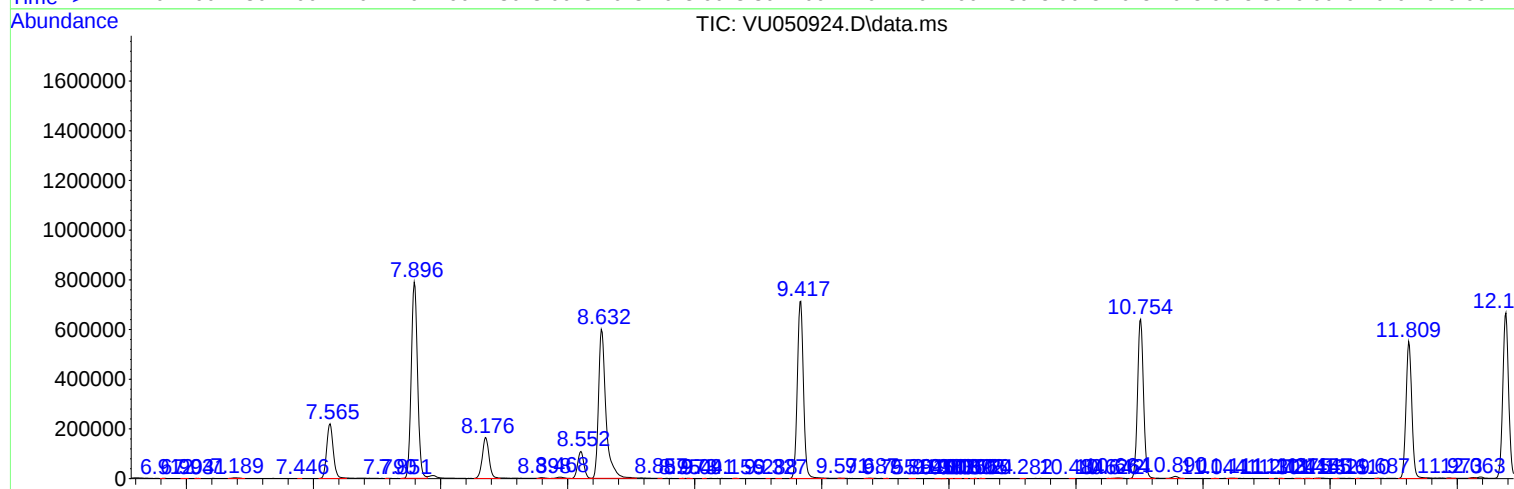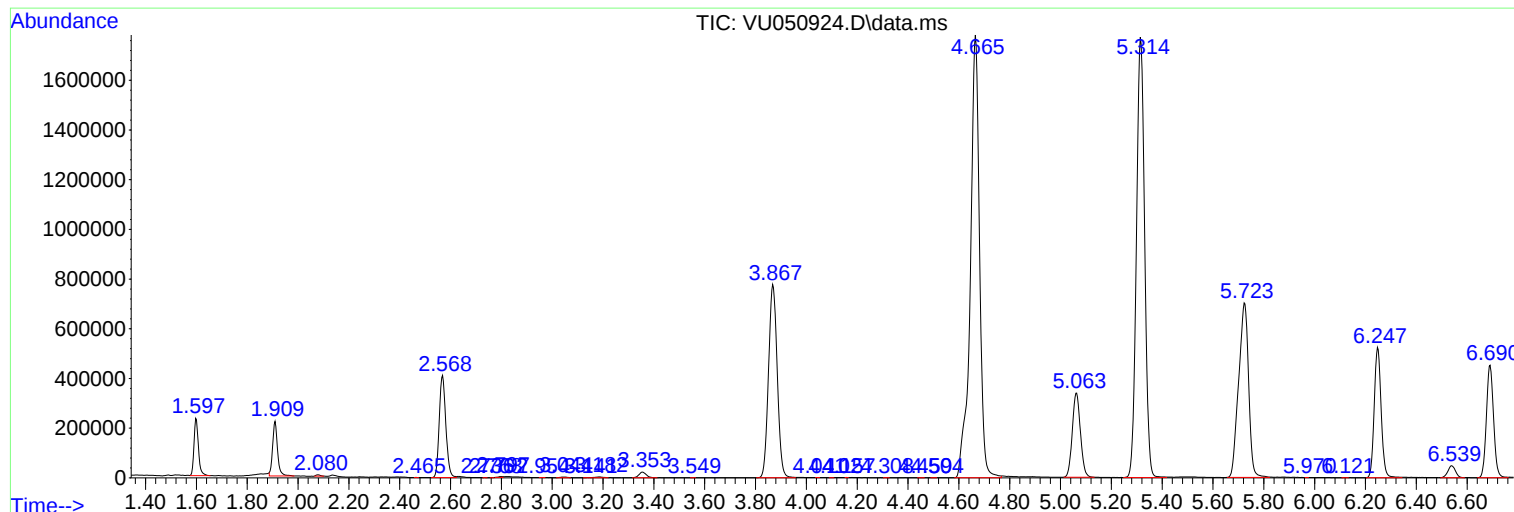

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050924.D
Acq On : 23 Sep 2022 16:54
Operator : JC/MD
Sample : N4650-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050924.D
Acq On : 23 Sep 2022 16:54
Operator : JC/MD
Sample : N4650-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc