

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050925.D
 Acq On : 23 Sep 2022 17:31
 Operator : JC/MD
 Sample : VIBLK138
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK138

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	102	rVB	235586	277940	14.87%	1.992%
2	1.912	171	178	198	rVB	206806	262900	14.07%	1.884%
3	2.568	370	382	403	rBV	369658	609021	32.59%	4.365%
4	2.935	494	496	498	rBV	176	117	0.01%	0.001%
5	3.047	523	531	541	rVB2	3961	7219	0.39%	0.052%
6	3.086	541	543	546	rBV	195	89	0.00%	0.001%
7	3.279	600	603	605	rBV2	286	197	0.01%	0.001%
8	3.334	617	620	622	rBV	234	153	0.01%	0.001%
9	3.356	625	627	630	rVV2	289	150	0.01%	0.001%
10	3.375	630	633	636	rVB	305	181	0.01%	0.001%
11	3.395	636	639	641	rBV2	302	200	0.01%	0.001%
12	3.453	653	657	659	rBV2	329	172	0.01%	0.001%
13	3.465	659	661	664	rVB	228	106	0.01%	0.001%
14	3.485	664	667	669	rBV	238	188	0.01%	0.001%
15	3.520	675	678	680	rBV2	205	111	0.01%	0.001%
16	3.536	680	683	684	rBV	187	115	0.01%	0.001%
17	3.559	689	690	691	rBV	269	93	0.00%	0.001%
18	3.626	706	711	714	rBV2	539	478	0.03%	0.003%
19	3.665	720	723	725	rVV	220	156	0.01%	0.001%
20	3.694	728	732	734	rBV	359	238	0.01%	0.002%
21	3.855	779	782	783	rBV3	613	398	0.02%	0.003%
22	3.932	804	806	809	rBV2	213	119	0.01%	0.001%
23	3.999	824	827	831	rBV2	163	143	0.01%	0.001%
24	4.035	835	838	840	rBV	219	153	0.01%	0.001%
25	4.109	857	861	863	rVV2	131	92	0.00%	0.001%
26	4.240	899	902	905	rVB2	132	95	0.01%	0.001%
27	4.398	945	951	954	rBV2	347	287	0.02%	0.002%
28	4.414	954	956	959	rVB3	181	119	0.01%	0.001%
29	4.433	959	962	968	rVB	191	189	0.01%	0.001%
30	4.465	968	972	974	rBV	227	188	0.01%	0.001%
31	4.501	981	983	987	rVB2	162	98	0.01%	0.001%
32	4.527	987	991	992	rBV2	178	111	0.01%	0.001%
33	4.552	997	999	1001	rVB2	245	117	0.01%	0.001%
34	4.629	1010	1023	1070	rBV2	189084	529366	28.33%	3.794%
35	5.063	1141	1158	1181	rBV	338886	747303	39.99%	5.356%
36	5.372	1249	1254	1255	rBV	805	527	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050925.D
 Acq On : 23 Sep 2022 17:31
 Operator : JC/MD
 Sample : VIBLK138
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK138

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	5.449	1276	1278	1280	rBV	190	120	0.01%	0.001%
38	5.507	1291	1296	1299	rBV2	314	319	0.02%	0.002%
39	5.549	1307	1309	1312	rBV2	185	104	0.01%	0.001%
40	5.568	1312	1315	1322	rVB3	406	370	0.02%	0.003%
41	5.620	1328	1331	1335	rVB2	325	222	0.01%	0.002%
42	5.649	1335	1340	1342	rBV	186	183	0.01%	0.001%
43	5.726	1342	1364	1395	rBV2	704046	1868607	100.00%	13.392%
44	6.073	1468	1472	1474	rBV2	270	189	0.01%	0.001%
45	6.092	1475	1478	1481	rVB2	307	205	0.01%	0.001%
46	6.108	1481	1483	1485	rBV	489	273	0.01%	0.002%
47	6.186	1505	1507	1511	rBV	324	177	0.01%	0.001%
48	6.250	1511	1527	1554	rBV	515874	987741	52.86%	7.079%
49	6.526	1603	1613	1632	rVB2	14859	29780	1.59%	0.213%
50	6.594	1632	1634	1636	rBV2	340	157	0.01%	0.001%
51	6.607	1636	1638	1641	rVB3	600	248	0.01%	0.002%
52	6.623	1641	1643	1645	rBV2	340	181	0.01%	0.001%
53	6.690	1648	1664	1690	rBV	444787	870215	46.57%	6.237%
54	6.941	1736	1742	1745	rBV3	292	299	0.02%	0.002%
55	6.977	1750	1753	1756	rBV3	359	212	0.01%	0.002%
56	7.092	1786	1789	1794	rBV3	327	302	0.02%	0.002%
57	7.182	1812	1817	1818	rBV	1435	1033	0.06%	0.007%
58	7.401	1884	1885	1888	rBV	183	111	0.01%	0.001%
59	7.459	1900	1903	1906	rBV2	139	103	0.01%	0.001%
60	7.517	1919	1921	1923	rBV	339	164	0.01%	0.001%
61	7.565	1923	1936	1960	rVV	218853	385673	20.64%	2.764%
62	7.803	2005	2010	2013	rVB3	485	424	0.02%	0.003%
63	7.835	2016	2020	2021	rBV2	207	122	0.01%	0.001%
64	7.899	2026	2040	2056	rBV	803756	1382476	73.98%	9.908%
65	8.096	2098	2101	2107	rVB	532	454	0.02%	0.003%
66	8.179	2115	2127	2147	rBV	155833	269560	14.43%	1.932%
67	8.517	2229	2232	2235	rBV4	505	394	0.02%	0.003%
68	8.552	2240	2243	2246	rBV4	1274	810	0.04%	0.006%
69	8.636	2257	2269	2302	rBV4	534471	1136566	60.82%	8.145%
70	9.038	2390	2394	2395	rBV2	301	245	0.01%	0.002%
71	9.099	2410	2413	2415	rBV	355	158	0.01%	0.001%
72	9.144	2421	2427	2428	rBV2	412	364	0.02%	0.003%
73	9.208	2441	2447	2448	rBV	285	293	0.02%	0.002%
74	9.234	2453	2455	2461	rVB2	418	326	0.02%	0.002%
75	9.333	2484	2486	2488	rBV	359	200	0.01%	0.001%
76	9.417	2499	2512	2535	rBV	761967	1258773	67.36%	9.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050925.D
 Acq On : 23 Sep 2022 17:31
 Operator : JC/MD
 Sample : VIBLK138
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK138

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	9.600	2566	2569	2572	rBV3	445	228	0.01%	0.002%
78	9.687	2593	2596	2600	rBV4	726	685	0.04%	0.005%
79	9.909	2661	2665	2668	rBV2	323	303	0.02%	0.002%
80	10.002	2687	2694	2699	rBV2	348	470	0.03%	0.003%
81	10.144	2735	2738	2739	rBV2	262	155	0.01%	0.001%
82	10.176	2745	2748	2750	rBV	305	206	0.01%	0.001%
83	10.234	2763	2766	2769	rBV2	287	209	0.01%	0.001%
84	10.613	2881	2884	2885	rBV	227	141	0.01%	0.001%
85	10.668	2893	2901	2908	rVB4	2521	3628	0.19%	0.026%
86	10.703	2909	2912	2914	rBV3	320	206	0.01%	0.001%
87	10.755	2915	2928	2949	rBV	638835	1018262	54.49%	7.298%
88	10.980	2995	2998	2999	rBV2	406	233	0.01%	0.002%
89	11.070	3022	3026	3027	rBV2	348	194	0.01%	0.001%
90	11.401	3122	3129	3130	rBV	397	434	0.02%	0.003%
91	11.449	3140	3144	3145	rBV2	1312	827	0.04%	0.006%
92	11.571	3180	3182	3184	rBV2	329	203	0.01%	0.001%
93	11.693	3215	3220	3226	rBV3	987	1193	0.06%	0.009%
94	11.812	3244	3257	3283	rBV	662238	1062478	56.86%	7.614%
95	12.192	3361	3375	3399	rBV	755871	1224219	65.52%	8.774%
96	12.494	3467	3469	3473	rBV2	390	235	0.01%	0.002%
97	12.729	3540	3542	3544	rBV2	334	220	0.01%	0.002%
98	12.893	3590	3593	3595	rBV2	414	306	0.02%	0.002%
99	13.417	3753	3756	3763	rBV4	447	479	0.03%	0.003%
100	14.504	4091	4094	4099	rBV3	593	631	0.03%	0.005%




Sum of corrected areas: 13953427

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050925.D
Acq On : 23 Sep 2022 17:31
Operator : JC/MD
Sample : VIBLK138
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

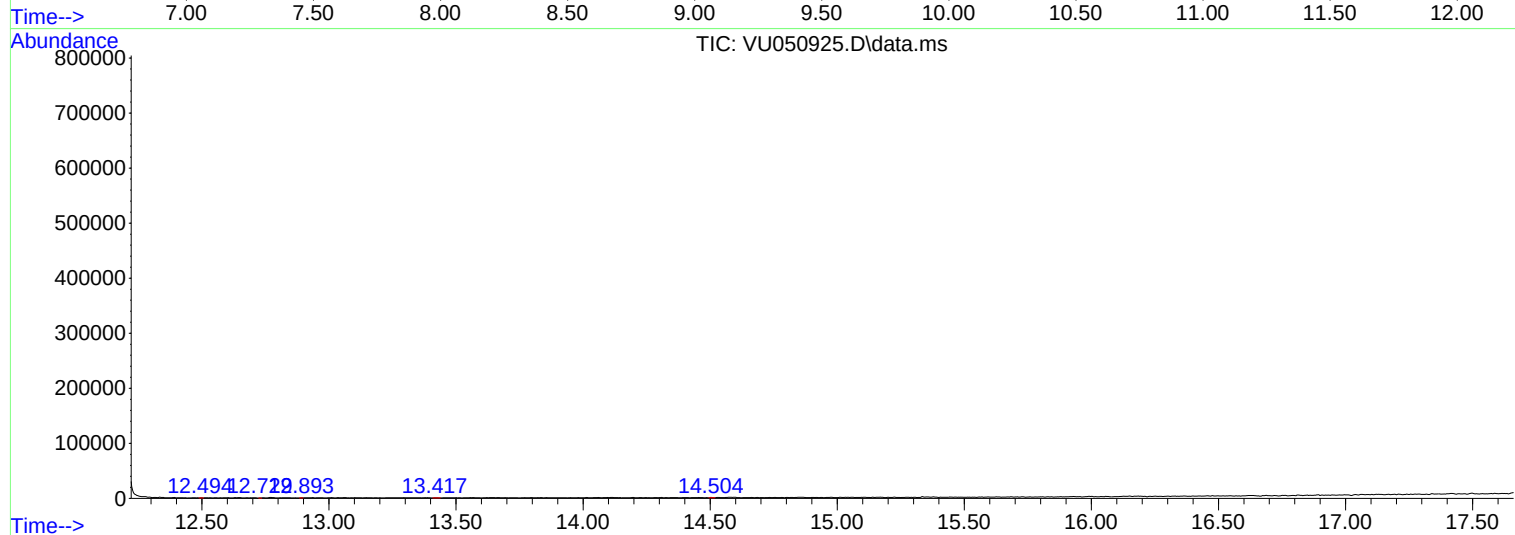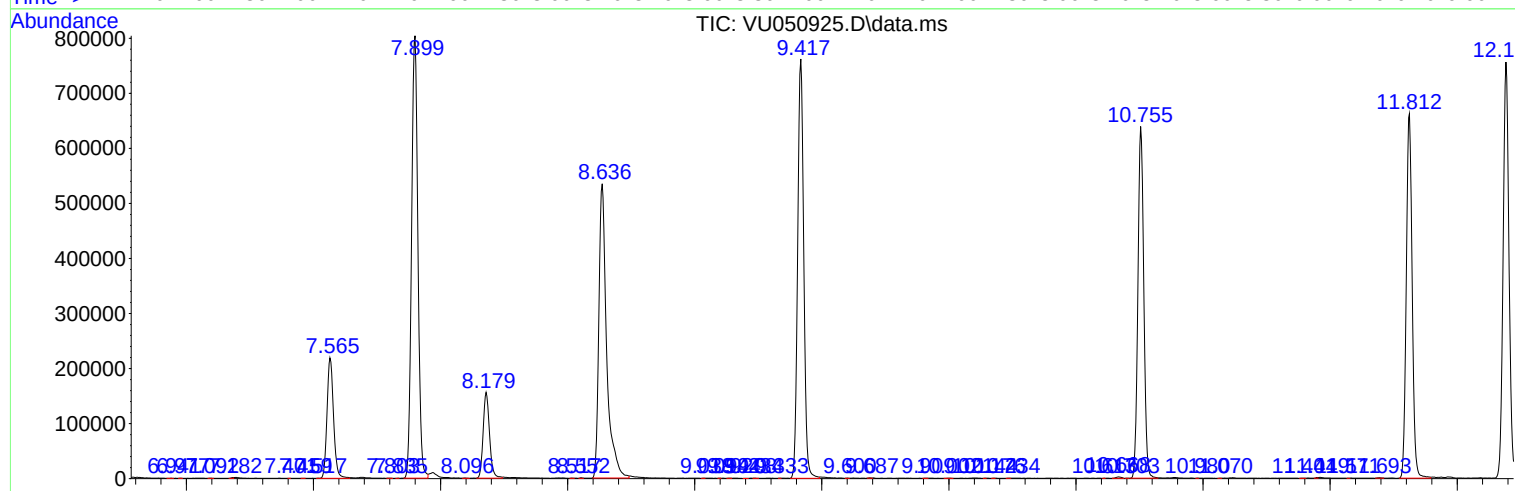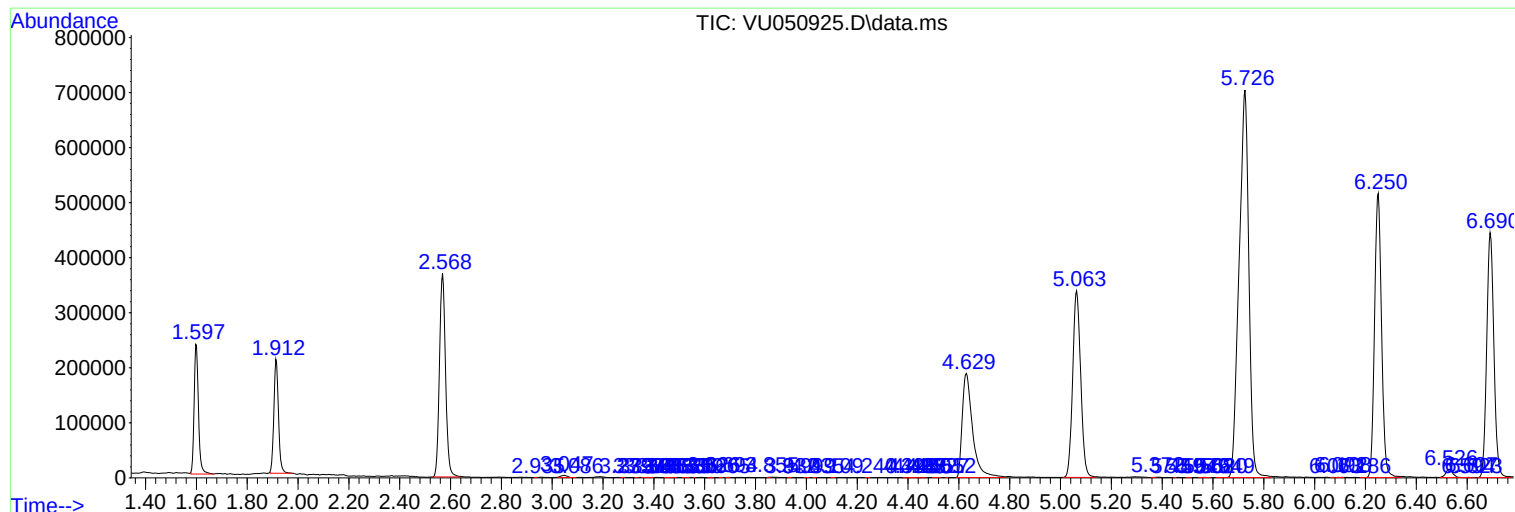

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050925.D
Acq On : 23 Sep 2022 17:31
Operator : JC/MD
Sample : VIBLK138
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050925.D
Acq On : 23 Sep 2022 17:31
Operator : JC/MD
Sample : VIBLK138
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
