

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050926.D
 Acq On : 23 Sep 2022 17:54
 Operator : JC/MD
 Sample : N4650-13DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ08DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	104	rVB	218356	264883	14.11%	1.849%
2	1.909	169	177	193	rVB	210829	276641	14.74%	1.931%
3	2.565	369	381	400	rBV	358768	607105	32.34%	4.238%
4	2.729	428	432	438	rVB3	728	807	0.04%	0.006%
5	2.909	486	488	493	rBV3	388	267	0.01%	0.002%
6	2.941	493	498	501	rBV3	312	344	0.02%	0.002%
7	3.047	521	531	541	rVB4	5646	10575	0.56%	0.074%
8	3.186	560	574	586	rBV2	4950	11590	0.62%	0.081%
9	3.263	596	598	606	rVB3	269	258	0.01%	0.002%
10	3.353	619	626	628	rBV2	2207	2525	0.13%	0.018%
11	3.507	671	674	678	rVB2	423	313	0.02%	0.002%
12	3.671	723	725	732	rVB3	347	322	0.02%	0.002%
13	3.780	754	759	763	rVB2	296	261	0.01%	0.002%
14	3.870	769	787	808	rBV2	75808	180819	9.63%	1.262%
15	4.147	870	873	879	rBV2	371	378	0.02%	0.003%
16	4.205	886	891	894	rVB2	417	334	0.02%	0.002%
17	4.340	930	933	939	rVB2	382	232	0.01%	0.002%
18	4.401	947	952	954	rBV2	428	354	0.02%	0.002%
19	4.462	968	971	975	rVV	386	256	0.01%	0.002%
20	4.626	1009	1022	1028	rBV	216235	483149	25.74%	3.372%
21	5.063	1142	1158	1178	rBV	340056	749704	39.93%	5.233%
22	5.314	1219	1236	1255	rBV2	175888	399804	21.30%	2.791%
23	5.533	1301	1304	1307	rVB2	510	290	0.02%	0.002%
24	5.607	1322	1327	1331	rBV3	325	323	0.02%	0.002%
25	5.722	1339	1363	1396	rBV3	689545	1877400	100.00%	13.104%
26	6.028	1456	1458	1461	rBV2	363	239	0.01%	0.002%
27	6.044	1461	1463	1465	rBV3	497	261	0.01%	0.002%
28	6.108	1476	1483	1485	rBV2	377	437	0.02%	0.003%
29	6.247	1508	1526	1558	rBV	549383	1035691	55.17%	7.229%
30	6.533	1604	1615	1630	rVB6	17402	36418	1.94%	0.254%
31	6.690	1648	1664	1685	rBV	448755	872264	46.46%	6.088%
32	6.877	1719	1722	1726	rBV2	568	351	0.02%	0.002%
33	6.899	1727	1729	1733	rVB3	668	399	0.02%	0.003%
34	7.044	1770	1774	1777	rBV	619	593	0.03%	0.004%
35	7.185	1808	1818	1836	rVB6	2485	5327	0.28%	0.037%
36	7.266	1841	1843	1849	rBV3	419	330	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050926.D
 Acq On : 23 Sep 2022 17:54
 Operator : JC/MD
 Sample : N4650-13DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ08DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.565	1922	1936	1955	rBV	218944	389769	20.76%	2.721%
38	7.690	1968	1975	1988	rVB9	1694	2904	0.15%	0.020%
39	7.896	2023	2039	2055	rBV	777920	1335435	71.13%	9.321%
40	8.179	2114	2127	2146	rBV	154719	269265	14.34%	1.879%
41	8.343	2175	2178	2181	rBV2	646	359	0.02%	0.003%
42	8.465	2214	2216	2226	rVB3	1282	1507	0.08%	0.011%
43	8.510	2226	2230	2234	rVB2	300	249	0.01%	0.002%
44	8.552	2234	2243	2256	rBV3	11680	19156	1.02%	0.134%
45	8.632	2256	2268	2297	rBV3	580518	1176848	62.68%	8.214%
46	8.861	2335	2339	2340	rBV2	397	300	0.02%	0.002%
47	8.906	2350	2353	2355	rBV2	467	293	0.02%	0.002%
48	8.999	2378	2382	2385	rBV2	399	323	0.02%	0.002%
49	9.070	2401	2404	2407	rBV3	330	232	0.01%	0.002%
50	9.240	2455	2457	2462	rVB2	317	292	0.02%	0.002%
51	9.359	2490	2494	2498	rBV2	362	296	0.02%	0.002%
52	9.417	2498	2512	2541	rBV	752408	1262678	67.26%	8.813%
53	9.639	2577	2581	2583	rBV2	372	277	0.01%	0.002%
54	9.690	2592	2597	2599	rBV2	839	725	0.04%	0.005%
55	9.806	2630	2633	2636	rBV2	372	257	0.01%	0.002%
56	9.854	2642	2648	2651	rBV	368	378	0.02%	0.003%
57	10.018	2690	2699	2703	rBV3	231	369	0.02%	0.003%
58	10.102	2720	2725	2730	rBV3	571	676	0.04%	0.005%
59	10.333	2793	2797	2802	rBV2	283	285	0.02%	0.002%
60	10.603	2877	2881	2884	rBV2	283	266	0.01%	0.002%
61	10.623	2885	2887	2892	rVV	359	263	0.01%	0.002%
62	10.668	2897	2901	2908	rVB5	1746	2158	0.11%	0.015%
63	10.754	2915	2928	2955	rBV	645004	1033646	55.06%	7.215%
64	10.877	2962	2966	2967	rBV2	495	366	0.02%	0.003%
65	10.893	2967	2971	2976	rVB5	1189	1373	0.07%	0.010%
66	10.989	2997	3001	3003	rBV	399	303	0.02%	0.002%
67	11.021	3008	3011	3012	rVV2	405	237	0.01%	0.002%
68	11.044	3015	3018	3021	rVV	430	292	0.02%	0.002%
69	11.089	3028	3032	3035	rBV3	557	505	0.03%	0.004%
70	11.118	3035	3041	3047	rVV5	1460	1944	0.10%	0.014%
71	11.147	3047	3050	3052	rVB2	505	296	0.02%	0.002%
72	11.172	3055	3058	3064	rBV2	268	302	0.02%	0.002%
73	11.314	3096	3102	3104	rBV2	705	610	0.03%	0.004%
74	11.410	3128	3132	3134	rBV	564	362	0.02%	0.003%
75	11.455	3137	3146	3149	rBV4	1140	1497	0.08%	0.010%
76	11.632	3196	3201	3205	rBV2	361	405	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050926.D
 Acq On : 23 Sep 2022 17:54
 Operator : JC/MD
 Sample : N4650-13DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ08DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.751	3235	3238	3244	rVB3	471	451	0.02%	0.003%
78	11.809	3244	3256	3280	rBV	576379	920411	49.03%	6.424%
79	11.973	3304	3307	3313	rVB4	1162	893	0.05%	0.006%
80	12.192	3358	3375	3398	rBV	660128	1065979	56.78%	7.440%
81	12.529	3477	3480	3486	rVB3	510	453	0.02%	0.003%
82	12.819	3567	3570	3573	rBV2	575	340	0.02%	0.002%
83	12.928	3600	3604	3607	rVB2	464	367	0.02%	0.003%
84	12.947	3607	3610	3612	rBV	589	362	0.02%	0.003%
85	12.999	3623	3626	3630	rVB2	417	316	0.02%	0.002%
86	13.057	3641	3644	3647	rBV2	534	372	0.02%	0.003%
87	13.176	3678	3681	3683	rBV	461	314	0.02%	0.002%
88	13.475	3770	3774	3776	rBV3	443	384	0.02%	0.003%
89	13.523	3787	3789	3795	rVB3	427	299	0.02%	0.002%
90	13.552	3795	3798	3801	rBV2	286	248	0.01%	0.002%
91	13.651	3825	3829	3833	rVB	553	440	0.02%	0.003%
92	13.680	3833	3838	3839	rBV2	505	421	0.02%	0.003%
93	13.909	3906	3909	3912	rBV3	378	244	0.01%	0.002%
94	14.584	4113	4119	4125	rVB5	1070	1181	0.06%	0.008%
95	14.793	4181	4184	4186	rBV	527	326	0.02%	0.002%
96	14.954	4231	4234	4239	rBV3	562	494	0.03%	0.003%
97	15.314	4343	4346	4347	rBV2	700	377	0.02%	0.003%
98	15.397	4370	4372	4377	rVB4	673	448	0.02%	0.003%
99	15.719	4469	4472	4476	rBV4	890	982	0.05%	0.007%
100	15.777	4487	4490	4496	rBV5	1317	1697	0.09%	0.012%




Sum of corrected areas: 14326741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050926.D
Acq On : 23 Sep 2022 17:54
Operator : JC/MD
Sample : N4650-13DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

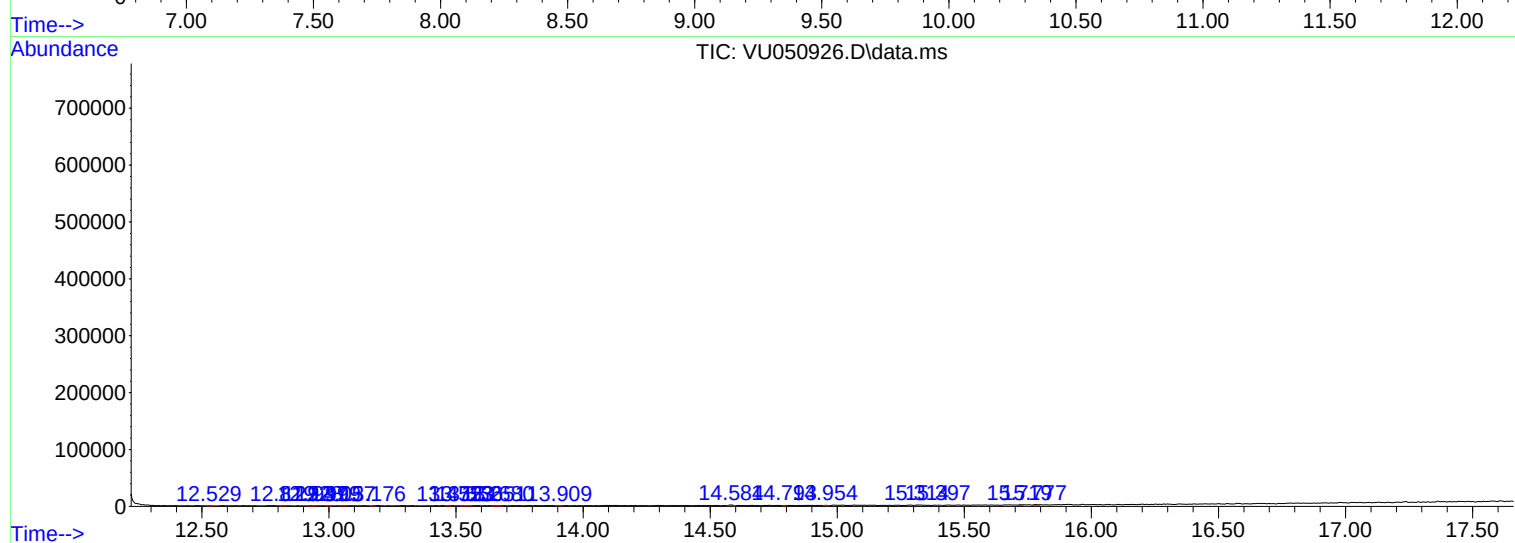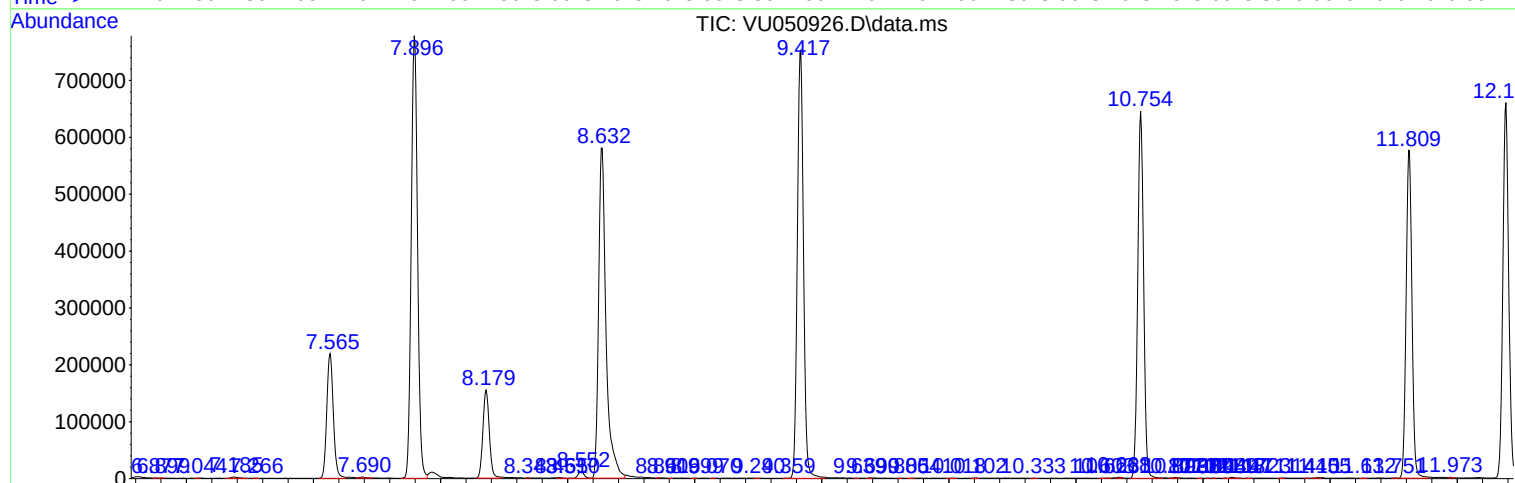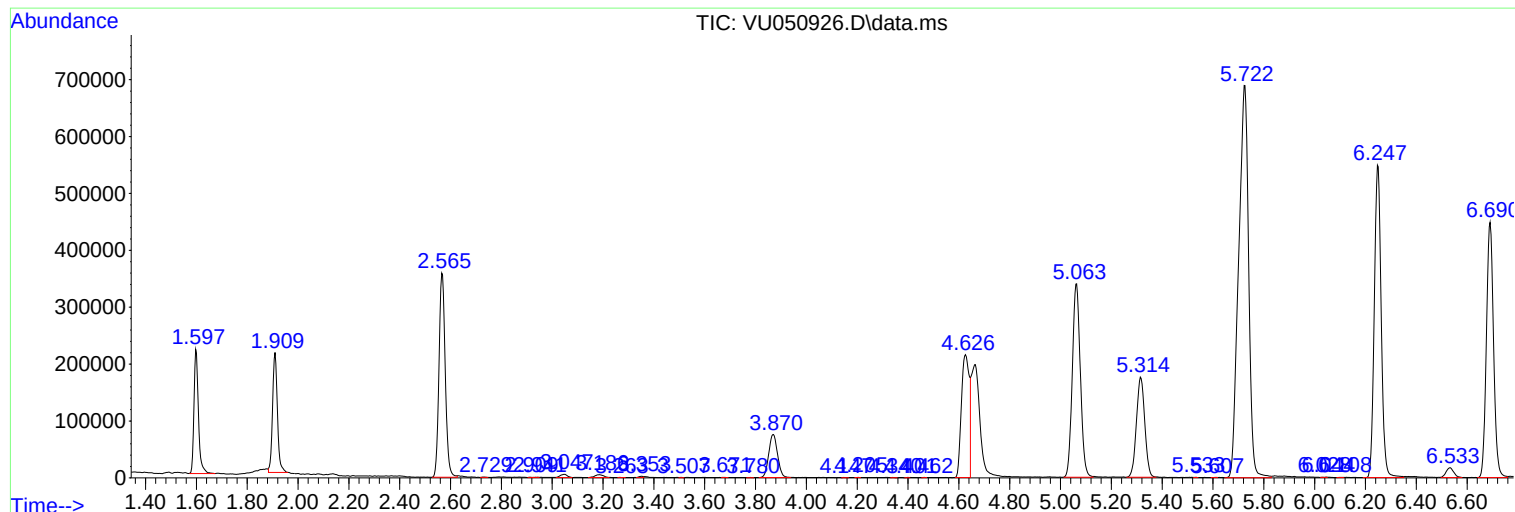

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050926.D
Acq On : 23 Sep 2022 17:54
Operator : JC/MD
Sample : N4650-13DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050926.D
Acq On : 23 Sep 2022 17:54
Operator : JC/MD
Sample : N4650-13DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc