

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050927.D
 Acq On : 23 Sep 2022 18:18
 Operator : JC/MD
 Sample : N4651-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	218717	258127	13.90%	1.908%
2	1.909	169	177	200	rVB	210719	285037	15.35%	2.107%
3	2.565	368	381	401	rBV	354114	590431	31.79%	4.365%
4	2.748	435	438	442	rBV3	324	249	0.01%	0.002%
5	2.957	496	503	511	rVB5	1033	1444	0.08%	0.011%
6	2.999	512	516	519	rVV2	495	399	0.02%	0.003%
7	3.047	520	531	542	rVB3	5566	10591	0.57%	0.078%
8	3.182	561	573	587	rVB2	4158	9143	0.49%	0.068%
9	3.256	591	596	600	rBV3	367	353	0.02%	0.003%
10	3.340	618	622	625	rBV2	399	361	0.02%	0.003%
11	3.494	666	670	672	rBV	313	274	0.01%	0.002%
12	3.542	680	685	690	rBV2	407	433	0.02%	0.003%
13	3.774	750	757	760	rBV	256	305	0.02%	0.002%
14	3.793	760	763	768	rVV2	283	285	0.02%	0.002%
15	3.822	768	772	776	rBV2	299	255	0.01%	0.002%
16	3.877	787	789	793	rVV2	267	225	0.01%	0.002%
17	3.919	798	802	806	rVB2	340	334	0.02%	0.002%
18	3.944	806	810	813	rBV	516	358	0.02%	0.003%
19	4.214	890	894	900	rVV2	461	462	0.02%	0.003%
20	4.340	928	933	938	rVB2	375	361	0.02%	0.003%
21	4.446	964	966	969	rVB	485	265	0.01%	0.002%
22	4.465	969	972	976	rBV	324	281	0.02%	0.002%
23	4.549	992	998	1000	rBV2	266	272	0.01%	0.002%
24	4.626	1009	1022	1060	rBV	210535	565781	30.46%	4.182%
25	4.848	1087	1091	1098	rVB5	584	750	0.04%	0.006%
26	5.063	1140	1158	1186	rBV	334553	740677	39.88%	5.475%
27	5.269	1218	1222	1223	rBV2	679	402	0.02%	0.003%
28	5.366	1249	1252	1256	rBV2	662	497	0.03%	0.004%
29	5.478	1282	1287	1290	rBV	577	450	0.02%	0.003%
30	5.542	1305	1307	1313	rVB2	500	310	0.02%	0.002%
31	5.722	1341	1363	1394	rBV2	677289	1857296	100.00%	13.729%
32	5.919	1421	1424	1425	rBV3	694	406	0.02%	0.003%
33	6.047	1462	1464	1473	rVB3	878	899	0.05%	0.007%
34	6.115	1483	1485	1491	rVB2	619	472	0.03%	0.003%
35	6.247	1511	1526	1547	rBV	503996	960554	51.72%	7.100%
36	6.530	1603	1614	1628	rVB2	14943	29304	1.58%	0.217%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050927.D
 Acq On : 23 Sep 2022 18:18
 Operator : JC/MD
 Sample : N4651-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.607	1634	1638	1640	rBV2	420	290	0.02%	0.002%
38	6.690	1646	1664	1687	rBV	445258	872369	46.97%	6.449%
39	6.928	1731	1738	1741	rBV5	604	801	0.04%	0.006%
40	6.986	1753	1756	1759	rBV3	437	270	0.01%	0.002%
41	7.050	1773	1776	1777	rBV	429	227	0.01%	0.002%
42	7.189	1812	1819	1829	rVV4	2326	4166	0.22%	0.031%
43	7.230	1829	1832	1835	rVB2	365	284	0.02%	0.002%
44	7.565	1922	1936	1961	rBV	214338	382353	20.59%	2.826%
45	7.693	1969	1976	1980	rVB6	1178	1498	0.08%	0.011%
46	7.790	1999	2006	2010	rBV3	560	545	0.03%	0.004%
47	7.896	2022	2039	2056	rBV	777230	1327952	71.50%	9.816%
48	8.025	2077	2079	2084	rVB3	555	276	0.01%	0.002%
49	8.073	2091	2094	2096	rBV2	325	228	0.01%	0.002%
50	8.179	2114	2127	2144	rBV	154779	267361	14.40%	1.976%
51	8.632	2254	2268	2317	rBV3	569748	1180986	63.59%	8.730%
52	8.851	2333	2336	2339	rVV3	653	334	0.02%	0.002%
53	8.976	2371	2375	2379	rBV3	429	529	0.03%	0.004%
54	9.021	2387	2389	2392	rBV2	384	228	0.01%	0.002%
55	9.156	2427	2431	2435	rBV2	403	285	0.02%	0.002%
56	9.356	2491	2493	2498	rBV2	296	242	0.01%	0.002%
57	9.417	2498	2512	2538	rBV	710075	1189046	64.02%	8.790%
58	9.552	2551	2554	2563	rVV4	812	751	0.04%	0.006%
59	9.690	2591	2597	2599	rBV2	798	677	0.04%	0.005%
60	9.780	2619	2625	2628	rBV2	409	398	0.02%	0.003%
61	10.063	2710	2713	2715	rBV	420	263	0.01%	0.002%
62	10.105	2723	2726	2730	rVB3	519	424	0.02%	0.003%
63	10.320	2789	2793	2797	rBV2	420	419	0.02%	0.003%
64	10.417	2818	2823	2826	rBV2	373	373	0.02%	0.003%
65	10.478	2840	2842	2846	rVB2	356	231	0.01%	0.002%
66	10.607	2879	2882	2885	rBV2	374	241	0.01%	0.002%
67	10.671	2893	2902	2909	rVB3	2178	2930	0.16%	0.022%
68	10.754	2915	2928	2951	rBV	640926	1031900	55.56%	7.628%
69	10.893	2968	2971	2979	rVB4	1090	1113	0.06%	0.008%
70	11.118	3035	3041	3046	rBV6	1428	1915	0.10%	0.014%
71	11.324	3100	3105	3110	rVB2	475	399	0.02%	0.003%
72	11.375	3119	3121	3126	rVB3	503	376	0.02%	0.003%
73	11.455	3139	3146	3149	rBV5	1201	1341	0.07%	0.010%
74	11.542	3167	3173	3175	rBV2	250	292	0.02%	0.002%
75	11.700	3218	3222	3228	rVB2	636	481	0.03%	0.004%
76	11.748	3234	3237	3242	rBV2	419	269	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050927.D
 Acq On : 23 Sep 2022 18:18
 Operator : JC/MD
 Sample : N4651-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.809	3243	3256	3278	rBV	533028	864819	46.56%	6.393%
78	11.941	3295	3297	3299	rVB2	791	250	0.01%	0.002%
79	11.954	3299	3301	3304	rVV3	616	486	0.03%	0.004%
80	11.970	3304	3306	3314	rVB5	1601	1585	0.09%	0.012%
81	12.037	3324	3327	3330	rVB2	393	255	0.01%	0.002%
82	12.092	3342	3344	3349	rVB	624	373	0.02%	0.003%
83	12.192	3360	3375	3399	rBV	646475	1058138	56.97%	7.822%
84	12.385	3427	3435	3437	rBV5	668	981	0.05%	0.007%
85	12.497	3468	3470	3475	rVB2	450	309	0.02%	0.002%
86	12.584	3494	3497	3499	rBV2	396	249	0.01%	0.002%
87	12.770	3551	3555	3559	rVB4	805	819	0.04%	0.006%
88	12.896	3591	3594	3597	rBV2	344	300	0.02%	0.002%
89	12.925	3600	3603	3607	rVV4	486	428	0.02%	0.003%
90	13.237	3698	3700	3704	rVV4	425	357	0.02%	0.003%
91	13.397	3746	3750	3753	rBV3	739	668	0.04%	0.005%
92	13.520	3784	3788	3794	rBV3	599	845	0.05%	0.006%
93	13.774	3863	3867	3870	rBV2	288	336	0.02%	0.002%
94	15.140	4290	4292	4296	rVB2	656	370	0.02%	0.003%
95	15.163	4296	4299	4304	rBV5	644	622	0.03%	0.005%
96	15.330	4349	4351	4352	rBV	607	250	0.01%	0.002%
97	15.381	4365	4367	4370	rVB	624	325	0.02%	0.002%
98	15.410	4373	4376	4381	rVB4	839	570	0.03%	0.004%
99	15.478	4390	4397	4401	rBV6	946	1164	0.06%	0.009%
100	15.500	4403	4404	4408	rBV3	667	398	0.02%	0.003%




Sum of corrected areas: 13528003

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050927.D
Acq On : 23 Sep 2022 18:18
Operator : JC/MD
Sample : N4651-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

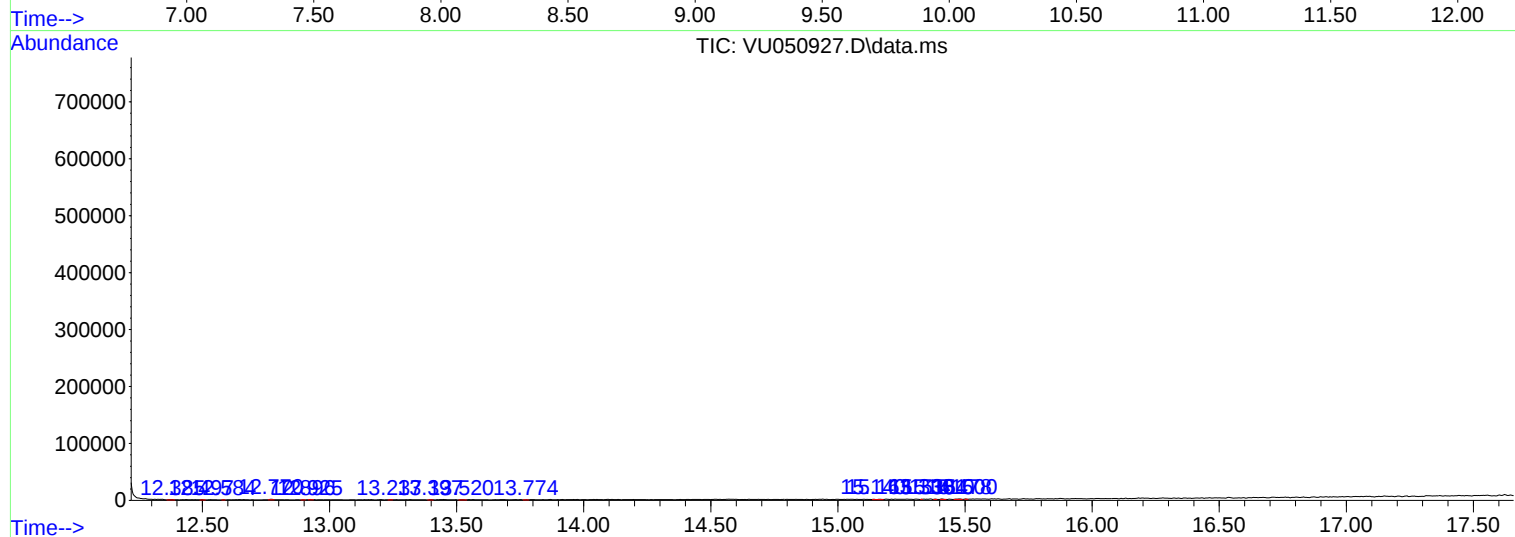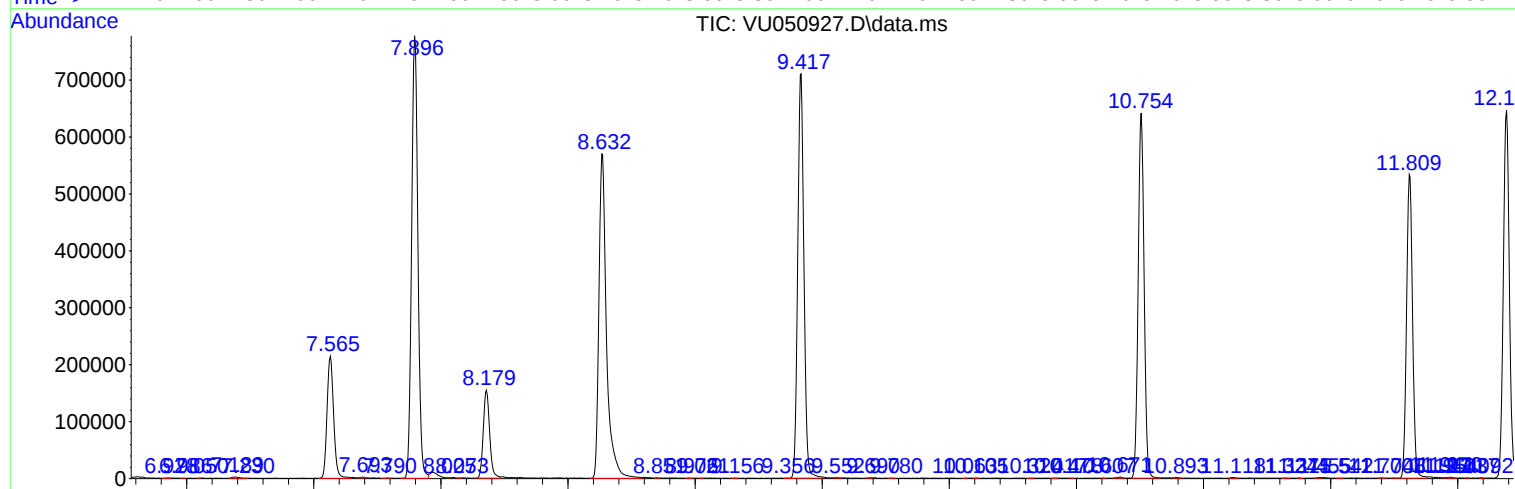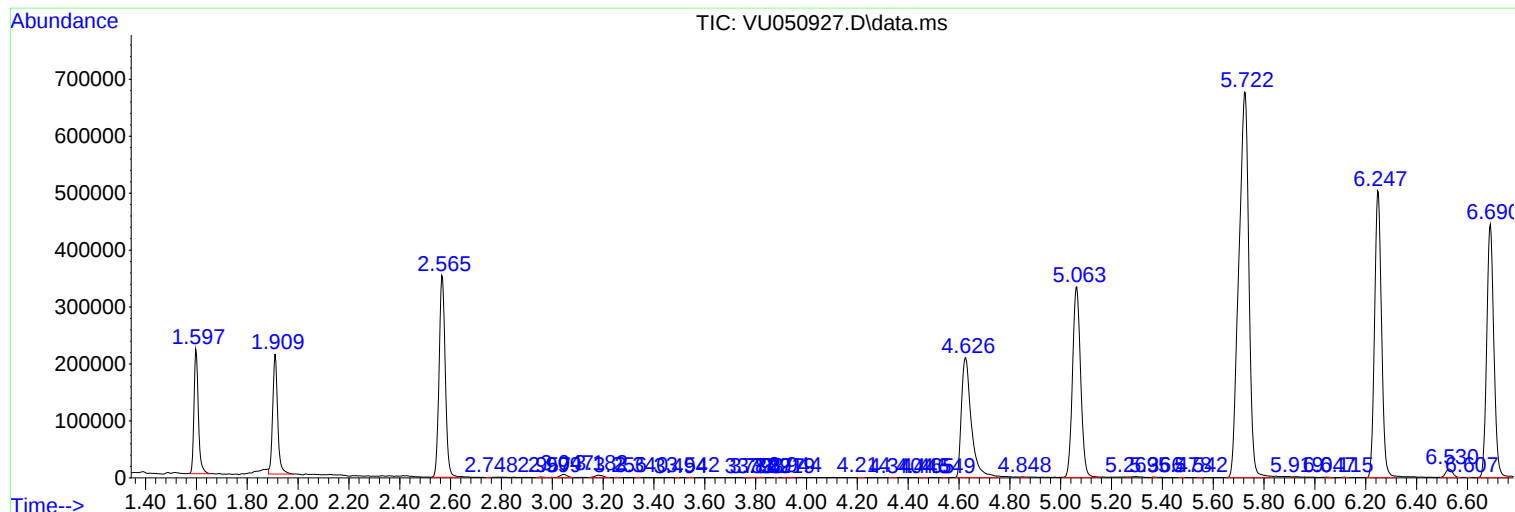

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050927.D
Acq On : 23 Sep 2022 18:18
Operator : JC/MD
Sample : N4651-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050927.D
Acq On : 23 Sep 2022 18:18
Operator : JC/MD
Sample : N4651-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc