

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050928.D
 Acq On : 23 Sep 2022 18:41
 Operator : JC/MD
 Sample : N4650-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	220605	263276	13.93%	1.909%
2	1.906	169	176	196	rVB	206485	276255	14.62%	2.004%
3	2.565	368	381	400	rBV	362732	601382	31.82%	4.362%
4	2.684	416	418	422	rVB3	521	301	0.02%	0.002%
5	2.742	433	436	439	rVB	410	268	0.01%	0.002%
6	2.765	440	443	445	rBV2	359	273	0.01%	0.002%
7	2.835	463	465	468	rVB2	650	292	0.02%	0.002%
8	2.858	468	472	477	rBV2	591	539	0.03%	0.004%
9	2.890	477	482	487	rBV2	829	931	0.05%	0.007%
10	2.954	500	502	505	rBV	412	336	0.02%	0.002%
11	2.970	505	507	512	rVB3	662	555	0.03%	0.004%
12	3.044	520	530	540	rVB3	4879	8879	0.47%	0.064%
13	3.183	564	573	584	rVB2	1687	3462	0.18%	0.025%
14	3.263	595	598	602	rVB2	363	236	0.01%	0.002%
15	3.321	610	616	620	rVB2	397	316	0.02%	0.002%
16	3.350	620	625	628	rBV2	314	282	0.01%	0.002%
17	3.404	638	642	647	rBV3	239	218	0.01%	0.002%
18	3.584	692	698	704	rBV2	241	313	0.02%	0.002%
19	3.655	715	720	722	rBV	367	289	0.02%	0.002%
20	3.748	744	749	755	rVB2	320	328	0.02%	0.002%
21	3.867	783	786	794	rVB3	379	388	0.02%	0.003%
22	4.031	833	837	842	rBV2	232	243	0.01%	0.002%
23	4.221	891	896	899	rBV	285	299	0.02%	0.002%
24	4.305	918	922	928	rVB3	296	339	0.02%	0.002%
25	4.504	982	984	988	rBV2	294	238	0.01%	0.002%
26	4.623	1008	1021	1059	rBV	211657	556664	29.46%	4.037%
27	4.961	1123	1126	1133	rBV2	316	342	0.02%	0.002%
28	4.996	1133	1137	1140	rBV	514	373	0.02%	0.003%
29	5.060	1140	1157	1183	rBV	339508	758748	40.15%	5.503%
30	5.504	1288	1295	1297	rBV2	421	386	0.02%	0.003%
31	5.600	1320	1325	1327	rBV2	283	205	0.01%	0.001%
32	5.723	1342	1363	1394	rBV2	696947	1889793	100.00%	13.706%
33	5.973	1437	1441	1444	rBV3	664	542	0.03%	0.004%
34	6.109	1480	1483	1487	rVV2	489	397	0.02%	0.003%
35	6.247	1512	1526	1550	rBV	510388	977627	51.73%	7.091%
36	6.436	1583	1585	1590	rVB4	462	379	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050928.D
 Acq On : 23 Sep 2022 18:41
 Operator : JC/MD
 Sample : N4650-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.526	1602	1613	1628	rVB4	15112	29899	1.58%	0.217%
38	6.690	1649	1664	1686	rBV	451198	886888	46.93%	6.432%
39	7.057	1774	1778	1781	rBV2	376	426	0.02%	0.003%
40	7.189	1812	1819	1828	rBV6	1914	3379	0.18%	0.025%
41	7.224	1828	1830	1834	rVB3	590	311	0.02%	0.002%
42	7.565	1922	1936	1952	rBV	219210	390130	20.64%	2.830%
43	7.896	2025	2039	2054	rBV	801987	1366801	72.33%	9.913%
44	8.179	2112	2127	2142	rBV2	157477	270239	14.30%	1.960%
45	8.517	2229	2232	2234	rBV	452	276	0.01%	0.002%
46	8.633	2256	2268	2306	rBV3	584405	1196369	63.31%	8.677%
47	9.243	2454	2458	2461	rVV	282	222	0.01%	0.002%
48	9.295	2472	2474	2478	rBV2	356	246	0.01%	0.002%
49	9.417	2498	2512	2538	rBV	715409	1202237	63.62%	8.720%
50	9.623	2573	2576	2579	rVB2	753	460	0.02%	0.003%
51	9.652	2583	2585	2589	rVB2	540	354	0.02%	0.003%
52	9.697	2591	2599	2608	rVB4	1297	1868	0.10%	0.014%
53	9.745	2609	2614	2619	rBV2	465	466	0.02%	0.003%
54	9.948	2675	2677	2681	rVB2	370	246	0.01%	0.002%
55	9.970	2681	2684	2686	rBV	295	217	0.01%	0.002%
56	10.005	2691	2695	2702	rBV2	361	395	0.02%	0.003%
57	10.095	2720	2723	2725	rBV2	531	287	0.02%	0.002%
58	10.124	2730	2732	2735	rVB3	380	223	0.01%	0.002%
59	10.253	2770	2772	2778	rVB2	303	241	0.01%	0.002%
60	10.308	2786	2789	2793	rBV	327	229	0.01%	0.002%
61	10.433	2825	2828	2833	rVB	350	261	0.01%	0.002%
62	10.459	2833	2836	2839	rBV2	416	346	0.02%	0.003%
63	10.485	2839	2844	2849	rBV2	411	555	0.03%	0.004%
64	10.607	2880	2882	2886	rVB	344	234	0.01%	0.002%
65	10.668	2891	2901	2910	rVB7	1653	3052	0.16%	0.022%
66	10.755	2915	2928	2946	rBV	644122	1045635	55.33%	7.584%
67	10.861	2958	2961	2964	rVB4	479	254	0.01%	0.002%
68	11.112	3034	3039	3044	rBV4	969	1367	0.07%	0.010%
69	11.214	3068	3071	3076	rBV2	327	307	0.02%	0.002%
70	11.327	3104	3106	3112	rBV	279	297	0.02%	0.002%
71	11.456	3138	3146	3159	rVB6	1457	2586	0.14%	0.019%
72	11.536	3167	3171	3175	rBV3	389	361	0.02%	0.003%
73	11.562	3176	3179	3181	rBV2	340	210	0.01%	0.002%
74	11.697	3213	3221	3223	rBV3	736	874	0.05%	0.006%
75	11.745	3232	3236	3237	rBV	485	270	0.01%	0.002%
76	11.809	3244	3256	3281	rBV	577497	918972	48.63%	6.665%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050928.D
 Acq On : 23 Sep 2022 18:41
 Operator : JC/MD
 Sample : N4650-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

77	11.931	3291	3294	3295	rBV3	827	476	0.03%	0.003%
78	12.070	3335	3337	3342	rBB	400	242	0.01%	0.002%
79	12.118	3347	3352	3355	rVB2	357	317	0.02%	0.002%
80	12.144	3357	3360	3361	rBV	422	241	0.01%	0.002%
81	12.192	3361	3375	3406	rVV	679702	1105728	58.51%	8.020%
82	12.459	3455	3458	3460	rBV2	404	268	0.01%	0.002%
83	12.497	3468	3470	3473	rBV2	519	267	0.01%	0.002%
84	12.581	3493	3496	3498	rBV2	577	313	0.02%	0.002%
85	12.755	3547	3550	3554	rBV3	533	535	0.03%	0.004%
86	12.825	3569	3572	3574	rBV	510	313	0.02%	0.002%
87	12.874	3584	3587	3589	rVB3	591	342	0.02%	0.002%
88	12.980	3617	3620	3623	rBV2	388	233	0.01%	0.002%
89	13.037	3635	3638	3641	rBV	315	212	0.01%	0.002%
90	13.070	3646	3648	3654	rVB3	390	315	0.02%	0.002%
91	13.156	3672	3675	3678	rVV2	468	354	0.02%	0.003%
92	13.205	3683	3690	3694	rBV3	665	848	0.04%	0.006%
93	13.263	3704	3708	3712	rVB2	386	318	0.02%	0.002%
94	13.285	3712	3715	3717	rBV2	448	345	0.02%	0.003%
95	13.298	3717	3719	3722	rVB	489	253	0.01%	0.002%
96	13.581	3804	3807	3811	rBV3	482	353	0.02%	0.003%
97	13.751	3858	3860	3863	rBV2	386	256	0.01%	0.002%
98	14.002	3935	3938	3941	rVB3	407	265	0.01%	0.002%
99	14.433	4068	4072	4074	rBV	496	414	0.02%	0.003%
100	15.279	4332	4335	4343	rVB4	956	922	0.05%	0.007%




Sum of corrected areas: 13787814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050928.D
Acq On : 23 Sep 2022 18:41
Operator : JC/MD
Sample : N4650-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

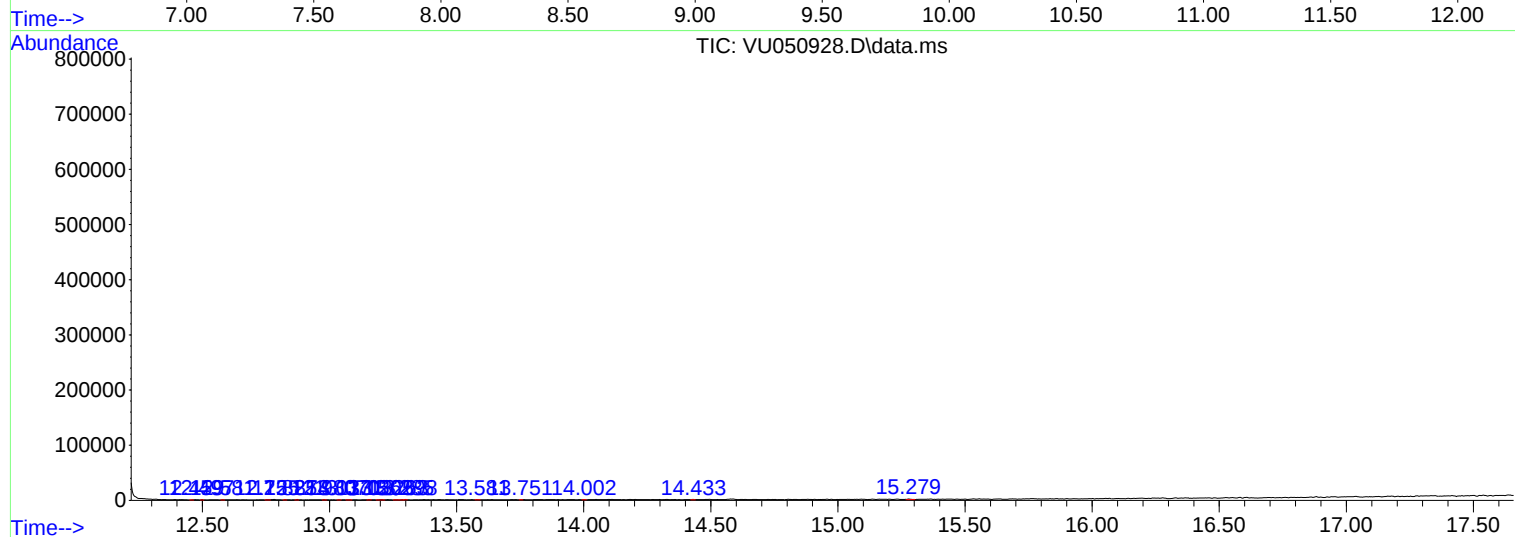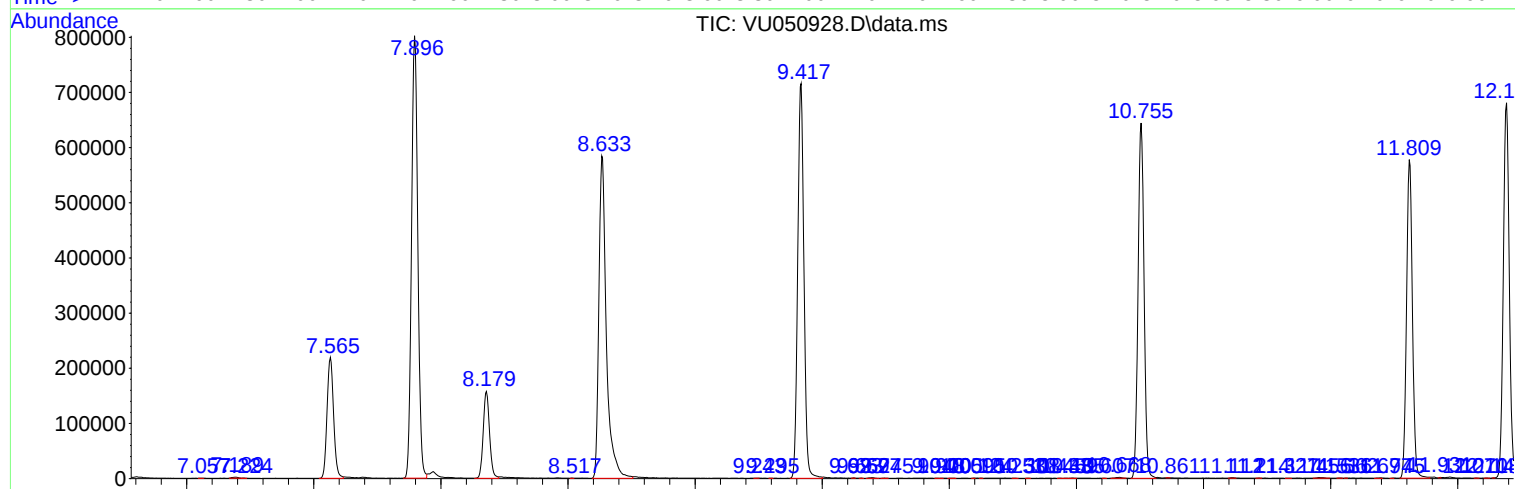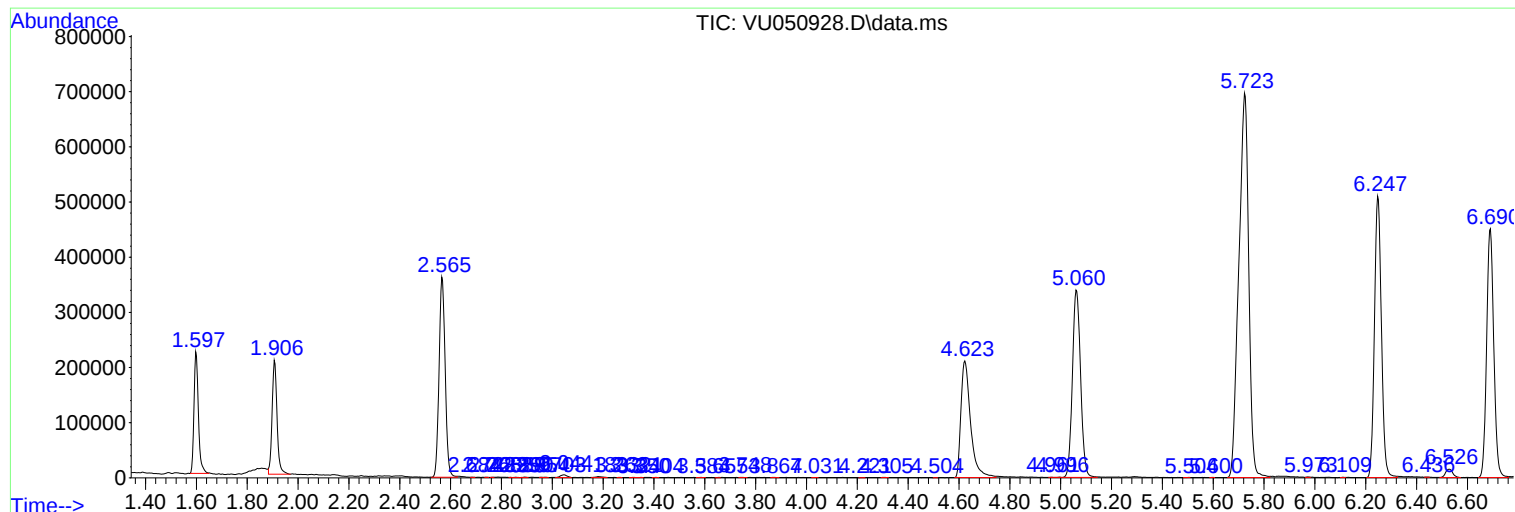

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050928.D
Acq On : 23 Sep 2022 18:41
Operator : JC/MD
Sample : N4650-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
Data File : VU050928.D
Acq On : 23 Sep 2022 18:41
Operator : JC/MD
Sample : N4650-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------