


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092322\
 Data File : VU050914.D
 Acq On : 23 Sep 2022 11:41
 Operator : JC/MD
 Sample : BFB130
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB130

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis
 Last Update : Mon Sep 26 20:52:47 2022

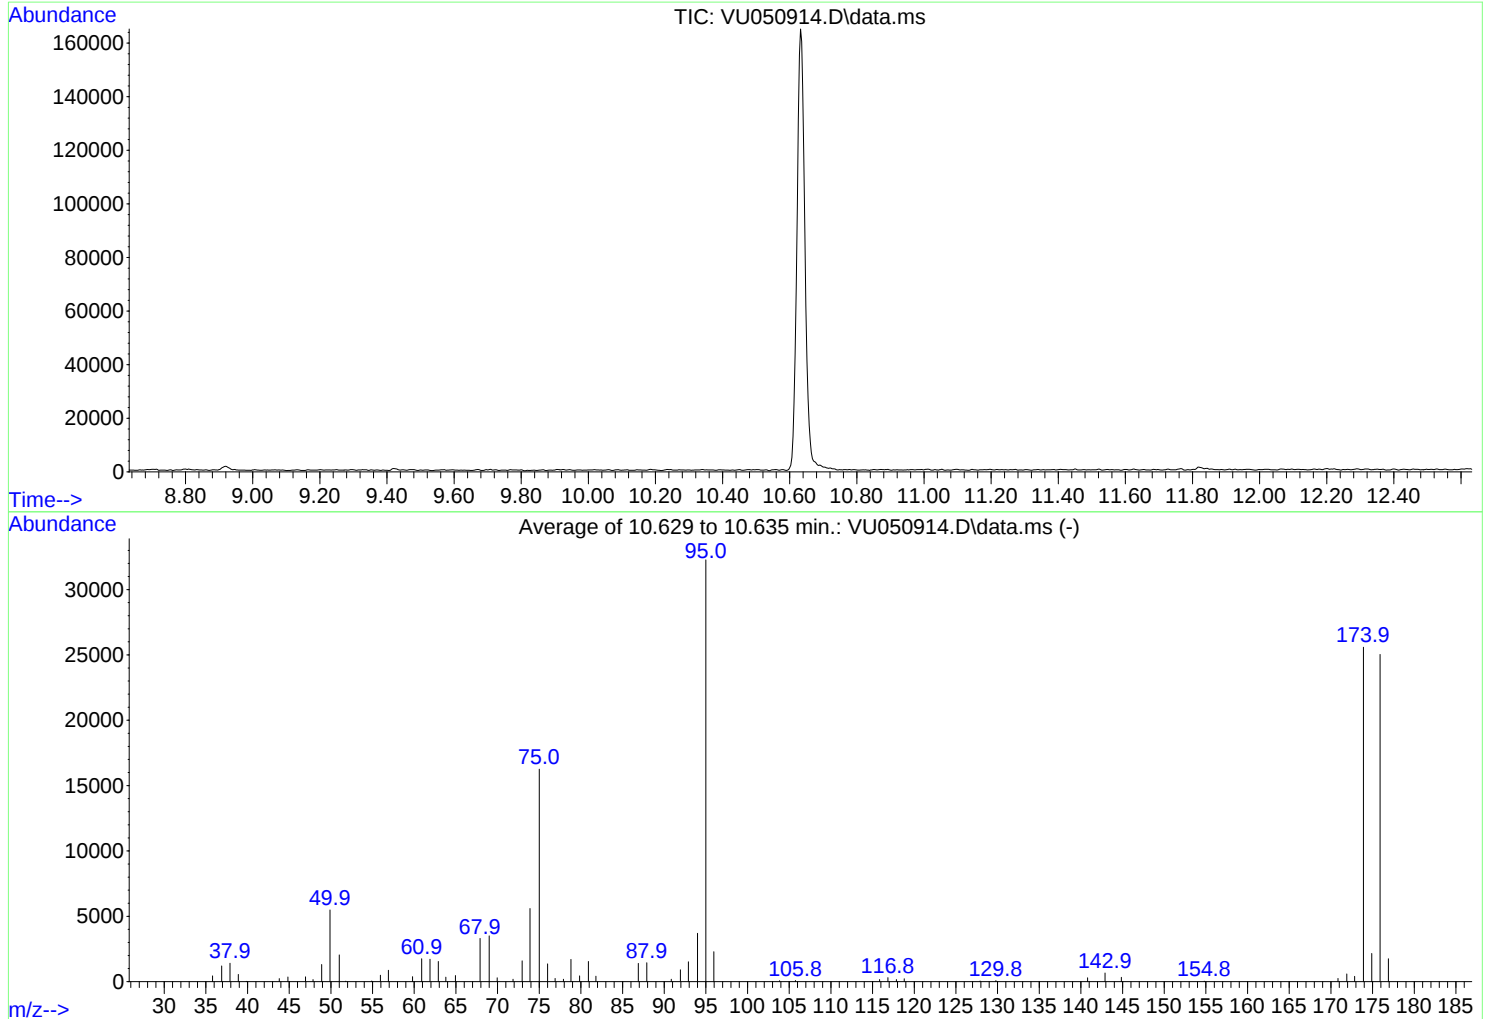

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	5481	PASS
75	95	30	80	50.4	16254	PASS
95	95	100	100	100.0	32275	PASS
96	95	5	9	7.1	2287	PASS
173	174	0.00	2	1.6	407	PASS
174	95	50	120	79.3	25592	PASS
175	174	5	9	8.4	2155	PASS
176	174	95	101	97.9	25043	PASS
177	176	5	9	7.0	1752	PASS

Scan 2878 (10.594 min): VU050914.D\data.ms
BFB130

m/z	Abundance
39.90	181.0
43.90	452.0

Instrument :
MSVOA_U
ClientSampleId :
BFB130

m/z	Abundance
35.80	456.0
36.90	1107.0
37.90	1307.0
38.90	529.0
39.80	208.0
43.80	639.0
44.80	310.0
47.00	411.0
47.90	154.0
48.90	1298.0
49.90	5370.0
51.00	2092.0
55.90	496.0
56.90	858.0
59.80	325.0
60.90	1705.0
61.90	1728.0
62.90	1534.0
63.80	320.0
65.00	446.0
67.90	3280.0
69.00	3507.0
70.00	315.0
71.90	192.0
72.90	1694.0
73.90	5576.0
75.00	15994.0
76.00	1422.0
76.90	209.0
77.90	163.0
78.80	1670.0
79.80	418.0
80.90	1443.0
81.80	444.0
86.90	1347.0
87.90	1330.0
90.80	150.0
92.00	904.0
92.90	1471.0
94.00	3636.0
95.00	31400.0
96.00	2167.0
103.90	116.0
105.80	121.0
115.80	164.0
116.90	311.0
118.00	137.0
118.90	226.0
129.80	128.0
140.80	309.0
142.90	620.0
144.90	322.0
170.80	231.0
171.90	569.0
173.00	344.0
173.90	24664.0
174.90	2107.0
175.90	23528.0
176.90	1655.0

Instrument :
MSVOA_U
ClientSampleId :
BFB130

m/z	Abundance
35.90	450.0
36.90	1230.0
37.90	1440.0
38.90	569.0
39.80	203.0
43.80	713.0
44.90	375.0
46.90	370.0
47.80	152.0
48.90	1355.0
49.90	5657.0
51.00	2127.0
55.90	522.0
56.90	870.0
59.80	388.0
60.90	1758.0
61.90	1748.0
62.90	1551.0
63.80	363.0
65.00	468.0
67.90	3358.0
69.00	3658.0
70.00	286.0
71.90	177.0
72.90	1682.0
73.90	5815.0
75.00	16784.0
76.00	1449.0
76.90	259.0
77.90	209.0
78.80	1758.0
79.90	425.0
80.90	1602.0
81.80	432.0
86.90	1453.0
87.90	1501.0
90.90	187.0
91.90	917.0
92.90	1600.0
94.00	3736.0
95.00	33336.0
96.00	2346.0
103.80	101.0
105.70	122.0
115.80	164.0
116.90	318.0
117.80	163.0
118.80	219.0
129.80	130.0
140.80	307.0
142.90	689.0
144.80	338.0
170.90	259.0
171.90	613.0
172.80	423.0
173.90	26424.0
174.90	2205.0
175.90	25632.0
176.90	1808.0

Instrument :
MSVOA_U
ClientSampleId :
BFB130

m/z	Abundance
35.80	402.0
36.90	1274.0
37.90	1484.0
38.90	561.0
39.90	223.0
43.80	690.0
44.90	370.0
47.00	306.0
47.80	165.0
48.90	1279.0
49.90	5415.0
51.00	1922.0
51.80	121.0
54.90	131.0
56.00	458.0
56.90	880.0
59.80	410.0
60.90	1798.0
61.90	1687.0
62.90	1556.0
63.80	342.0
64.90	491.0
67.90	3263.0
69.00	3332.0
69.90	277.0
71.80	172.0
73.00	1415.0
73.90	5389.0
75.00	15985.0
76.00	1224.0
76.90	256.0
77.90	192.0
78.80	1699.0
79.90	477.0
80.90	1593.0
81.80	377.0
86.90	1376.0
87.90	1515.0
90.90	201.0
91.90	891.0
92.90	1497.0
94.00	3733.0
95.00	32088.0
95.90	2348.0
115.90	141.0
116.80	302.0
117.80	179.0
118.70	214.0
127.90	139.0
140.80	265.0
142.90	681.0
144.80	344.0
154.80	109.0
170.90	245.0
171.90	603.0
172.80	455.0
173.90	25688.0
174.90	2153.0
175.90	25968.0
176.90	1793.0

Instrument :
MSVOA_U
ClientSampleId :
BFB130