

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050939.D
 Acq On : 26 Sep 2022 12:05
 Operator : JC/MD
 Sample : N4747-09DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	102	rVB2	305118	371486	19.89%	2.647%
2	1.912	169	178	194	rVB	193980	255090	13.66%	1.817%
3	2.568	369	382	411	rVB	365144	598859	32.07%	4.267%
4	2.787	440	450	451	rBV4	1375	1511	0.08%	0.011%
5	2.829	460	463	465	rBV2	480	318	0.02%	0.002%
6	2.867	471	475	478	rBV2	456	377	0.02%	0.003%
7	2.941	493	498	500	rBV2	339	298	0.02%	0.002%
8	3.044	521	530	541	rVB2	5534	9546	0.51%	0.068%
9	3.182	559	573	593	rBV2	11051	24345	1.30%	0.173%
10	3.356	616	627	641	rBV2	10754	20351	1.09%	0.145%
11	3.459	653	659	661	rBV2	377	408	0.02%	0.003%
12	3.623	705	710	713	rBV2	360	291	0.02%	0.002%
13	3.681	723	728	733	rBV2	508	607	0.03%	0.004%
14	3.864	778	785	786	rBV3	923	731	0.04%	0.005%
15	4.218	892	895	903	rVB2	292	361	0.02%	0.003%
16	4.308	918	923	929	rBV2	199	268	0.01%	0.002%
17	4.552	994	999	1001	rBV	381	284	0.02%	0.002%
18	4.620	1007	1020	1027	rBV	229948	511610	27.40%	3.645%
19	4.919	1111	1113	1119	rVB3	651	495	0.03%	0.004%
20	5.063	1141	1158	1180	rBV	341834	750300	40.18%	5.346%
21	5.269	1220	1222	1224	rBV2	479	294	0.02%	0.002%
22	5.343	1242	1245	1248	rVB2	638	442	0.02%	0.003%
23	5.366	1248	1252	1253	rBV	817	442	0.02%	0.003%
24	5.391	1258	1260	1263	rVB3	738	388	0.02%	0.003%
25	5.478	1283	1287	1296	rVB2	275	355	0.02%	0.003%
26	5.523	1298	1301	1303	rBV2	421	301	0.02%	0.002%
27	5.536	1303	1305	1309	rVV2	421	265	0.01%	0.002%
28	5.726	1342	1364	1397	rBV2	682742	1867368	100.00%	13.305%
29	5.976	1438	1442	1443	rBV3	476	347	0.02%	0.002%
30	6.089	1474	1477	1481	rVB2	307	258	0.01%	0.002%
31	6.160	1496	1499	1502	rBV2	329	257	0.01%	0.002%
32	6.250	1512	1527	1554	rBV	500361	949263	50.83%	6.763%
33	6.401	1571	1574	1582	rVB4	1083	1145	0.06%	0.008%
34	6.436	1582	1585	1587	rVB2	414	233	0.01%	0.002%
35	6.452	1587	1590	1593	rBV3	508	311	0.02%	0.002%
36	6.475	1594	1597	1602	rVV2	407	371	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050939.D
 Acq On : 26 Sep 2022 12:05
 Operator : JC/MD
 Sample : N4747-09DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.529	1602	1614	1629	rVB3	17526	33623	1.80%	0.240%
38	6.690	1648	1664	1683	rBV	451024	872283	46.71%	6.215%
39	6.870	1718	1720	1724	rVB3	432	236	0.01%	0.002%
40	6.931	1736	1739	1742	rVB	410	229	0.01%	0.002%
41	7.050	1770	1776	1780	rVV2	443	652	0.03%	0.005%
42	7.099	1789	1791	1795	rVB3	437	307	0.02%	0.002%
43	7.185	1812	1818	1828	rVV7	2474	3937	0.21%	0.028%
44	7.385	1875	1880	1884	rBV	346	299	0.02%	0.002%
45	7.427	1884	1893	1898	rBV	197	312	0.02%	0.002%
46	7.459	1900	1903	1907	rVB	385	290	0.02%	0.002%
47	7.565	1922	1936	1961	rBV	228291	399842	21.41%	2.849%
48	7.787	2002	2005	2006	rBV3	448	270	0.01%	0.002%
49	7.800	2006	2009	2014	rVB2	1259	1043	0.06%	0.007%
50	7.899	2024	2040	2055	rBV	797021	1373418	73.55%	9.785%
51	8.179	2114	2127	2149	rBV	161592	276747	14.82%	1.972%
52	8.394	2193	2194	2200	rVB4	557	267	0.01%	0.002%
53	8.452	2208	2212	2213	rBV	430	272	0.01%	0.002%
54	8.500	2224	2227	2233	rVB4	569	511	0.03%	0.004%
55	8.555	2241	2244	2251	rVB5	700	718	0.04%	0.005%
56	8.632	2252	2268	2304	rBV2	579746	1185720	63.50%	8.448%
57	9.417	2498	2512	2536	rBV	721116	1201685	64.35%	8.562%
58	9.565	2555	2558	2564	rVB3	1114	1049	0.06%	0.007%
59	9.642	2578	2582	2587	rVB3	462	401	0.02%	0.003%
60	9.780	2620	2625	2628	rBV2	260	272	0.01%	0.002%
61	10.098	2718	2724	2726	rBV4	618	693	0.04%	0.005%
62	10.481	2836	2843	2846	rBV2	1141	1190	0.06%	0.008%
63	10.677	2890	2904	2908	rBV8	1604	2696	0.14%	0.019%
64	10.754	2915	2928	2946	rBV	655355	1052312	56.35%	7.497%
65	10.979	2994	2998	3003	rBV2	357	381	0.02%	0.003%
66	11.166	3052	3056	3059	rVB2	342	260	0.01%	0.002%
67	11.375	3117	3121	3125	rBV2	388	396	0.02%	0.003%
68	11.420	3131	3135	3138	rVV3	541	331	0.02%	0.002%
69	11.471	3141	3151	3160	rVB3	6879	10764	0.58%	0.077%
70	11.542	3170	3173	3181	rVB	346	335	0.02%	0.002%
71	11.581	3181	3185	3189	rBV3	428	359	0.02%	0.003%
72	11.693	3215	3220	3221	rBV2	717	544	0.03%	0.004%
73	11.751	3232	3238	3244	rBV3	1542	1519	0.08%	0.011%
74	11.809	3244	3256	3280	rBV	626493	999420	53.52%	7.121%
75	12.076	3335	3339	3341	rBV3	881	772	0.04%	0.006%
76	12.192	3361	3375	3396	rBV	756109	1220548	65.36%	8.696%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050939.D
 Acq On : 26 Sep 2022 12:05
 Operator : JC/MD
 Sample : N4747-09DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.311	3410	3412	3414	rVB3	805	358	0.02%	0.003%
78	12.336	3418	3420	3425	rVB4	775	472	0.03%	0.003%
79	12.568	3489	3492	3493	rBV	383	236	0.01%	0.002%
80	12.629	3508	3511	3515	rVB3	344	241	0.01%	0.002%
81	12.745	3544	3547	3549	rBV3	519	294	0.02%	0.002%
82	12.767	3549	3554	3558	rBV3	832	912	0.05%	0.006%
83	12.825	3570	3572	3575	rBV2	358	266	0.01%	0.002%
84	12.976	3614	3619	3622	rBV4	870	782	0.04%	0.006%
85	13.028	3630	3635	3636	rBV3	553	386	0.02%	0.003%
86	13.060	3642	3645	3647	rBV2	451	261	0.01%	0.002%
87	13.150	3669	3673	3674	rBV	527	278	0.01%	0.002%
88	13.224	3691	3696	3706	rVB6	1833	2611	0.14%	0.019%
89	13.323	3722	3727	3729	rBV2	494	459	0.02%	0.003%
90	13.401	3747	3751	3755	rBV4	490	561	0.03%	0.004%
91	13.449	3764	3766	3773	rBV3	489	450	0.02%	0.003%
92	13.587	3807	3809	3811	rBV2	409	272	0.01%	0.002%
93	13.674	3833	3836	3839	rBV2	415	245	0.01%	0.002%
94	13.844	3883	3889	3897	rBV6	2236	3057	0.16%	0.022%
95	14.092	3960	3966	3979	rVB3	3229	4472	0.24%	0.032%
96	14.687	4149	4151	4154	rVB	462	276	0.01%	0.002%
97	14.809	4186	4189	4196	rBV4	786	807	0.04%	0.006%
98	14.838	4196	4198	4202	rBV3	500	330	0.02%	0.002%
99	15.323	4345	4349	4351	rBV3	785	609	0.03%	0.004%
100	15.397	4370	4372	4375	rBV2	815	426	0.02%	0.003%


Sum of corrected areas: 14035540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
Data File : VU050939.D
Acq On : 26 Sep 2022 12:05
Operator : JC/MD
Sample : N4747-09DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

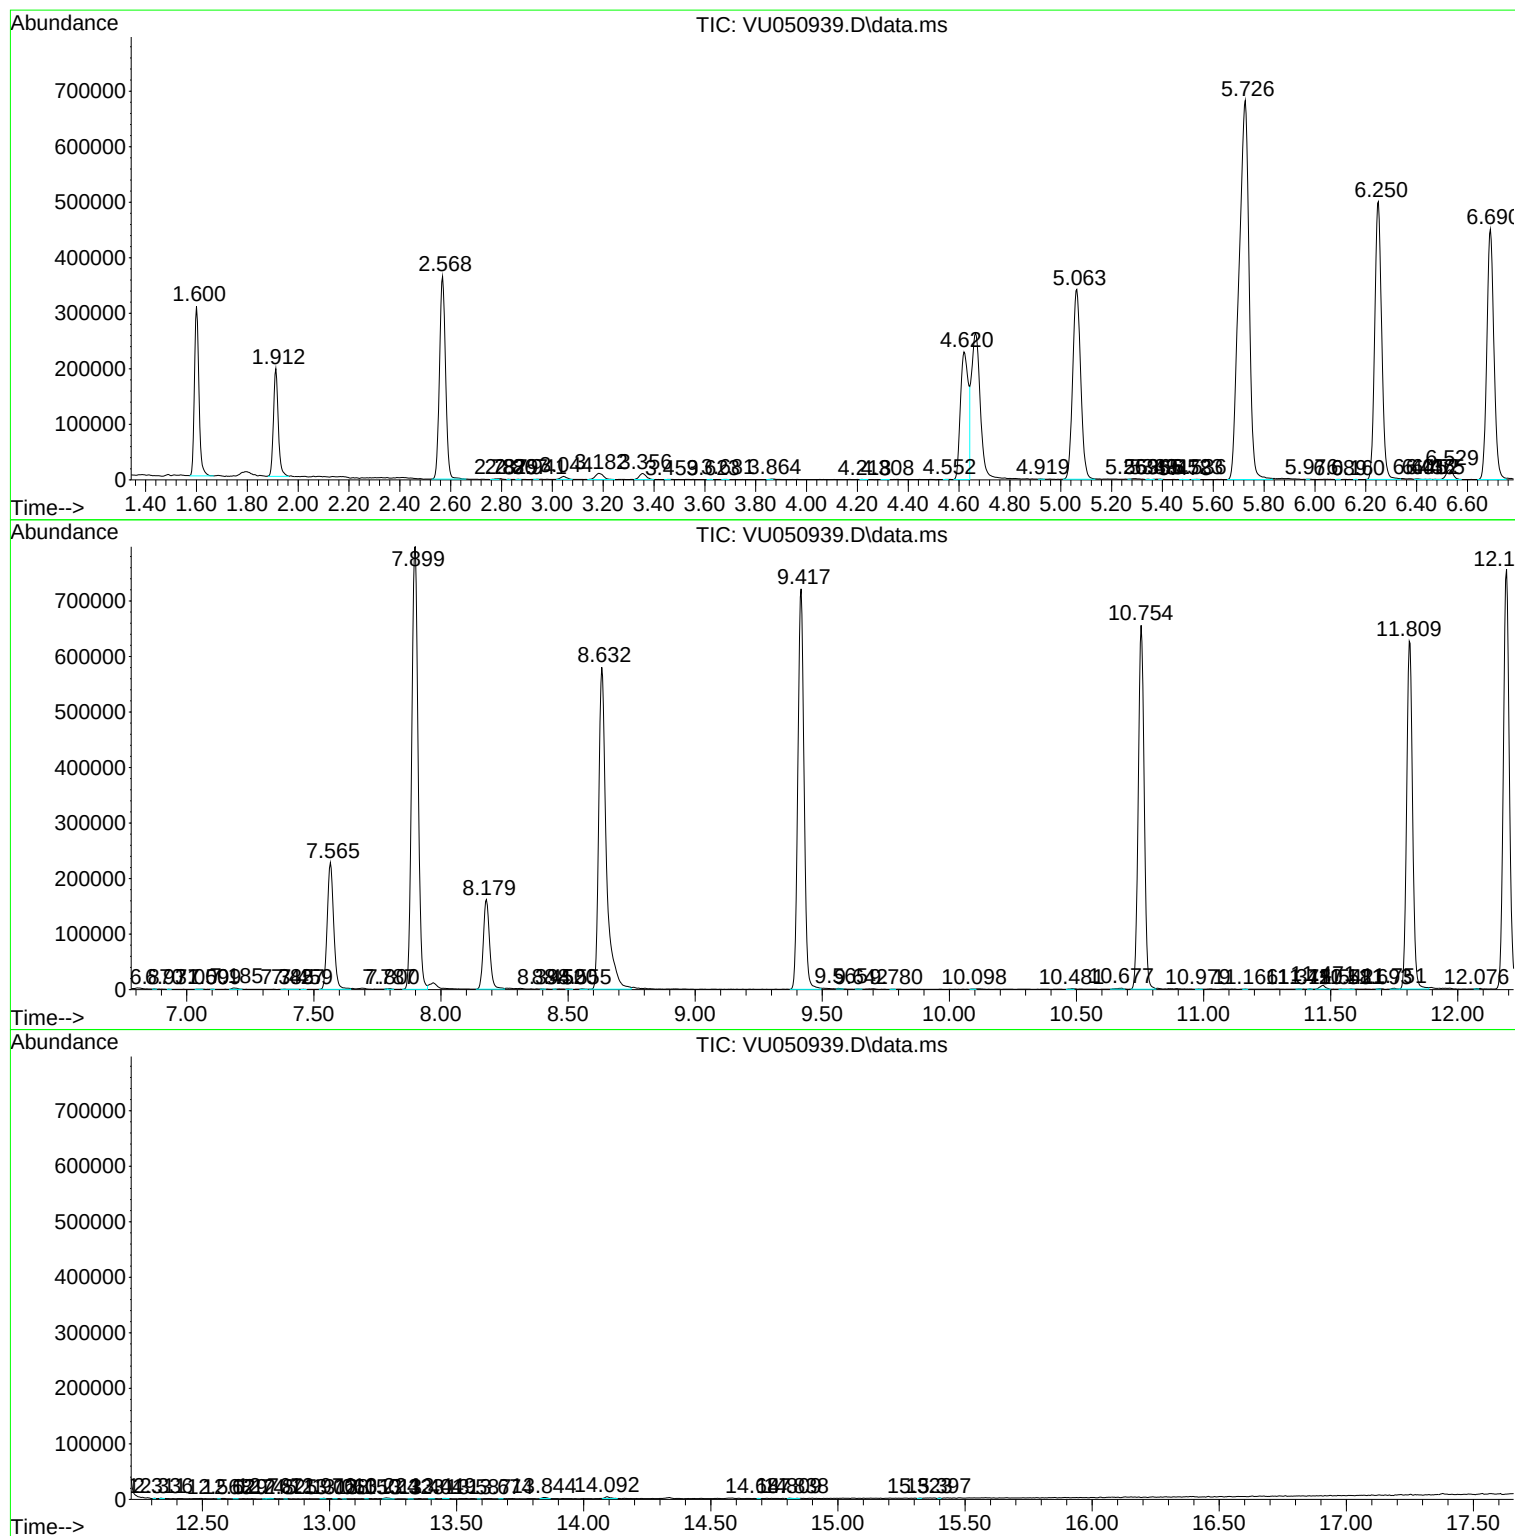

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
Data File : VU050939.D
Acq On : 26 Sep 2022 12:05
Operator : JC/MD
Sample : N4747-09DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
Data File : VU050939.D
Acq On : 26 Sep 2022 12:05
Operator : JC/MD
Sample : N4747-09DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------