

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050944.D
 Acq On : 26 Sep 2022 14:08
 Operator : JC/MD
 Sample : N4748-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rVB	188042	221477	13.02%	1.742%
2	1.912	170	178	196	rVB	169347	218536	12.85%	1.719%
3	2.568	369	382	397	rBV	312298	513913	30.22%	4.042%
4	2.687	416	419	424	rVB3	361	272	0.02%	0.002%
5	2.758	435	441	443	rBV3	799	823	0.05%	0.006%
6	2.774	443	446	449	rVV3	648	495	0.03%	0.004%
7	2.867	471	475	478	rBV3	385	246	0.01%	0.002%
8	2.922	489	492	495	rBV2	411	242	0.01%	0.002%
9	3.047	520	531	541	rBV4	2609	4804	0.28%	0.038%
10	3.182	562	573	574	rBV3	1162	1461	0.09%	0.011%
11	3.427	647	649	654	rVB2	399	300	0.02%	0.002%
12	3.645	714	717	723	rVV2	335	330	0.02%	0.003%
13	3.681	723	728	731	rVV	310	297	0.02%	0.002%
14	3.813	765	769	772	rBV2	313	300	0.02%	0.002%
15	3.861	779	784	786	rVB	346	269	0.02%	0.002%
16	3.916	799	801	807	rVV2	342	332	0.02%	0.003%
17	3.973	816	819	825	rVV2	391	437	0.03%	0.003%
18	4.022	828	834	839	rVB2	261	354	0.02%	0.003%
19	4.227	894	898	901	rVV	302	286	0.02%	0.002%
20	4.247	901	904	910	rVB2	352	301	0.02%	0.002%
21	4.620	1008	1020	1051	rBV	196101	494399	29.07%	3.889%
22	5.063	1139	1158	1184	rBV	319194	703584	41.37%	5.534%
23	5.346	1241	1246	1249	rBV	433	354	0.02%	0.003%
24	5.726	1342	1364	1386	rBV2	623000	1700726	100.00%	13.377%
25	5.967	1436	1439	1443	rBV3	543	422	0.02%	0.003%
26	5.999	1443	1449	1455	rVB4	566	710	0.04%	0.006%
27	6.250	1512	1527	1552	rBV	440910	851394	50.06%	6.697%
28	6.375	1564	1566	1571	rVB3	671	406	0.02%	0.003%
29	6.481	1595	1599	1602	rBV	622	416	0.02%	0.003%
30	6.530	1602	1614	1625	rBV4	17923	34857	2.05%	0.274%
31	6.597	1632	1635	1637	rBV	350	252	0.01%	0.002%
32	6.690	1649	1664	1684	rBV	417496	812196	47.76%	6.388%
33	6.883	1721	1724	1729	rVB2	750	597	0.04%	0.005%
34	6.915	1729	1734	1742	rBV3	423	509	0.03%	0.004%
35	7.009	1759	1763	1767	rVB2	271	258	0.02%	0.002%
36	7.047	1767	1775	1777	rBV3	514	715	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050944.D
 Acq On : 26 Sep 2022 14:08
 Operator : JC/MD
 Sample : N4748-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.108	1791	1794	1797	rVB2	487	384	0.02%	0.003%
38	7.189	1813	1819	1830	rVB3	2017	2997	0.18%	0.024%
39	7.259	1836	1841	1847	rVB2	295	348	0.02%	0.003%
40	7.359	1870	1872	1875	rBV	437	256	0.02%	0.002%
41	7.462	1900	1904	1905	rBV	385	247	0.01%	0.002%
42	7.565	1921	1936	1960	rBV	199734	357539	21.02%	2.812%
43	7.693	1972	1976	1983	rVB5	1223	1597	0.09%	0.013%
44	7.899	2024	2040	2057	rBV	717619	1237298	72.75%	9.732%
45	8.089	2096	2099	2107	rVB4	430	470	0.03%	0.004%
46	8.179	2115	2127	2150	rBV	148036	254806	14.98%	2.004%
47	8.443	2204	2209	2212	rBV4	431	423	0.02%	0.003%
48	8.475	2216	2219	2223	rVB3	647	573	0.03%	0.005%
49	8.632	2256	2268	2307	rBV2	519612	1079920	63.50%	8.494%
50	8.838	2330	2332	2336	rBV3	768	599	0.04%	0.005%
51	8.890	2346	2348	2352	rVB2	685	408	0.02%	0.003%
52	8.925	2355	2359	2363	rVV4	566	557	0.03%	0.004%
53	8.951	2363	2367	2370	rVB3	428	338	0.02%	0.003%
54	8.996	2379	2381	2386	rBV2	458	362	0.02%	0.003%
55	9.089	2406	2410	2413	rVB2	404	267	0.02%	0.002%
56	9.163	2429	2433	2435	rBV	514	282	0.02%	0.002%
57	9.195	2438	2443	2446	rBV2	236	254	0.01%	0.002%
58	9.272	2463	2467	2471	rVB	404	287	0.02%	0.002%
59	9.314	2474	2480	2483	rVV	375	326	0.02%	0.003%
60	9.417	2497	2512	2534	rBV	672865	1113269	65.46%	8.756%
61	9.562	2554	2557	2560	rBV2	640	503	0.03%	0.004%
62	9.655	2583	2586	2589	rVB2	405	271	0.02%	0.002%
63	9.674	2589	2592	2594	rBV2	540	340	0.02%	0.003%
64	9.845	2642	2645	2649	rBV2	400	298	0.02%	0.002%
65	9.947	2675	2677	2683	rVB2	331	270	0.02%	0.002%
66	9.980	2683	2687	2691	rBV2	317	265	0.02%	0.002%
67	10.240	2765	2768	2776	rBV2	309	451	0.03%	0.004%
68	10.317	2786	2792	2796	rBV2	206	263	0.02%	0.002%
69	10.619	2880	2886	2892	rBV2	324	480	0.03%	0.004%
70	10.671	2893	2902	2909	rBV4	1529	2289	0.13%	0.018%
71	10.706	2909	2913	2915	rBV	804	681	0.04%	0.005%
72	10.754	2916	2928	2950	rVV	611796	981581	57.72%	7.721%
73	10.886	2965	2969	2973	rBV5	1270	1458	0.09%	0.011%
74	10.992	2998	3002	3004	rBV	357	263	0.02%	0.002%
75	11.250	3078	3082	3085	rVB2	407	330	0.02%	0.003%
76	11.468	3139	3150	3156	rBV5	1378	2514	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050944.D
 Acq On : 26 Sep 2022 14:08
 Operator : JC/MD
 Sample : N4748-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.584	3183	3186	3188	rBV2	382	278	0.02%	0.002%
78	11.690	3212	3219	3220	rBV2	560	530	0.03%	0.004%
79	11.745	3232	3236	3243	rBV3	770	914	0.05%	0.007%
80	11.812	3244	3257	3280	rBV	579886	931584	54.78%	7.327%
81	12.057	3330	3333	3334	rBV	857	420	0.02%	0.003%
82	12.073	3334	3338	3348	rVB4	1844	2509	0.15%	0.020%
83	12.192	3360	3375	3400	rBV	700169	1155741	67.96%	9.090%
84	12.330	3416	3418	3424	rVB2	889	814	0.05%	0.006%
85	12.436	3446	3451	3456	rBV4	749	782	0.05%	0.006%
86	12.674	3520	3525	3528	rBV	605	622	0.04%	0.005%
87	12.835	3571	3575	3577	rBV2	356	307	0.02%	0.002%
88	12.925	3600	3603	3605	rBV2	456	321	0.02%	0.003%
89	13.021	3630	3633	3637	rVB	623	415	0.02%	0.003%
90	13.134	3666	3668	3673	rVB2	457	305	0.02%	0.002%
91	13.160	3673	3676	3680	rBV3	378	406	0.02%	0.003%
92	13.224	3690	3696	3699	rBV3	910	1082	0.06%	0.009%
93	13.272	3708	3711	3713	rBV2	621	397	0.02%	0.003%
94	13.520	3786	3788	3792	rVB	495	275	0.02%	0.002%
95	13.658	3828	3831	3833	rBV	346	263	0.02%	0.002%
96	13.844	3886	3889	3893	rBV3	625	610	0.04%	0.005%
97	14.176	3989	3992	3995	rBV2	492	311	0.02%	0.002%
98	14.336	4039	4042	4046	rVB3	648	531	0.03%	0.004%
99	14.359	4046	4049	4051	rBV3	567	319	0.02%	0.003%
100	15.159	4295	4298	4303	rBV	559	721	0.04%	0.006%




Sum of corrected areas: 12713791

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
Data File : VU050944.D
Acq On : 26 Sep 2022 14:08
Operator : JC/MD
Sample : N4748-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

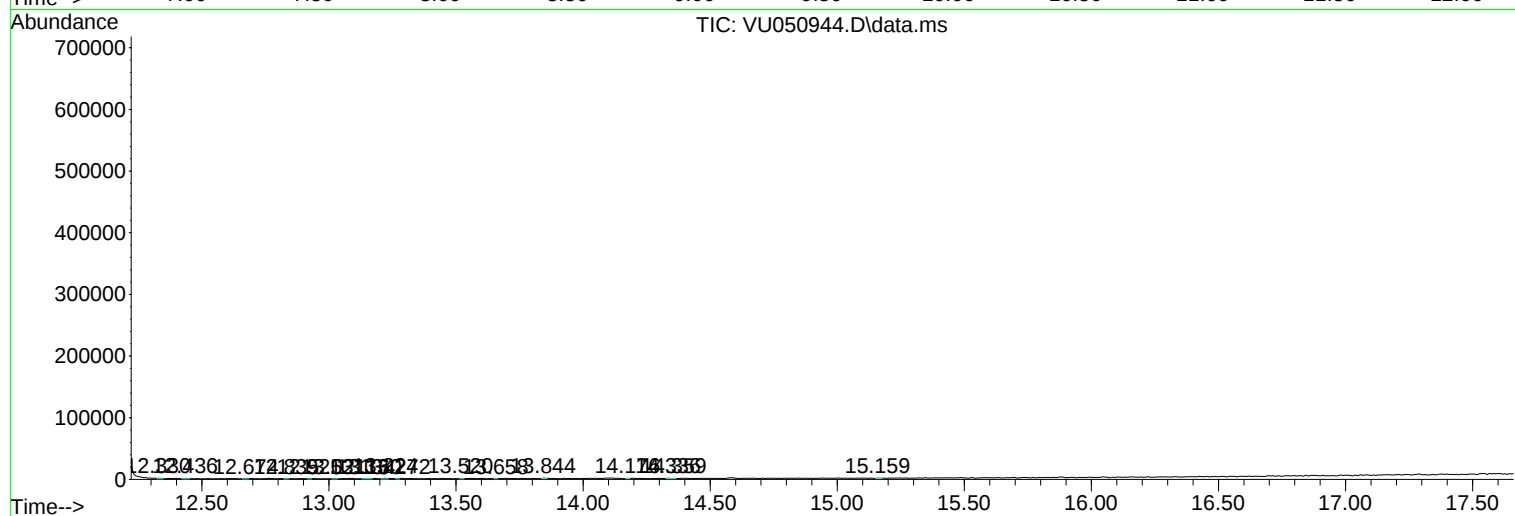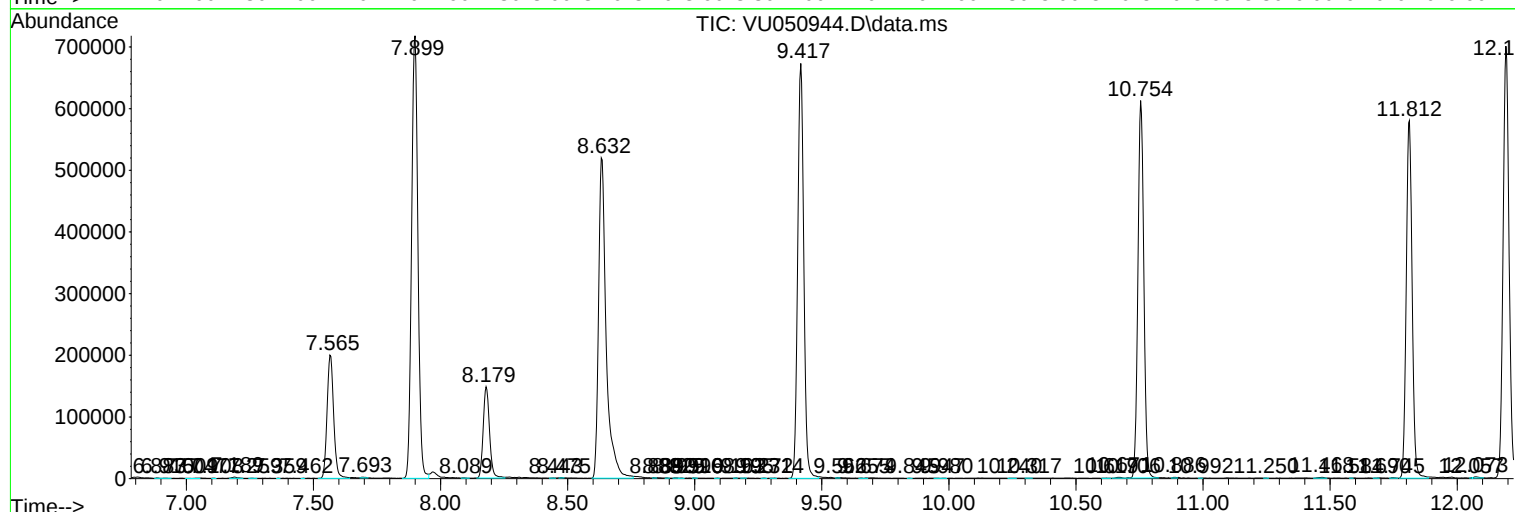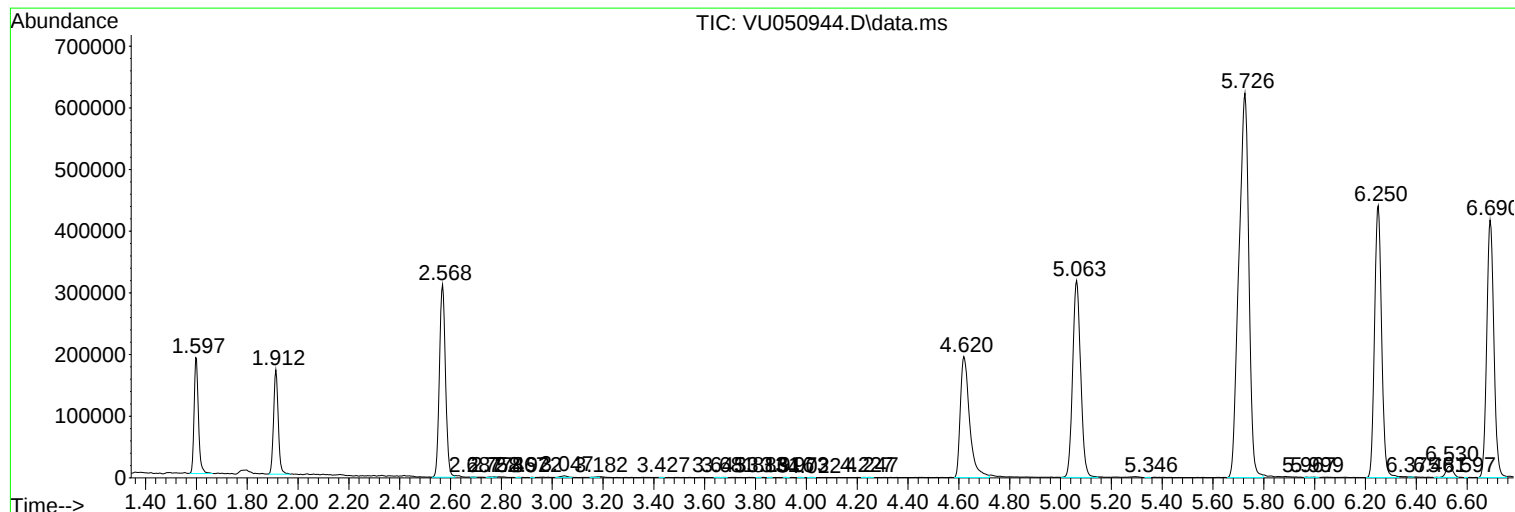

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
Data File : VU050944.D
Acq On : 26 Sep 2022 14:08
Operator : JC/MD
Sample : N4748-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
Data File : VU050944.D
Acq On : 26 Sep 2022 14:08
Operator : JC/MD
Sample : N4748-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------