

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050947.D
 Acq On : 26 Sep 2022 15:19
 Operator : JC/MD
 Sample : N4748-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rVB	204181	238878	13.63%	1.833%
2	1.912	169	178	196	rVB	181671	234094	13.35%	1.796%
3	2.568	369	382	397	rBV	329170	540528	30.83%	4.148%
4	2.790	445	451	452	rBV3	651	605	0.03%	0.005%
5	2.819	458	460	464	rVB	679	338	0.02%	0.003%
6	2.961	501	504	509	rBV3	403	421	0.02%	0.003%
7	3.041	520	529	541	rVV3	4746	8408	0.48%	0.065%
8	3.186	561	574	587	rBV2	4679	10640	0.61%	0.082%
9	3.273	597	601	607	rBV	419	476	0.03%	0.004%
10	3.363	627	629	634	rBV2	305	181	0.01%	0.001%
11	3.568	690	693	700	rVB	406	302	0.02%	0.002%
12	3.613	704	707	709	rBV2	279	179	0.01%	0.001%
13	3.674	723	726	729	rBV	379	319	0.02%	0.002%
14	3.723	738	741	745	rBV2	211	198	0.01%	0.002%
15	3.813	765	769	772	rBV2	209	172	0.01%	0.001%
16	4.070	846	849	854	rBV2	223	210	0.01%	0.002%
17	4.128	860	867	868	rBV2	265	301	0.02%	0.002%
18	4.154	872	875	881	rVV2	348	391	0.02%	0.003%
19	4.205	885	891	894	rVV2	461	494	0.03%	0.004%
20	4.298	915	920	923	rBV	402	394	0.02%	0.003%
21	4.620	1007	1020	1056	rBV2	207492	532338	30.37%	4.085%
22	4.916	1108	1112	1115	rBV2	396	347	0.02%	0.003%
23	5.063	1140	1158	1186	rBV	322643	713638	40.71%	5.476%
24	5.292	1223	1229	1235	rVV5	1162	1692	0.10%	0.013%
25	5.366	1249	1252	1255	rBV4	670	499	0.03%	0.004%
26	5.517	1296	1299	1302	rBV2	270	183	0.01%	0.001%
27	5.539	1302	1306	1310	rVB2	246	180	0.01%	0.001%
28	5.723	1341	1363	1390	rBV2	636513	1753061	100.00%	13.453%
29	6.041	1460	1462	1470	rVB3	844	853	0.05%	0.007%
30	6.105	1478	1482	1486	rVB3	497	407	0.02%	0.003%
31	6.128	1486	1489	1492	rVB4	261	181	0.01%	0.001%
32	6.170	1499	1502	1505	rBV3	445	336	0.02%	0.003%
33	6.250	1512	1527	1552	rBV	452272	862523	49.20%	6.619%
34	6.469	1591	1595	1598	rVB2	354	302	0.02%	0.002%
35	6.530	1602	1614	1626	rVB3	17060	30995	1.77%	0.238%
36	6.597	1632	1635	1639	rBV3	327	269	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050947.D
 Acq On : 26 Sep 2022 15:19
 Operator : JC/MD
 Sample : N4748-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.690	1646	1664	1687	rBV	426993	830241	47.36%	6.371%
38	7.047	1772	1775	1780	rVV3	473	421	0.02%	0.003%
39	7.108	1790	1794	1798	rBV2	169	170	0.01%	0.001%
40	7.186	1811	1818	1820	rBV5	1650	1962	0.11%	0.015%
41	7.343	1862	1867	1871	rVB2	426	497	0.03%	0.004%
42	7.366	1871	1874	1877	rBV	454	393	0.02%	0.003%
43	7.404	1882	1886	1889	rBV2	295	256	0.01%	0.002%
44	7.565	1921	1936	1954	rBV	202787	364449	20.79%	2.797%
45	7.684	1971	1973	1984	rVB7	1573	2445	0.14%	0.019%
46	7.796	2003	2008	2013	rBV4	609	499	0.03%	0.004%
47	7.896	2024	2039	2056	rBV	732148	1273134	72.62%	9.770%
48	8.115	2104	2107	2108	rBV2	496	266	0.02%	0.002%
49	8.179	2115	2127	2147	rBV	147908	254983	14.55%	1.957%
50	8.459	2210	2214	2217	rBV3	731	600	0.03%	0.005%
51	8.552	2240	2243	2249	rVB3	513	497	0.03%	0.004%
52	8.581	2249	2252	2253	rBV	349	222	0.01%	0.002%
53	8.632	2256	2268	2300	rBV4	546234	1122972	64.06%	8.618%
54	8.925	2353	2359	2363	rVB3	930	1051	0.06%	0.008%
55	9.002	2378	2383	2385	rBV2	461	385	0.02%	0.003%
56	9.038	2390	2394	2398	rVV3	432	426	0.02%	0.003%
57	9.092	2408	2411	2415	rBV2	329	308	0.02%	0.002%
58	9.237	2454	2456	2463	rBV2	299	211	0.01%	0.002%
59	9.417	2498	2512	2538	rBV	681665	1121565	63.98%	8.607%
60	9.607	2568	2571	2572	rBV	443	197	0.01%	0.002%
61	9.649	2582	2584	2586	rVB	394	173	0.01%	0.001%
62	9.687	2592	2596	2599	rBV3	597	621	0.04%	0.005%
63	9.742	2609	2613	2619	rBV	229	359	0.02%	0.003%
64	9.767	2619	2621	2629	rVB2	523	497	0.03%	0.004%
65	9.822	2635	2638	2640	rBV2	319	218	0.01%	0.002%
66	9.935	2671	2673	2679	rVB	383	197	0.01%	0.002%
67	10.025	2697	2701	2706	rBV2	407	345	0.02%	0.003%
68	10.050	2706	2709	2714	rBB2	279	237	0.01%	0.002%
69	10.079	2714	2718	2720	rBV	291	200	0.01%	0.002%
70	10.099	2720	2724	2728	rBV3	638	647	0.04%	0.005%
71	10.205	2753	2757	2760	rBV2	451	269	0.02%	0.002%
72	10.275	2775	2779	2782	rBV	393	351	0.02%	0.003%
73	10.488	2841	2845	2849	rVB	566	440	0.03%	0.003%
74	10.616	2882	2885	2891	rBV2	355	291	0.02%	0.002%
75	10.674	2896	2903	2911	rVB4	1477	1944	0.11%	0.015%
76	10.755	2914	2928	2957	rVV	623736	1015982	57.95%	7.797%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050947.D
 Acq On : 26 Sep 2022 15:19
 Operator : JC/MD
 Sample : N4748-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	10.880	2965	2967	2969	rBV2	310	177	0.01%	0.001%
78	10.999	3001	3004	3008	rVB2	607	476	0.03%	0.004%
79	11.070	3019	3026	3029	rBV2	497	553	0.03%	0.004%
80	11.163	3051	3055	3058	rBV2	310	259	0.01%	0.002%
81	11.420	3133	3135	3140	rVB2	354	222	0.01%	0.002%
82	11.459	3140	3147	3152	rBV5	1278	1783	0.10%	0.014%
83	11.526	3165	3168	3171	rBV2	277	237	0.01%	0.002%
84	11.623	3196	3198	3204	rBV2	314	271	0.02%	0.002%
85	11.745	3233	3236	3240	rVB3	549	397	0.02%	0.003%
86	11.809	3244	3256	3276	rBV	578787	928346	52.96%	7.124%
87	12.079	3337	3340	3345	rBV3	697	506	0.03%	0.004%
88	12.124	3351	3354	3359	rVB3	381	260	0.01%	0.002%
89	12.192	3362	3375	3399	rBV	697451	1157033	66.00%	8.879%
90	12.735	3541	3544	3545	rBV	551	269	0.02%	0.002%
91	12.999	3623	3626	3627	rBV	283	171	0.01%	0.001%
92	13.208	3687	3691	3692	rBV3	622	404	0.02%	0.003%
93	13.304	3717	3721	3723	rBV2	623	509	0.03%	0.004%
94	13.780	3865	3869	3871	rBV3	390	343	0.02%	0.003%
95	13.809	3875	3878	3882	rBV3	423	366	0.02%	0.003%
96	14.192	3994	3997	4001	rBV	528	415	0.02%	0.003%
97	14.266	4017	4020	4023	rBV	1049	703	0.04%	0.005%
98	14.838	4195	4198	4200	rBV2	673	434	0.02%	0.003%
99	14.960	4234	4236	4239	rBV3	601	352	0.02%	0.003%
100	15.147	4292	4294	4296	rBV	632	271	0.02%	0.002%




Sum of corrected areas: 13031011

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
Data File : VU050947.D
Acq On : 26 Sep 2022 15:19
Operator : JC/MD
Sample : N4748-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

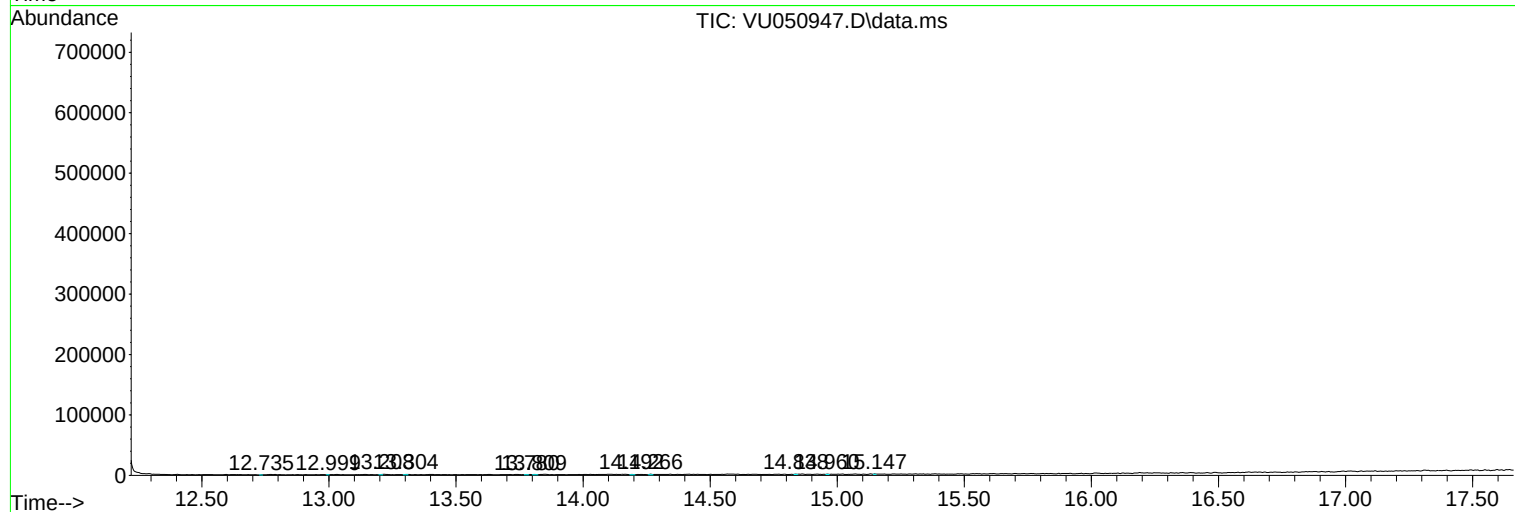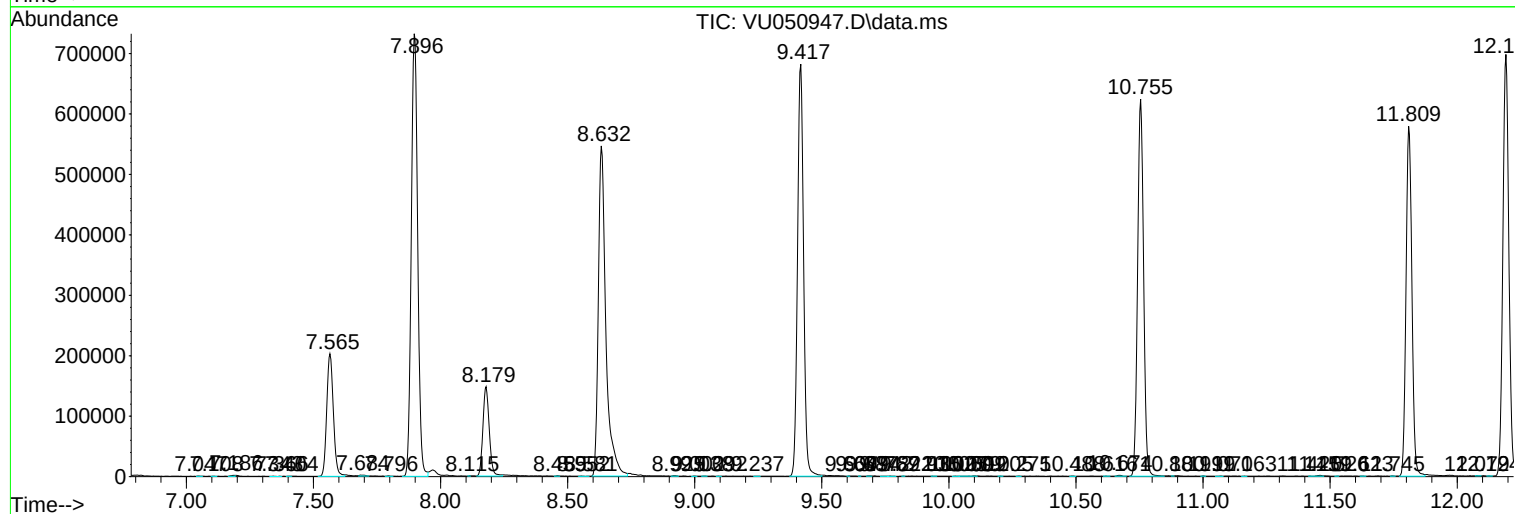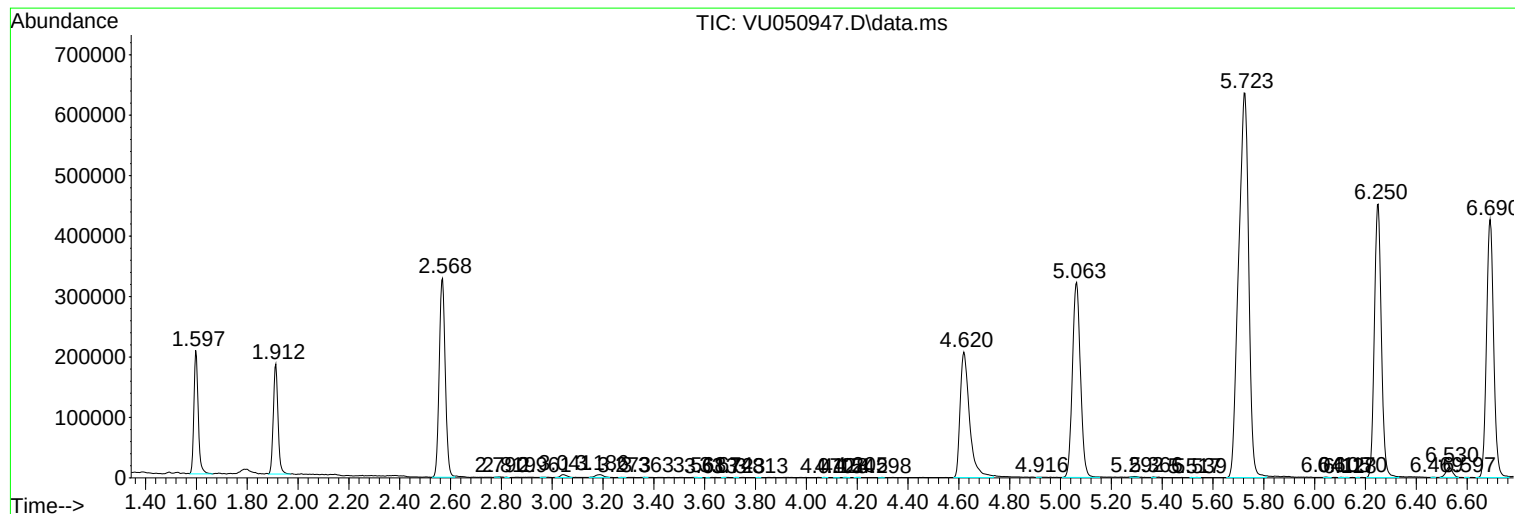

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
Data File : VU050947.D
Acq On : 26 Sep 2022 15:19
Operator : JC/MD
Sample : N4748-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
Data File : VU050947.D
Acq On : 26 Sep 2022 15:19
Operator : JC/MD
Sample : N4748-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------