


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092622\
 Data File : VU050935.D
 Acq On : 26 Sep 2022 09:03
 Operator : JC/MD
 Sample : BFB131
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB131

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis
 Last Update : Mon Sep 26 20:52:47 2022

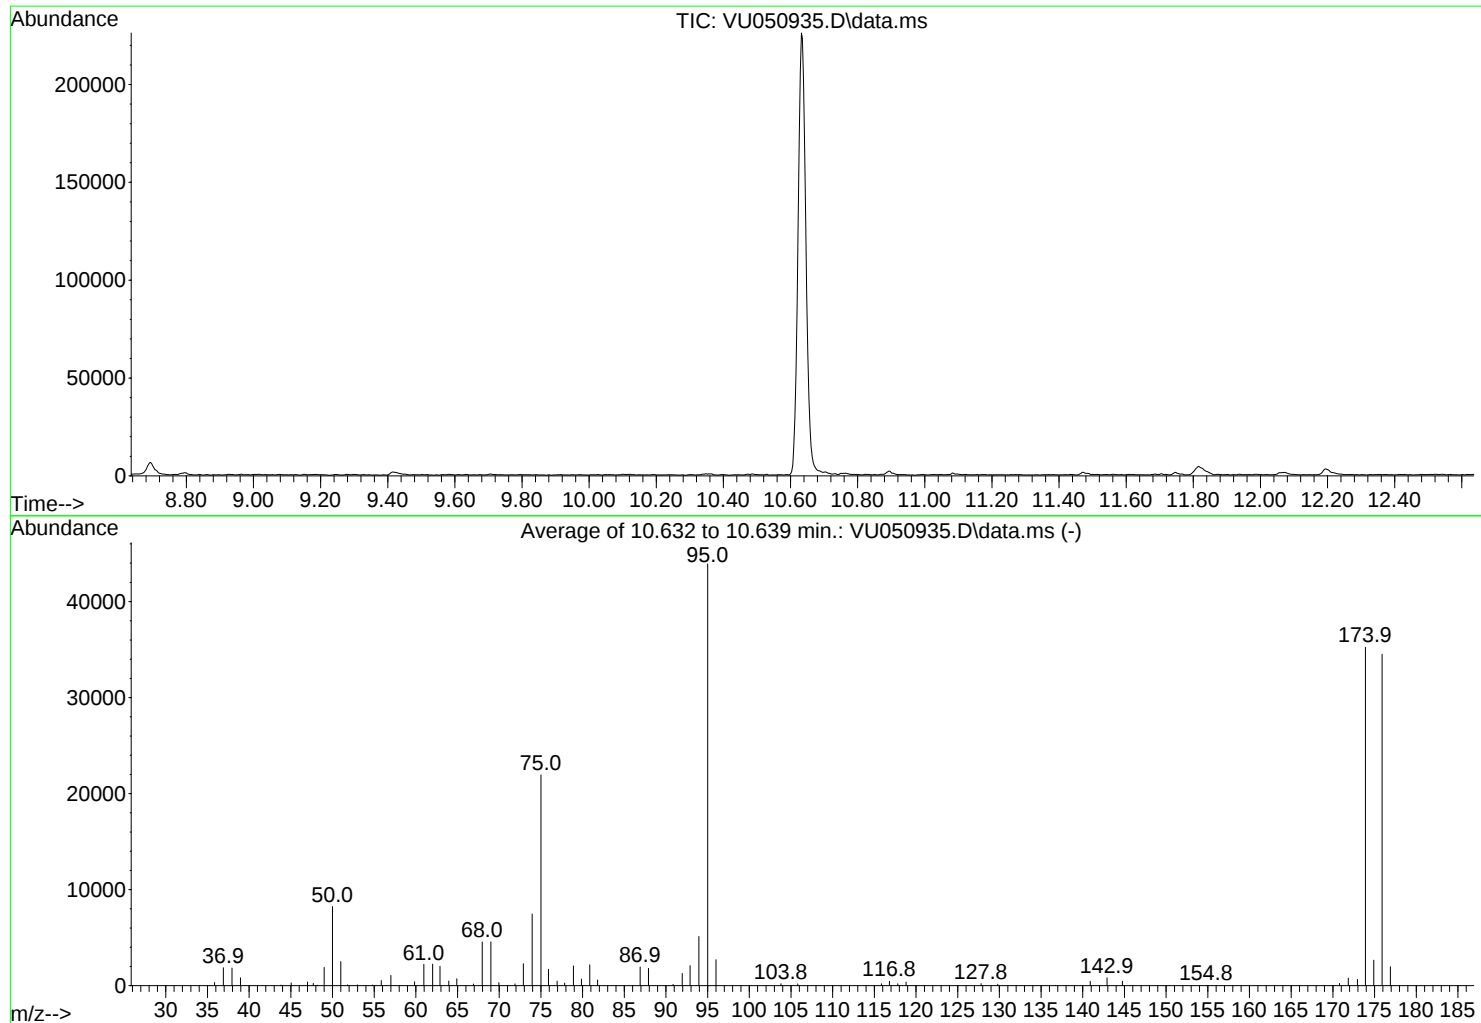

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	8227	PASS
75	95	30	80	49.9	21941	PASS
95	95	100	100	100.0	43928	PASS
96	95	5	9	6.2	2703	PASS
173	174	0.00	2	1.8	647	PASS
174	95	50	120	80.2	35237	PASS
175	174	5	9	7.5	2647	PASS
176	174	95	101	97.9	34509	PASS
177	176	5	9	5.7	1968	PASS

m/z	Abundance
39.90	195.0
43.80	402.0

Instrument :
MSVOA_U
ClientSampleId :
BFB131

m/z	Abundance
35.90	342.0
36.90	2010.0
37.90	1798.0
39.00	932.0
39.80	156.0
43.80	505.0
45.10	330.0
47.00	451.0
47.70	236.0
49.00	2216.0
50.00	8790.0
51.00	2789.0
51.80	148.0
55.10	126.0
55.80	498.0
57.00	1080.0
59.80	516.0
60.90	2363.0
62.00	2343.0
62.90	2187.0
64.00	495.0
64.90	624.0
66.90	168.0
68.00	4718.0
69.00	4819.0
70.00	324.0
71.90	166.0
72.90	2399.0
73.90	7847.0
75.00	23672.0
75.90	1729.0
77.00	509.0
77.80	246.0
78.90	2332.0
79.90	601.0
80.80	2290.0
81.80	567.0
86.90	1876.0
87.90	1907.0
90.90	146.0
92.00	1346.0
92.90	2062.0
93.90	5194.0
95.00	45304.0
96.00	2850.0
103.80	224.0
105.70	218.0
115.90	205.0
116.80	416.0
117.80	202.0
118.80	390.0
127.80	183.0
129.80	104.0
140.90	440.0
142.90	907.0
144.80	489.0
145.70	106.0
154.80	115.0
170.70	240.0
171.90	748.0
173.00	650.0
173.90	36040.0
174.90	2797.0
175.90	35752.0
176.90	2045.0

Instrument :
MSVOA_U
ClientSampleId :
BFB131

m/z	Abundance
35.90	338.0
36.90	1849.0
37.90	1853.0
38.90	816.0
39.90	158.0
43.80	454.0
45.10	296.0
47.00	391.0
47.70	252.0
49.00	1945.0
50.00	8559.0
51.00	2598.0
51.80	109.0
53.00	139.0
54.80	114.0
55.90	545.0
57.00	1115.0
59.80	384.0
61.00	2279.0
62.00	2287.0
62.90	2057.0
63.90	490.0
64.90	780.0
66.90	180.0
68.00	4696.0
69.00	4694.0
69.90	322.0
71.90	188.0
72.90	2355.0
74.00	7590.0
75.00	22560.0
75.90	1801.0
77.00	542.0
77.80	274.0
78.90	2111.0
79.80	657.0
80.80	2223.0
81.80	617.0
86.90	1998.0
87.90	1896.0
90.90	133.0
92.00	1305.0
92.90	2179.0
93.90	5205.0
95.00	45464.0
96.00	2707.0
103.80	209.0
105.80	179.0
115.90	217.0
116.80	492.0
117.80	201.0
118.80	375.0
127.80	229.0
129.80	155.0
140.90	482.0
142.90	798.0
144.70	479.0
170.80	215.0
171.90	804.0
172.90	695.0
173.90	36048.0
174.90	2717.0
175.90	35640.0
176.90	2029.0

Instrument :
MSVOA_U
ClientSampleId :
BFB131

m/z	Abundance
35.80	294.0
36.90	1723.0
38.00	1827.0
38.90	684.0
40.00	205.0
43.90	384.0
45.00	245.0
47.00	303.0
47.70	216.0
48.20	161.0
49.00	1535.0
50.00	7333.0
51.00	2103.0
53.00	131.0
54.80	111.0
55.90	585.0
57.00	1025.0
59.90	318.0
60.90	1999.0
62.00	2049.0
62.90	1792.0
63.90	450.0
64.90	757.0
66.90	147.0
67.90	4240.0
69.00	4204.0
69.90	297.0
71.90	186.0
72.90	2112.0
74.00	6958.0
75.00	19592.0
75.90	1598.0
76.90	374.0
77.90	288.0
78.90	1724.0
79.80	773.0
80.90	1987.0
81.80	591.0
86.90	1974.0
87.90	1605.0
90.80	130.0
91.90	1168.0
92.90	2002.0
94.00	4973.0
95.00	41016.0
96.00	2552.0
103.80	168.0
105.90	148.0
115.80	170.0
116.80	458.0
117.80	181.0
118.80	335.0
127.80	233.0
129.80	192.0
136.70	106.0
140.90	415.0
142.90	771.0
144.70	408.0
170.90	224.0
171.80	796.0
172.90	596.0
173.90	33624.0
174.90	2427.0
175.90	32136.0
176.90	1831.0

Instrument :
MSVOA_U
ClientSampleId :
BFB131