

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050958.D
 Acq On : 27 Sep 2022 15:45
 Operator : JC/MD
 Sample : N4854-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J17

Quant Time: Sep 28 02:02:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 28 01:59:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	324807	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	352699	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	140225	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	115402	34.293	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	68.580%	
7) Chloroethane-d5	1.909	69	106243	44.329	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	88.660%	
11) 1,1-Dichloroethene-d2	2.565	63	154134	29.435	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	58.880%#	
21) 2-Butanone-d5	4.617	46	259500	119.443	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	119.440%	
24) Chloroform-d	5.060	84	263823	50.026	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.060%	
26) 1,2-Dichloroethane-d4	5.700	65	175551	54.015	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	108.020%	
32) Benzene-d6	5.726	84	497793	42.850	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	85.700%	
36) 1,2-Dichloropropane-d6	6.690	67	180093	45.927	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	91.860%	
41) Toluene-d8	7.896	98	409865	40.362	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	80.720%	
43) trans-1,3-Dichloroprop...	8.179	79	71953	42.179	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.360%	
47) 2-Hexanone-d5	8.629	63	146298	90.532	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	90.530%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	286040	47.845	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	95.700%	
66) 1,2-Dichlorobenzene-d4	12.192	152	155695	53.030	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	106.060%	
Target Compounds						
						Qvalue
13) Acetone	2.623	43	78342	42.586	ug/L	99
34) Trichloroethene	6.539	95	24507	8.128	ug/L	97
46) Tetrachloroethene	8.552	164	325023	150.011	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050958.D
Acq On : 27 Sep 2022 15:45
Operator : JC/MD
Sample : N4854-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J17

Quant Time: Sep 28 02:02:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 28 01:59:42 2022
Response via : Initial Calibration

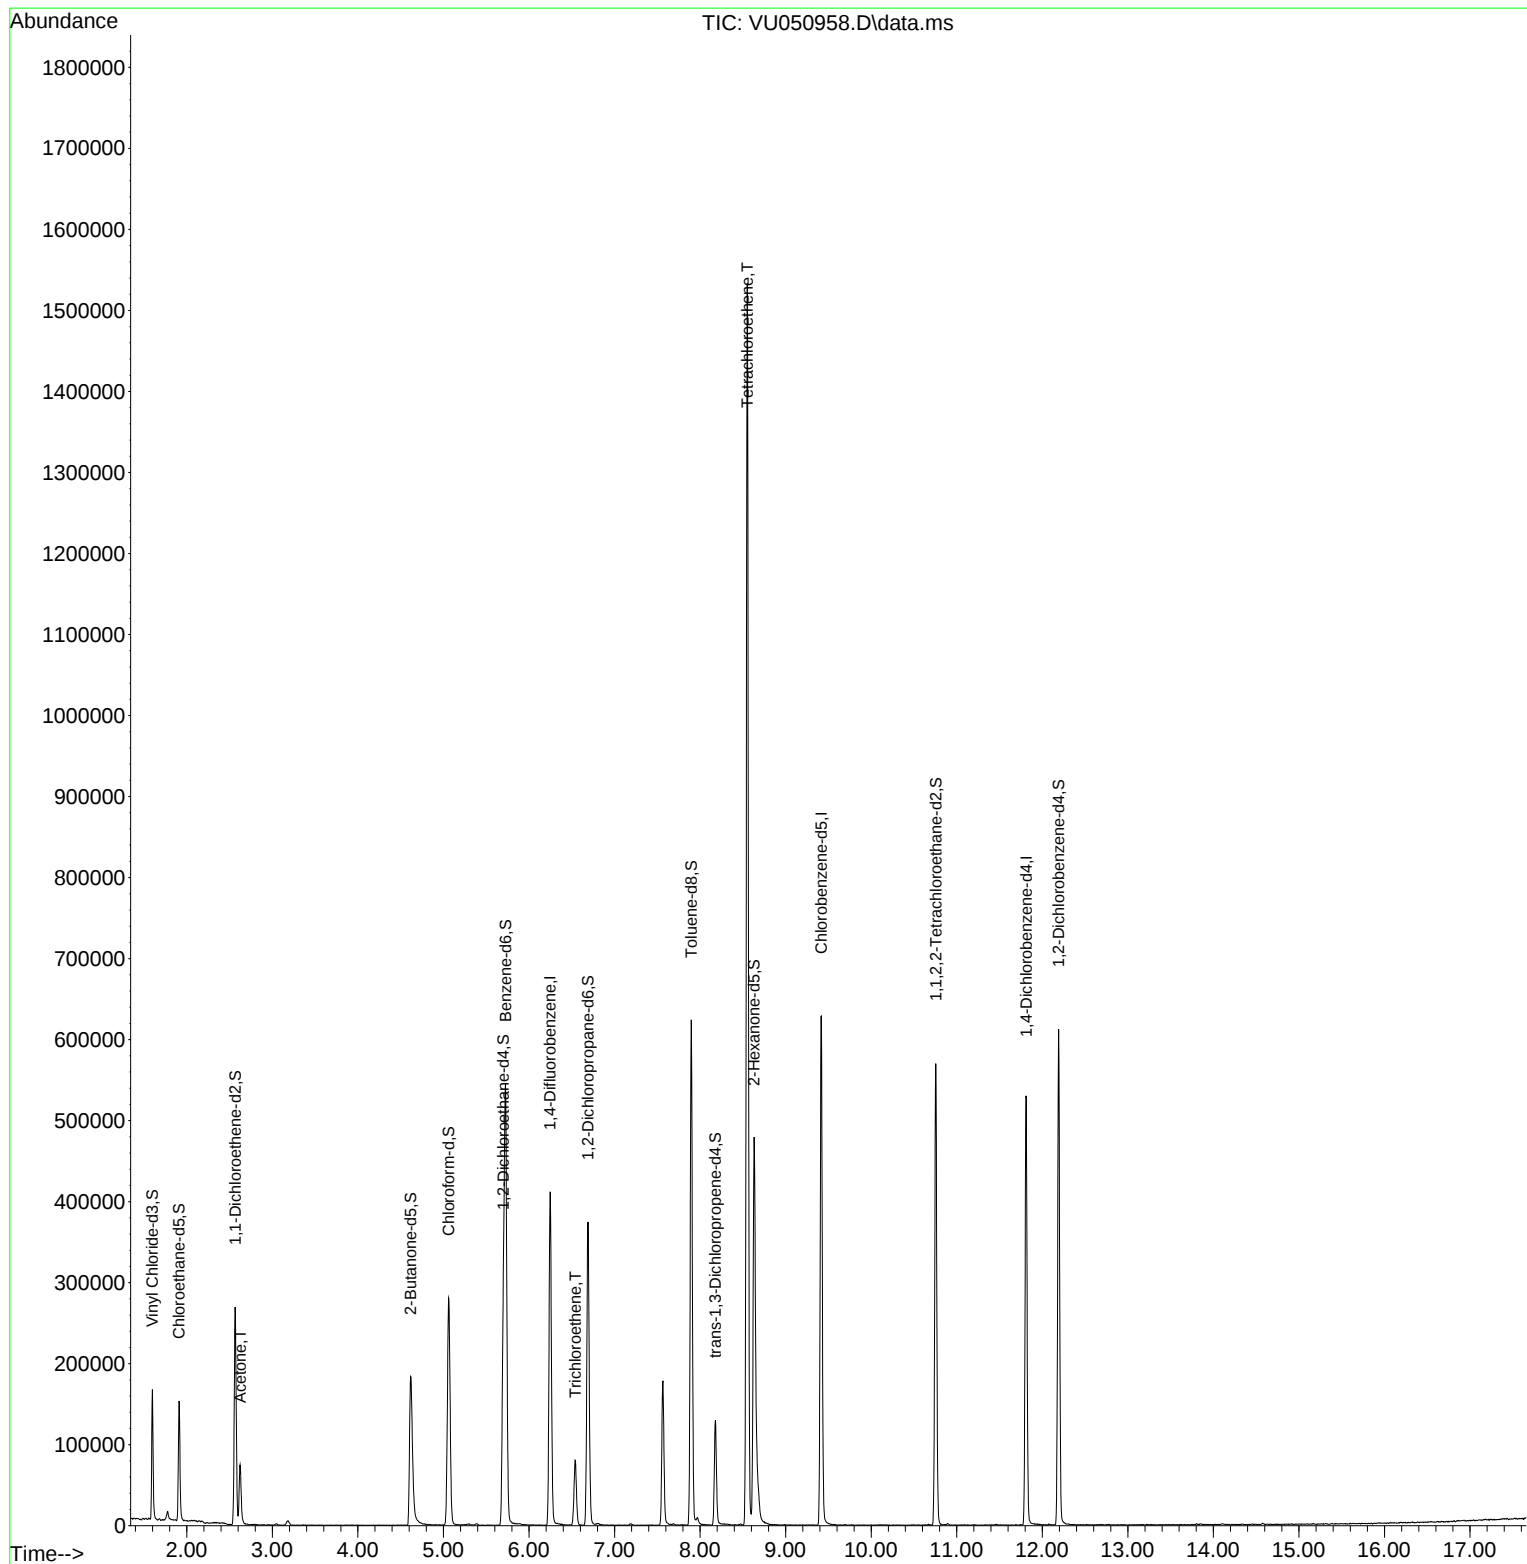

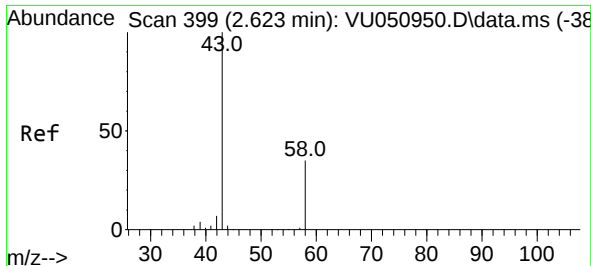

#13

Acetone

Concen: 42.586 ug/L

RT: 2.623 min Scan# 399

Delta R.T. -0.000 min

Lab File: VU050958.D

Acq: 27 Sep 2022 15:45

Instrument :

MSVOA_U

ClientSampleId :





F5J17

Tgt Ion: 43 Resp: 78342

Ion Ratio Lower Upper

43 100

58 35.4 0.0 71.4

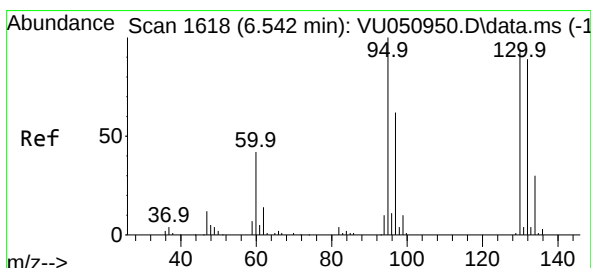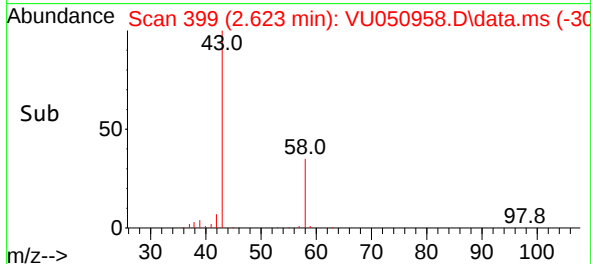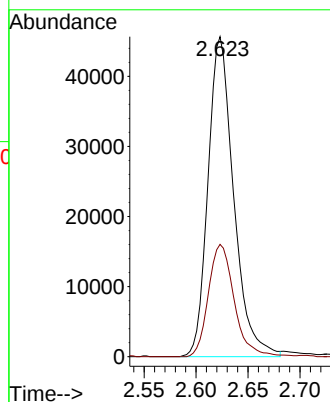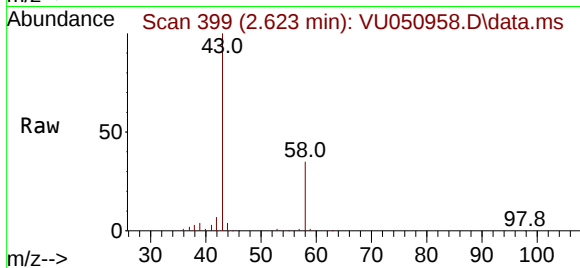

#34

Trichloroethene

Concen: 8.128 ug/L

RT: 6.539 min Scan# 1617

Delta R.T. -0.003 min

Lab File: VU050958.D

Acq: 27 Sep 2022 15:45

Tgt Ion: 95 Resp: 24507




Ion Ratio Lower Upper


95 100

97 65.1 43.9 81.5

132 92.9 63.1 117.1


130 97.7 65.9 122.3

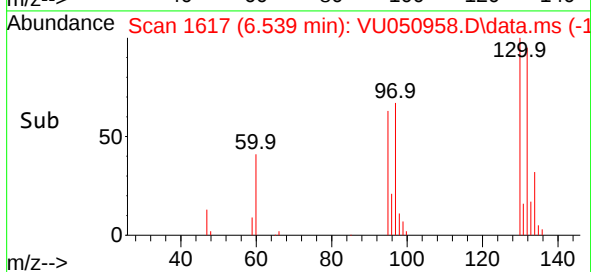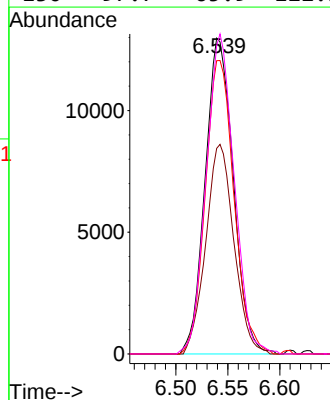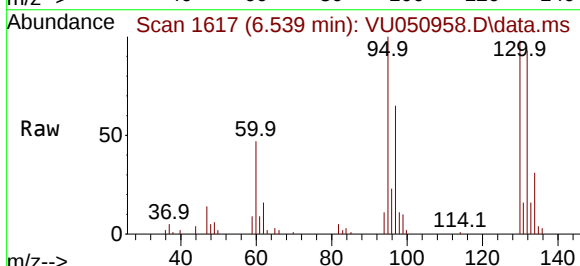

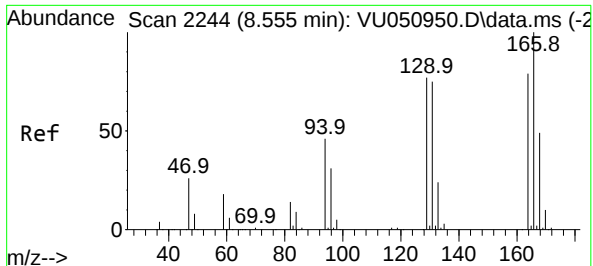

#46
Tetrachloroethene
Concen: 150.011 ug/L
RT: 8.552 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU050958.D
Acq: 27 Sep 2022 15:45

Instrument :
MSVOA_U
ClientSampleId :
F5J17

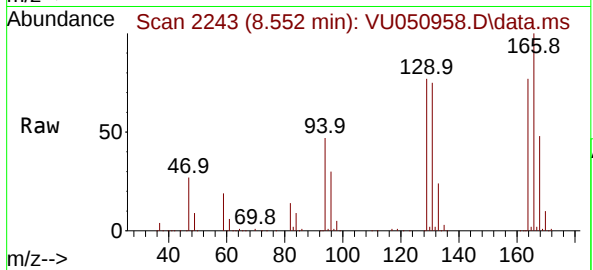

Tgt Ion:	164	Resp:	325023
Ion	Ratio	Lower	Upper
164	100		
129	100.6	68.5	127.3
131	98.3	66.1	122.7
166	130.6	88.8	164.8

