

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050953.D
 Acq On : 27 Sep 2022 13:47
 Operator : JC/MD
 Sample : N4854-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	153989	176575	1.63%	0.776%
2	1.913	170	178	194	rVB	144650	186446	1.73%	0.819%
3	2.568	369	382	397	rBV	259430	427450	3.96%	1.877%
4	2.684	414	418	420	rBV3	395	311	0.00%	0.001%
5	2.800	446	454	461	rVB2	1558	2150	0.02%	0.009%
6	3.044	522	530	539	rBV3	3210	5505	0.05%	0.024%
7	3.128	548	556	559	rBV2	294	362	0.00%	0.002%
8	3.176	559	571	572	rBV5	2499	2833	0.03%	0.012%
9	3.289	604	606	612	rVB2	372	307	0.00%	0.001%
10	3.366	617	630	644	rVV3	5983	13064	0.12%	0.057%
11	3.511	669	675	678	rBV2	290	319	0.00%	0.001%
12	3.552	683	688	696	rBV3	417	617	0.01%	0.003%
13	3.793	758	763	769	rBV2	199	238	0.00%	0.001%
14	4.285	913	916	922	rBV	463	349	0.00%	0.002%
15	4.623	1008	1021	1048	rBV	164995	441677	4.09%	1.940%
16	4.941	1118	1120	1124	rVB4	454	274	0.00%	0.001%
17	4.990	1131	1135	1141	rVB2	380	360	0.00%	0.002%
18	5.064	1141	1158	1185	rBV	275731	613881	5.68%	2.696%
19	5.179	1191	1194	1197	rVB3	446	263	0.00%	0.001%
20	5.211	1200	1204	1207	rVB3	376	245	0.00%	0.001%
21	5.228	1207	1209	1213	rBV2	414	267	0.00%	0.001%
22	5.285	1221	1227	1229	rBV3	1267	1212	0.01%	0.005%
23	5.372	1249	1254	1257	rBV3	483	485	0.00%	0.002%
24	5.494	1286	1292	1295	rBV	421	419	0.00%	0.002%
25	5.517	1295	1299	1305	rVB3	368	339	0.00%	0.001%
26	5.726	1342	1364	1396	rBV2	528024	1467347	13.58%	6.445%
27	6.115	1477	1485	1486	rBV2	452	549	0.01%	0.002%
28	6.199	1507	1511	1512	rBV2	324	243	0.00%	0.001%
29	6.250	1512	1527	1548	rBV	420674	797199	7.38%	3.501%
30	6.414	1575	1578	1581	rVB3	735	546	0.01%	0.002%
31	6.543	1603	1618	1635	rBV	343070	649997	6.02%	2.855%
32	6.690	1649	1664	1686	rBV2	358239	704394	6.52%	3.094%
33	6.919	1729	1735	1740	rBV3	782	1044	0.01%	0.005%
34	6.948	1742	1744	1749	rVV2	466	523	0.00%	0.002%
35	7.102	1784	1792	1798	rBV3	795	1133	0.01%	0.005%
36	7.186	1809	1818	1826	rBV6	2109	3385	0.03%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050953.D
 Acq On : 27 Sep 2022 13:47
 Operator : JC/MD
 Sample : N4854-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.218	1826	1828	1831	rVB2	662	355	0.00%	0.002%
38	7.353	1863	1870	1871	rBV	207	243	0.00%	0.001%
39	7.565	1919	1936	1954	rBV	177029	313219	2.90%	1.376%
40	7.797	2005	2008	2009	rBV2	510	309	0.00%	0.001%
41	7.899	2026	2040	2055	rBV	613948	1045792	9.68%	4.593%
42	8.031	2078	2081	2083	rVB3	669	382	0.00%	0.002%
43	8.086	2096	2098	2100	rBV2	592	306	0.00%	0.001%
44	8.179	2115	2127	2141	rBV	127373	216490	2.00%	0.951%
45	8.295	2160	2163	2166	rBV3	816	624	0.01%	0.003%
46	8.404	2194	2197	2200	rBV3	532	407	0.00%	0.002%
47	8.472	2209	2218	2226	rBV3	3881	6914	0.06%	0.030%
48	8.555	2228	2244	2258	rBV	6471895	10802791	100.00%	47.448%
49	8.636	2259	2269	2305	rVB3	468798	1020848	9.45%	4.484%
50	8.893	2347	2349	2354	rVB3	446	402	0.00%	0.002%
51	9.038	2391	2394	2399	rBV2	289	309	0.00%	0.001%
52	9.417	2499	2512	2548	rBV	646441	1059954	9.81%	4.656%
53	9.568	2555	2559	2568	rVB	1663	2247	0.02%	0.010%
54	9.636	2576	2580	2582	rBV3	467	427	0.00%	0.002%
55	9.661	2585	2588	2591	rVB2	382	295	0.00%	0.001%
56	9.694	2591	2598	2599	rBV4	1414	1372	0.01%	0.006%
57	9.755	2614	2617	2619	rBV	397	292	0.00%	0.001%
58	9.870	2651	2653	2657	rBV3	432	231	0.00%	0.001%
59	9.896	2657	2661	2665	rBV2	488	506	0.00%	0.002%
60	9.928	2668	2671	2677	rBV2	367	360	0.00%	0.002%
61	9.960	2677	2681	2684	rBV2	502	415	0.00%	0.002%
62	10.002	2689	2694	2697	rBV2	247	261	0.00%	0.001%
63	10.089	2717	2721	2722	rBV2	450	294	0.00%	0.001%
64	10.105	2723	2726	2737	rVB6	1817	2225	0.02%	0.010%
65	10.240	2763	2768	2773	rVB2	389	431	0.00%	0.002%
66	10.298	2781	2786	2789	rBV2	465	438	0.00%	0.002%
67	10.349	2798	2802	2809	rBV3	254	360	0.00%	0.002%
68	10.456	2830	2835	2837	rBV2	280	251	0.00%	0.001%
69	10.488	2841	2845	2847	rVV3	656	641	0.01%	0.003%
70	10.517	2851	2854	2857	rBV	359	272	0.00%	0.001%
71	10.639	2886	2892	2896	rBV4	1034	1324	0.01%	0.006%
72	10.755	2916	2928	2946	rBV	542453	873859	8.09%	3.838%
73	10.893	2964	2971	2982	rVB4	4944	7894	0.07%	0.035%
74	10.970	2993	2995	2999	rVB	468	312	0.00%	0.001%
75	11.002	2999	3005	3007	rBV2	561	568	0.01%	0.002%
76	11.092	3026	3033	3040	rBV4	806	1304	0.01%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050953.D
 Acq On : 27 Sep 2022 13:47
 Operator : JC/MD
 Sample : N4854-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.221	3070	3073	3076	rBV2	417	256	0.00%	0.001%
78	11.359	3112	3116	3119	rBV2	546	469	0.00%	0.002%
79	11.468	3143	3150	3161	rVB7	1850	3153	0.03%	0.014%
80	11.639	3199	3203	3205	rBV2	372	252	0.00%	0.001%
81	11.687	3215	3218	3220	rBV2	436	302	0.00%	0.001%
82	11.700	3220	3222	3225	rVB2	713	420	0.00%	0.002%
83	11.745	3230	3236	3245	rBV7	1890	2376	0.02%	0.010%
84	11.812	3245	3257	3274	rBV	555449	888009	8.22%	3.900%
85	12.073	3336	3338	3340	rBV2	542	234	0.00%	0.001%
86	12.192	3362	3375	3397	rBV	602529	986681	9.13%	4.334%
87	12.603	3500	3503	3505	rBV2	377	271	0.00%	0.001%
88	12.774	3546	3556	3563	rBV3	1312	2471	0.02%	0.011%
89	12.906	3594	3597	3604	rVB3	716	628	0.01%	0.003%
90	13.002	3623	3627	3631	rBV2	532	369	0.00%	0.002%
91	13.169	3676	3679	3683	rBV3	576	511	0.00%	0.002%
92	13.192	3683	3686	3688	rVV2	602	452	0.00%	0.002%
93	13.224	3692	3696	3709	rVV6	2381	3560	0.03%	0.016%
94	13.288	3713	3716	3721	rVV2	427	358	0.00%	0.002%
95	13.433	3756	3761	3765	rVB2	417	472	0.00%	0.002%
96	13.848	3885	3890	3897	rVB6	1842	2421	0.02%	0.011%
97	14.195	3996	3998	4009	rVB3	790	1094	0.01%	0.005%
98	14.336	4036	4042	4051	rVB6	1976	3016	0.03%	0.013%
99	14.571	4112	4115	4117	rBV3	1148	881	0.01%	0.004%
100	14.642	4131	4137	4138	rBV	526	582	0.01%	0.003%




Sum of corrected areas: 22767470

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050953.D
Acq On : 27 Sep 2022 13:47
Operator : JC/MD
Sample : N4854-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

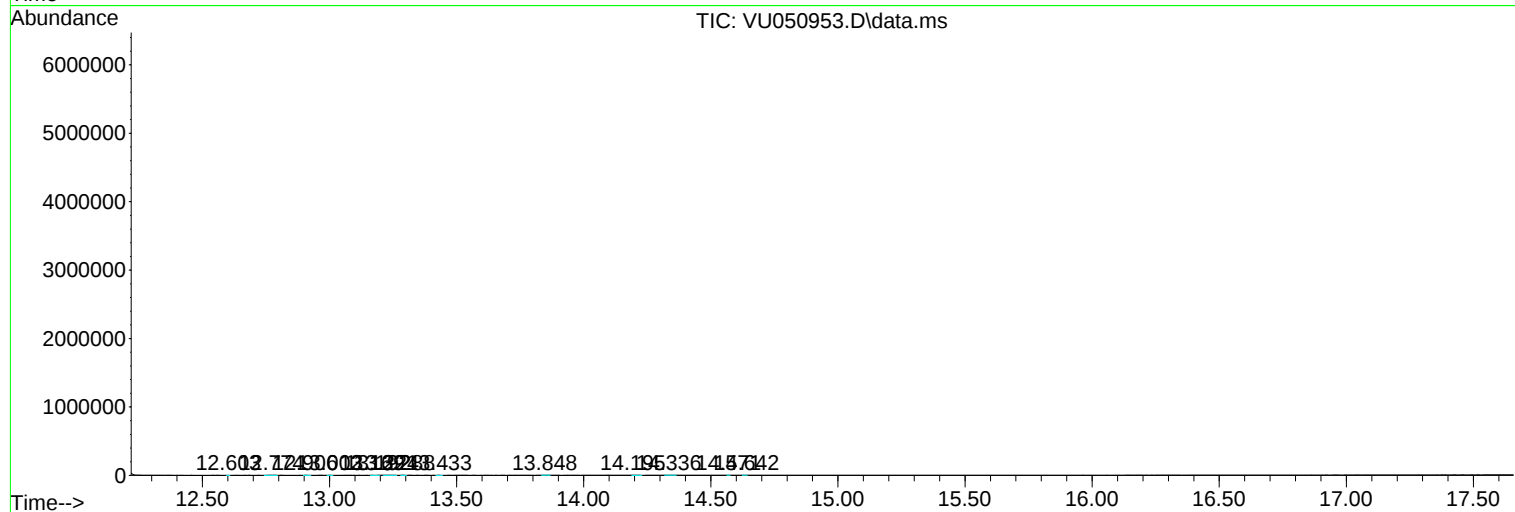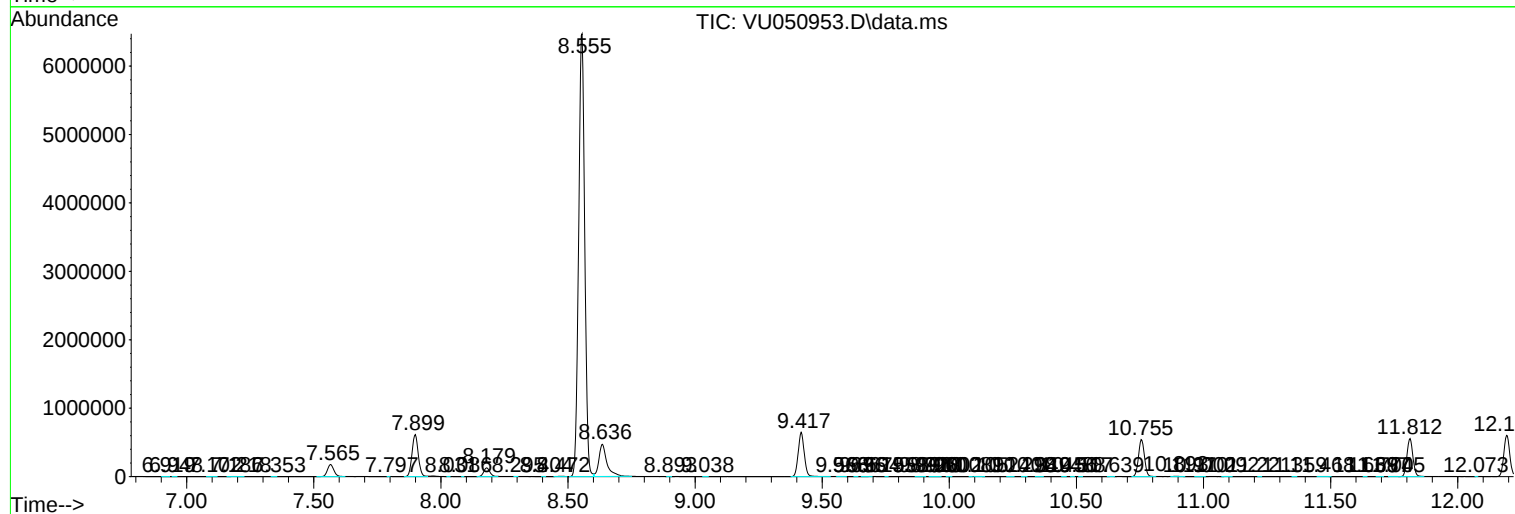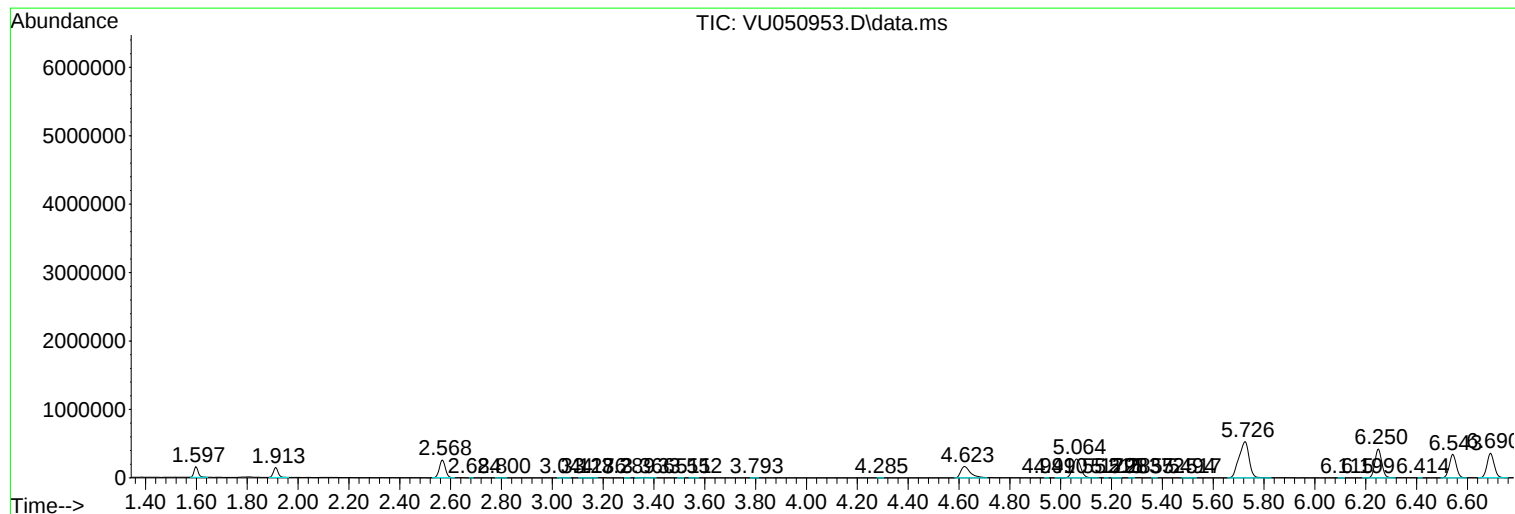

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050953.D
Acq On : 27 Sep 2022 13:47
Operator : JC/MD
Sample : N4854-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050953.D
Acq On : 27 Sep 2022 13:47
Operator : JC/MD
Sample : N4854-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------