

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050957.D
 Acq On : 27 Sep 2022 15:21
 Operator : JC/MD
 Sample : N4854-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	162839	186040	6.30%	1.285%
2	1.913	169	178	193	rVB	145468	193274	6.54%	1.335%
3	2.565	367	381	398	rBV	267175	442219	14.97%	3.054%
4	2.697	417	422	423	rBV2	371	337	0.01%	0.002%
5	2.938	494	497	501	rBV	385	286	0.01%	0.002%
6	3.044	521	530	538	rBV4	2233	3243	0.11%	0.022%
7	3.356	614	627	630	rBV5	3868	5699	0.19%	0.039%
8	3.427	646	649	652	rBV2	324	255	0.01%	0.002%
9	3.543	681	685	690	rVB3	362	378	0.01%	0.003%
10	3.591	693	700	704	rVV2	335	469	0.02%	0.003%
11	3.617	704	708	713	rVV	387	320	0.01%	0.002%
12	3.864	782	785	789	rVV3	307	320	0.01%	0.002%
13	3.890	789	793	797	rVB3	453	373	0.01%	0.003%
14	4.044	835	841	844	rBV2	399	327	0.01%	0.002%
15	4.218	891	895	897	rBV2	285	251	0.01%	0.002%
16	4.494	977	981	984	rVB2	450	345	0.01%	0.002%
17	4.530	990	992	1000	rVB2	218	246	0.01%	0.002%
18	4.617	1006	1019	1046	rBV	186984	463985	15.71%	3.205%
19	4.832	1083	1086	1089	rBV2	552	365	0.01%	0.003%
20	5.060	1139	1157	1184	rBV	289825	637568	21.59%	4.404%
21	5.369	1248	1253	1254	rBV2	414	333	0.01%	0.002%
22	5.469	1281	1284	1290	rVB2	341	342	0.01%	0.002%
23	5.507	1293	1296	1301	rBV3	300	251	0.01%	0.002%
24	5.723	1341	1363	1386	rBV2	552978	1534771	51.96%	10.600%
25	6.028	1454	1458	1460	rBV2	557	433	0.01%	0.003%
26	6.115	1481	1485	1491	rVB3	541	561	0.02%	0.004%
27	6.153	1495	1497	1501	rBV2	346	279	0.01%	0.002%
28	6.250	1512	1527	1550	rBV	397590	754853	25.56%	5.214%
29	6.485	1598	1600	1604	rVB3	367	273	0.01%	0.002%
30	6.533	1604	1615	1628	rVV5	16696	32947	1.12%	0.228%
31	6.690	1649	1664	1683	rBV	377210	736745	24.94%	5.089%
32	6.854	1714	1715	1719	rVB2	691	358	0.01%	0.002%
33	7.051	1773	1776	1779	rVV2	389	337	0.01%	0.002%
34	7.141	1801	1804	1807	rBV	325	283	0.01%	0.002%
35	7.186	1811	1818	1828	rVV6	1953	3758	0.13%	0.026%
36	7.388	1874	1881	1884	rBV	228	259	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050957.D
 Acq On : 27 Sep 2022 15:21
 Operator : JC/MD
 Sample : N4854-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.446	1895	1899	1904	rBV2	261	292	0.01%	0.002%
38	7.565	1923	1936	1965	rBV	182860	329762	11.16%	2.278%
39	7.687	1970	1974	1978	rVV2	1039	836	0.03%	0.006%
40	7.751	1990	1994	2002	rVB3	499	640	0.02%	0.004%
41	7.790	2002	2006	2009	rBV2	384	437	0.01%	0.003%
42	7.896	2025	2039	2055	rBV	633184	1083223	36.68%	7.482%
43	8.073	2092	2094	2100	rVB3	823	674	0.02%	0.005%
44	8.179	2115	2127	2152	rBV	131761	229173	7.76%	1.583%
45	8.321	2167	2171	2175	rBV3	874	770	0.03%	0.005%
46	8.385	2186	2191	2197	rBV4	342	410	0.01%	0.003%
47	8.475	2206	2219	2224	rBV6	1135	2165	0.07%	0.015%
48	8.552	2228	2243	2257	rBV	1779695	2953569	100.00%	20.400%
49	8.632	2257	2268	2302	rVB2	485712	1038645	35.17%	7.174%
50	8.912	2351	2355	2357	rBV3	490	363	0.01%	0.003%
51	9.166	2431	2434	2438	rBV3	397	294	0.01%	0.002%
52	9.231	2449	2454	2456	rBV2	395	303	0.01%	0.002%
53	9.350	2489	2491	2496	rVB2	524	390	0.01%	0.003%
54	9.417	2496	2512	2552	rBV	602280	1006242	34.07%	6.950%
55	9.626	2573	2577	2581	rVB2	348	315	0.01%	0.002%
56	9.694	2594	2598	2601	rBV3	560	544	0.02%	0.004%
57	9.841	2640	2644	2649	rVV3	380	358	0.01%	0.002%
58	9.874	2652	2654	2658	rVB2	389	262	0.01%	0.002%
59	10.050	2705	2709	2711	rBV2	515	272	0.01%	0.002%
60	10.369	2804	2808	2816	rVB3	542	652	0.02%	0.005%
61	10.446	2830	2832	2839	rVB2	324	270	0.01%	0.002%
62	10.481	2840	2843	2846	rBV2	338	256	0.01%	0.002%
63	10.565	2863	2869	2871	rBV2	298	316	0.01%	0.002%
64	10.671	2894	2902	2908	rBV4	1135	1407	0.05%	0.010%
65	10.755	2915	2928	2947	rBV	576791	933245	31.60%	6.446%
66	10.874	2962	2965	2967	rBV3	997	611	0.02%	0.004%
67	11.166	3052	3056	3062	rVB2	494	481	0.02%	0.003%
68	11.247	3077	3081	3084	rBV	295	332	0.01%	0.002%
69	11.308	3097	3100	3106	rVB2	421	362	0.01%	0.003%
70	11.456	3140	3146	3148	rBV3	922	980	0.03%	0.007%
71	11.517	3163	3165	3171	rBV2	484	490	0.02%	0.003%
72	11.636	3199	3202	3208	rBV2	265	274	0.01%	0.002%
73	11.748	3233	3237	3243	rVB4	1401	1285	0.04%	0.009%
74	11.809	3243	3256	3273	rBV	533061	836713	28.33%	5.779%
75	11.970	3303	3306	3307	rBV	788	501	0.02%	0.003%
76	12.015	3317	3320	3326	rVB2	394	357	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050957.D
 Acq On : 27 Sep 2022 15:21
 Operator : JC/MD
 Sample : N4854-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.070	3330	3337	3342	rBV3	2525	3142	0.11%	0.022%
78	12.192	3361	3375	3399	rBV	625838	1026891	34.77%	7.093%
79	12.320	3413	3415	3420	rVB3	847	476	0.02%	0.003%
80	12.459	3456	3458	3461	rVB3	676	407	0.01%	0.003%
81	12.513	3472	3475	3480	rBV3	547	518	0.02%	0.004%
82	12.565	3489	3491	3494	rBV2	547	340	0.01%	0.002%
83	12.655	3517	3519	3524	rBV2	305	282	0.01%	0.002%
84	12.838	3572	3576	3579	rBV4	746	725	0.02%	0.005%
85	12.896	3590	3594	3595	rBV2	482	356	0.01%	0.002%
86	13.108	3657	3660	3664	rVB2	703	550	0.02%	0.004%
87	13.131	3664	3667	3671	rBV2	499	461	0.02%	0.003%
88	13.153	3671	3674	3676	rBV	483	304	0.01%	0.002%
89	13.218	3691	3694	3696	rBV3	601	436	0.01%	0.003%
90	13.507	3781	3784	3790	rBV2	659	559	0.02%	0.004%
91	13.642	3822	3826	3831	rBV3	650	652	0.02%	0.005%
92	13.774	3865	3867	3870	rVB	790	381	0.01%	0.003%
93	13.796	3870	3874	3878	rBV3	541	455	0.02%	0.003%
94	13.848	3885	3890	3894	rBV5	1054	955	0.03%	0.007%
95	14.037	3942	3949	3957	rVB9	3936	5538	0.19%	0.038%
96	14.269	4018	4021	4025	rBV2	632	620	0.02%	0.004%
97	14.333	4038	4041	4043	rBV3	877	460	0.02%	0.003%
98	15.269	4329	4332	4335	rBV2	588	476	0.02%	0.003%
99	15.439	4382	4385	4388	rBV2	863	553	0.02%	0.004%
100	15.587	4427	4431	4435	rBV5	1217	1209	0.04%	0.008%




Sum of corrected areas: 14478300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050957.D
Acq On : 27 Sep 2022 15:21
Operator : JC/MD
Sample : N4854-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

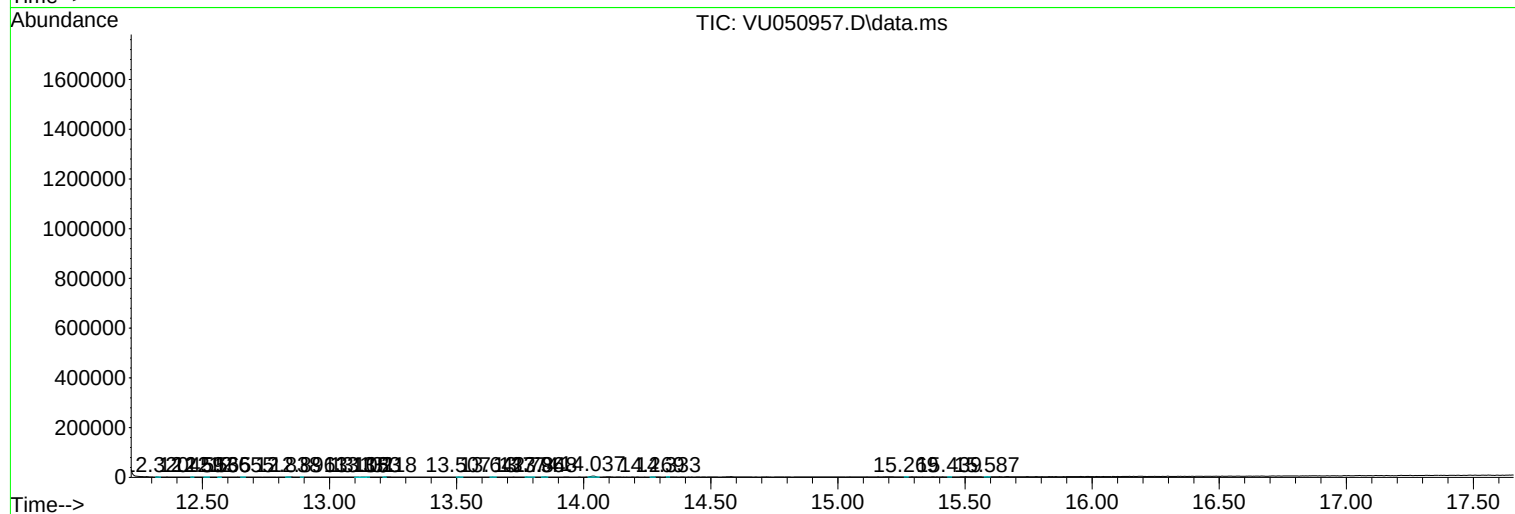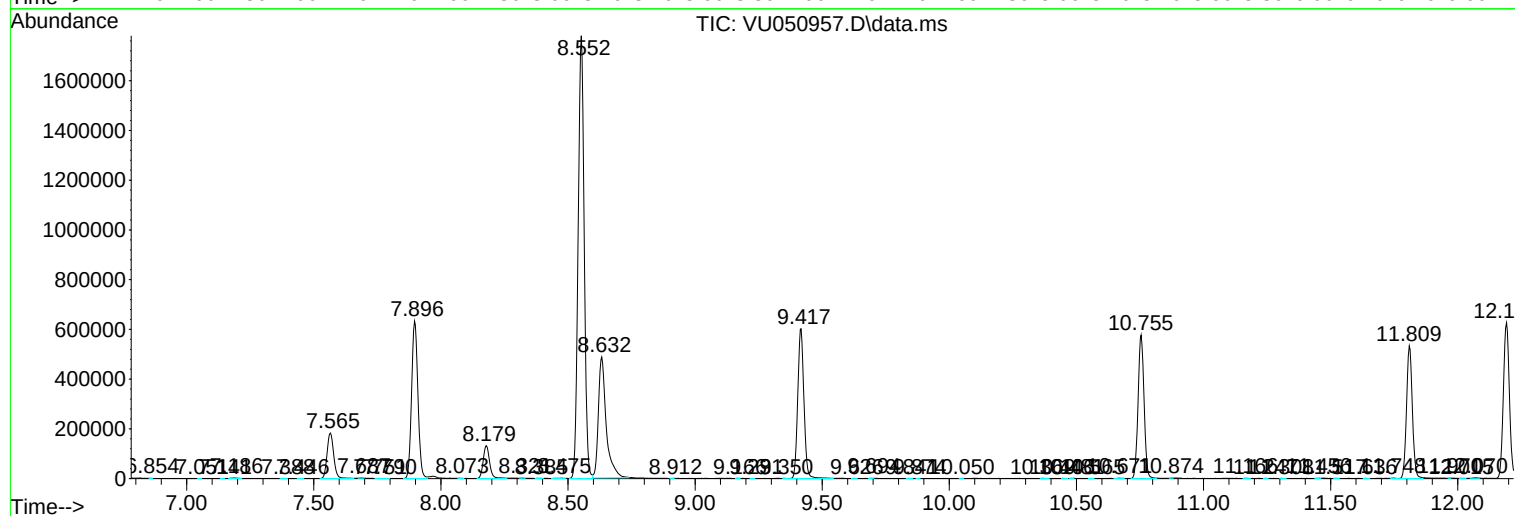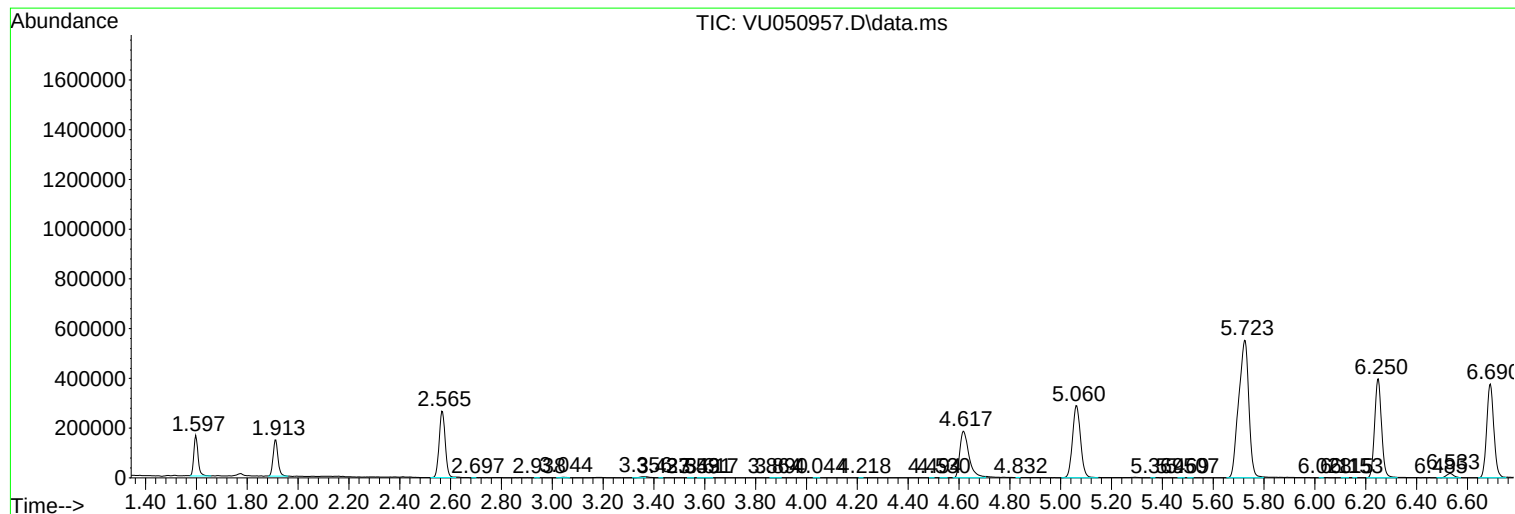

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050957.D
Acq On : 27 Sep 2022 15:21
Operator : JC/MD
Sample : N4854-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050957.D
Acq On : 27 Sep 2022 15:21
Operator : JC/MD
Sample : N4854-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------