

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050959.D
 Acq On : 27 Sep 2022 16:08
 Operator : JC/MD
 Sample : N4854-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	660	662	668	rVB2	260	200	0.01%	0.011%
2	3.527	677	680	683	rVB	283	172	0.01%	0.009%
3	3.591	697	700	701	rBV2	251	119	0.01%	0.006%
4	3.678	724	727	732	rVB2	368	302	0.02%	0.016%
5	3.710	732	737	742	rBV2	373	444	0.03%	0.024%
6	3.829	771	774	779	rBV	336	270	0.02%	0.015%
7	4.022	832	834	837	rBV2	169	112	0.01%	0.006%
8	4.073	847	850	854	rBV2	166	179	0.01%	0.010%
9	4.138	868	870	872	rVB	377	147	0.01%	0.008%
10	4.186	883	885	886	rBV	206	100	0.01%	0.005%
11	4.331	928	930	934	rVB2	242	106	0.01%	0.006%
12	4.353	934	937	939	rBV	163	104	0.01%	0.006%
13	4.787	1070	1072	1075	rVB	263	93	0.01%	0.005%
14	4.839	1083	1088	1092	rBV2	348	297	0.02%	0.016%
15	4.874	1092	1099	1103	rBV2	233	358	0.02%	0.019%
16	4.941	1118	1120	1124	rBV2	194	148	0.01%	0.008%
17	5.273	1220	1223	1224	rBV2	413	269	0.02%	0.014%
18	5.369	1250	1253	1257	rVB2	430	305	0.02%	0.016%
19	5.507	1292	1296	1302	rVB2	343	392	0.02%	0.021%
20	5.536	1302	1305	1307	rBV	297	217	0.01%	0.012%
21	5.601	1322	1325	1328	rBV2	135	86	0.00%	0.005%
22	5.620	1328	1331	1333	rBV	235	159	0.01%	0.009%
23	5.658	1340	1343	1344	rBV2	128	72	0.00%	0.004%
24	5.707	1349	1358	1365	rBV6	2454	5087	0.29%	0.274%
25	5.996	1442	1448	1454	rBV2	311	500	0.03%	0.027%
26	6.141	1492	1493	1494	rBB	22	12	0.00%	0.001%
27	6.250	1517	1527	1537	rBV2	2195	3688	0.21%	0.198%
28	6.340	1550	1555	1557	rBV2	328	257	0.01%	0.014%
29	6.443	1583	1587	1590	rBV2	252	185	0.01%	0.010%
30	6.546	1610	1619	1629	rVB4	3837	6566	0.37%	0.353%
31	6.652	1650	1652	1654	rBV	149	95	0.01%	0.005%
32	6.681	1657	1661	1662	rBV2	677	416	0.02%	0.022%
33	6.755	1682	1684	1687	rVB	257	129	0.01%	0.007%
34	6.777	1687	1691	1694	rBV2	262	247	0.01%	0.013%
35	6.816	1700	1703	1706	rBV	240	144	0.01%	0.008%
36	6.948	1741	1744	1752	rBV2	346	444	0.03%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050959.D
 Acq On : 27 Sep 2022 16:08
 Operator : JC/MD
 Sample : N4854-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.051	1773	1776	1780	rBV	142	110	0.01%	0.006%
38	7.105	1788	1793	1802	rVB3	1102	1620	0.09%	0.087%
39	7.228	1826	1831	1837	rBV2	260	302	0.02%	0.016%
40	7.282	1845	1848	1851	rBV2	179	128	0.01%	0.007%
41	7.392	1879	1882	1883	rBV	155	89	0.01%	0.005%
42	7.555	1931	1933	1934	rBV	375	181	0.01%	0.010%
43	7.687	1971	1974	1977	rBV2	247	192	0.01%	0.010%
44	7.771	1998	2000	2001	rBV2	184	64	0.00%	0.003%
45	7.858	2025	2027	2028	rBV	186	60	0.00%	0.003%
46	7.903	2032	2041	2051	rVB2	3783	6616	0.37%	0.356%
47	8.041	2081	2084	2087	rBV2	232	221	0.01%	0.012%
48	8.176	2120	2126	2128	rBV2	578	621	0.04%	0.033%
49	8.234	2138	2144	2147	rBV3	591	631	0.04%	0.034%
50	8.552	2229	2243	2270	rBV	1036555	1768522	100.00%	95.102%
51	9.006	2382	2384	2385	rBV	249	86	0.00%	0.005%
52	9.231	2452	2454	2456	rBV	292	132	0.01%	0.007%
53	9.353	2487	2492	2495	rBV2	423	457	0.03%	0.025%
54	9.424	2503	2514	2520	rBV4	6007	9942	0.56%	0.535%
55	9.507	2537	2540	2542	rBV2	308	219	0.01%	0.012%
56	9.536	2547	2549	2552	rBV2	226	164	0.01%	0.009%
57	9.761	2616	2619	2622	rBV	393	323	0.02%	0.017%
58	10.597	2877	2879	2885	rBV2	351	293	0.02%	0.016%
59	10.887	2964	2969	2970	rBV2	2381	1811	0.10%	0.097%
60	11.751	3235	3238	3243	rVB3	545	450	0.03%	0.024%
61	11.816	3249	3258	3272	rBV3	15196	24851	1.41%	1.336%
62	12.195	3368	3376	3387	rBV4	12273	18935	1.07%	1.018%
63	12.806	3564	3566	3568	rBV	278	160	0.01%	0.009%




Sum of corrected areas: 1859601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050959.D
Acq On : 27 Sep 2022 16:08
Operator : JC/MD
Sample : N4854-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

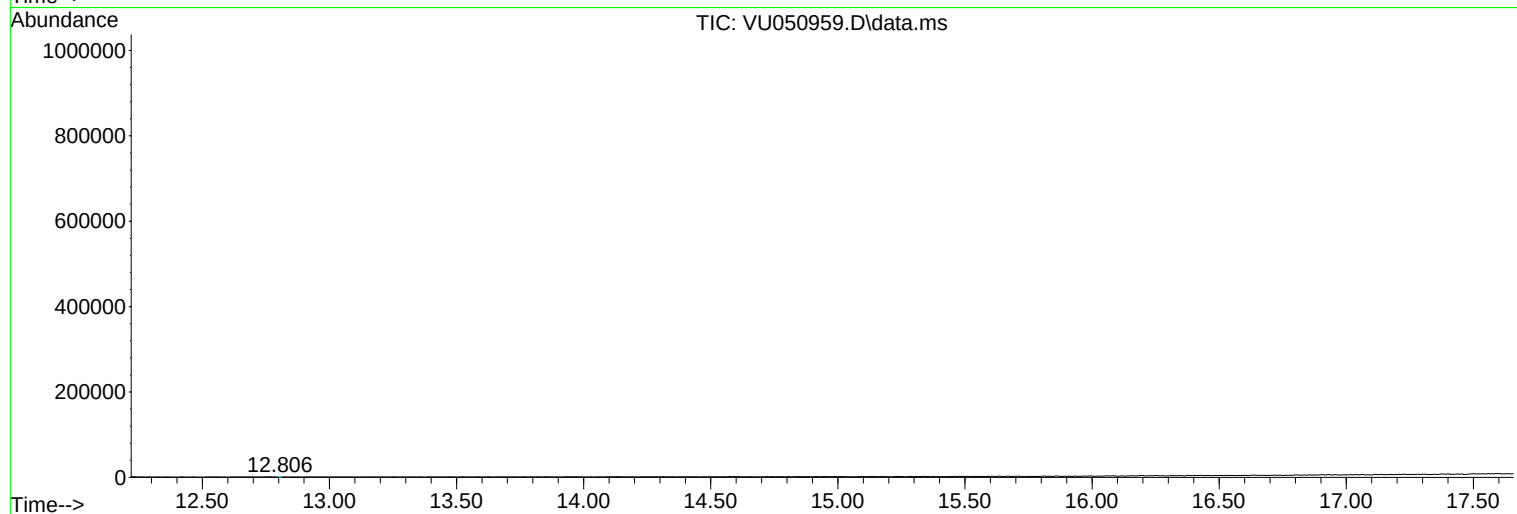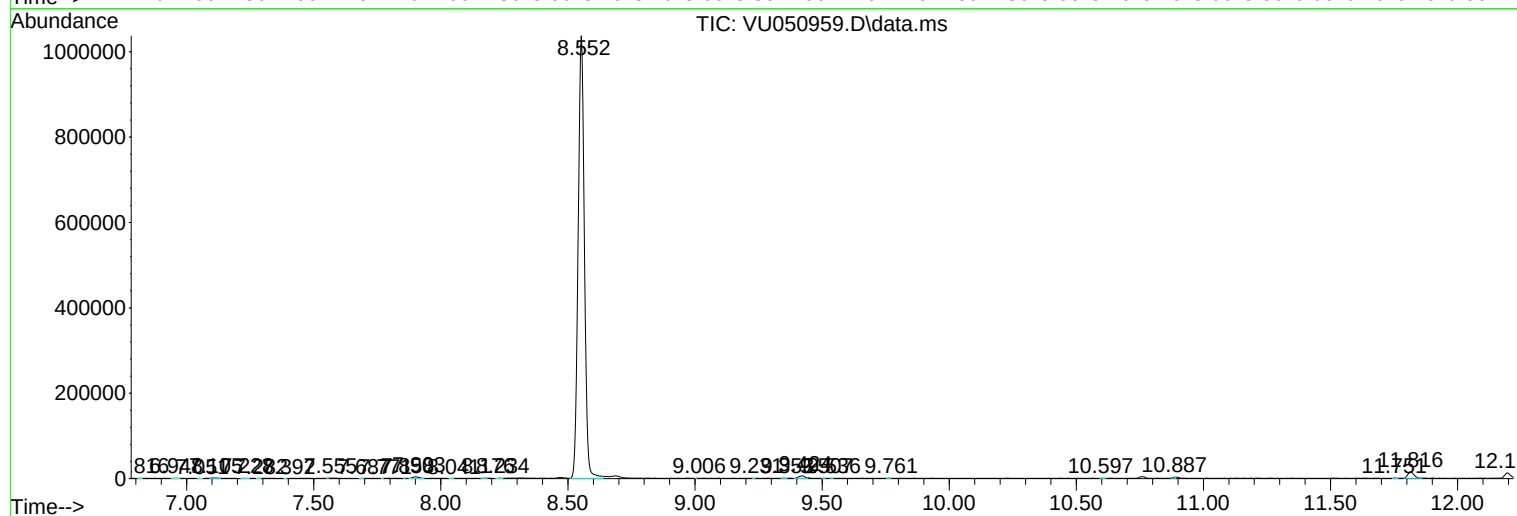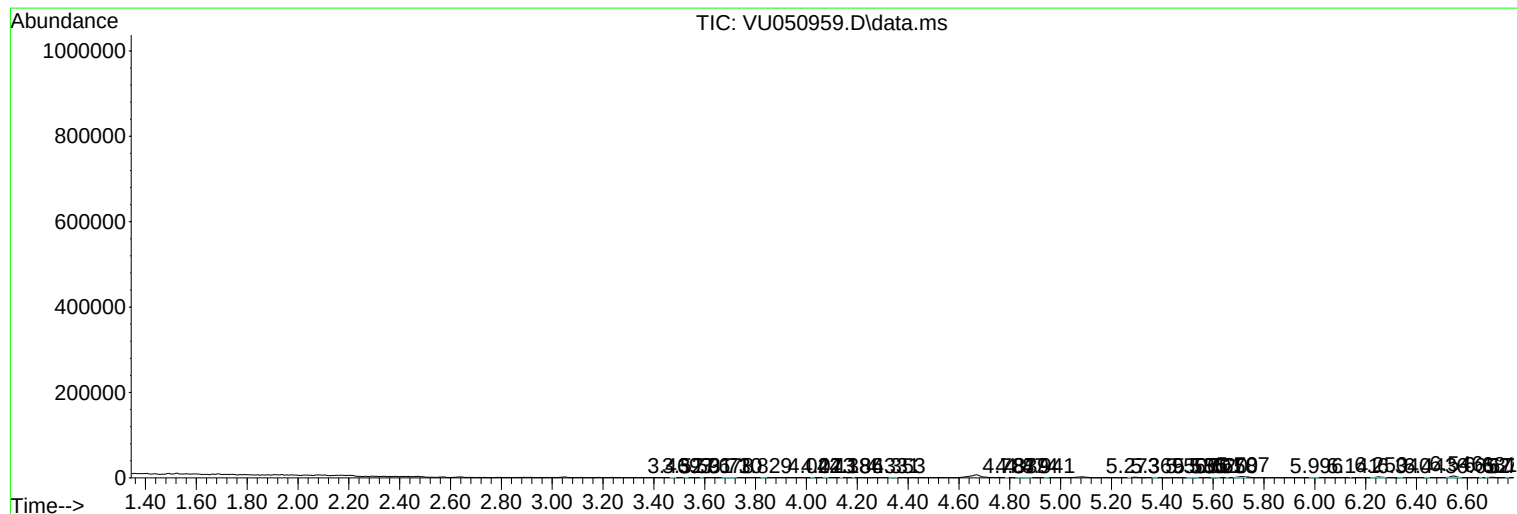

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050959.D
Acq On : 27 Sep 2022 16:08
Operator : JC/MD
Sample : N4854-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050959.D
Acq On : 27 Sep 2022 16:08
Operator : JC/MD
Sample : N4854-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------