

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050963.D
 Acq On : 27 Sep 2022 17:42
 Operator : JC/MD
 Sample : N4854-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050963.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	151280	171646	5.69%	1.236%
2	1.912	170	178	191	rVB	138657	179331	5.95%	1.292%
3	2.565	369	381	412	rVB	248082	411459	13.65%	2.964%
4	2.748	436	438	440	rVB2	544	218	0.01%	0.002%
5	2.780	446	448	450	rBV2	419	276	0.01%	0.002%
6	2.874	472	477	479	rBV2	278	286	0.01%	0.002%
7	3.044	523	530	539	rBV2	2251	3775	0.13%	0.027%
8	3.179	563	572	574	rBV4	1390	1874	0.06%	0.013%
9	3.362	616	629	639	rBV7	3660	6992	0.23%	0.050%
10	3.443	651	654	657	rBV2	448	304	0.01%	0.002%
11	3.645	712	717	719	rBV2	438	366	0.01%	0.003%
12	3.787	755	761	764	rBV3	249	258	0.01%	0.002%
13	3.877	785	789	793	rBV	282	339	0.01%	0.002%
14	4.031	835	837	843	rVB2	222	222	0.01%	0.002%
15	4.144	870	872	878	rVB2	313	289	0.01%	0.002%
16	4.285	912	916	919	rBV	329	264	0.01%	0.002%
17	4.333	927	931	936	rBV2	255	268	0.01%	0.002%
18	4.446	962	966	971	rBV2	229	220	0.01%	0.002%
19	4.472	971	974	979	rVB	387	256	0.01%	0.002%
20	4.616	1007	1019	1047	rBV2	173535	432649	14.35%	3.117%
21	4.829	1082	1085	1089	rVB3	556	416	0.01%	0.003%
22	4.899	1104	1107	1111	rVB4	539	383	0.01%	0.003%
23	5.063	1140	1158	1183	rBV	273205	612770	20.33%	4.414%
24	5.288	1220	1228	1238	rBV6	1531	2727	0.09%	0.020%
25	5.456	1277	1280	1284	rBV2	336	273	0.01%	0.002%
26	5.722	1342	1363	1382	rBV2	516207	1429823	47.43%	10.300%
27	5.970	1438	1440	1444	rVB2	489	355	0.01%	0.003%
28	6.250	1512	1527	1549	rBV	386907	737762	24.47%	5.315%
29	6.468	1593	1595	1599	rVB2	387	244	0.01%	0.002%
30	6.533	1599	1615	1628	rBV7	16078	36046	1.20%	0.260%
31	6.632	1643	1646	1650	rVB	380	244	0.01%	0.002%
32	6.690	1650	1664	1686	rBV	355747	696912	23.12%	5.020%
33	6.973	1748	1752	1754	rVV2	323	278	0.01%	0.002%
34	7.038	1767	1772	1773	rBV2	450	290	0.01%	0.002%
35	7.105	1781	1793	1804	rVB3	5795	9867	0.33%	0.071%
36	7.182	1812	1817	1819	rBV3	1680	1653	0.05%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050963.D
 Acq On : 27 Sep 2022 17:42
 Operator : JC/MD
 Sample : N4854-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.250	1833	1838	1844	rBV2	307	312	0.01%	0.002%
38	7.382	1872	1879	1883	rBV2	447	470	0.02%	0.003%
39	7.423	1890	1892	1895	rVB2	453	306	0.01%	0.002%
40	7.456	1895	1902	1905	rBV2	455	643	0.02%	0.005%
41	7.565	1924	1936	1958	rBV2	167638	296992	9.85%	2.139%
42	7.809	2008	2012	2017	rBV4	311	345	0.01%	0.002%
43	7.896	2026	2039	2055	rBV	571115	984674	32.66%	7.093%
44	8.076	2093	2095	2101	rVB4	467	267	0.01%	0.002%
45	8.179	2115	2127	2143	rBV	122075	206710	6.86%	1.489%
46	8.455	2209	2213	2214	rBV	575	388	0.01%	0.003%
47	8.552	2229	2243	2257	rBV	1789219	3014515	100.00%	21.716%
48	8.632	2258	2268	2302	rVB3	467237	979294	32.49%	7.055%
49	8.992	2378	2380	2387	rVB3	525	513	0.02%	0.004%
50	9.034	2391	2393	2399	rVB3	506	404	0.01%	0.003%
51	9.095	2408	2412	2413	rBV3	435	279	0.01%	0.002%
52	9.240	2453	2457	2461	rBV2	270	347	0.01%	0.002%
53	9.417	2497	2512	2540	rBV	596182	998842	33.13%	7.195%
54	9.539	2548	2550	2555	rBV3	483	375	0.01%	0.003%
55	9.581	2561	2563	2569	rVB5	815	752	0.02%	0.005%
56	9.700	2594	2600	2605	rVB3	817	900	0.03%	0.006%
57	9.729	2605	2609	2613	rBV	317	324	0.01%	0.002%
58	9.867	2646	2652	2656	rBV2	353	454	0.02%	0.003%
59	10.012	2693	2697	2701	rBV3	422	332	0.01%	0.002%
60	10.079	2714	2718	2723	rVB2	590	635	0.02%	0.005%
61	10.118	2723	2730	2733	rBV2	549	581	0.02%	0.004%
62	10.211	2753	2759	2761	rBV3	422	443	0.01%	0.003%
63	10.491	2842	2846	2850	rVB2	593	507	0.02%	0.004%
64	10.664	2897	2900	2907	rVB2	1003	888	0.03%	0.006%
65	10.754	2914	2928	2948	rBV	560116	899921	29.85%	6.483%
66	10.896	2970	2972	2982	rVB3	1626	1515	0.05%	0.011%
67	10.979	2996	2998	3004	rVB3	490	306	0.01%	0.002%
68	11.092	3029	3033	3040	rBV4	478	559	0.02%	0.004%
69	11.137	3044	3047	3052	rBV2	344	279	0.01%	0.002%
70	11.298	3090	3097	3103	rBV3	411	573	0.02%	0.004%
71	11.343	3108	3111	3120	rVB3	428	489	0.02%	0.004%
72	11.388	3120	3125	3127	rBV3	334	321	0.01%	0.002%
73	11.452	3141	3145	3147	rBV2	917	732	0.02%	0.005%
74	11.696	3217	3221	3227	rBV2	484	635	0.02%	0.005%
75	11.745	3234	3236	3240	rVB3	565	369	0.01%	0.003%
76	11.809	3243	3256	3285	rBV	494372	797712	26.46%	5.746%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050963.D
 Acq On : 27 Sep 2022 17:42
 Operator : JC/MD
 Sample : N4854-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.066	3334	3336	3339	rBV2	312	239	0.01%	0.002%
78	12.082	3339	3341	3345	rVB2	562	375	0.01%	0.003%
79	12.192	3362	3375	3392	rBV	569811	933233	30.96%	6.723%
80	12.340	3418	3421	3425	rBV3	758	619	0.02%	0.004%
81	12.626	3504	3510	3513	rBV2	582	636	0.02%	0.005%
82	12.960	3612	3614	3620	rVB3	500	489	0.02%	0.004%
83	12.983	3620	3621	3626	rBV3	321	234	0.01%	0.002%
84	13.021	3630	3633	3635	rBV2	357	235	0.01%	0.002%
85	13.397	3748	3750	3753	rBV	449	283	0.01%	0.002%
86	13.581	3805	3807	3810	rVB2	477	288	0.01%	0.002%
87	14.410	4063	4065	4067	rBV2	469	294	0.01%	0.002%
88	14.462	4078	4081	4087	rVB2	1431	1210	0.04%	0.009%
89	14.574	4110	4116	4121	rBV3	1491	1874	0.06%	0.013%
90	14.684	4148	4150	4151	rBV	520	250	0.01%	0.002%
91	14.738	4163	4167	4170	rBV2	612	508	0.02%	0.004%
92	14.761	4171	4174	4178	rVV2	979	676	0.02%	0.005%
93	14.802	4185	4187	4190	rBV2	803	457	0.02%	0.003%
94	14.995	4245	4247	4250	rBV2	668	313	0.01%	0.002%
95	15.092	4273	4277	4283	rBV3	588	709	0.02%	0.005%
96	15.121	4283	4286	4289	rVB2	892	572	0.02%	0.004%
97	15.327	4347	4350	4351	rBV2	628	383	0.01%	0.003%
98	15.362	4359	4361	4364	rBV2	617	378	0.01%	0.003%
99	15.397	4369	4372	4377	rBV3	740	699	0.02%	0.005%
100	15.497	4400	4403	4407	rVB3	990	587	0.02%	0.004%




Sum of corrected areas: 13881779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050963.D
Acq On : 27 Sep 2022 17:42
Operator : JC/MD
Sample : N4854-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

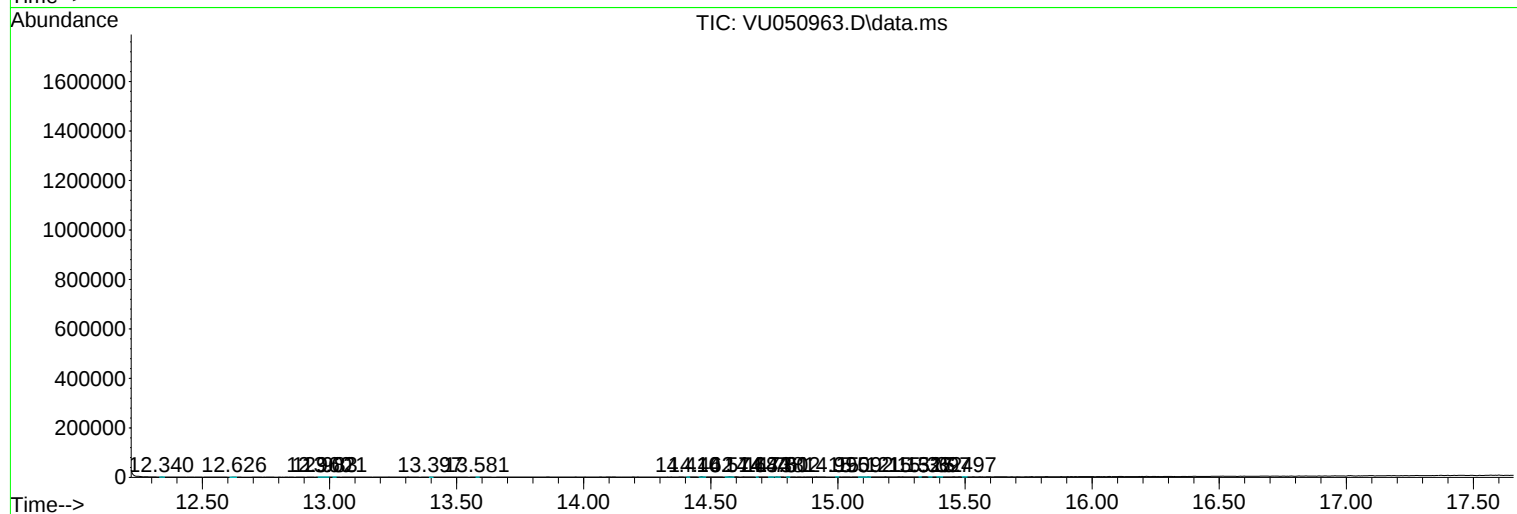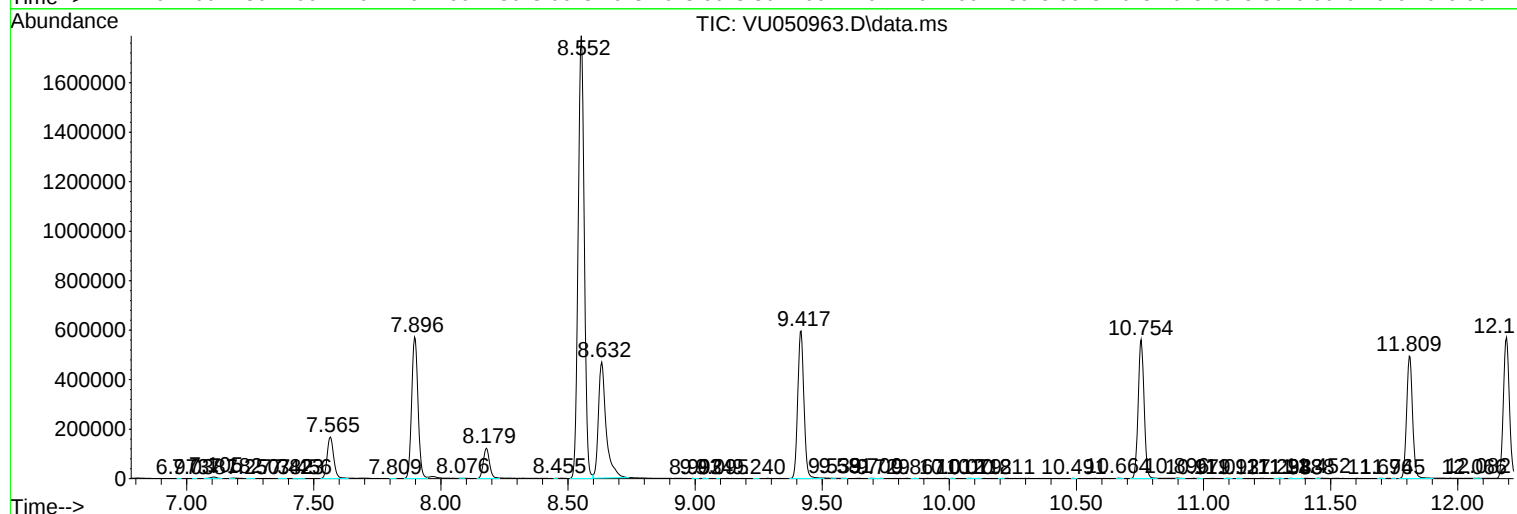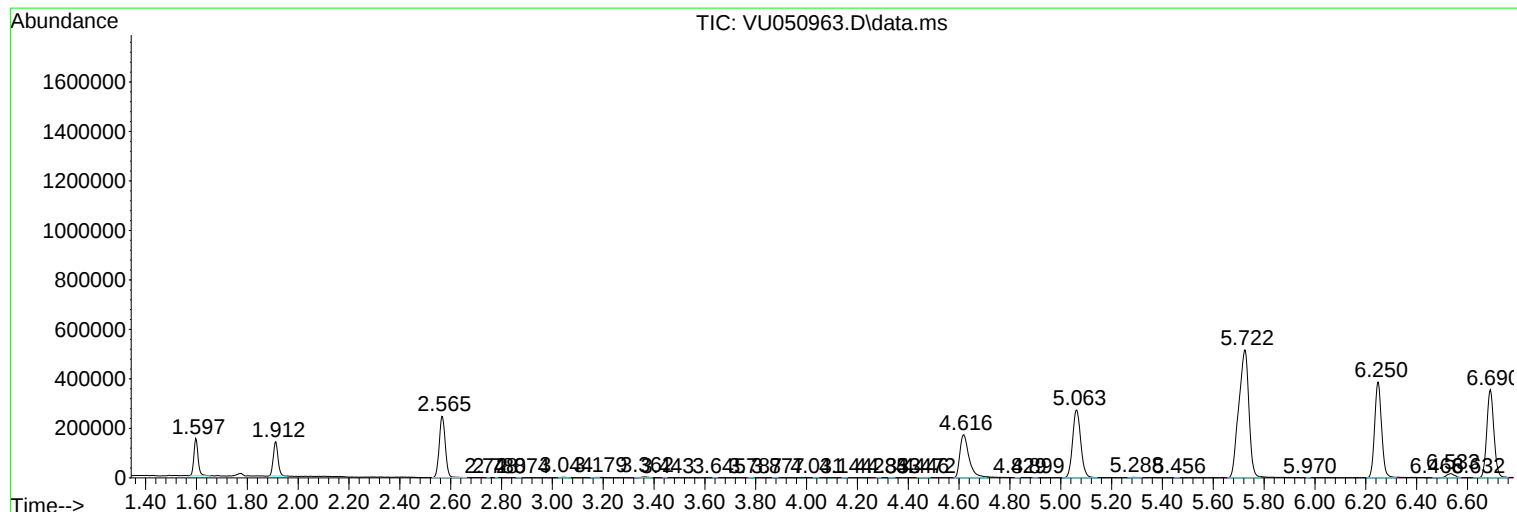

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050963.D
Acq On : 27 Sep 2022 17:42
Operator : JC/MD
Sample : N4854-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050963.D
Acq On : 27 Sep 2022 17:42
Operator : JC/MD
Sample : N4854-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------