

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050964.D
 Acq On : 27 Sep 2022 18:06
 Operator : JC/MD
 Sample : N4854-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	147025	172162	11.88%	1.451%
2	1.912	170	178	199	rVB	140264	186154	12.85%	1.569%
3	2.568	369	382	402	rBV	249177	412428	28.47%	3.477%
4	2.719	427	429	434	rBV2	279	257	0.02%	0.002%
5	2.787	447	450	461	rVB4	610	924	0.06%	0.008%
6	2.899	480	485	488	rBV3	305	359	0.02%	0.003%
7	2.954	496	502	509	rBV3	586	895	0.06%	0.008%
8	3.044	524	530	539	rVB4	1878	3117	0.22%	0.026%
9	3.128	553	556	559	rBV	341	273	0.02%	0.002%
10	3.189	563	575	583	rVV3	1312	3097	0.21%	0.026%
11	3.324	611	617	622	rBV2	290	362	0.02%	0.003%
12	3.362	622	629	639	rVV4	1092	1697	0.12%	0.014%
13	3.623	706	710	713	rBV	402	244	0.02%	0.002%
14	3.645	713	717	721	rVB	289	245	0.02%	0.002%
15	3.706	732	736	738	rBV2	344	242	0.02%	0.002%
16	3.771	751	756	759	rBV	281	276	0.02%	0.002%
17	3.806	762	767	769	rBV2	321	274	0.02%	0.002%
18	4.150	869	874	877	rBV2	260	236	0.02%	0.002%
19	4.275	908	913	916	rBV2	378	333	0.02%	0.003%
20	4.549	995	998	1001	rVB2	326	238	0.02%	0.002%
21	4.616	1006	1019	1050	rBV	178740	447196	30.87%	3.770%
22	4.935	1115	1118	1122	rBV3	369	334	0.02%	0.003%
23	4.964	1125	1127	1133	rVB3	626	551	0.04%	0.005%
24	4.996	1133	1137	1140	rBV2	461	341	0.02%	0.003%
25	5.060	1140	1157	1181	rBV	276940	607843	41.95%	5.124%
26	5.253	1213	1217	1220	rVB3	589	398	0.03%	0.003%
27	5.362	1248	1251	1253	rBV2	391	233	0.02%	0.002%
28	5.378	1253	1256	1261	rVB4	603	434	0.03%	0.004%
29	5.497	1289	1293	1294	rBV2	325	222	0.02%	0.002%
30	5.584	1313	1320	1323	rBV	423	495	0.03%	0.004%
31	5.722	1342	1363	1390	rBV2	520850	1448808	100.00%	12.213%
32	5.925	1424	1426	1430	rVB3	559	299	0.02%	0.003%
33	6.034	1454	1460	1467	rVB4	572	746	0.05%	0.006%
34	6.121	1480	1487	1492	rBV3	562	750	0.05%	0.006%
35	6.185	1503	1507	1509	rBV3	422	270	0.02%	0.002%
36	6.250	1513	1527	1550	rVV	413512	789215	54.47%	6.653%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050964.D
 Acq On : 27 Sep 2022 18:06
 Operator : JC/MD
 Sample : N4854-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.417	1577	1579	1583	rVB4	451	241	0.02%	0.002%
38	6.472	1591	1596	1597	rBV2	413	328	0.02%	0.003%
39	6.529	1602	1614	1628	rVB3	13167	25429	1.76%	0.214%
40	6.690	1649	1664	1685	rBV	355859	699342	48.27%	5.895%
41	6.809	1698	1701	1702	rBV2	768	474	0.03%	0.004%
42	6.870	1718	1720	1725	rVB3	507	462	0.03%	0.004%
43	6.976	1749	1753	1755	rBV2	273	220	0.02%	0.002%
44	7.044	1769	1774	1776	rBV2	454	479	0.03%	0.004%
45	7.099	1788	1791	1795	rBV2	349	268	0.02%	0.002%
46	7.189	1812	1819	1832	rVB6	2223	4034	0.28%	0.034%
47	7.237	1832	1834	1840	rVB	390	293	0.02%	0.002%
48	7.449	1896	1900	1905	rBV2	359	306	0.02%	0.003%
49	7.565	1921	1936	1956	rBV	170486	304000	20.98%	2.563%
50	7.693	1966	1976	1981	rBV4	1687	2380	0.16%	0.020%
51	7.896	2025	2039	2054	rBV	582855	1001686	69.14%	8.444%
52	8.115	2104	2107	2111	rBV3	414	237	0.02%	0.002%
53	8.179	2115	2127	2148	rBV	124453	212634	14.68%	1.792%
54	8.291	2160	2162	2167	rVB3	630	431	0.03%	0.004%
55	8.471	2213	2218	2228	rVB4	1284	1549	0.11%	0.013%
56	8.552	2230	2243	2257	rBV	472901	797125	55.02%	6.719%
57	8.632	2257	2268	2302	rVB2	456412	955403	65.94%	8.054%
58	8.835	2329	2331	2333	rBV	462	286	0.02%	0.002%
59	8.893	2347	2349	2352	rBV3	487	253	0.02%	0.002%
60	8.954	2366	2368	2372	rVB2	451	253	0.02%	0.002%
61	8.973	2372	2374	2380	rVB3	341	234	0.02%	0.002%
62	9.028	2386	2391	2396	rBV3	239	320	0.02%	0.003%
63	9.317	2476	2481	2489	rVB3	284	432	0.03%	0.004%
64	9.369	2493	2497	2498	rBV	373	257	0.02%	0.002%
65	9.417	2498	2512	2535	rBV	645112	1059273	73.11%	8.929%
66	9.664	2586	2589	2592	rVB	436	247	0.02%	0.002%
67	9.690	2592	2597	2605	rVB5	657	953	0.07%	0.008%
68	9.873	2651	2654	2660	rVV4	415	529	0.04%	0.004%
69	9.918	2665	2668	2672	rVV2	362	251	0.02%	0.002%
70	9.979	2685	2687	2692	rVB2	358	242	0.02%	0.002%
71	10.018	2697	2699	2706	rVB4	432	427	0.03%	0.004%
72	10.073	2712	2716	2719	rBV	344	291	0.02%	0.002%
73	10.201	2752	2756	2760	rBV2	404	353	0.02%	0.003%
74	10.262	2769	2775	2777	rBV	465	382	0.03%	0.003%
75	10.603	2878	2881	2885	rBV	374	340	0.02%	0.003%
76	10.664	2896	2900	2901	rBV	794	432	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050964.D
 Acq On : 27 Sep 2022 18:06
 Operator : JC/MD
 Sample : N4854-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	10.754	2914	2928	2954	rBV	567153	907060	62.61%	7.646%
78	10.848	2954	2957	2958	rBV	366	231	0.02%	0.002%
79	10.883	2966	2968	2969	rBV	704	323	0.02%	0.003%
80	10.896	2970	2972	2977	rVB2	1495	1023	0.07%	0.009%
81	10.954	2987	2990	2997	rVB3	423	482	0.03%	0.004%
82	11.057	3017	3022	3028	rBV2	430	595	0.04%	0.005%
83	11.249	3078	3082	3085	rVV2	398	269	0.02%	0.002%
84	11.266	3085	3087	3091	rVB	390	225	0.02%	0.002%
85	11.327	3100	3106	3110	rBV3	473	598	0.04%	0.005%
86	11.458	3144	3147	3151	rVV2	604	479	0.03%	0.004%
87	11.700	3217	3222	3225	rBV4	525	420	0.03%	0.004%
88	11.812	3244	3257	3275	rBV	527346	846002	58.39%	7.131%
89	12.085	3339	3342	3344	rVB3	594	368	0.03%	0.003%
90	12.192	3360	3375	3395	rBV	580639	945840	65.28%	7.973%
91	12.423	3444	3447	3450	rVB3	574	398	0.03%	0.003%
92	12.767	3551	3554	3559	rBV2	510	567	0.04%	0.005%
93	12.847	3575	3579	3585	rBV3	438	457	0.03%	0.004%
94	13.217	3689	3694	3695	rBV3	663	544	0.04%	0.005%
95	13.349	3732	3735	3738	rBV3	415	268	0.02%	0.002%
96	13.468	3769	3772	3777	rVB2	623	454	0.03%	0.004%
97	13.494	3777	3780	3783	rBV2	642	531	0.04%	0.004%
98	13.542	3793	3795	3797	rBV	358	225	0.02%	0.002%
99	13.986	3930	3933	3934	rBV	500	320	0.02%	0.003%
100	14.076	3958	3961	3965	rBV3	412	328	0.02%	0.003%




Sum of corrected areas: 11863031

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050964.D
Acq On : 27 Sep 2022 18:06
Operator : JC/MD
Sample : N4854-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

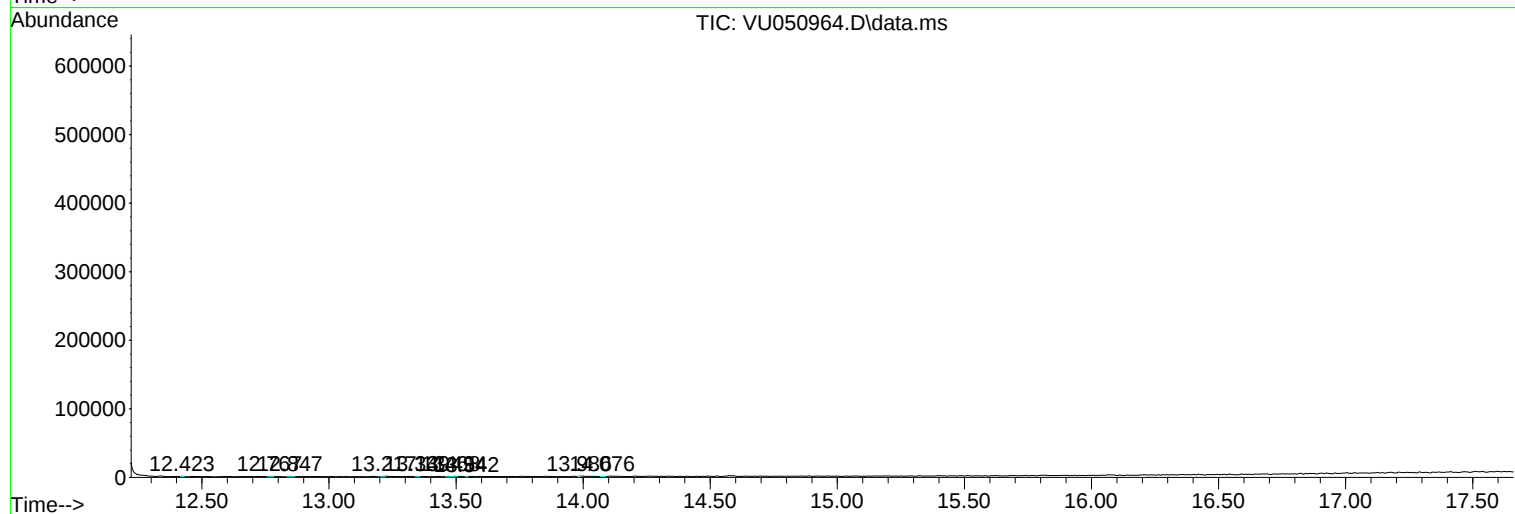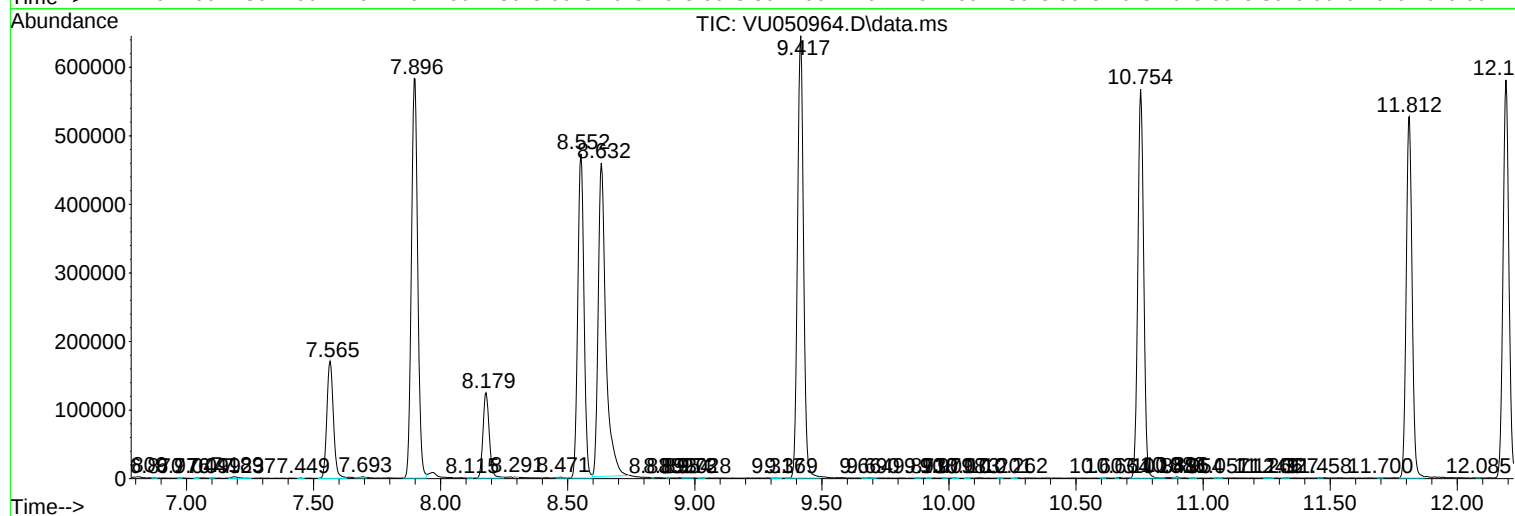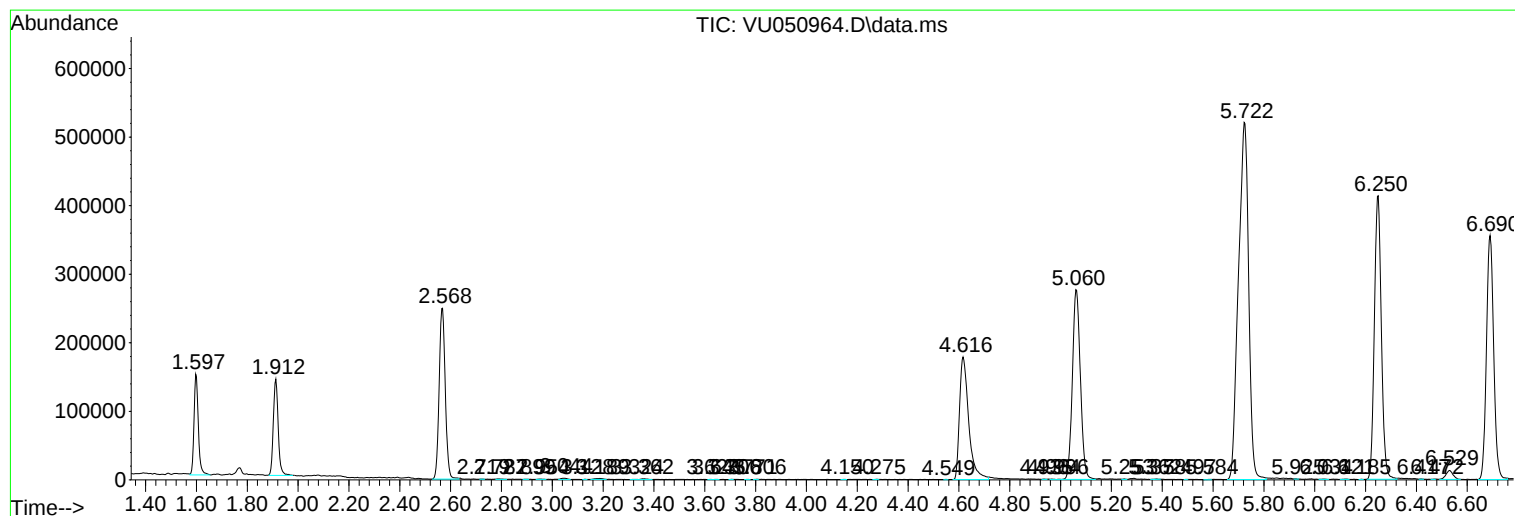

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050964.D
Acq On : 27 Sep 2022 18:06
Operator : JC/MD
Sample : N4854-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050964.D
Acq On : 27 Sep 2022 18:06
Operator : JC/MD
Sample : N4854-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------