

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050966.D
 Acq On : 27 Sep 2022 18:53
 Operator : JC/MD
 Sample : N4854-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	97	rVB	148291	169625	11.66%	1.427%
2	1.912	170	178	195	rVB	140132	182469	12.54%	1.535%
3	2.504	360	362	365	rBV2	421	266	0.02%	0.002%
4	2.568	369	382	395	rBV	247780	407672	28.02%	3.429%
5	2.706	422	425	430	rBV3	435	408	0.03%	0.003%
6	2.761	439	442	445	rBV	491	392	0.03%	0.003%
7	2.874	475	477	481	rVB2	461	319	0.02%	0.003%
8	2.899	481	485	487	rBV	363	291	0.02%	0.002%
9	2.951	494	501	503	rBV3	624	625	0.04%	0.005%
10	3.041	522	529	531	rBV4	1401	1367	0.09%	0.011%
11	3.092	542	545	548	rBV2	394	293	0.02%	0.002%
12	3.189	562	575	584	rVV4	2354	5227	0.36%	0.044%
13	3.266	593	599	601	rBV3	287	326	0.02%	0.003%
14	3.378	632	634	640	rVB2	656	533	0.04%	0.004%
15	3.478	661	665	668	rBV	364	341	0.02%	0.003%
16	3.613	703	707	714	rVB2	378	404	0.03%	0.003%
17	3.658	718	721	726	rVB2	376	312	0.02%	0.003%
18	4.218	887	895	899	rBV	282	348	0.02%	0.003%
19	4.269	906	911	913	rBV2	340	296	0.02%	0.002%
20	4.327	926	929	935	rVV2	322	313	0.02%	0.003%
21	4.382	939	946	951	rBV2	230	290	0.02%	0.002%
22	4.616	1007	1019	1050	rBV	183348	456728	31.39%	3.841%
23	4.845	1087	1090	1093	rBV2	407	311	0.02%	0.003%
24	5.063	1140	1158	1181	rBV	276640	611369	42.02%	5.142%
25	5.240	1210	1213	1217	rVV3	424	300	0.02%	0.003%
26	5.263	1217	1220	1223	rVV3	608	543	0.04%	0.005%
27	5.288	1225	1228	1241	rVB4	1549	2285	0.16%	0.019%
28	5.349	1243	1247	1250	rVB2	393	297	0.02%	0.002%
29	5.372	1250	1254	1255	rBV2	679	381	0.03%	0.003%
30	5.382	1255	1257	1263	rVB2	908	721	0.05%	0.006%
31	5.465	1276	1283	1286	rVB2	343	286	0.02%	0.002%
32	5.520	1294	1300	1302	rBV2	340	316	0.02%	0.003%
33	5.726	1341	1364	1392	rBV2	520070	1454959	100.00%	12.237%
34	6.086	1474	1476	1480	rVB2	353	259	0.02%	0.002%
35	6.134	1483	1491	1496	rVB4	560	844	0.06%	0.007%
36	6.160	1496	1499	1504	rBV2	360	267	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050966.D
 Acq On : 27 Sep 2022 18:53
 Operator : JC/MD
 Sample : N4854-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.246	1509	1526	1548	rBV	410497	785117	53.96%	6.603%
38	6.455	1586	1591	1593	rBV2	363	310	0.02%	0.003%
39	6.533	1603	1615	1630	rVB6	11393	23458	1.61%	0.197%
40	6.690	1649	1664	1684	rBV	361117	706709	48.57%	5.944%
41	7.189	1807	1819	1825	rBV6	1991	3346	0.23%	0.028%
42	7.262	1837	1842	1844	rBV	359	398	0.03%	0.003%
43	7.565	1923	1936	1950	rBV	168217	297683	20.46%	2.504%
44	7.690	1969	1975	1984	rVB6	1472	2432	0.17%	0.020%
45	7.896	2026	2039	2055	rBV	587446	1008691	69.33%	8.484%
46	8.179	2115	2127	2145	rBV	123255	209705	14.41%	1.764%
47	8.478	2211	2220	2224	rBV3	1342	1828	0.13%	0.015%
48	8.552	2230	2243	2256	rBV	458924	769175	52.87%	6.469%
49	8.632	2257	2268	2308	rVB3	458605	978360	67.24%	8.229%
50	8.864	2337	2340	2341	rBV3	632	313	0.02%	0.003%
51	8.947	2363	2366	2371	rVB2	380	341	0.02%	0.003%
52	9.121	2415	2420	2421	rBV2	373	277	0.02%	0.002%
53	9.243	2454	2458	2463	rVB	307	274	0.02%	0.002%
54	9.352	2489	2492	2495	rVB2	451	308	0.02%	0.003%
55	9.417	2499	2512	2535	rBV	622114	1045477	71.86%	8.793%
56	9.558	2553	2556	2558	rBV4	637	432	0.03%	0.004%
57	9.597	2566	2568	2571	rBV3	413	264	0.02%	0.002%
58	9.613	2571	2573	2575	rVV	450	290	0.02%	0.002%
59	9.690	2591	2597	2600	rBV2	903	885	0.06%	0.007%
60	9.748	2611	2615	2623	rVB	379	364	0.03%	0.003%
61	10.092	2720	2722	2725	rVV	356	255	0.02%	0.002%
62	10.143	2735	2738	2742	rVB2	418	339	0.02%	0.003%
63	10.172	2742	2747	2751	rBV2	325	344	0.02%	0.003%
64	10.423	2819	2825	2827	rBV	358	335	0.02%	0.003%
65	10.481	2841	2843	2847	rVB	420	292	0.02%	0.002%
66	10.671	2894	2902	2908	rBV4	1094	1222	0.08%	0.010%
67	10.754	2912	2928	2947	rBV	581105	921676	63.35%	7.752%
68	10.886	2965	2969	2979	rVB3	1475	1904	0.13%	0.016%
69	11.127	3041	3044	3049	rVB2	325	271	0.02%	0.002%
70	11.211	3067	3070	3074	rVB3	375	285	0.02%	0.002%
71	11.362	3111	3117	3123	rBV2	255	383	0.03%	0.003%
72	11.455	3140	3146	3148	rBV2	967	684	0.05%	0.006%
73	11.600	3182	3191	3194	rBV3	587	862	0.06%	0.007%
74	11.703	3217	3223	3232	rBV3	610	963	0.07%	0.008%
75	11.754	3232	3239	3241	rBV5	610	751	0.05%	0.006%
76	11.809	3243	3256	3275	rBV	517375	842587	57.91%	7.087%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050966.D
 Acq On : 27 Sep 2022 18:53
 Operator : JC/MD
 Sample : N4854-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.060	3330	3334	3338	rBV2	336	348	0.02%	0.003%
78	12.192	3360	3375	3399	rBV	598796	966537	66.43%	8.129%
79	12.359	3425	3427	3432	rVB3	497	320	0.02%	0.003%
80	12.417	3441	3445	3447	rBV	517	380	0.03%	0.003%
81	12.574	3491	3494	3497	rBV	511	413	0.03%	0.003%
82	12.632	3509	3512	3519	rVB4	516	594	0.04%	0.005%
83	12.841	3574	3577	3581	rBV2	483	354	0.02%	0.003%
84	12.918	3598	3601	3607	rBV2	752	824	0.06%	0.007%
85	13.053	3637	3643	3647	rBV3	603	677	0.05%	0.006%
86	13.111	3659	3661	3665	rVB2	507	304	0.02%	0.003%
87	13.378	3741	3744	3747	rBV2	468	347	0.02%	0.003%
88	13.420	3754	3757	3762	rVB2	391	367	0.03%	0.003%
89	13.561	3799	3801	3806	rBV2	419	351	0.02%	0.003%
90	13.613	3814	3817	3824	rBV	493	593	0.04%	0.005%
91	13.860	3889	3894	3897	rBV4	710	661	0.05%	0.006%
92	13.928	3911	3915	3920	rBV2	559	540	0.04%	0.005%
93	14.420	4065	4068	4073	rVB2	594	456	0.03%	0.004%
94	15.140	4290	4292	4297	rBV4	604	641	0.04%	0.005%
95	15.188	4304	4307	4309	rBV	570	383	0.03%	0.003%
96	15.439	4381	4385	4388	rBV2	1224	1066	0.07%	0.009%
97	15.564	4421	4424	4429	rBV4	790	726	0.05%	0.006%
98	15.757	4481	4484	4485	rBV	803	458	0.03%	0.004%
99	15.780	4489	4491	4493	rBV2	769	437	0.03%	0.004%
100	15.873	4517	4520	4521	rBV3	857	527	0.04%	0.004%




Sum of corrected areas: 11889877

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050966.D
Acq On : 27 Sep 2022 18:53
Operator : JC/MD
Sample : N4854-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

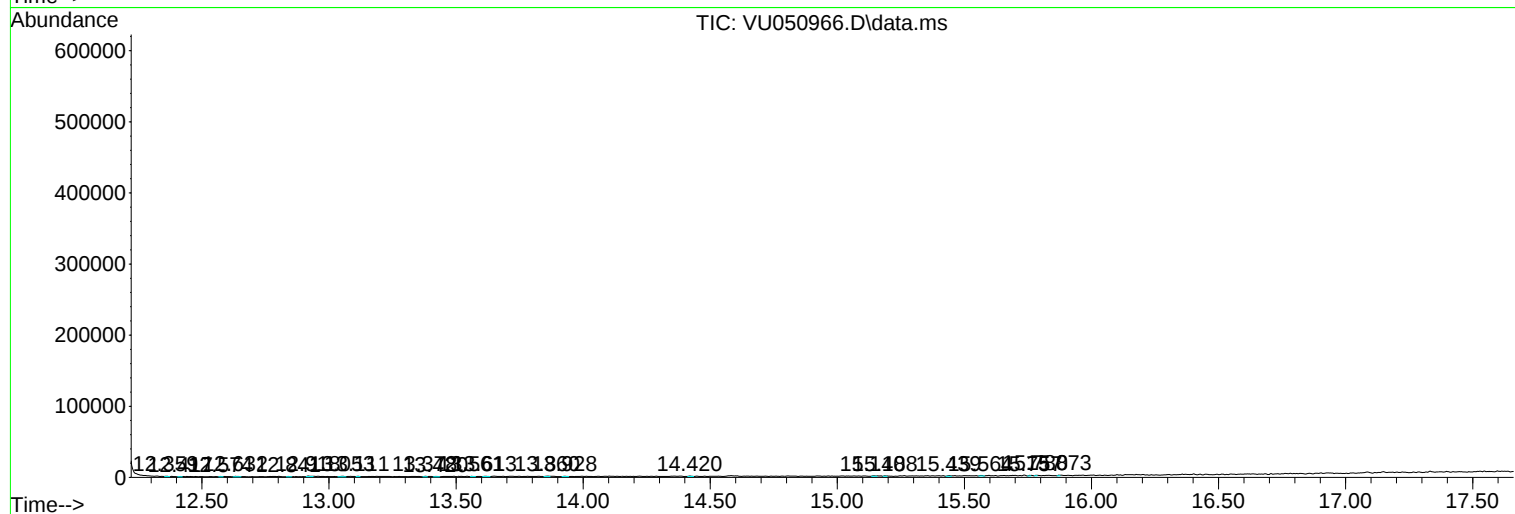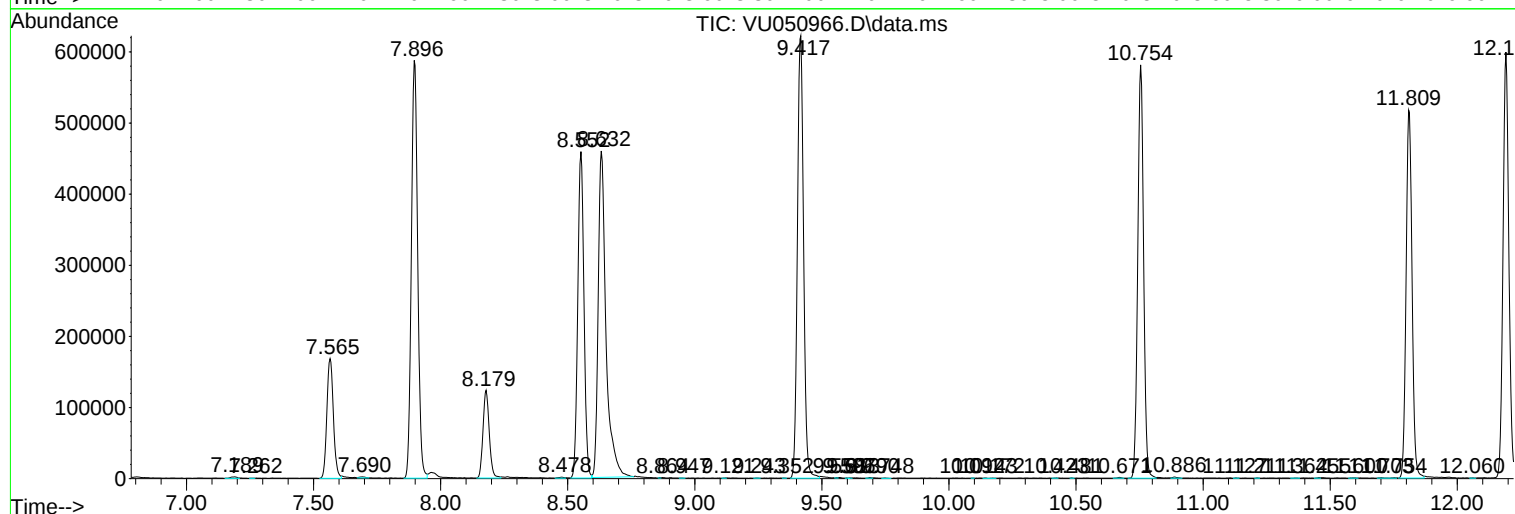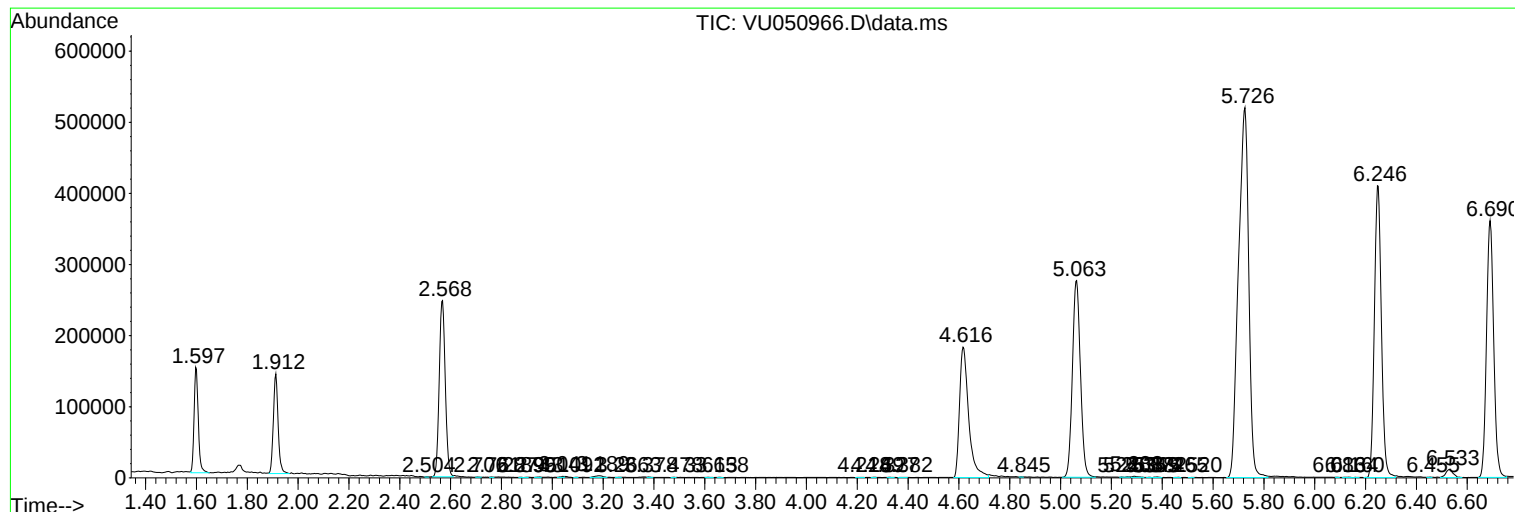

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050966.D
Acq On : 27 Sep 2022 18:53
Operator : JC/MD
Sample : N4854-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050966.D
Acq On : 27 Sep 2022 18:53
Operator : JC/MD
Sample : N4854-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc