

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050967.D
 Acq On : 27 Sep 2022 19:16
 Operator : JC/MD
 Sample : VIBLK139
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK139

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	160614	188953	12.04%	1.600%
2	1.912	170	178	192	rVB	150051	195168	12.44%	1.652%
3	2.568	368	382	400	rBV	274769	449970	28.68%	3.810%
4	2.739	433	435	440	rBV2	462	327	0.02%	0.003%
5	2.954	498	502	505	rBV2	321	322	0.02%	0.003%
6	3.044	519	530	546	rVB2	18247	34022	2.17%	0.288%
7	3.186	561	574	590	rVB3	9680	22299	1.42%	0.189%
8	3.401	636	641	649	rVB2	304	448	0.03%	0.004%
9	3.446	653	655	662	rVB2	417	325	0.02%	0.003%
10	3.491	662	669	674	rBV3	292	399	0.03%	0.003%
11	3.616	703	708	710	rBV2	369	317	0.02%	0.003%
12	3.636	710	714	718	rVB2	562	441	0.03%	0.004%
13	3.674	718	726	729	rBV	387	408	0.03%	0.003%
14	3.694	729	732	738	rBV2	320	321	0.02%	0.003%
15	3.864	782	785	788	rVB2	488	341	0.02%	0.003%
16	4.095	854	857	859	rBV	394	280	0.02%	0.002%
17	4.121	862	865	869	rVB3	382	307	0.02%	0.003%
18	4.218	891	895	899	rBV2	250	278	0.02%	0.002%
19	4.523	987	990	997	rVB2	444	442	0.03%	0.004%
20	4.616	1006	1019	1054	rBV	198658	501921	31.99%	4.250%
21	4.861	1093	1095	1099	rVB3	692	394	0.03%	0.003%
22	4.993	1134	1136	1141	rVB3	574	370	0.02%	0.003%
23	5.063	1141	1158	1184	rBV	293656	649237	41.38%	5.497%
24	5.176	1190	1193	1198	rBV4	467	568	0.04%	0.005%
25	5.282	1220	1226	1227	rBV2	813	773	0.05%	0.007%
26	5.317	1235	1237	1239	rVB2	679	284	0.02%	0.002%
27	5.330	1239	1241	1246	rVB2	603	381	0.02%	0.003%
28	5.372	1251	1254	1261	rVB3	758	737	0.05%	0.006%
29	5.501	1292	1294	1298	rVB2	543	361	0.02%	0.003%
30	5.726	1342	1364	1393	rBV2	564737	1568968	100.00%	13.284%
31	5.999	1447	1449	1454	rVB3	511	325	0.02%	0.003%
32	6.070	1468	1471	1475	rVB2	435	318	0.02%	0.003%
33	6.092	1475	1478	1481	rBV	326	280	0.02%	0.002%
34	6.121	1481	1487	1490	rVV3	600	497	0.03%	0.004%
35	6.247	1512	1526	1553	rBV	406030	783455	49.93%	6.633%
36	6.484	1597	1600	1602	rVB2	709	412	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050967.D
 Acq On : 27 Sep 2022 19:16
 Operator : JC/MD
 Sample : VIBLK139
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK139

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.526	1602	1613	1630	rVB4	10962	20893	1.33%	0.177%
38	6.690	1649	1664	1685	rBV	393912	756010	48.19%	6.401%
39	6.925	1734	1737	1744	rVB3	299	285	0.02%	0.002%
40	7.028	1765	1769	1771	rBV2	451	326	0.02%	0.003%
41	7.185	1807	1818	1830	rBV5	2474	3827	0.24%	0.032%
42	7.234	1830	1833	1838	rVB2	428	316	0.02%	0.003%
43	7.472	1903	1907	1912	rBV2	300	298	0.02%	0.003%
44	7.565	1920	1936	1955	rBV	180631	320854	20.45%	2.717%
45	7.674	1967	1970	1971	rBV2	676	440	0.03%	0.004%
46	7.690	1971	1975	1978	rVV2	714	845	0.05%	0.007%
47	7.751	1990	1994	1998	rBV4	635	683	0.04%	0.006%
48	7.896	2025	2039	2055	rBV	639579	1094774	69.78%	9.269%
49	8.070	2091	2093	2099	rVB4	473	396	0.03%	0.003%
50	8.179	2113	2127	2149	rBV	135474	234997	14.98%	1.990%
51	8.282	2157	2159	2162	rBV3	463	359	0.02%	0.003%
52	8.465	2213	2216	2220	rBV4	552	558	0.04%	0.005%
53	8.552	2233	2243	2255	rVB2	17971	28964	1.85%	0.245%
54	8.632	2255	2268	2296	rBV3	486767	1029302	65.60%	8.715%
55	8.825	2325	2328	2332	rVB3	665	602	0.04%	0.005%
56	8.947	2364	2366	2371	rVB4	626	482	0.03%	0.004%
57	9.041	2391	2395	2399	rVB3	422	341	0.02%	0.003%
58	9.417	2497	2512	2543	rBV	623104	1040741	66.33%	8.812%
59	9.568	2553	2559	2567	rVB5	939	1625	0.10%	0.014%
60	9.632	2572	2579	2585	rBV3	436	637	0.04%	0.005%
61	9.693	2589	2598	2606	rBV4	921	1361	0.09%	0.012%
62	9.806	2625	2633	2639	rBV3	556	829	0.05%	0.007%
63	9.947	2673	2677	2681	rBV	345	303	0.02%	0.003%
64	10.301	2779	2787	2790	rBV	461	605	0.04%	0.005%
65	10.324	2790	2794	2801	rVV	358	398	0.03%	0.003%
66	10.671	2894	2902	2909	rBV4	1270	1445	0.09%	0.012%
67	10.754	2914	2928	2948	rVV	602218	969020	61.76%	8.205%
68	10.825	2948	2950	2957	rVB3	744	665	0.04%	0.006%
69	10.870	2961	2964	2965	rBV	442	268	0.02%	0.002%
70	11.063	3021	3024	3029	rBV2	438	376	0.02%	0.003%
71	11.092	3029	3033	3035	rBV2	345	289	0.02%	0.002%
72	11.185	3057	3062	3064	rBV	351	318	0.02%	0.003%
73	11.439	3138	3141	3143	rBV2	417	296	0.02%	0.003%
74	11.462	3143	3148	3153	rVB5	820	886	0.06%	0.008%
75	11.809	3242	3256	3278	rBV	529740	838552	53.45%	7.100%
76	12.192	3361	3375	3405	rBV	636391	1040063	66.29%	8.806%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050967.D
 Acq On : 27 Sep 2022 19:16
 Operator : JC/MD
 Sample : VIBLK139
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK139

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.378	3429	3433	3437	rBV3	519	518	0.03%	0.004%
78	12.410	3440	3443	3447	rVV3	470	275	0.02%	0.002%
79	12.581	3490	3496	3500	rBV2	444	630	0.04%	0.005%
80	12.674	3523	3525	3528	rVB3	509	284	0.02%	0.002%
81	12.764	3550	3553	3555	rBV2	506	310	0.02%	0.003%
82	12.835	3572	3575	3580	rVV2	519	444	0.03%	0.004%
83	12.880	3587	3589	3595	rVB4	438	360	0.02%	0.003%
84	12.909	3595	3598	3601	rBV2	610	466	0.03%	0.004%
85	13.057	3641	3644	3646	rBV	413	293	0.02%	0.002%
86	13.085	3650	3653	3654	rBV2	520	296	0.02%	0.003%
87	13.124	3661	3665	3667	rBV2	484	323	0.02%	0.003%
88	13.159	3673	3676	3677	rBV	444	308	0.02%	0.003%
89	13.503	3780	3783	3788	rBV2	618	619	0.04%	0.005%
90	13.577	3804	3806	3810	rVB2	553	301	0.02%	0.003%
91	13.645	3824	3827	3829	rBV2	439	272	0.02%	0.002%
92	13.774	3862	3867	3871	rBV	620	725	0.05%	0.006%
93	13.867	3890	3896	3900	rBV3	701	870	0.06%	0.007%
94	13.921	3911	3913	3917	rVB	481	273	0.02%	0.002%
95	14.230	4005	4009	4010	rBV	394	308	0.02%	0.003%
96	14.365	4048	4051	4053	rBV2	519	301	0.02%	0.003%
97	14.577	4113	4117	4127	rVB3	1641	2172	0.14%	0.018%
98	15.359	4358	4360	4363	rBV3	546	273	0.02%	0.002%
99	15.391	4367	4370	4373	rBV2	704	458	0.03%	0.004%
100	15.706	4466	4468	4473	rBV5	1000	715	0.05%	0.006%




Sum of corrected areas: 11810672

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050967.D
Acq On : 27 Sep 2022 19:16
Operator : JC/MD
Sample : VIBLK139
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK139

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

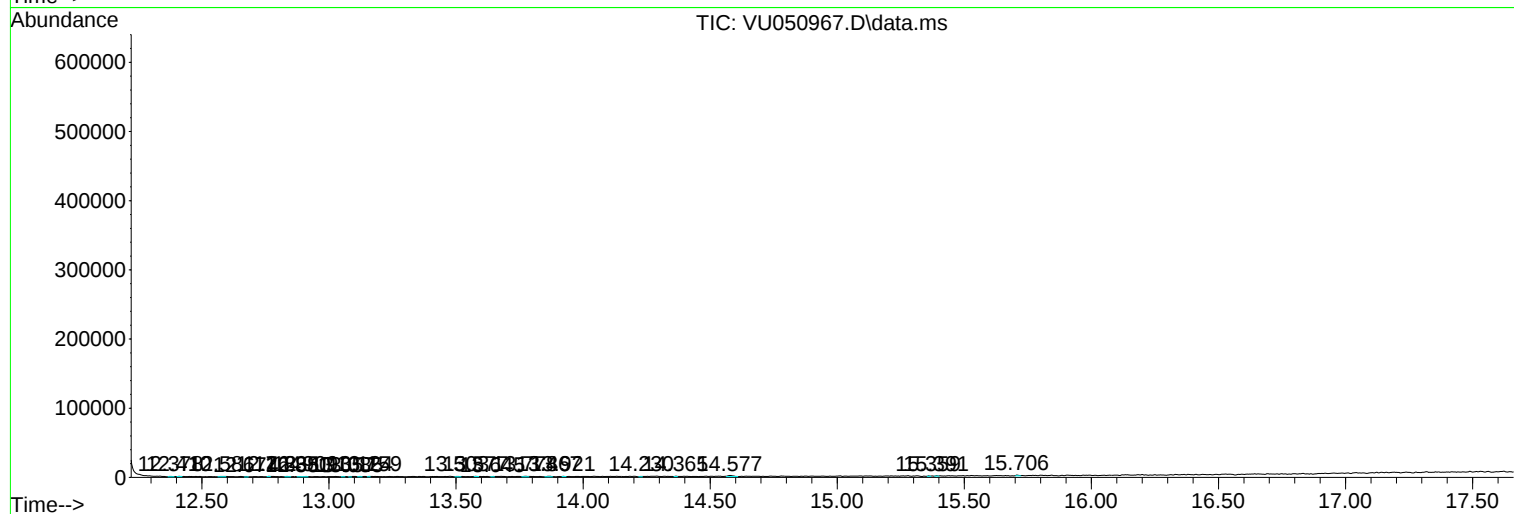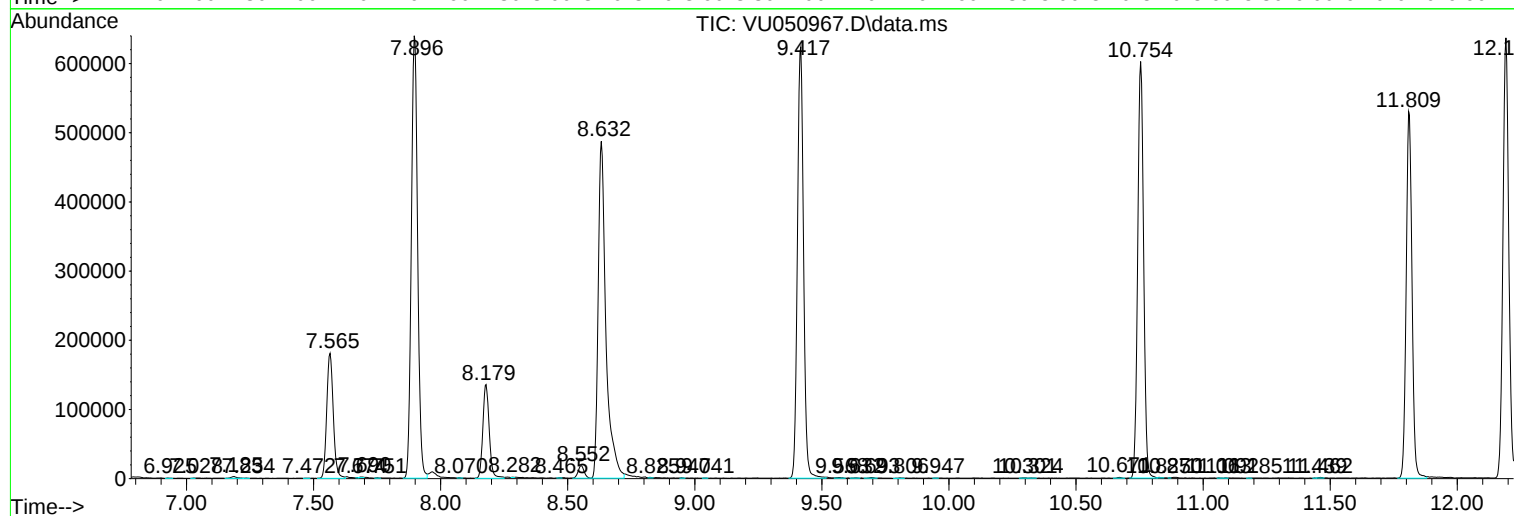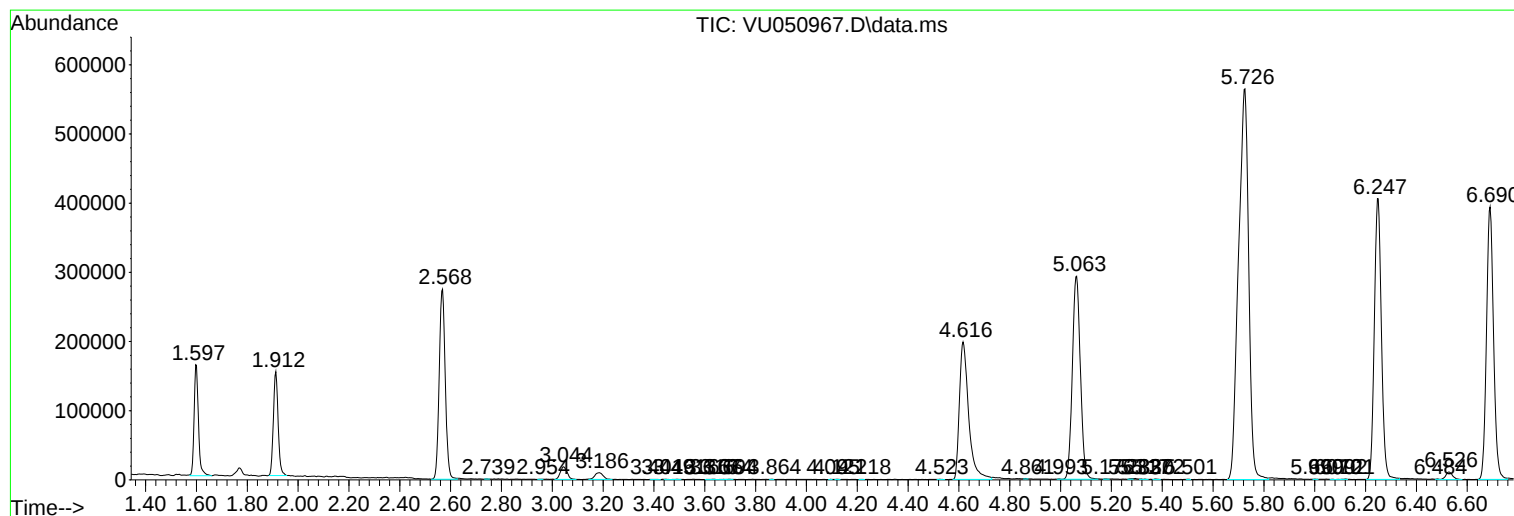

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050967.D
Acq On : 27 Sep 2022 19:16
Operator : JC/MD
Sample : VIBLK139
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK139

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
Data File : VU050967.D
Acq On : 27 Sep 2022 19:16
Operator : JC/MD
Sample : VIBLK139
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK139

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------