
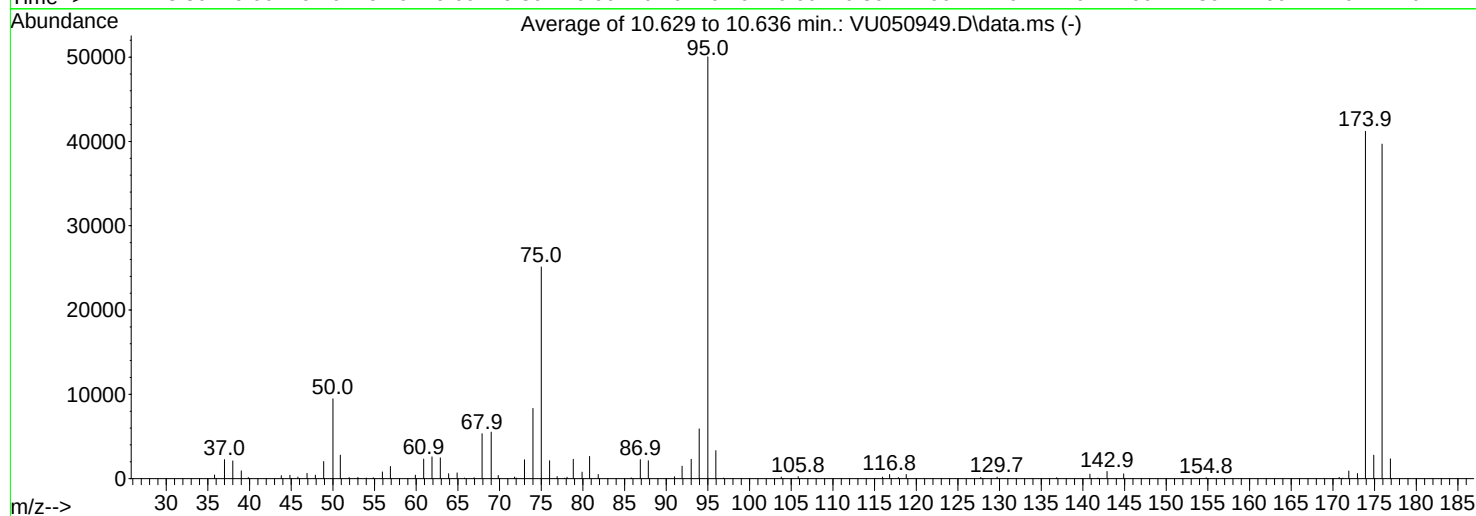


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092722\
 Data File : VU050949.D
 Acq On : 27 Sep 2022 10:24
 Operator : JC/MD
 Sample : BFB132
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB132

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 28 01:59:42 2022

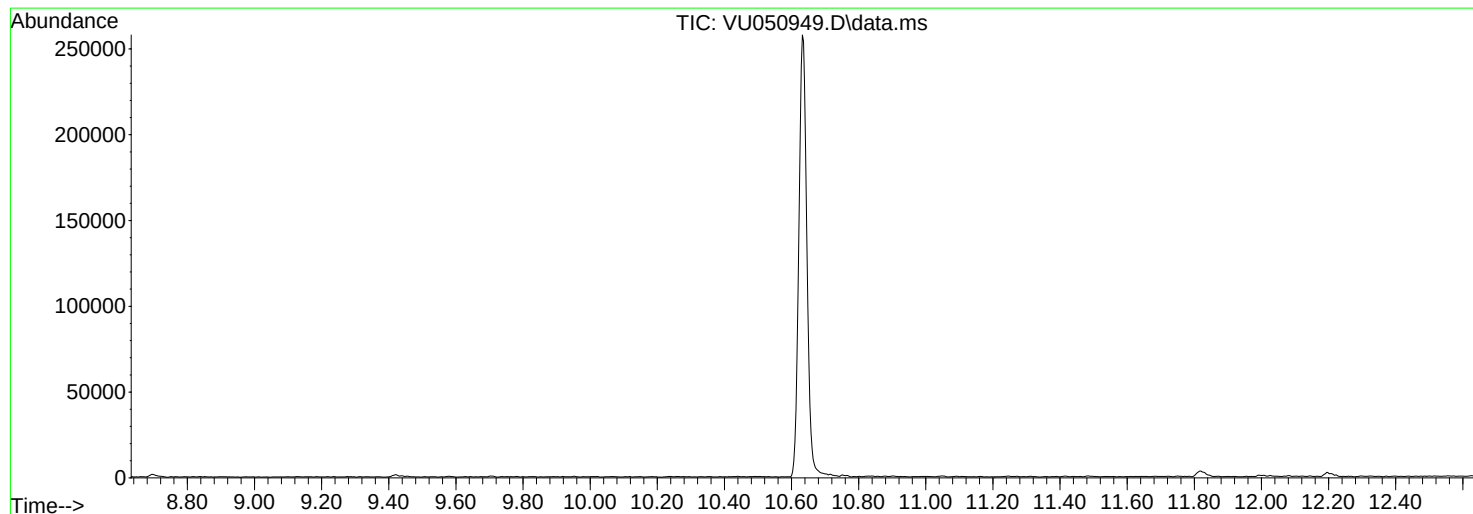

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	9476	PASS
75	95	30	80	50.2	25115	PASS
95	95	100	100	100.0	50037	PASS
96	95	5	9	6.7	3330	PASS
173	174	0.00	2	1.5	601	PASS
174	95	50	120	82.4	41216	PASS
175	174	5	9	6.8	2783	PASS
176	174	95	101	96.3	39696	PASS
177	176	5	9	5.9	2359	PASS

Scan 2878 (10.594 min): VU050949.D\data.ms
BFB132

m/z	Abundance
39.80	194.0
43.80	423.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132

m/z	Abundance
35.80	388.0
37.00	2339.0
38.00	2133.0
39.00	891.0
39.90	258.0
43.80	765.0
44.90	336.0
45.80	234.0
46.90	647.0
47.90	440.0
48.90	2035.0
50.00	9198.0
50.90	2604.0
52.00	138.0
53.00	149.0
54.00	129.0
54.90	108.0
55.90	920.0
56.90	1394.0
59.90	401.0
60.90	2208.0
61.90	2508.0
62.90	2340.0
63.90	624.0
64.90	620.0
67.00	108.0
67.90	5196.0
69.00	5413.0
69.80	351.0
71.80	308.0
73.00	2222.0
74.00	7939.0
75.00	24688.0
76.00	2309.0
76.90	236.0
78.10	254.0
78.90	2162.0
79.90	715.0
80.80	2590.0
81.90	511.0
85.80	149.0
86.90	2132.0
87.90	2088.0
91.00	223.0
91.90	1478.0
93.00	2179.0
94.00	6055.0
95.00	47768.0
95.90	3235.0
103.80	165.0
105.80	202.0
116.00	195.0
116.80	469.0
117.80	131.0
118.80	407.0
127.80	152.0
129.70	153.0
136.90	117.0
140.90	413.0
142.90	846.0
144.90	596.0
156.80	100.0
170.70	144.0
171.20	159.0
171.90	795.0
172.90	597.0
173.90	38672.0
174.90	2583.0
175.90	36592.0
176.90	2250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132

m/z	Abundance
35.80	474.0
37.00	2321.0
38.00	2180.0
39.00	938.0
39.90	343.0
43.90	793.0
44.90	420.0
45.80	216.0
46.90	610.0
47.90	436.0
48.90	2092.0
50.00	9782.0
50.90	2801.0
51.90	143.0
53.00	155.0
54.00	101.0
54.90	131.0
56.00	827.0
56.90	1519.0
59.90	439.0
60.90	2350.0
61.90	2677.0
62.90	2489.0
63.90	580.0
64.90	703.0
65.80	113.0
67.00	130.0
67.90	5551.0
69.00	5807.0
69.90	372.0
71.80	280.0
73.00	2263.0
74.00	8471.0
75.00	25760.0
76.00	2163.0
76.90	250.0
78.10	259.0
78.90	2317.0
79.90	832.0
80.80	2720.0
81.90	509.0
85.80	130.0
86.90	2310.0
87.90	2232.0
91.00	241.0
91.90	1523.0
93.00	2346.0
93.90	6045.0
95.00	51664.0
96.00	3416.0
96.90	101.0
103.80	202.0
105.80	262.0
115.90	185.0
116.80	502.0
117.80	143.0
118.80	503.0
127.70	142.0
129.70	205.0
136.80	109.0
140.80	578.0
141.80	111.0
142.90	848.0
144.90	589.0
154.80	144.0
170.80	147.0
171.90	927.0
172.90	603.0
173.90	42392.0
174.90	2867.0
175.90	40880.0
176.90	2432.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132

m/z	Abundance
35.80	457.0
37.00	2142.0
38.00	2024.0
39.00	958.0
39.90	368.0
43.90	805.0
44.80	465.0
45.80	111.0
46.90	606.0
47.90	379.0
48.90	1948.0
50.00	9448.0
50.90	2961.0
51.90	118.0
53.00	171.0
54.80	130.0
56.00	656.0
56.90	1388.0
59.90	434.0
60.90	2401.0
61.90	2566.0
62.90	2583.0
63.90	563.0
64.90	714.0
65.80	107.0
66.90	130.0
67.90	5241.0
69.00	5367.0
69.90	411.0
72.00	236.0
73.00	2249.0
74.00	8620.0
75.00	24896.0
76.00	1912.0
76.90	230.0
77.80	196.0
78.80	2437.0
79.90	798.0
80.80	2599.0
81.80	478.0
86.90	2322.0
87.80	2070.0
91.00	210.0
91.90	1446.0
93.00	2359.0
93.90	5624.0
95.00	50680.0
96.00	3338.0
96.90	128.0
103.80	204.0
105.90	273.0
115.90	185.0
116.80	522.0
117.90	156.0
118.80	550.0
127.70	156.0
129.70	213.0
136.80	112.0
140.80	598.0
141.80	106.0
142.90	871.0
144.90	538.0
154.80	210.0
170.80	162.0
171.90	1014.0
173.00	602.0
173.90	42584.0
174.90	2899.0
175.90	41616.0
176.90	2394.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132