




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051044.D
 Acq On : 30 Sep 2022 19:17
 Operator : JC/MD
 Sample : N4859-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10048

Manual IntegrationsAPPROVED

Quant Time: Oct 01 01:28:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 01 01:23:58 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/03/2022
 Supervised By :Mahesh Dadoda 10/05/2022

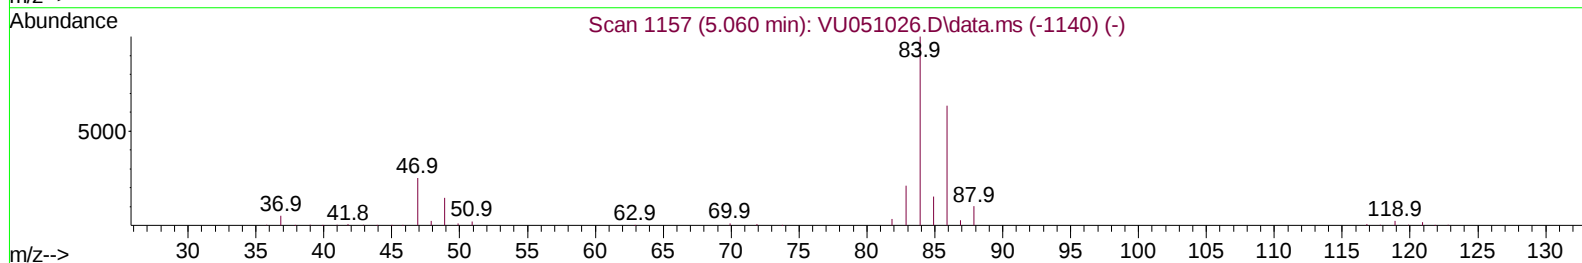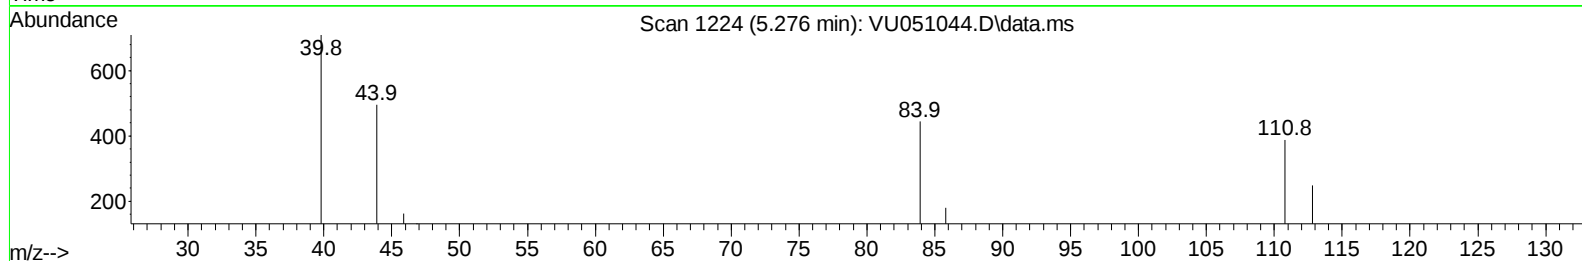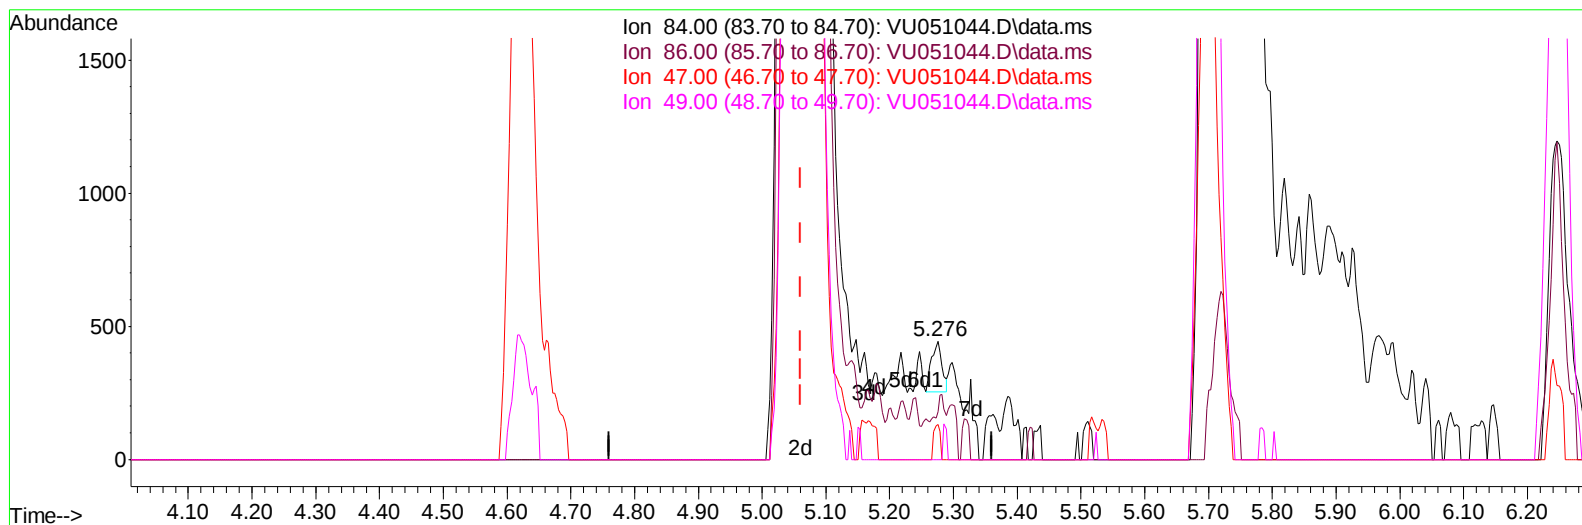

TIC: VU051044.D\data.ms

(24) Chloroform-d (S)

5.276min (+ 0.215) 0.03 ug/L

response 219

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.40	66.21
47.00	41.40	41.55
49.00	25.40	21.92




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051044.D
 Acq On : 30 Sep 2022 19:17
 Operator : JC/MD
 Sample : N4859-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10048

Manual IntegrationsAPPROVED

Quant Time: Oct 01 01:28:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 01 01:23:58 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/03/2022
 Supervised By :Mahesh Dadoda 10/05/2022

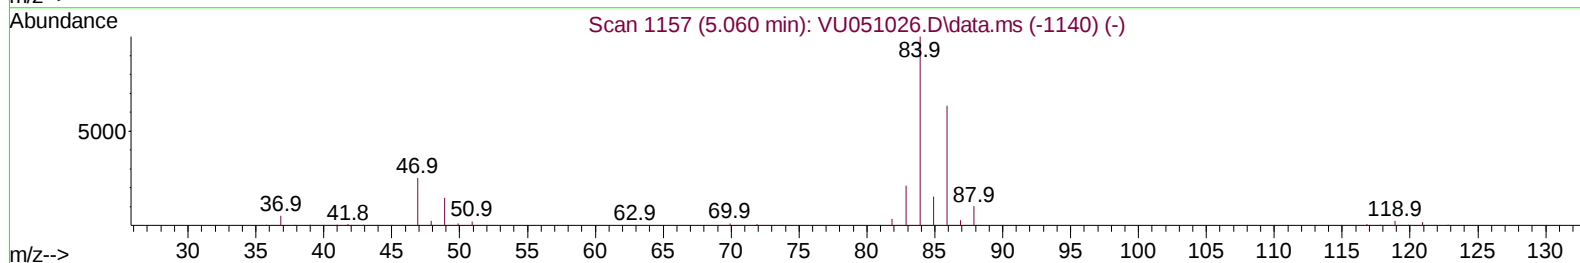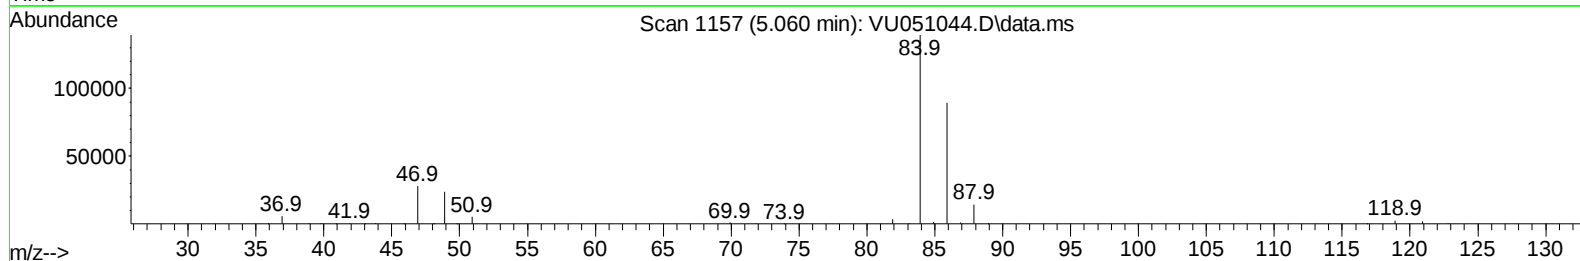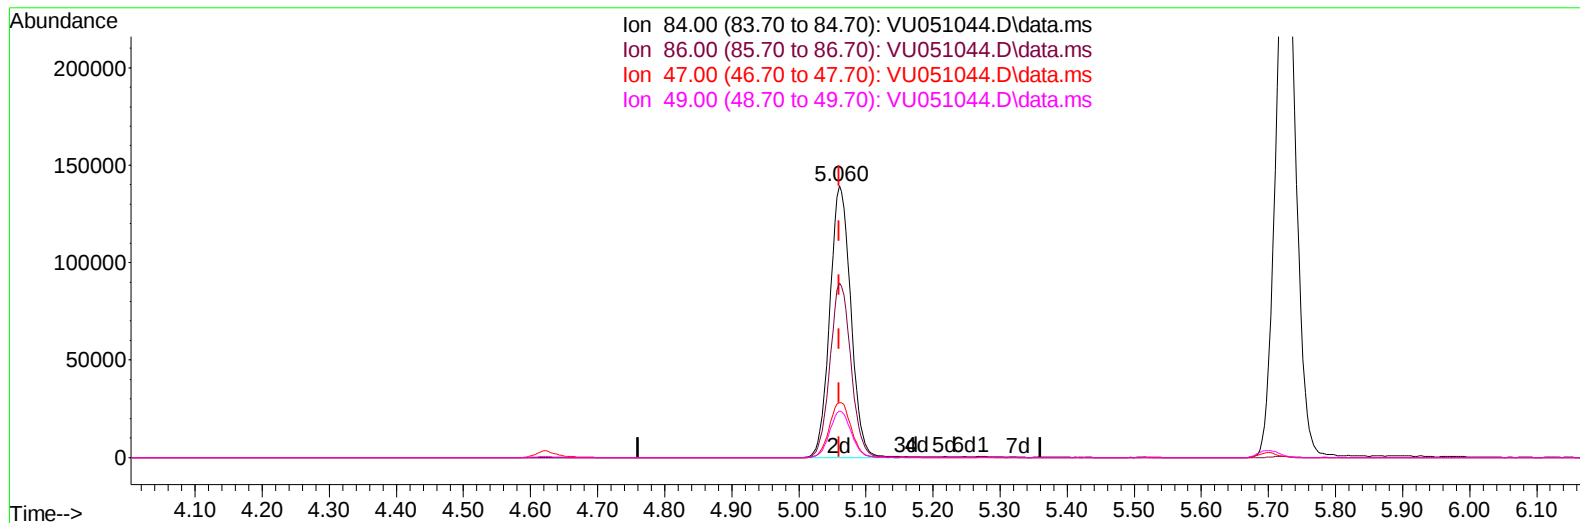

TIC: VU051044.D\data.ms

(24) Chloroform-d (S)

5.060min (+ 0.000) 44.59 ug/L m

response 302592

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.40	0.05#
47.00	41.40	0.03#
49.00	25.40	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051044.D
 Acq On : 30 Sep 2022 19:17
 Operator : JC/MD
 Sample : N4859-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10048

Manual IntegrationsAPPROVED

Quant Time: Oct 01 01:28:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 01 01:23:58 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/03/2022
 Supervised By :Mahesh Dadoda 10/05/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.247	114		415633	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117		404216	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152		149700	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.597	65		148301	35.207	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	70.420%	
7) Chloroethane-d5	1.903	69		140009	35.782	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	71.560%	
11) 1,1-Dichloroethene-d2	2.565	63		194108	31.196	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	62.400%	
21) 2-Butanone-d5	4.620	46		289679	106.032	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	106.030%	
24) Chloroform-d	5.060	84		302592m	44.588	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	89.180%	
26) 1,2-Dichloroethane-d4	5.700	65		198210	47.187	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	94.380%	
32) Benzene-d6	5.726	84		598312	50.546	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	101.100%	
36) 1,2-Dichloropropane-d6	6.687	67		206845	53.852	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	107.700%	
41) Toluene-d8	7.896	98		489204	44.732	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	89.460%	
43) trans-1,3-Dichloroprop...	8.179	79		85604	46.726	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	93.460%	
47) 2-Hexanone-d5	8.632	63		149474	96.377	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	96.380%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84		305717	45.542	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	91.080%	
66) 1,2-Dichlorobenzene-d4	12.192	152		162990	50.966	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	101.940%	
Target Compounds							
13) Acetone	2.630	43		5072	2.325	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051044.D
Acq On : 30 Sep 2022 19:17
Operator : JC/MD
Sample : N4859-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10048

Manual IntegrationsAPPROVED

Quant Time: Oct 01 01:28:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 01 01:23:58 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/03/2022
Supervised By :Mahesh Dadoda 10/05/2022

