

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU093022\  
 Data File : VU051069.D  
 Acq On : 01 Oct 2022 05:22  
 Operator : JC/MD  
 Sample : N4880-15  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 47 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BGS4

Quant Time: Oct 03 00:02:36 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM092922WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Oct 01 03:04:59 2022  
 Response via : Initial Calibration


| Compound                      | R.T. QIon |                | Response | Conc        | Units | Dev(Min)  |
|-------------------------------|-----------|----------------|----------|-------------|-------|-----------|
| -----                         |           |                |          |             |       |           |
| Internal Standards            |           |                |          |             |       |           |
| 1) 1,4-Difluorobenzene        | 6.247     | 114            | 384676   | 50.000      | ug/L  | 0.00      |
| 28) Chlorobenzene-d5          | 9.414     | 117            | 386294   | 50.000      | ug/L  | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    | 11.809    | 152            | 142541   | 50.000      | ug/L  | 0.00      |
| System Monitoring Compounds   |           |                |          |             |       |           |
| 4) Vinyl Chloride-d3          | 1.597     | 65             | 208294   | 53.429      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 60 - 135 | Recovery | = 106.860%  |       |           |
| 7) Chloroethane-d5            | 1.900     | 69             | 177864   | 49.115      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 70 - 130 | Recovery | = 98.220%   |       |           |
| 11) 1,1-Dichloroethene-d2     | 2.562     | 63             | 245069   | 42.556      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 60 - 125 | Recovery | = 85.120%   |       |           |
| 21) 2-Butanone-d5             | 4.617     | 46             | 296408   | 117.227     | ug/L  | -0.01     |
| Spiked Amount                 | 100.000   | Range 40 - 130 | Recovery | = 117.230%  |       |           |
| 24) Chloroform-d              | 5.060     | 84             | 347942   | 55.397      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 70 - 125 | Recovery | = 110.800%  |       |           |
| 26) 1,2-Dichloroethane-d4     | 5.700     | 65             | 228608   | 58.803      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 70 - 125 | Recovery | = 117.600%  |       |           |
| 32) Benzene-d6                | 5.726     | 84             | 696330   | 61.556      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 70 - 125 | Recovery | = 123.120%  |       |           |
| 36) 1,2-Dichloropropane-d6    | 6.687     | 67             | 233781   | 63.689      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 70 - 120 | Recovery | = 127.380%# |       |           |
| 41) Toluene-d8                | 7.896     | 98             | 571356   | 54.667      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 80 - 120 | Recovery | = 109.340%  |       |           |
| 43) trans-1,3-Dichloroprop... | 8.176     | 79             | 92640    | 52.913      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 60 - 125 | Recovery | = 105.820%  |       |           |
| 47) 2-Hexanone-d5             | 8.629     | 63             | 161050   | 108.659     | ug/L  | 0.00      |
| Spiked Amount                 | 100.000   | Range 45 - 130 | Recovery | = 108.660%  |       |           |
| 56) 1,1,2,2-Tetrachloroeth... | 10.755    | 84             | 359229   | 55.996      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 65 - 120 | Recovery | = 112.000%  |       |           |
| 66) 1,2-Dichlorobenzene-d4    | 12.192    | 152            | 193172   | 63.438      | ug/L  | 0.00      |
| Spiked Amount                 | 50.000    | Range 80 - 120 | Recovery | = 126.880%# |       |           |
| Target Compounds              |           |                |          |             |       |           |
| 13) Acetone                   | 2.626     | 43             | 5635     | 2.791       | ug/L  | Qvalue 91 |
| -----                         |           |                |          |             |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU093022\  
Data File : VU051069.D  
Acq On : 01 Oct 2022 05:22  
Operator : JC/MD  
Sample : N4880-15  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 47 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BGS4

Quant Time: Oct 03 00:02:36 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM092922WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Oct 01 03:04:59 2022  
Response via : Initial Calibration

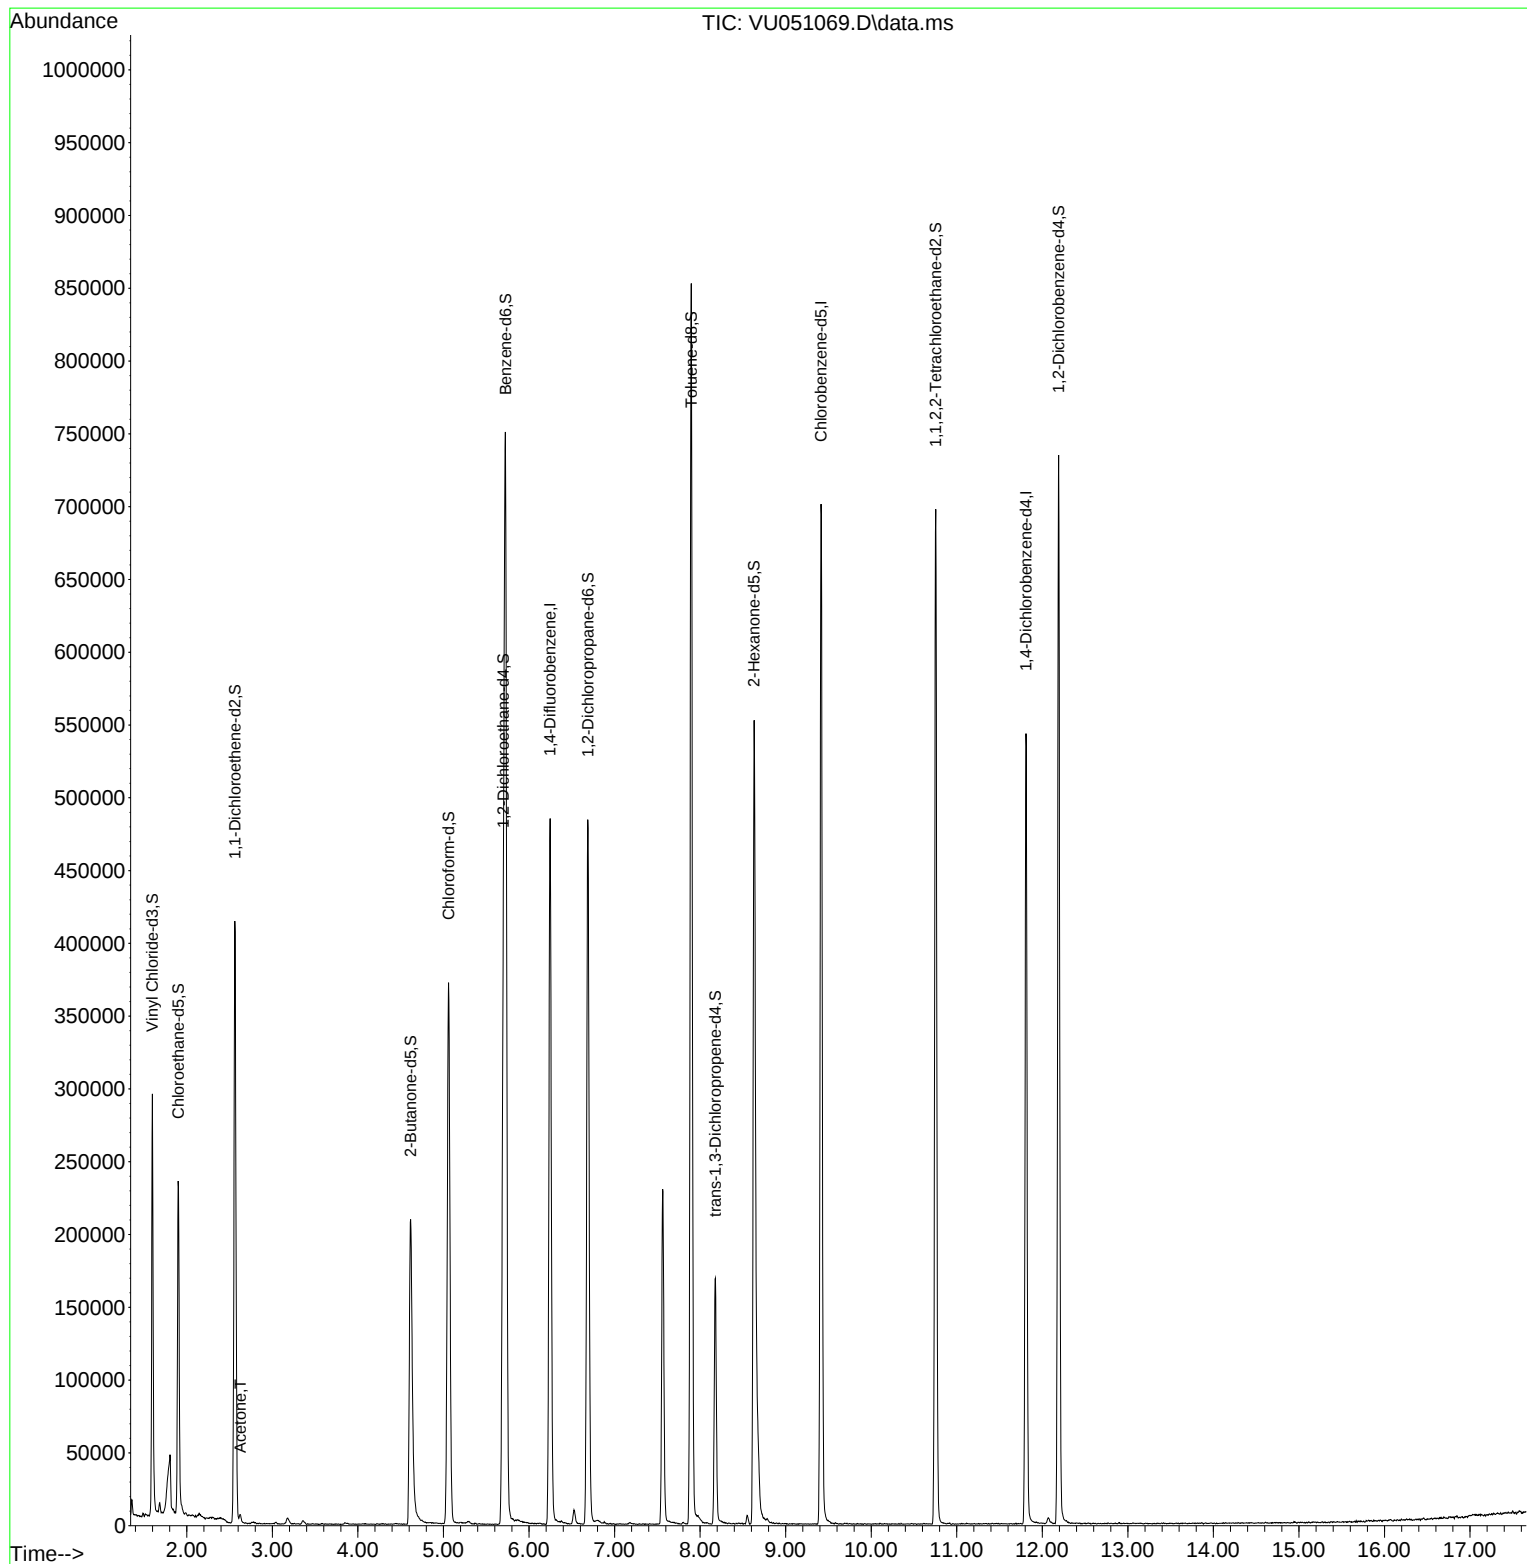

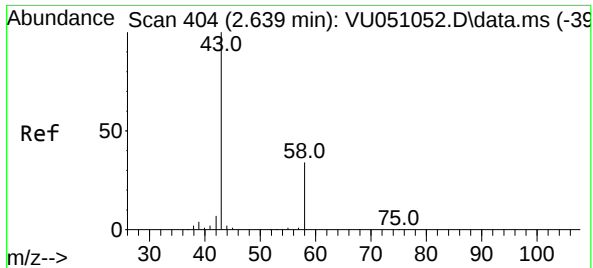

#13  
 Acetone  
 Concen: 2.791 ug/L  
 RT: 2.626 min Scan# 40  
 Delta R.T. -0.013 min  
 Lab File: VU051069.D  
 Acq: 01 Oct 2022 05:22

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BGS4

Tgt Ion: 43 Resp: 5635  
 Ion Ratio Lower Upper  
 43 100  
 58 31.2 0.0 73.6

