

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051029.D
 Acq On : 30 Sep 2022 13:28
 Operator : JC/MD
 Sample : N4854-07 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rVB	224832	276662	14.81%	2.024%
2	1.909	170	177	205	rVB	267157	390222	20.89%	2.854%
3	2.565	368	381	398	rBV	365278	594311	31.82%	4.347%
4	2.883	477	480	483	rBV2	328	253	0.01%	0.002%
5	3.041	521	529	538	rVB6	2597	4838	0.26%	0.035%
6	3.118	550	553	555	rBV	356	222	0.01%	0.002%
7	3.572	688	694	695	rBV	301	245	0.01%	0.002%
8	3.581	695	697	699	rVV2	302	141	0.01%	0.001%
9	3.607	703	705	709	rVB	283	199	0.01%	0.001%
10	3.707	732	736	740	rBV	191	164	0.01%	0.001%
11	3.809	763	768	771	rBV2	135	147	0.01%	0.001%
12	3.829	771	774	776	rBV2	196	108	0.01%	0.001%
13	3.874	786	788	789	rBV	204	83	0.00%	0.001%
14	3.928	802	805	806	rBV2	242	135	0.01%	0.001%
15	3.954	810	813	816	rBV2	315	221	0.01%	0.002%
16	4.031	832	837	838	rBV2	397	305	0.02%	0.002%
17	4.099	854	858	860	rBV2	235	173	0.01%	0.001%
18	4.179	879	883	886	rBV	247	184	0.01%	0.001%
19	4.211	891	893	896	rBV	204	104	0.01%	0.001%
20	4.231	896	899	901	rBV	193	112	0.01%	0.001%
21	4.289	913	917	919	rBV	263	194	0.01%	0.001%
22	4.317	924	926	931	rVB2	213	154	0.01%	0.001%
23	4.369	939	942	946	rVB	364	227	0.01%	0.002%
24	4.407	950	954	959	rBV	263	251	0.01%	0.002%
25	4.465	969	972	974	rBV2	225	147	0.01%	0.001%
26	4.523	985	990	994	rVB2	370	348	0.02%	0.003%
27	4.549	994	998	999	rBV2	215	161	0.01%	0.001%
28	4.581	1005	1008	1009	rBV2	201	104	0.01%	0.001%
29	4.626	1009	1022	1064	rVV	186027	514756	27.56%	3.765%
30	5.060	1141	1157	1183	rBV	340139	753189	40.32%	5.509%
31	5.359	1248	1250	1253	rBV2	665	502	0.03%	0.004%
32	5.440	1272	1275	1276	rBV	229	102	0.01%	0.001%
33	5.517	1297	1299	1301	rBV	190	120	0.01%	0.001%
34	5.571	1311	1316	1321	rBV3	332	371	0.02%	0.003%
35	5.597	1321	1324	1325	rBV	215	119	0.01%	0.001%
36	5.652	1338	1341	1342	rBV	317	146	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051029.D
 Acq On : 30 Sep 2022 13:28
 Operator : JC/MD
 Sample : N4854-07 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	5.723	1342	1363	1393	rBV2	685462	1868013	100.00%	13.663%
38	6.028	1456	1458	1462	rBV5	565	402	0.02%	0.003%
39	6.063	1466	1469	1473	rVB3	448	301	0.02%	0.002%
40	6.083	1473	1475	1478	rBV2	237	138	0.01%	0.001%
41	6.147	1493	1495	1499	rVB2	423	234	0.01%	0.002%
42	6.173	1499	1503	1509	rBV2	516	471	0.03%	0.003%
43	6.247	1509	1526	1553	rBV	520880	988086	52.90%	7.227%
44	6.526	1601	1613	1627	rBV3	15029	29617	1.59%	0.217%
45	6.639	1646	1648	1649	rBV3	174	91	0.00%	0.001%
46	6.690	1649	1664	1685	rBV	451279	875324	46.86%	6.402%
47	6.932	1735	1739	1742	rBB3	315	215	0.01%	0.002%
48	6.964	1747	1749	1755	rBV3	354	270	0.01%	0.002%
49	6.986	1755	1756	1759	rVB	247	103	0.01%	0.001%
50	7.015	1760	1765	1773	rVB3	406	540	0.03%	0.004%
51	7.050	1773	1776	1777	rBV	224	98	0.01%	0.001%
52	7.089	1784	1788	1790	rBV2	370	304	0.02%	0.002%
53	7.102	1790	1792	1794	rBV2	256	118	0.01%	0.001%
54	7.147	1802	1806	1809	rBV2	118	83	0.00%	0.001%
55	7.166	1810	1812	1813	rBV	329	113	0.01%	0.001%
56	7.198	1813	1822	1828	rBV6	1283	2317	0.12%	0.017%
57	7.269	1841	1844	1850	rVB2	315	241	0.01%	0.002%
58	7.510	1916	1919	1921	rBV	160	93	0.00%	0.001%
59	7.565	1922	1936	1960	rBV	215021	387686	20.75%	2.836%
60	7.896	2026	2039	2058	rBV	765056	1338264	71.64%	9.788%
61	8.179	2114	2127	2149	rBV	158177	270311	14.47%	1.977%
62	8.517	2228	2232	2234	rBV	379	290	0.02%	0.002%
63	8.552	2234	2243	2256	rVB2	21385	35663	1.91%	0.261%
64	8.636	2256	2269	2308	rBV4	477295	1081440	57.89%	7.910%
65	8.938	2359	2363	2368	rVB4	506	414	0.02%	0.003%
66	8.996	2378	2381	2385	rBV2	380	311	0.02%	0.002%
67	9.230	2450	2454	2460	rVB	416	464	0.02%	0.003%
68	9.272	2464	2467	2469	rBV	342	217	0.01%	0.002%
69	9.417	2497	2512	2545	rBV	748736	1249497	66.89%	9.139%
70	9.648	2581	2584	2586	rBV	388	257	0.01%	0.002%
71	9.687	2593	2596	2599	rBV	615	521	0.03%	0.004%
72	9.716	2603	2605	2609	rVB2	318	205	0.01%	0.001%
73	9.790	2626	2628	2632	rVB	238	135	0.01%	0.001%
74	9.816	2632	2636	2637	rBV	409	222	0.01%	0.002%
75	9.851	2645	2647	2649	rBV2	221	96	0.01%	0.001%
76	9.928	2665	2671	2676	rBV3	276	300	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051029.D
 Acq On : 30 Sep 2022 13:28
 Operator : JC/MD
 Sample : N4854-07 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	9.989	2687	2690	2692	rBV2	174	133	0.01%	0.001%
78	10.095	2720	2723	2725	rBV2	571	373	0.02%	0.003%
79	10.214	2754	2760	2762	rBV	314	326	0.02%	0.002%
80	10.253	2769	2772	2773	rBV2	142	91	0.00%	0.001%
81	10.378	2808	2811	2814	rVB2	396	198	0.01%	0.001%
82	10.407	2814	2820	2821	rBV	235	222	0.01%	0.002%
83	10.754	2916	2928	2949	rBV	632142	1015875	54.38%	7.430%
84	10.928	2980	2982	2984	rBV	259	95	0.01%	0.001%
85	11.118	3037	3041	3046	rBV4	842	638	0.03%	0.005%
86	11.221	3070	3073	3075	rBV	229	128	0.01%	0.001%
87	11.320	3102	3104	3109	rBV2	299	243	0.01%	0.002%
88	11.414	3129	3133	3138	rVB3	567	524	0.03%	0.004%
89	11.449	3139	3144	3146	rBV2	343	304	0.02%	0.002%
90	11.497	3157	3159	3164	rVB3	477	294	0.02%	0.002%
91	11.523	3164	3167	3171	rBV2	446	410	0.02%	0.003%
92	11.619	3193	3197	3199	rBV	345	256	0.01%	0.002%
93	11.809	3244	3256	3283	rBV	575317	916781	49.08%	6.706%
94	12.192	3362	3375	3400	rBV	652854	1059307	56.71%	7.748%
95	12.623	3506	3509	3514	rBV	447	330	0.02%	0.002%
96	13.131	3664	3667	3671	rBV2	519	331	0.02%	0.002%
97	13.275	3709	3712	3716	rBV2	636	516	0.03%	0.004%
98	13.340	3729	3732	3736	rBV2	653	383	0.02%	0.003%
99	13.735	3852	3855	3857	rBV	515	309	0.02%	0.002%
100	14.455	4076	4079	4084	rBV2	694	806	0.04%	0.006%




Sum of corrected areas: 13672058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051029.D
Acq On : 30 Sep 2022 13:28
Operator : JC/MD
Sample : N4854-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

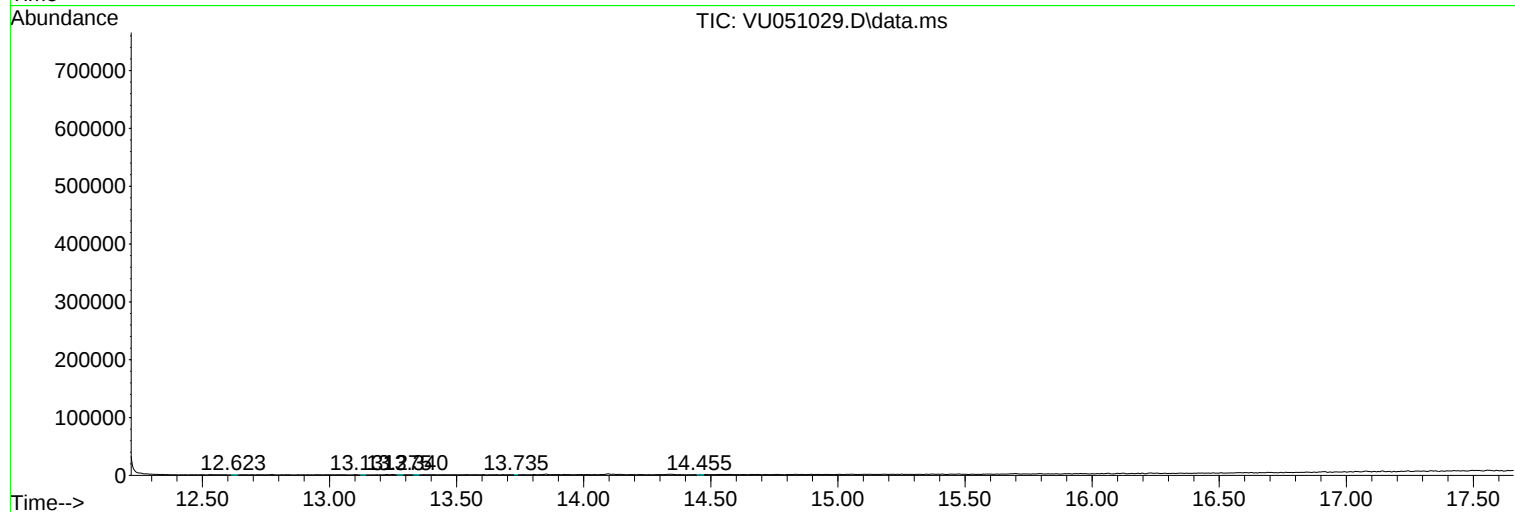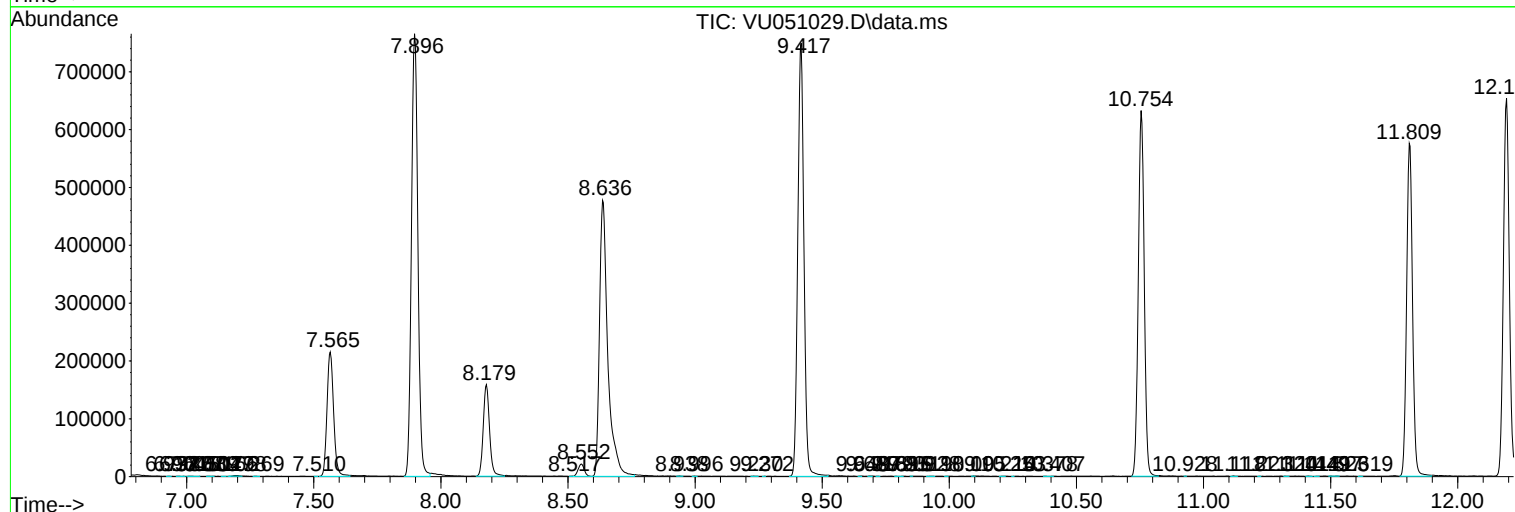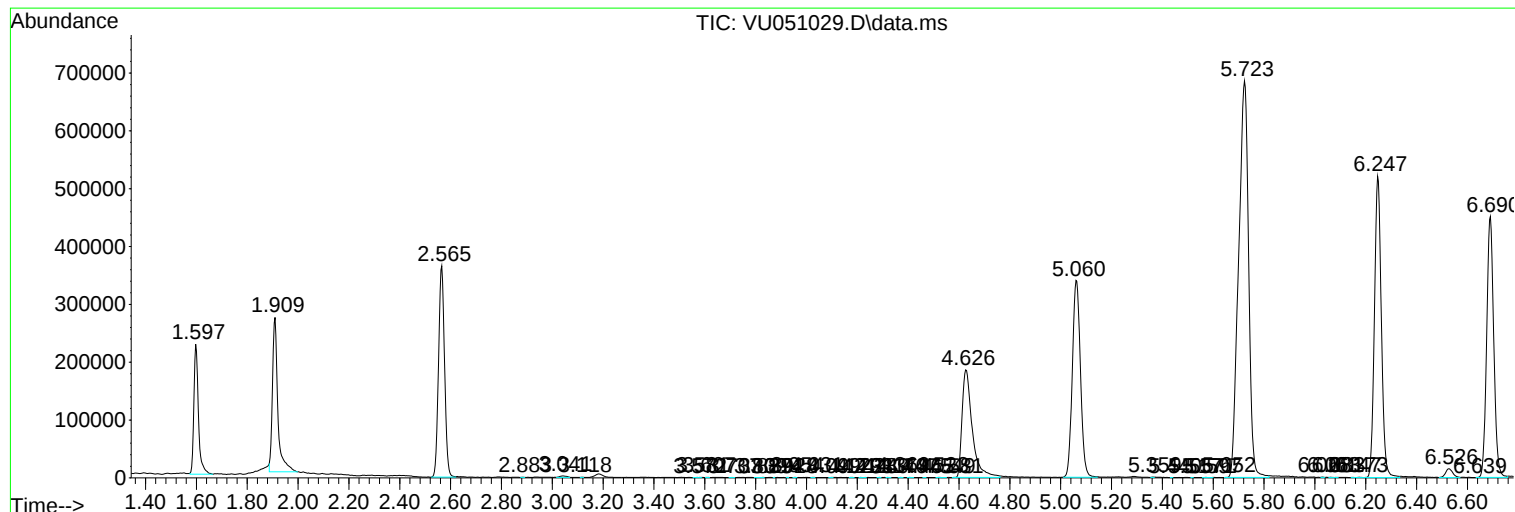

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051029.D
Acq On : 30 Sep 2022 13:28
Operator : JC/MD
Sample : N4854-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051029.D
Acq On : 30 Sep 2022 13:28
Operator : JC/MD
Sample : N4854-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------