

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051036.D
 Acq On : 30 Sep 2022 16:11
 Operator : JC/MD
 Sample : N4854-19 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	103	rVB	197034	241856	14.29%	1.952%
2	1.903	167	175	196	rVB	181508	255933	15.12%	2.065%
3	2.565	368	381	396	rVV	325479	527670	31.17%	4.258%
4	2.761	440	442	446	rVV4	372	288	0.02%	0.002%
5	3.041	520	529	544	rVV2	7608	14746	0.87%	0.119%
6	3.183	559	573	595	rBV2	20870	50490	2.98%	0.407%
7	3.321	612	616	619	rBV3	435	398	0.02%	0.003%
8	3.414	642	645	649	rVB	331	239	0.01%	0.002%
9	3.443	649	654	659	rBV2	269	330	0.02%	0.003%
10	3.764	750	754	759	rVB2	317	343	0.02%	0.003%
11	3.922	799	803	809	rBV3	237	243	0.01%	0.002%
12	3.990	820	824	826	rBV	320	237	0.01%	0.002%
13	4.038	831	839	842	rBV2	293	377	0.02%	0.003%
14	4.102	852	859	868	rBV2	311	415	0.02%	0.003%
15	4.221	893	896	900	rVB2	401	238	0.01%	0.002%
16	4.414	953	956	963	rBV3	437	509	0.03%	0.004%
17	4.501	974	983	989	rBV2	481	527	0.03%	0.004%
18	4.552	996	999	1005	rVB2	288	254	0.02%	0.002%
19	4.623	1007	1021	1051	rBV	187332	493587	29.16%	3.983%
20	5.060	1140	1157	1182	rBV	315996	696532	41.14%	5.621%
21	5.356	1246	1249	1251	rBV2	445	302	0.02%	0.002%
22	5.382	1253	1257	1262	rVB4	604	630	0.04%	0.005%
23	5.523	1295	1301	1306	rVB2	226	229	0.01%	0.002%
24	5.723	1341	1363	1384	rBV2	624953	1692924	100.00%	13.662%
25	5.970	1438	1440	1445	rVB4	735	585	0.03%	0.005%
26	6.022	1450	1456	1459	rBV3	477	555	0.03%	0.004%
27	6.070	1468	1471	1474	rVB2	311	230	0.01%	0.002%
28	6.115	1482	1485	1493	rVB3	889	961	0.06%	0.008%
29	6.182	1503	1506	1512	rVB3	378	339	0.02%	0.003%
30	6.247	1512	1526	1550	rBV	491594	926684	54.74%	7.479%
31	6.526	1603	1613	1628	rVB2	15549	31033	1.83%	0.250%
32	6.626	1642	1644	1648	rVB2	521	279	0.02%	0.002%
33	6.690	1648	1664	1683	rBV	413657	807820	47.72%	6.519%
34	7.083	1780	1786	1790	rVB3	364	341	0.02%	0.003%
35	7.192	1805	1820	1821	rBV4	1383	2099	0.12%	0.017%
36	7.234	1831	1833	1840	rVB2	309	252	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051036.D
 Acq On : 30 Sep 2022 16:11
 Operator : JC/MD
 Sample : N4854-19 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.565	1923	1936	1954	rBV	196064	348209	20.57%	2.810%
38	7.745	1988	1992	1996	rVB2	527	408	0.02%	0.003%
39	7.771	1996	2000	2003	rBV3	391	268	0.02%	0.002%
40	7.796	2003	2008	2011	rBV3	598	567	0.03%	0.005%
41	7.816	2011	2014	2019	rVB2	886	584	0.03%	0.005%
42	7.896	2025	2039	2072	rBV	687707	1199662	70.86%	9.682%
43	8.086	2094	2098	2102	rBV3	566	499	0.03%	0.004%
44	8.121	2107	2109	2113	rVB2	555	363	0.02%	0.003%
45	8.179	2115	2127	2144	rBV	140988	240983	14.23%	1.945%
46	8.391	2190	2193	2197	rVB3	812	603	0.04%	0.005%
47	8.423	2197	2203	2209	rBV3	627	1069	0.06%	0.009%
48	8.552	2231	2243	2256	rBV2	16422	26489	1.56%	0.214%
49	8.636	2256	2269	2302	rBV2	441522	988099	58.37%	7.974%
50	8.912	2352	2355	2357	rBV2	545	401	0.02%	0.003%
51	8.964	2369	2371	2373	rVV	481	289	0.02%	0.002%
52	8.976	2373	2375	2382	rVB3	518	507	0.03%	0.004%
53	9.009	2382	2385	2388	rBV	309	224	0.01%	0.002%
54	9.128	2419	2422	2426	rBV	300	240	0.01%	0.002%
55	9.234	2449	2455	2463	rVV	361	465	0.03%	0.004%
56	9.288	2469	2472	2477	rVB2	429	285	0.02%	0.002%
57	9.356	2488	2493	2496	rBV2	385	301	0.02%	0.002%
58	9.417	2498	2512	2538	rBV	698715	1161361	68.60%	9.373%
59	9.645	2580	2583	2586	rBV2	280	221	0.01%	0.002%
60	9.703	2599	2601	2607	rVB3	685	492	0.03%	0.004%
61	9.848	2643	2646	2649	rBV2	409	296	0.02%	0.002%
62	9.915	2664	2667	2671	rVB2	384	354	0.02%	0.003%
63	9.938	2671	2674	2680	rBV2	283	289	0.02%	0.002%
64	10.321	2789	2793	2796	rBV2	308	227	0.01%	0.002%
65	10.436	2825	2829	2834	rVB3	496	482	0.03%	0.004%
66	10.465	2834	2838	2841	rBV2	513	343	0.02%	0.003%
67	10.488	2841	2845	2848	rVV	380	346	0.02%	0.003%
68	10.517	2851	2854	2861	rVB2	357	352	0.02%	0.003%
69	10.648	2891	2895	2899	rVV3	335	324	0.02%	0.003%
70	10.755	2914	2928	2952	rBV	583533	935894	55.28%	7.553%
71	10.973	2990	2996	3004	rVV2	298	556	0.03%	0.004%
72	11.012	3005	3008	3012	rVB	566	394	0.02%	0.003%
73	11.378	3121	3122	3129	rVB2	434	249	0.01%	0.002%
74	11.427	3131	3137	3138	rBV	362	264	0.02%	0.002%
75	11.600	3187	3191	3193	rBV2	324	237	0.01%	0.002%
76	11.735	3231	3233	3238	rVB2	353	226	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051036.D
 Acq On : 30 Sep 2022 16:11
 Operator : JC/MD
 Sample : N4854-19 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.761	3238	3241	3244	rBV3	303	283	0.02%	0.002%
78	11.809	3244	3256	3278	rBV	489783	802780	47.42%	6.479%
79	11.999	3310	3315	3321	rBV3	791	825	0.05%	0.007%
80	12.192	3361	3375	3399	rBV	559702	914963	54.05%	7.384%
81	12.780	3555	3558	3562	rBV3	385	360	0.02%	0.003%
82	12.832	3571	3574	3579	rVB3	333	262	0.02%	0.002%
83	12.857	3579	3582	3586	rBV4	317	311	0.02%	0.003%
84	12.925	3600	3603	3605	rBV3	380	250	0.01%	0.002%
85	13.304	3716	3721	3726	rBV3	543	734	0.04%	0.006%
86	13.340	3729	3732	3735	rVB3	497	338	0.02%	0.003%
87	13.417	3750	3756	3760	rBV4	586	704	0.04%	0.006%
88	13.488	3774	3778	3781	rVB2	416	375	0.02%	0.003%
89	13.510	3783	3785	3789	rBV3	412	317	0.02%	0.003%
90	13.600	3806	3813	3816	rBV3	535	742	0.04%	0.006%
91	13.690	3837	3841	3844	rBV3	621	559	0.03%	0.005%
92	13.745	3855	3858	3862	rBV3	395	344	0.02%	0.003%
93	13.838	3884	3887	3890	rBV	353	227	0.01%	0.002%
94	13.886	3899	3902	3908	rBV2	501	439	0.03%	0.004%
95	13.960	3919	3925	3930	rBV2	557	671	0.04%	0.005%
96	14.005	3936	3939	3943	rVB	544	338	0.02%	0.003%
97	14.208	3999	4002	4004	rBV2	376	268	0.02%	0.002%
98	14.568	4110	4114	4118	rBV3	493	520	0.03%	0.004%
99	14.754	4170	4172	4175	rVB2	533	242	0.01%	0.002%
100	14.803	4185	4187	4191	rBV2	457	281	0.02%	0.002%




Sum of corrected areas: 12391030

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051036.D
Acq On : 30 Sep 2022 16:11
Operator : JC/MD
Sample : N4854-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

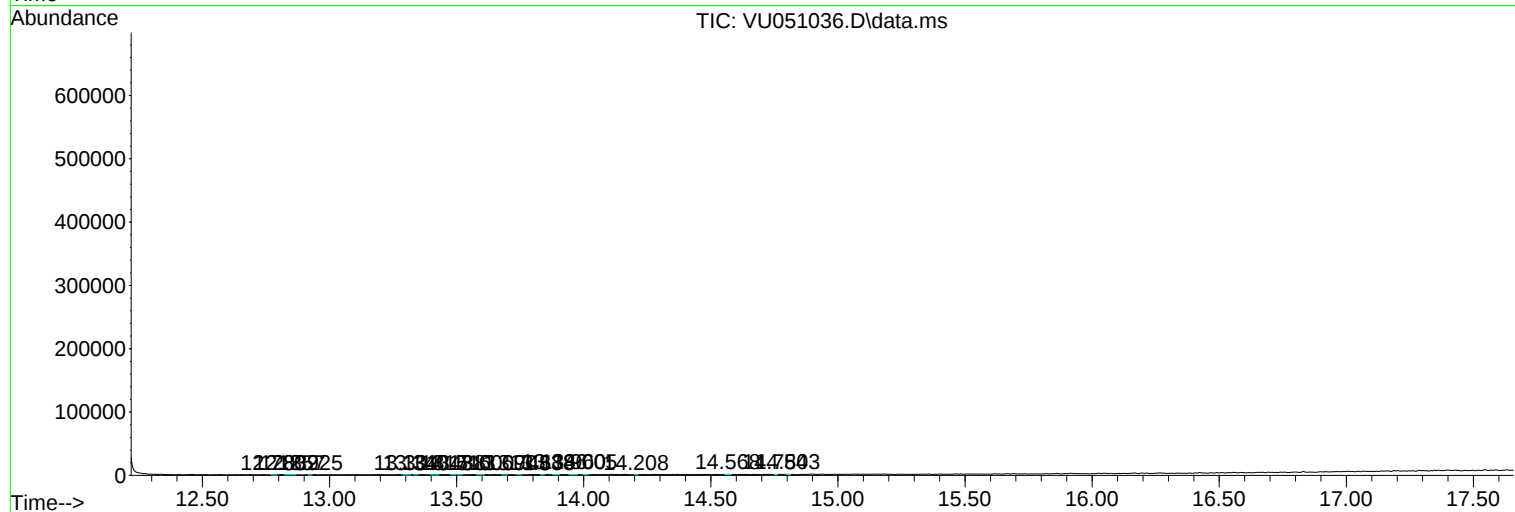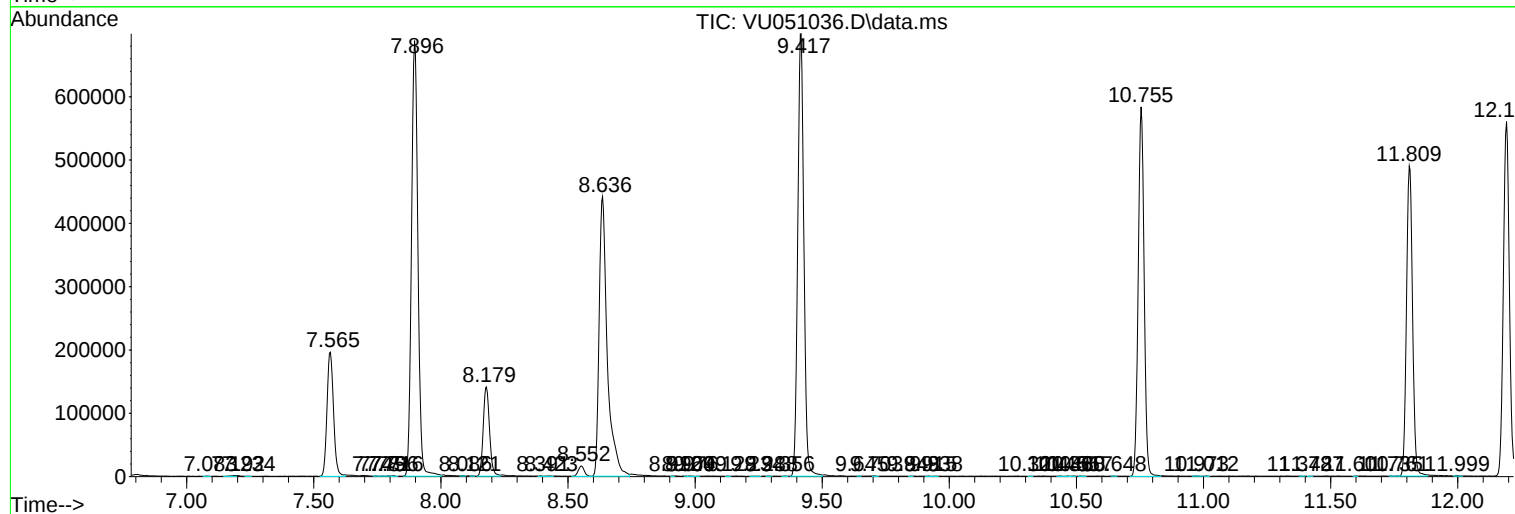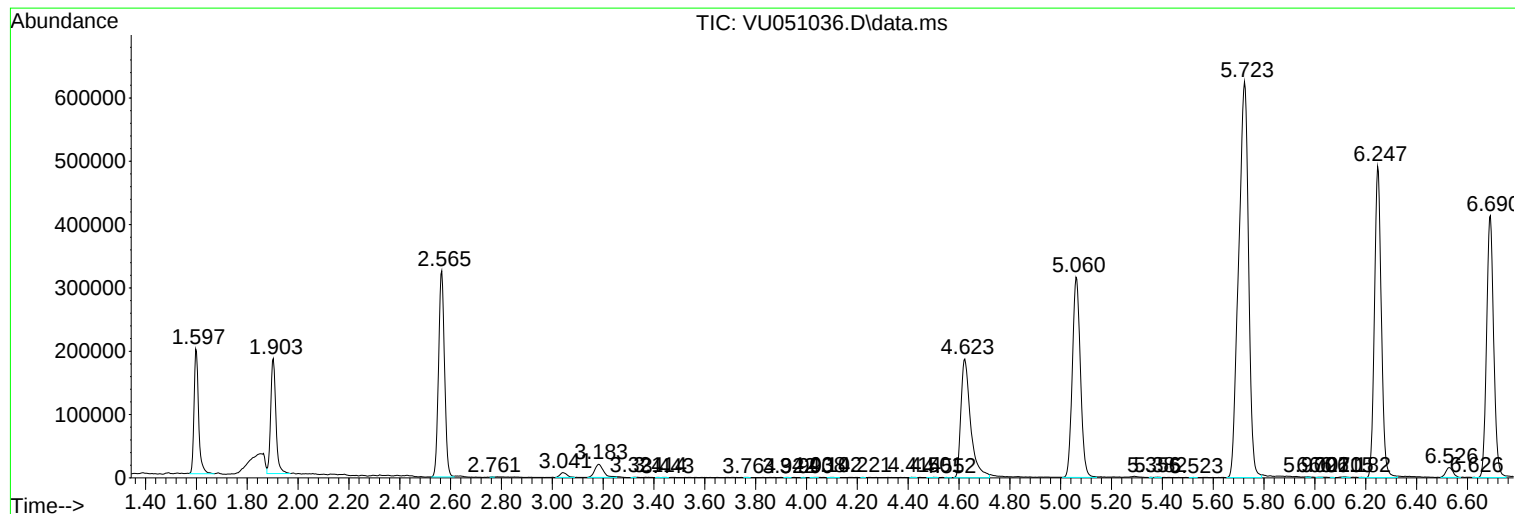

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051036.D
Acq On : 30 Sep 2022 16:11
Operator : JC/MD
Sample : N4854-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051036.D
Acq On : 30 Sep 2022 16:11
Operator : JC/MD
Sample : N4854-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------