

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051037.D
 Acq On : 30 Sep 2022 16:34
 Operator : JC/MD
 Sample : N4854-20 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	202216	245126	13.77%	1.901%
2	1.903	168	175	193	rVB	195572	268082	15.06%	2.079%
3	2.565	368	381	399	rBV	335781	548692	30.82%	4.255%
4	2.790	445	451	454	rBV5	874	994	0.06%	0.008%
5	2.912	486	489	491	rBV	513	315	0.02%	0.002%
6	2.967	504	506	510	rVB4	411	219	0.01%	0.002%
7	3.041	513	529	544	rVB3	13526	26465	1.49%	0.205%
8	3.102	544	548	554	rVB2	403	458	0.03%	0.004%
9	3.182	556	573	588	rBV2	18527	45165	2.54%	0.350%
10	3.343	621	623	627	rBV2	371	234	0.01%	0.002%
11	3.391	636	638	641	rBV2	354	243	0.01%	0.002%
12	3.613	705	707	711	rVV2	404	312	0.02%	0.002%
13	3.748	745	749	752	rBV2	362	313	0.02%	0.002%
14	3.832	773	775	780	rVB2	329	238	0.01%	0.002%
15	3.957	810	814	817	rBV2	383	306	0.02%	0.002%
16	4.192	882	887	890	rBV2	339	258	0.01%	0.002%
17	4.272	909	912	918	rVB2	373	368	0.02%	0.003%
18	4.314	918	925	928	rBV2	355	422	0.02%	0.003%
19	4.433	949	962	974	rVB6	4478	11292	0.63%	0.088%
20	4.485	974	978	980	rBV2	277	219	0.01%	0.002%
21	4.623	1008	1021	1050	rBV2	186141	503387	28.27%	3.903%
22	4.903	1106	1108	1111	rBV2	399	278	0.02%	0.002%
23	4.973	1127	1130	1132	rBV2	467	250	0.01%	0.002%
24	5.060	1140	1157	1182	rBV	328016	722737	40.59%	5.604%
25	5.247	1209	1215	1217	rBV4	687	727	0.04%	0.006%
26	5.366	1249	1252	1253	rBV2	475	252	0.01%	0.002%
27	5.459	1268	1281	1296	rVB7	12309	27852	1.56%	0.216%
28	5.722	1342	1363	1387	rBV2	655376	1780429	100.00%	13.805%
29	5.970	1436	1440	1445	rVB6	1091	932	0.05%	0.007%
30	6.044	1460	1463	1464	rBV	443	299	0.02%	0.002%
31	6.118	1482	1486	1491	rVB2	644	631	0.04%	0.005%
32	6.173	1500	1503	1507	rBV2	461	435	0.02%	0.003%
33	6.247	1512	1526	1550	rBV	495733	949155	53.31%	7.360%
34	6.369	1562	1564	1567	rBV3	917	623	0.03%	0.005%
35	6.475	1595	1597	1601	rVB2	468	268	0.02%	0.002%
36	6.529	1601	1614	1626	rVB3	15301	28343	1.59%	0.220%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051037.D
 Acq On : 30 Sep 2022 16:34
 Operator : JC/MD
 Sample : N4854-20 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.584	1626	1631	1637	rBV6	689	698	0.04%	0.005%
38	6.690	1648	1664	1690	rBV	432500	843080	47.35%	6.537%
39	6.944	1741	1743	1747	rVB3	652	427	0.02%	0.003%
40	7.031	1767	1770	1774	rVB2	437	370	0.02%	0.003%
41	7.066	1774	1781	1784	rBV	477	598	0.03%	0.005%
42	7.185	1811	1818	1828	rBV5	1699	3038	0.17%	0.024%
43	7.256	1828	1840	1853	rVB6	7750	15492	0.87%	0.120%
44	7.382	1864	1879	1889	rBV5	7077	13902	0.78%	0.108%
45	7.513	1915	1920	1923	rBV2	304	273	0.02%	0.002%
46	7.565	1923	1936	1955	rBV	202949	363164	20.40%	2.816%
47	7.690	1970	1975	1977	rBV4	1089	987	0.06%	0.008%
48	7.800	2006	2009	2014	rVB3	625	461	0.03%	0.004%
49	7.896	2025	2039	2057	rBV	731199	1252840	70.37%	9.714%
50	8.121	2105	2109	2115	rBV4	434	524	0.03%	0.004%
51	8.179	2115	2127	2145	rBV	146819	251896	14.15%	1.953%
52	8.353	2178	2181	2186	rVB3	589	545	0.03%	0.004%
53	8.475	2216	2219	2222	rBV2	382	254	0.01%	0.002%
54	8.491	2222	2224	2227	rVB	474	279	0.02%	0.002%
55	8.523	2231	2234	2236	rVB	398	230	0.01%	0.002%
56	8.552	2236	2243	2253	rBV6	2771	4583	0.26%	0.036%
57	8.635	2256	2269	2310	rBV2	469961	1024337	57.53%	7.943%
58	8.890	2345	2348	2353	rVB3	440	423	0.02%	0.003%
59	9.092	2408	2411	2416	rVB2	308	219	0.01%	0.002%
60	9.163	2430	2433	2435	rBV	458	328	0.02%	0.003%
61	9.343	2481	2489	2496	rBV5	1146	1799	0.10%	0.014%
62	9.417	2498	2512	2538	rBV	703288	1186076	66.62%	9.197%
63	9.539	2548	2550	2553	rVB3	584	286	0.02%	0.002%
64	9.693	2595	2598	2606	rBV2	501	532	0.03%	0.004%
65	9.787	2623	2627	2632	rVB2	541	489	0.03%	0.004%
66	10.008	2693	2696	2701	rBV	381	353	0.02%	0.003%
67	10.044	2704	2707	2713	rBV2	240	264	0.01%	0.002%
68	10.143	2732	2738	2744	rBV2	281	254	0.01%	0.002%
69	10.185	2746	2751	2754	rBV2	310	299	0.02%	0.002%
70	10.401	2815	2818	2826	rBV2	216	232	0.01%	0.002%
71	10.664	2896	2900	2905	rVB2	360	329	0.02%	0.003%
72	10.693	2905	2909	2912	rBV2	783	777	0.04%	0.006%
73	10.754	2915	2928	2950	rVV	603726	970449	54.51%	7.525%
74	10.880	2963	2967	2974	rVB2	471	620	0.03%	0.005%
75	11.015	3006	3009	3015	rBV2	496	564	0.03%	0.004%
76	11.118	3037	3041	3042	rBV	359	255	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051037.D
 Acq On : 30 Sep 2022 16:34
 Operator : JC/MD
 Sample : N4854-20 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.179	3057	3060	3061	rBV	437	259	0.01%	0.002%
78	11.369	3115	3119	3120	rBV	316	222	0.01%	0.002%
79	11.404	3126	3130	3131	rBV	341	224	0.01%	0.002%
80	11.629	3198	3200	3205	rVB2	392	219	0.01%	0.002%
81	11.809	3244	3256	3273	rBV	509347	817508	45.92%	6.339%
82	11.992	3310	3313	3317	rVB3	440	287	0.02%	0.002%
83	12.018	3318	3321	3327	rBV3	305	268	0.02%	0.002%
84	12.108	3345	3349	3351	rBV2	360	289	0.02%	0.002%
85	12.124	3352	3354	3356	rVB3	541	240	0.01%	0.002%
86	12.192	3361	3375	3393	rBV	590864	961417	54.00%	7.455%
87	12.410	3441	3443	3446	rBV2	493	400	0.02%	0.003%
88	12.552	3484	3487	3490	rBV	442	363	0.02%	0.003%
89	12.809	3564	3567	3569	rBV2	477	309	0.02%	0.002%
90	12.848	3576	3579	3582	rBV2	510	390	0.02%	0.003%
91	12.902	3593	3596	3600	rVB2	521	373	0.02%	0.003%
92	12.999	3623	3626	3631	rBV3	432	427	0.02%	0.003%
93	13.076	3646	3650	3653	rBV2	506	394	0.02%	0.003%
94	13.378	3739	3744	3749	rBV3	362	416	0.02%	0.003%
95	13.471	3771	3773	3777	rVB2	554	337	0.02%	0.003%
96	13.909	3906	3909	3913	rBV2	527	394	0.02%	0.003%
97	14.317	4033	4036	4043	rBV3	581	583	0.03%	0.005%
98	15.127	4285	4288	4290	rBV2	618	334	0.02%	0.003%
99	15.201	4309	4311	4315	rBV2	608	449	0.03%	0.003%
100	15.867	4512	4518	4523	rBV7	1259	1674	0.09%	0.013%




Sum of corrected areas: 12896621

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051037.D
Acq On : 30 Sep 2022 16:34
Operator : JC/MD
Sample : N4854-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

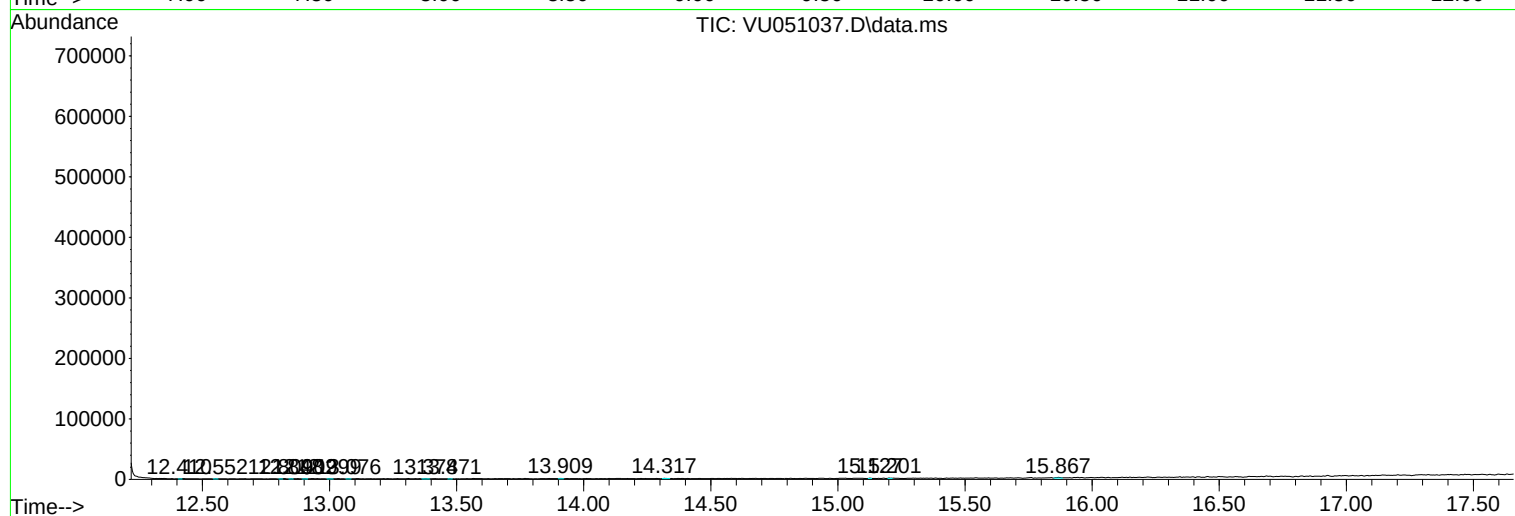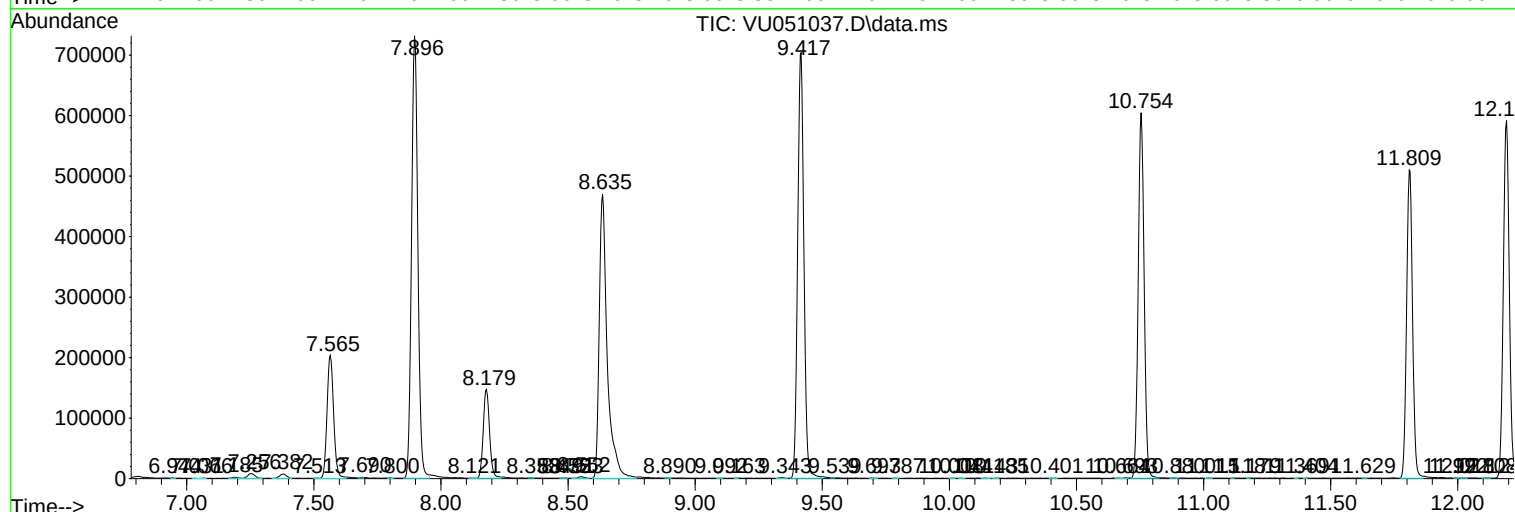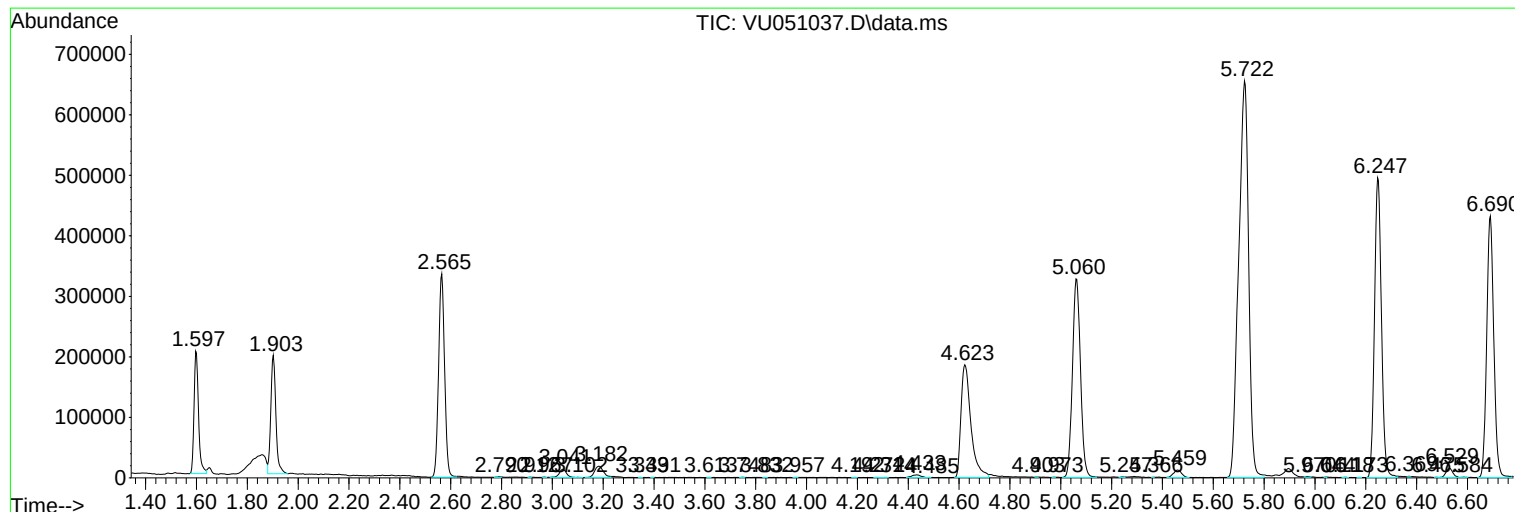

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051037.D
Acq On : 30 Sep 2022 16:34
Operator : JC/MD
Sample : N4854-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051037.D
Acq On : 30 Sep 2022 16:34
Operator : JC/MD
Sample : N4854-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------