

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051038.D
 Acq On : 30 Sep 2022 16:58
 Operator : JC/MD
 Sample : N4854-16 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	202247	245370	14.03%	1.853%
2	1.903	168	175	192	rVB	188757	256084	14.65%	1.934%
3	2.565	368	381	398	rBV	330973	541757	30.98%	4.092%
4	3.044	522	530	542	rVB4	3222	5639	0.32%	0.043%
5	3.186	560	574	588	rBV	16033	37615	2.15%	0.284%
6	3.346	621	624	625	rBV	887	505	0.03%	0.004%
7	3.533	680	682	685	rBV	283	128	0.01%	0.001%
8	3.703	730	735	738	rBV	382	306	0.02%	0.002%
9	3.848	778	780	784	rBV2	261	169	0.01%	0.001%
10	4.076	848	851	853	rBV	147	100	0.01%	0.001%
11	4.115	860	863	865	rBV2	236	159	0.01%	0.001%
12	4.131	865	868	871	rVV2	455	307	0.02%	0.002%
13	4.150	871	874	880	rVB	252	226	0.01%	0.002%
14	4.182	880	884	886	rBV2	200	157	0.01%	0.001%
15	4.250	902	905	909	rVB	329	197	0.01%	0.001%
16	4.311	921	924	926	rBV	211	136	0.01%	0.001%
17	4.350	934	936	940	rBV2	205	179	0.01%	0.001%
18	4.459	966	970	973	rBV2	218	161	0.01%	0.001%
19	4.517	985	988	990	rBV2	429	261	0.01%	0.002%
20	4.623	1006	1021	1069	rBV	183431	497376	28.45%	3.757%
21	4.986	1132	1134	1136	rBV2	315	103	0.01%	0.001%
22	5.060	1142	1157	1185	rVB	324976	716834	41.00%	5.414%
23	5.359	1248	1250	1251	rBV2	388	174	0.01%	0.001%
24	5.420	1264	1269	1274	rVB3	383	505	0.03%	0.004%
25	5.446	1274	1277	1280	rVB2	246	113	0.01%	0.001%
26	5.469	1280	1284	1289	rBV	199	233	0.01%	0.002%
27	5.526	1299	1302	1304	rVB2	287	145	0.01%	0.001%
28	5.578	1317	1318	1320	rVB2	123	25	0.00%	0.000%
29	5.629	1331	1334	1336	rBV	220	166	0.01%	0.001%
30	5.723	1341	1363	1383	rBV2	651943	1748516	100.00%	13.206%
31	6.041	1459	1462	1467	rBV2	894	711	0.04%	0.005%
32	6.112	1478	1484	1485	rBV4	333	306	0.02%	0.002%
33	6.247	1512	1526	1549	rBV	479708	911240	52.12%	6.882%
34	6.530	1603	1614	1627	rBV5	15971	32047	1.83%	0.242%
35	6.690	1649	1664	1684	rBV	424391	827989	47.35%	6.254%
36	6.919	1733	1735	1739	rVB4	311	213	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051038.D
 Acq On : 30 Sep 2022 16:58
 Operator : JC/MD
 Sample : N4854-16 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.034	1769	1771	1774	rVB	264	167	0.01%	0.001%
38	7.176	1810	1815	1816	rBV2	1215	856	0.05%	0.006%
39	7.304	1853	1855	1856	rBV2	183	64	0.00%	0.000%
40	7.346	1865	1868	1871	rVB2	114	69	0.00%	0.001%
41	7.366	1871	1874	1877	rBV2	240	217	0.01%	0.002%
42	7.513	1915	1920	1923	rBV	400	345	0.02%	0.003%
43	7.565	1923	1936	1962	rBV2	198718	360720	20.63%	2.724%
44	7.758	1992	1996	1997	rBV	357	281	0.02%	0.002%
45	7.841	2019	2022	2024	rBV	237	145	0.01%	0.001%
46	7.896	2026	2039	2057	rBV	724941	1231371	70.42%	9.300%
47	8.179	2115	2127	2146	rBV	144893	247719	14.17%	1.871%
48	8.494	2221	2225	2227	rBV3	335	269	0.02%	0.002%
49	8.552	2230	2243	2257	rBV	427663	721504	41.26%	5.449%
50	8.636	2258	2269	2307	rVB3	452084	993312	56.81%	7.502%
51	8.867	2339	2341	2343	rVB	358	134	0.01%	0.001%
52	8.912	2353	2355	2358	rBV2	402	195	0.01%	0.001%
53	9.047	2395	2397	2398	rBV	246	120	0.01%	0.001%
54	9.118	2417	2419	2421	rBV2	252	149	0.01%	0.001%
55	9.128	2421	2422	2423	rBV	328	119	0.01%	0.001%
56	9.153	2428	2430	2433	rVB	296	171	0.01%	0.001%
57	9.237	2453	2456	2457	rBV	236	125	0.01%	0.001%
58	9.417	2498	2512	2535	rBV	684520	1143501	65.40%	8.637%
59	9.655	2582	2586	2591	rBV2	305	382	0.02%	0.003%
60	9.774	2619	2623	2626	rBV2	293	249	0.01%	0.002%
61	10.160	2740	2743	2745	rBV	184	117	0.01%	0.001%
62	10.459	2832	2836	2837	rBV	260	174	0.01%	0.001%
63	10.491	2843	2846	2848	rBV2	335	207	0.01%	0.002%
64	10.754	2914	2928	2951	rBV	593514	954792	54.61%	7.211%
65	11.070	3021	3026	3029	rBV3	494	425	0.02%	0.003%
66	11.111	3037	3039	3042	rBV3	555	337	0.02%	0.003%
67	11.140	3047	3048	3051	rBV	286	106	0.01%	0.001%
68	11.156	3051	3053	3056	rBV2	277	155	0.01%	0.001%
69	11.214	3068	3071	3074	rBV2	524	529	0.03%	0.004%
70	11.333	3105	3108	3111	rBV	249	148	0.01%	0.001%
71	11.507	3160	3162	3168	rBV2	292	271	0.02%	0.002%
72	11.581	3182	3185	3188	rBV2	462	345	0.02%	0.003%
73	11.809	3244	3256	3278	rBV	495233	796751	45.57%	6.018%
74	12.192	3362	3375	3403	rBV	578998	955788	54.66%	7.219%
75	12.652	3512	3518	3519	rBV3	435	464	0.03%	0.004%
76	13.722	3848	3851	3854	rVB2	692	482	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051038.D
Acq On : 30 Sep 2022 16:58
Operator : JC/MD
Sample : N4854-16 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J07

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Title : VOC Analysis

77	13.745	3854	3858	3861	rBV2	781	632	0.04%	0.005%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 13240059

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051038.D
Acq On : 30 Sep 2022 16:58
Operator : JC/MD
Sample : N4854-16 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

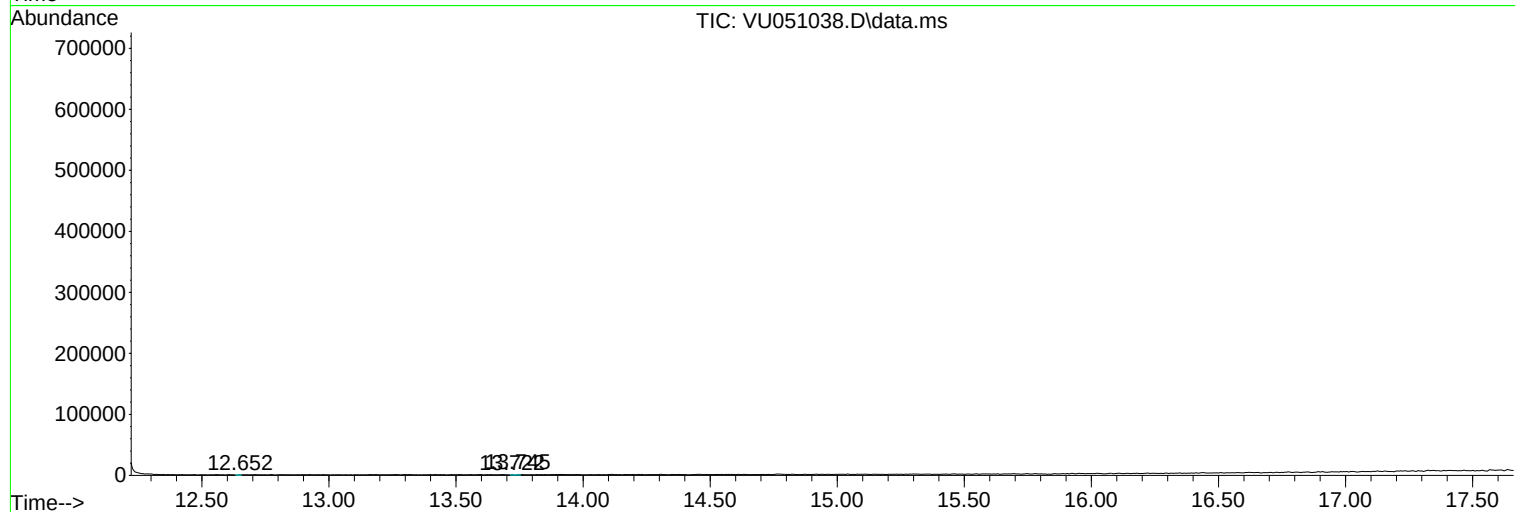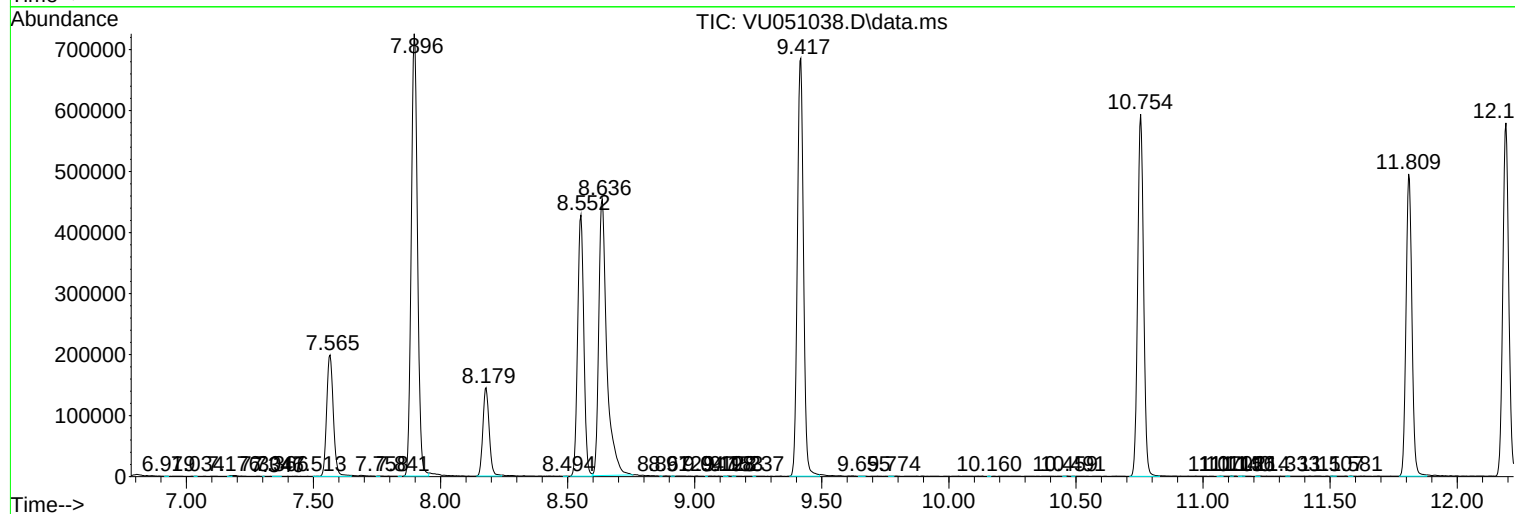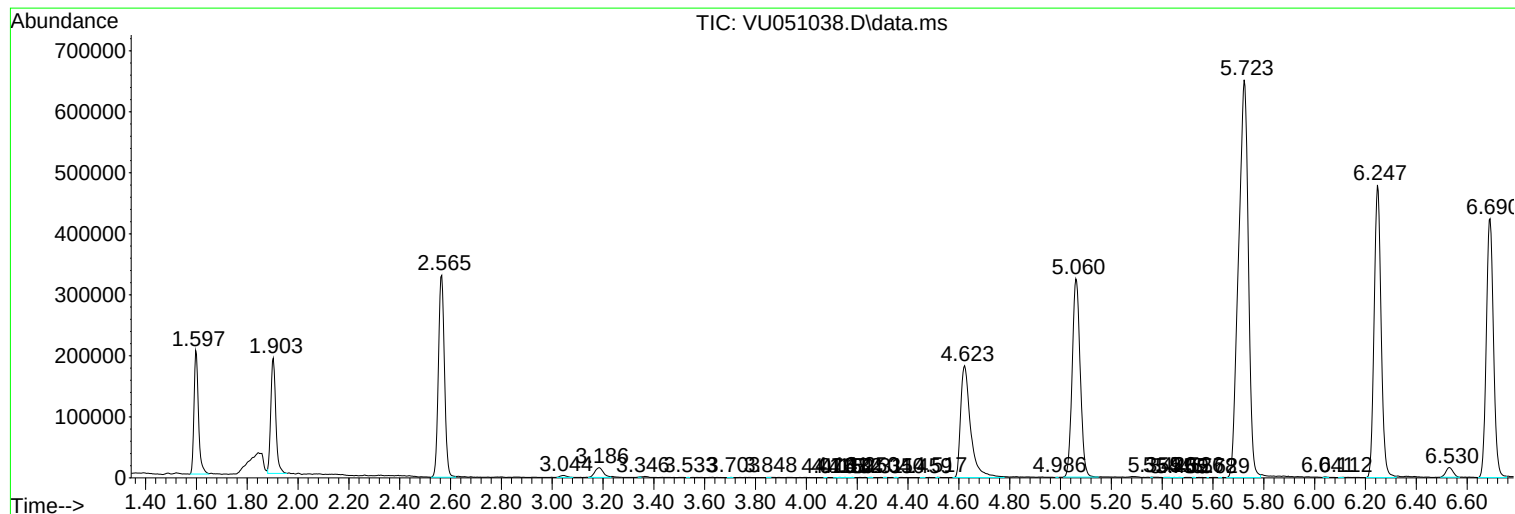

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051038.D
Acq On : 30 Sep 2022 16:58
Operator : JC/MD
Sample : N4854-16 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051038.D
Acq On : 30 Sep 2022 16:58
Operator : JC/MD
Sample : N4854-16 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc