

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051039.D
 Acq On : 30 Sep 2022 17:21
 Operator : JC/MD
 Sample : N4854-17 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	74	80	97	rVB	221849	264810	15.01%	2.015%
2	1.910	171	177	204	rVB	250418	378252	21.44%	2.879%
3	2.565	372	381	399	rVB	361954	580057	32.88%	4.414%
4	4.626	1011	1022	1063	rBV	182620	520947	29.53%	3.964%
5	5.064	1144	1158	1179	rVB	336091	730797	41.43%	5.561%
6	5.723	1343	1363	1384	rBV2	659856	1764047	100.00%	13.425%
7	6.247	1513	1526	1550	rBV	511298	972785	55.15%	7.403%
8	6.527	1603	1613	1628	rBV4	15429	30125	1.71%	0.229%
9	6.691	1649	1664	1683	rBV	430754	848548	48.10%	6.458%
10	7.060	1776	1779	1786	rBV2	572	691	0.04%	0.005%
11	7.192	1813	1820	1821	rBV4	1337	1309	0.07%	0.010%
12	7.231	1829	1832	1836	rVB2	718	574	0.03%	0.004%
13	7.398	1882	1884	1891	rVB2	402	387	0.02%	0.003%
14	7.440	1891	1897	1904	rBV2	468	528	0.03%	0.004%
15	7.475	1904	1908	1911	rBV	461	338	0.02%	0.003%
16	7.565	1923	1936	1964	rBV	205348	368845	20.91%	2.807%
17	7.768	1996	1999	2005	rVB4	721	674	0.04%	0.005%
18	7.800	2005	2009	2011	rBV2	528	454	0.03%	0.003%
19	7.896	2024	2039	2061	rBV	745356	1271419	72.07%	9.676%
20	8.179	2115	2127	2145	rBV	146830	256286	14.53%	1.950%
21	8.318	2167	2170	2175	rVB5	440	335	0.02%	0.003%
22	8.443	2205	2209	2212	rVB3	354	308	0.02%	0.002%
23	8.462	2212	2215	2218	rBV3	565	316	0.02%	0.002%
24	8.478	2218	2220	2226	rVV3	449	387	0.02%	0.003%
25	8.549	2236	2242	2250	rBV7	4164	6499	0.37%	0.049%
26	8.636	2256	2269	2308	rBV2	472088	1054804	59.79%	8.027%
27	8.871	2340	2342	2344	rVV3	593	318	0.02%	0.002%
28	8.957	2366	2369	2372	rVV2	504	341	0.02%	0.003%
29	9.051	2395	2398	2401	rBV	624	414	0.02%	0.003%
30	9.189	2436	2441	2446	rVB3	403	394	0.02%	0.003%
31	9.244	2453	2458	2460	rBV2	328	324	0.02%	0.002%
32	9.260	2460	2463	2466	rVB2	435	307	0.02%	0.002%
33	9.327	2481	2484	2487	rBV3	468	331	0.02%	0.003%
34	9.414	2498	2511	2531	rBV	734711	1223596	69.36%	9.312%
35	9.610	2568	2572	2573	rBV2	578	326	0.02%	0.002%
36	9.649	2582	2584	2587	rBV2	686	371	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051039.D
 Acq On : 30 Sep 2022 17:21
 Operator : JC/MD
 Sample : N4854-17 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	9.687	2593	2596	2600	rVV	407	329	0.02%	0.003%
38	9.723	2604	2607	2610	rVB	750	460	0.03%	0.004%
39	9.739	2610	2612	2619	rVB3	418	412	0.02%	0.003%
40	9.816	2634	2636	2642	rVB2	555	444	0.03%	0.003%
41	9.906	2661	2664	2668	rBV2	378	310	0.02%	0.002%
42	10.060	2709	2712	2719	rVB2	670	727	0.04%	0.006%
43	10.109	2722	2727	2731	rVB2	615	533	0.03%	0.004%
44	10.221	2756	2762	2766	rBV2	256	349	0.02%	0.003%
45	10.273	2775	2778	2783	rVB2	407	334	0.02%	0.003%
46	10.308	2783	2789	2795	rBV2	527	611	0.03%	0.005%
47	10.340	2795	2799	2801	rBV2	440	331	0.02%	0.003%
48	10.485	2840	2844	2852	rVB3	864	955	0.05%	0.007%
49	10.755	2915	2928	2946	rBV	613094	992491	56.26%	7.553%
50	10.877	2963	2966	2970	rVB3	392	350	0.02%	0.003%
51	10.932	2979	2983	2985	rBV	616	444	0.03%	0.003%
52	11.057	3016	3022	3027	rBV2	450	537	0.03%	0.004%
53	11.080	3027	3029	3035	rVV	332	314	0.02%	0.002%
54	11.121	3039	3042	3046	rVV2	353	300	0.02%	0.002%
55	11.330	3099	3107	3113	rBV2	458	702	0.04%	0.005%
56	11.388	3122	3125	3130	rVB2	587	456	0.03%	0.003%
57	11.453	3139	3145	3149	rBV2	401	348	0.02%	0.003%
58	11.572	3179	3182	3186	rBV2	520	477	0.03%	0.004%
59	11.809	3243	3256	3275	rBV	538036	854356	48.43%	6.502%
60	12.009	3315	3318	3322	rBV3	651	433	0.02%	0.003%
61	12.054	3330	3332	3336	rVB	572	340	0.02%	0.003%
62	12.137	3355	3358	3362	rVB2	580	509	0.03%	0.004%
63	12.192	3362	3375	3396	rBV	594889	982602	55.70%	7.478%
64	12.440	3447	3452	3454	rBV	432	323	0.02%	0.002%
65	12.549	3482	3486	3488	rBV2	751	598	0.03%	0.005%
66	12.600	3497	3502	3508	rBV3	629	879	0.05%	0.007%
67	12.633	3509	3512	3517	rVB3	682	498	0.03%	0.004%
68	12.842	3574	3577	3582	rVB2	429	341	0.02%	0.003%
69	12.890	3587	3592	3596	rVB3	914	903	0.05%	0.007%
70	12.925	3599	3603	3606	rBV2	478	384	0.02%	0.003%
71	12.996	3620	3625	3630	rBV3	586	791	0.04%	0.006%
72	13.076	3648	3650	3654	rVB3	549	297	0.02%	0.002%
73	13.105	3654	3659	3664	rVB3	534	454	0.03%	0.003%
74	13.141	3664	3670	3672	rBV3	403	434	0.02%	0.003%
75	13.305	3718	3721	3726	rVB2	350	318	0.02%	0.002%
76	13.343	3730	3733	3738	rVB3	555	524	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051039.D
 Acq On : 30 Sep 2022 17:21
 Operator : JC/MD
 Sample : N4854-17 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	13.469	3769	3772	3776	rVV3	491	464	0.03%	0.004%
78	13.520	3785	3788	3791	rVB	783	514	0.03%	0.004%
79	13.552	3795	3798	3809	rVV3	545	757	0.04%	0.006%
80	13.739	3852	3856	3858	rVB	443	301	0.02%	0.002%
81	13.858	3891	3893	3897	rVB2	499	312	0.02%	0.002%
82	13.890	3897	3903	3906	rVB3	623	702	0.04%	0.005%
83	13.909	3906	3909	3914	rBV3	310	307	0.02%	0.002%
84	13.970	3924	3928	3929	rBV	658	424	0.02%	0.003%
85	14.076	3958	3961	3964	rBV2	475	355	0.02%	0.003%
86	14.411	4062	4065	4067	rBV	553	376	0.02%	0.003%
87	14.478	4083	4086	4088	rBV2	623	417	0.02%	0.003%
88	14.562	4110	4112	4115	rVB4	760	337	0.02%	0.003%
89	14.581	4115	4118	4119	rBV2	531	320	0.02%	0.002%
90	14.620	4126	4130	4132	rBV2	444	375	0.02%	0.003%
91	14.999	4246	4248	4252	rVB2	576	362	0.02%	0.003%
92	15.147	4292	4294	4299	rVB3	639	371	0.02%	0.003%
93	15.218	4313	4316	4319	rBV2	531	472	0.03%	0.004%
94	15.279	4331	4335	4339	rBV3	844	809	0.05%	0.006%
95	15.353	4355	4358	4360	rBV	653	345	0.02%	0.003%
96	15.395	4368	4371	4374	rBV3	870	624	0.04%	0.005%
97	15.677	4456	4459	4462	rBV3	1085	853	0.05%	0.006%
98	15.748	4478	4481	4486	rBV4	770	799	0.05%	0.006%
99	15.777	4486	4490	4492	rBV4	1014	765	0.04%	0.006%
100	16.131	4596	4600	4601	rBV2	892	656	0.04%	0.005%




Sum of corrected areas: 13140459

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051039.D
Acq On : 30 Sep 2022 17:21
Operator : JC/MD
Sample : N4854-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

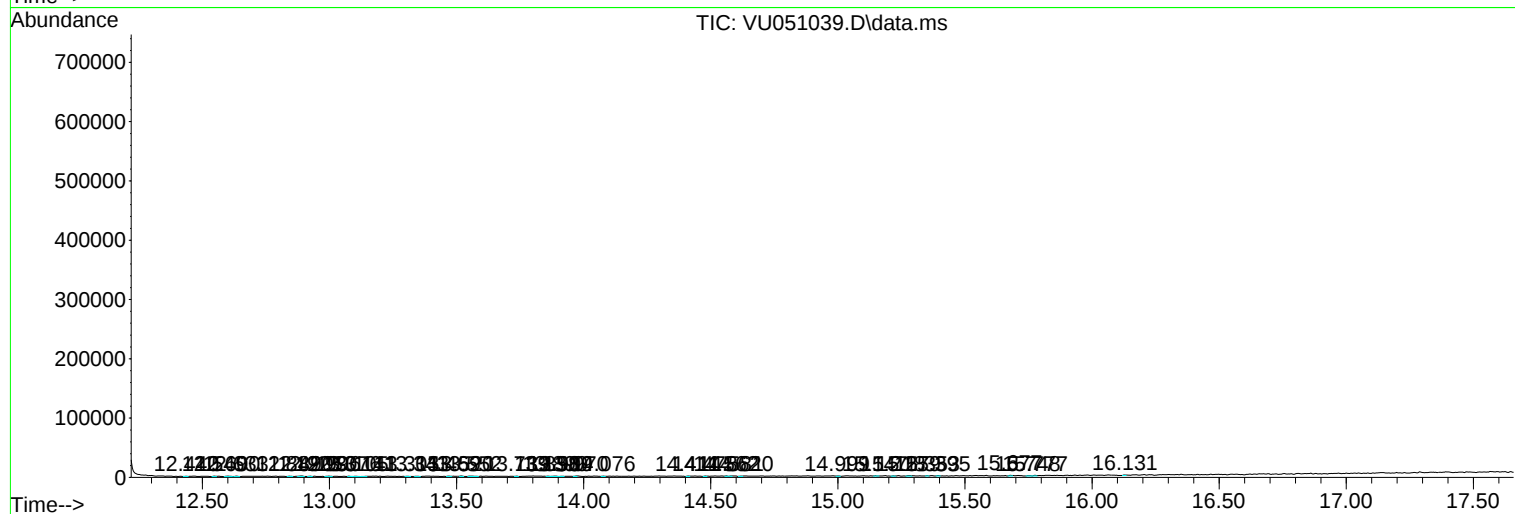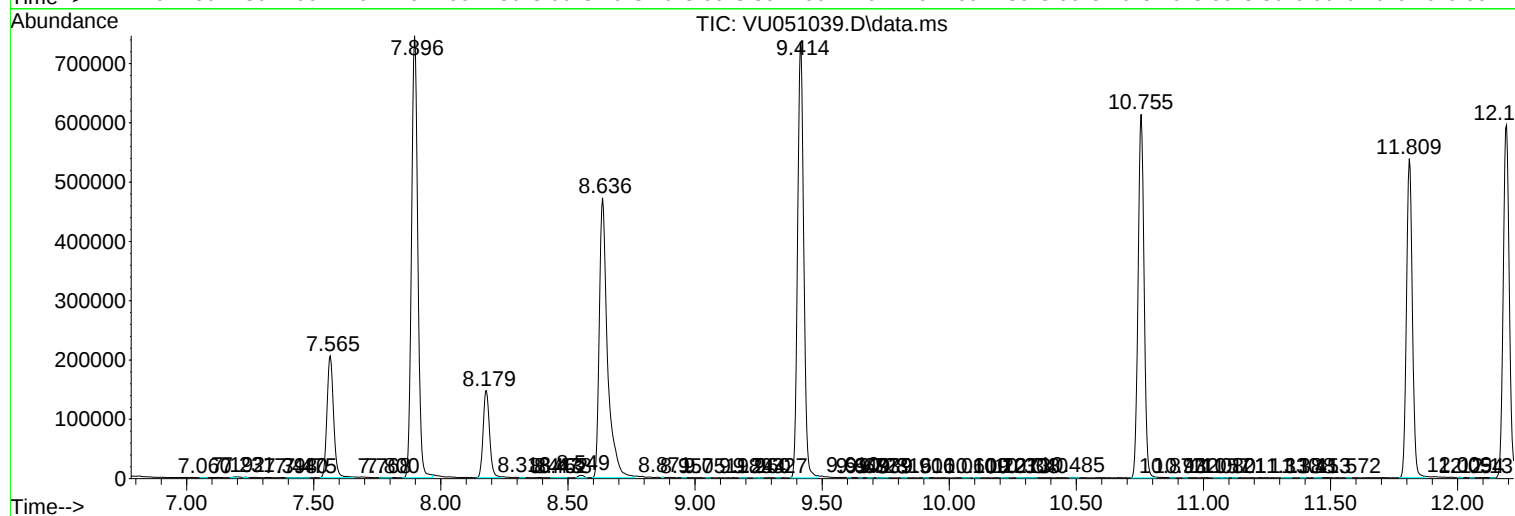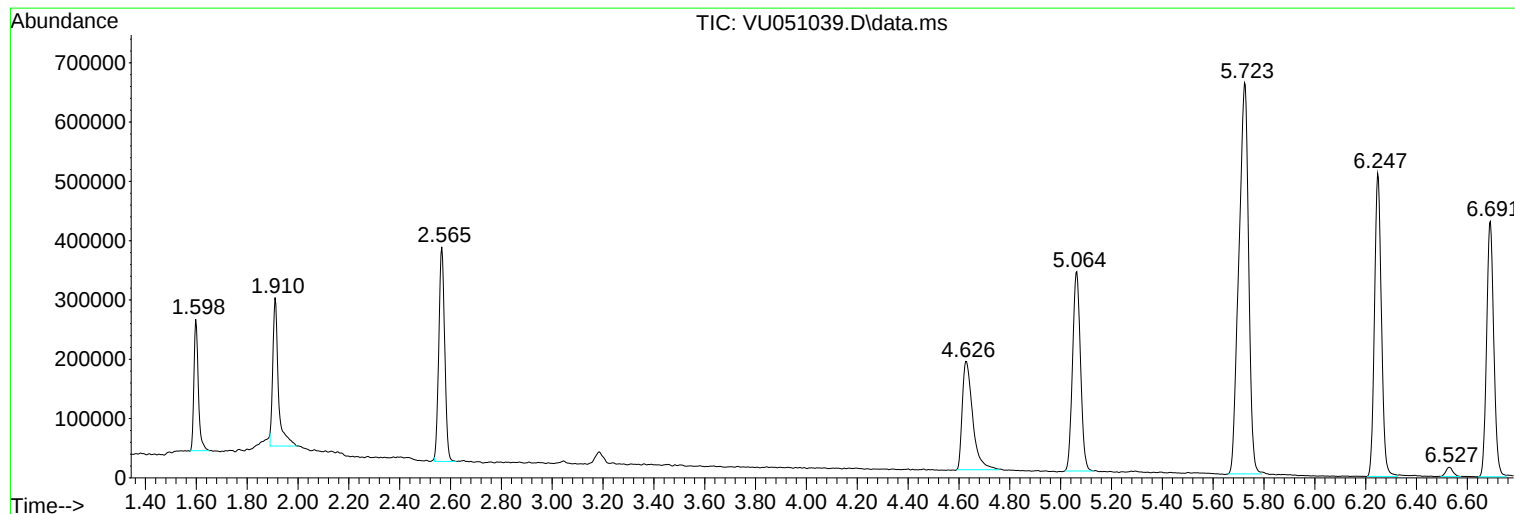

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051039.D
Acq On : 30 Sep 2022 17:21
Operator : JC/MD
Sample : N4854-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051039.D
Acq On : 30 Sep 2022 17:21
Operator : JC/MD
Sample : N4854-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc