

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051040.D
 Acq On : 30 Sep 2022 17:44
 Operator : JC/MD
 Sample : N4854-21 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	208696	250712	14.39%	1.936%
2	1.900	165	174	197	rVB	182015	254389	14.60%	1.964%
3	2.562	368	380	399	rBV	334877	541909	31.11%	4.184%
4	2.748	435	438	443	rBV2	566	601	0.03%	0.005%
5	3.041	517	529	544	rVB2	8004	15337	0.88%	0.118%
6	3.131	553	557	559	rVV2	524	446	0.03%	0.003%
7	3.182	559	573	600	rVB	22358	53826	3.09%	0.416%
8	3.305	607	611	614	rVB	527	380	0.02%	0.003%
9	3.440	648	653	655	rBV2	492	480	0.03%	0.004%
10	3.555	685	689	692	rBV	382	338	0.02%	0.003%
11	3.690	727	731	734	rBV3	430	322	0.02%	0.002%
12	3.726	738	742	745	rBV	336	327	0.02%	0.003%
13	3.771	753	756	758	rBV	513	343	0.02%	0.003%
14	3.957	812	814	821	rVB2	513	407	0.02%	0.003%
15	4.028	833	836	841	rBV3	439	354	0.02%	0.003%
16	4.256	901	907	909	rBV	323	367	0.02%	0.003%
17	4.414	953	956	959	rVV2	463	351	0.02%	0.003%
18	4.575	1002	1006	1007	rBV2	532	321	0.02%	0.002%
19	4.616	1007	1019	1051	rBV	190308	492167	28.25%	3.800%
20	4.993	1131	1136	1138	rBV4	418	373	0.02%	0.003%
21	5.060	1141	1157	1181	rVV	326072	710796	40.80%	5.488%
22	5.285	1224	1227	1229	rBV3	682	482	0.03%	0.004%
23	5.350	1241	1247	1249	rBV2	567	568	0.03%	0.004%
24	5.372	1251	1254	1263	rVV3	732	1124	0.06%	0.009%
25	5.449	1273	1278	1282	rVB3	333	342	0.02%	0.003%
26	5.636	1332	1336	1341	rVB	444	426	0.02%	0.003%
27	5.723	1341	1363	1388	rBV2	638927	1742122	100.00%	13.450%
28	5.999	1446	1449	1455	rVB3	351	378	0.02%	0.003%
29	6.044	1457	1463	1469	rVV4	497	803	0.05%	0.006%
30	6.247	1511	1526	1554	rBV	502131	955815	54.86%	7.379%
31	6.526	1603	1613	1628	rVB3	15291	30485	1.75%	0.235%
32	6.687	1648	1663	1682	rBV	421271	819427	47.04%	6.326%
33	6.912	1729	1733	1742	rVB3	489	683	0.04%	0.005%
34	6.957	1742	1747	1749	rBV	554	410	0.02%	0.003%
35	7.015	1758	1765	1771	rVB2	515	608	0.03%	0.005%
36	7.182	1807	1817	1830	rBV7	1127	2456	0.14%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051040.D
 Acq On : 30 Sep 2022 17:44
 Operator : JC/MD
 Sample : N4854-21 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.253	1835	1839	1845	rBV2	405	344	0.02%	0.003%
38	7.565	1923	1936	1954	rBV2	196384	348741	20.02%	2.692%
39	7.748	1991	1993	1996	rVB2	790	450	0.03%	0.003%
40	7.796	2002	2008	2011	rBV4	748	695	0.04%	0.005%
41	7.848	2020	2024	2025	rBV2	567	328	0.02%	0.003%
42	7.896	2025	2039	2057	rBV	712464	1220701	70.07%	9.425%
43	8.083	2094	2097	2105	rBV2	383	374	0.02%	0.003%
44	8.179	2115	2127	2148	rBV	144673	246963	14.18%	1.907%
45	8.311	2164	2168	2172	rBV4	444	376	0.02%	0.003%
46	8.407	2193	2198	2201	rBV	930	608	0.03%	0.005%
47	8.488	2218	2223	2228	rBV3	531	576	0.03%	0.004%
48	8.552	2232	2243	2252	rBV3	9232	15124	0.87%	0.117%
49	8.632	2252	2268	2305	rBV4	478822	1054888	60.55%	8.144%
50	8.899	2347	2351	2355	rVB3	561	452	0.03%	0.003%
51	8.941	2360	2364	2367	rVB	539	454	0.03%	0.004%
52	8.992	2376	2380	2384	rBV4	548	560	0.03%	0.004%
53	9.041	2391	2395	2399	rBV3	487	349	0.02%	0.003%
54	9.082	2404	2408	2414	rBV3	455	481	0.03%	0.004%
55	9.176	2433	2437	2440	rBV2	685	575	0.03%	0.004%
56	9.272	2464	2467	2473	rBV2	381	389	0.02%	0.003%
57	9.304	2473	2477	2480	rBV2	427	320	0.02%	0.002%
58	9.356	2490	2493	2497	rBV2	491	394	0.02%	0.003%
59	9.417	2497	2512	2533	rBV	734113	1211450	69.54%	9.353%
60	9.581	2561	2563	2574	rVB4	1108	1232	0.07%	0.010%
61	9.629	2574	2578	2580	rBV2	443	337	0.02%	0.003%
62	9.655	2582	2586	2591	rBV	1027	1034	0.06%	0.008%
63	9.774	2620	2623	2631	rVB	374	484	0.03%	0.004%
64	9.822	2631	2638	2640	rBV2	462	532	0.03%	0.004%
65	9.848	2643	2646	2650	rBV2	540	343	0.02%	0.003%
66	10.066	2710	2714	2717	rVB2	452	338	0.02%	0.003%
67	10.140	2735	2737	2743	rVB2	440	399	0.02%	0.003%
68	10.192	2750	2753	2759	rVB	602	591	0.03%	0.005%
69	10.664	2896	2900	2905	rBV3	344	350	0.02%	0.003%
70	10.754	2914	2928	2951	rBV	622462	997461	57.26%	7.701%
71	10.886	2964	2969	2974	rBV2	640	865	0.05%	0.007%
72	10.992	2999	3002	3006	rBV2	521	477	0.03%	0.004%
73	11.124	3039	3043	3047	rBV2	554	486	0.03%	0.004%
74	11.311	3099	3101	3111	rVB2	329	347	0.02%	0.003%
75	11.401	3124	3129	3132	rVB2	358	321	0.02%	0.002%
76	11.423	3132	3136	3139	rBV3	759	673	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051040.D
 Acq On : 30 Sep 2022 17:44
 Operator : JC/MD
 Sample : N4854-21 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.526	3163	3168	3172	rVB	688	577	0.03%	0.004%
78	11.680	3211	3216	3219	rBV2	369	374	0.02%	0.003%
79	11.809	3243	3256	3272	rBV	568205	908715	52.16%	7.016%
80	12.008	3315	3318	3323	rBV3	574	550	0.03%	0.004%
81	12.063	3333	3335	3339	rVB3	514	346	0.02%	0.003%
82	12.192	3362	3375	3401	rBV	638217	1039258	59.65%	8.024%
83	12.629	3508	3511	3516	rVB2	399	389	0.02%	0.003%
84	12.703	3530	3534	3535	rBV2	629	431	0.02%	0.003%
85	12.902	3591	3596	3598	rBV3	392	385	0.02%	0.003%
86	13.044	3636	3640	3644	rVV3	543	504	0.03%	0.004%
87	13.182	3678	3683	3685	rBV2	653	545	0.03%	0.004%
88	13.256	3703	3706	3709	rVB2	602	363	0.02%	0.003%
89	13.275	3709	3712	3716	rBV3	452	346	0.02%	0.003%
90	13.610	3809	3816	3819	rBV2	578	653	0.04%	0.005%
91	13.873	3895	3898	3904	rBV	542	604	0.03%	0.005%
92	14.211	3999	4003	4008	rVB	479	458	0.03%	0.004%
93	14.796	4180	4185	4187	rBV3	667	718	0.04%	0.006%
94	14.976	4237	4241	4246	rBV2	730	812	0.05%	0.006%
95	15.037	4256	4260	4266	rBV3	875	899	0.05%	0.007%
96	15.089	4272	4276	4279	rBV4	700	851	0.05%	0.007%
97	15.208	4311	4313	4317	rVB2	837	420	0.02%	0.003%
98	15.401	4369	4373	4375	rBV4	682	573	0.03%	0.004%
99	15.420	4377	4379	4381	rVV	691	349	0.02%	0.003%
100	15.703	4465	4467	4473	rVB4	941	761	0.04%	0.006%




Sum of corrected areas: 12952418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051040.D
Acq On : 30 Sep 2022 17:44
Operator : JC/MD
Sample : N4854-21 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

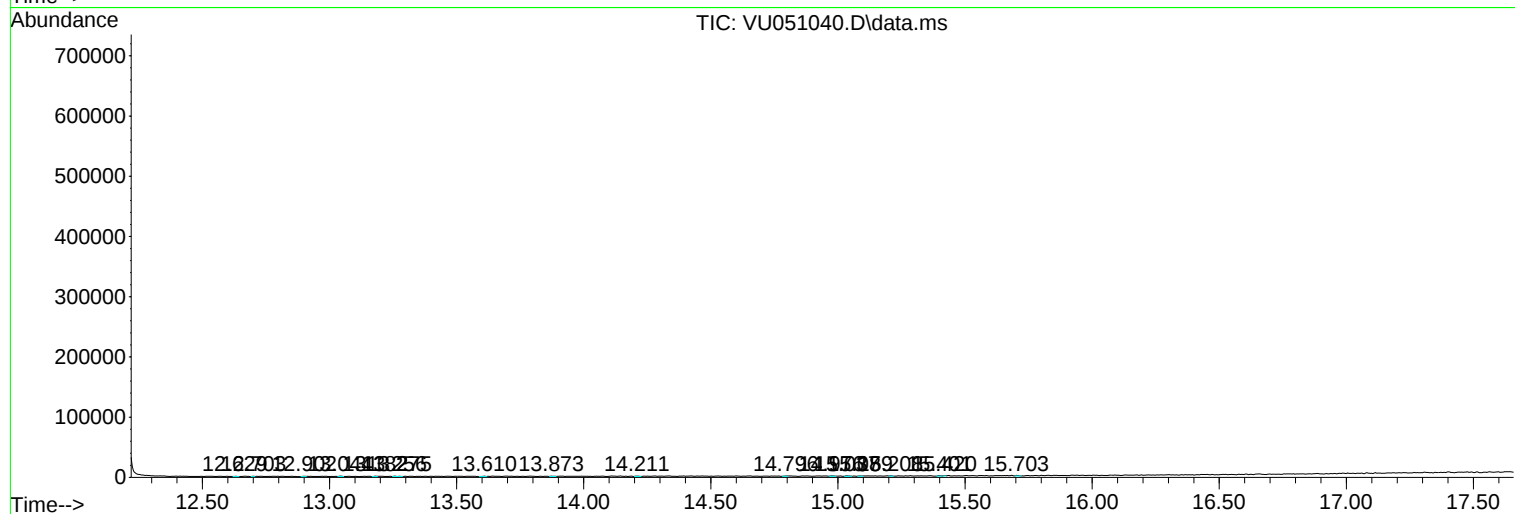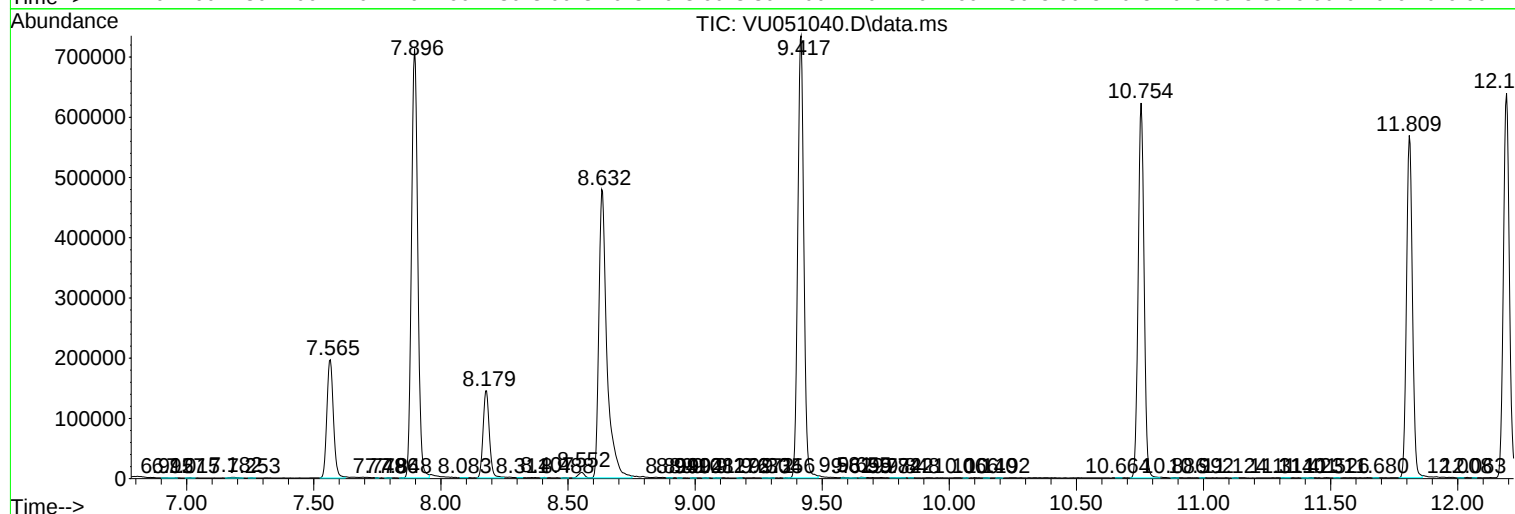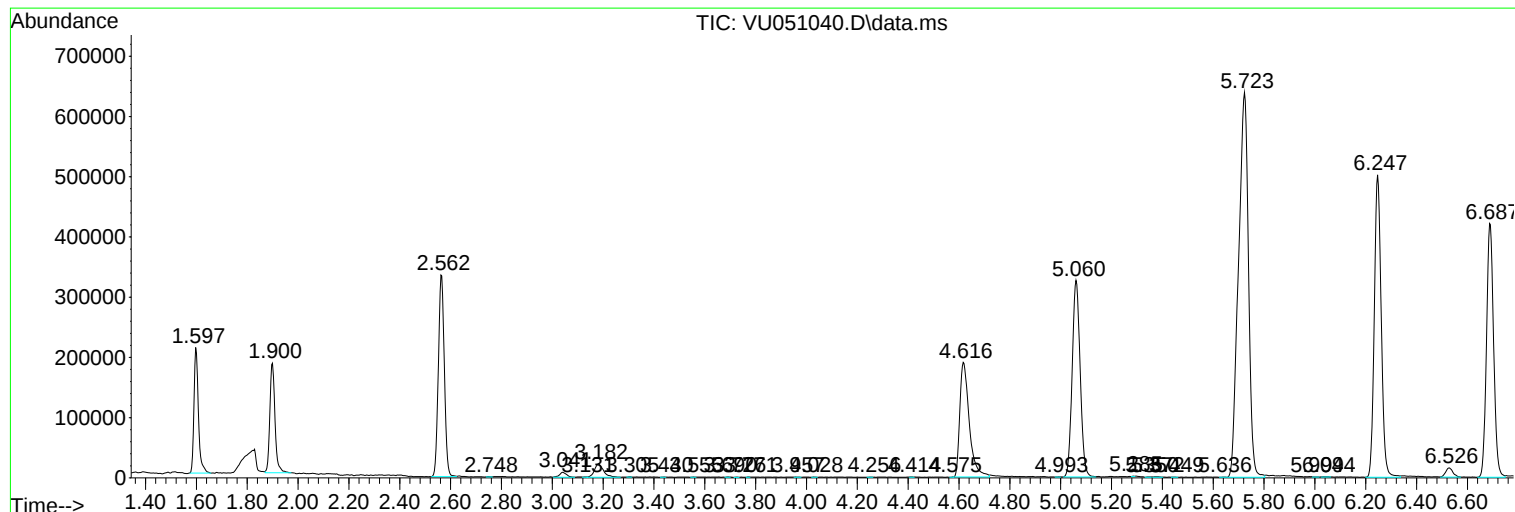

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051040.D
Acq On : 30 Sep 2022 17:44
Operator : JC/MD
Sample : N4854-21 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051040.D
Acq On : 30 Sep 2022 17:44
Operator : JC/MD
Sample : N4854-21 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------