

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051045.D
 Acq On : 30 Sep 2022 19:40
 Operator : JC/MD
 Sample : N4859-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	97	rVB	193974	226880	13.11%	1.780%
2	1.903	168	175	192	rVB	175965	232007	13.41%	1.820%
3	2.565	369	381	394	rBV	321666	517216	29.89%	4.058%
4	2.729	430	432	434	rBV	307	135	0.01%	0.001%
5	2.999	514	516	517	rBV	465	207	0.01%	0.002%
6	3.141	558	560	561	rBV	170	76	0.00%	0.001%
7	3.189	562	575	586	rVV7	2554	6269	0.36%	0.049%
8	3.298	602	609	611	rBV2	640	634	0.04%	0.005%
9	3.385	634	636	638	rBV	159	53	0.00%	0.000%
10	3.401	638	641	644	rBV2	341	241	0.01%	0.002%
11	3.440	650	653	656	rBV	279	152	0.01%	0.001%
12	3.523	674	679	681	rBV3	295	245	0.01%	0.002%
13	3.588	697	699	702	rBV	270	108	0.01%	0.001%
14	3.646	714	717	720	rBV2	283	209	0.01%	0.002%
15	3.668	720	724	732	rBV2	732	1119	0.06%	0.009%
16	3.871	784	787	792	rBV	468	456	0.03%	0.004%
17	3.983	820	822	825	rBV2	313	184	0.01%	0.001%
18	4.115	859	863	865	rBV2	364	288	0.02%	0.002%
19	4.343	931	934	937	rBV	303	268	0.02%	0.002%
20	4.391	943	949	953	rVB2	481	478	0.03%	0.004%
21	4.411	953	955	960	rBV2	221	190	0.01%	0.001%
22	4.453	964	968	970	rBV2	297	186	0.01%	0.001%
23	4.620	1007	1020	1058	rBV	200584	508290	29.37%	3.988%
24	5.060	1141	1157	1184	rBV	314150	699285	40.41%	5.487%
25	5.404	1262	1264	1269	rVB	333	217	0.01%	0.002%
26	5.526	1292	1302	1316	rVB3	19914	42987	2.48%	0.337%
27	5.578	1316	1318	1320	rBV	301	183	0.01%	0.001%
28	5.623	1328	1332	1334	rBV2	404	222	0.01%	0.002%
29	5.723	1342	1363	1387	rBV2	635503	1730511	100.00%	13.578%
30	6.089	1473	1477	1481	rBV	385	331	0.02%	0.003%
31	6.108	1481	1483	1485	rBV2	565	363	0.02%	0.003%
32	6.147	1492	1495	1497	rBV2	280	159	0.01%	0.001%
33	6.247	1512	1526	1552	rBV	504835	958934	55.41%	7.524%
34	6.533	1603	1615	1628	rBV6	23559	52689	3.04%	0.413%
35	6.636	1643	1647	1649	rBV2	394	324	0.02%	0.003%
36	6.690	1649	1664	1682	rBV	415306	808721	46.73%	6.346%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051045.D
 Acq On : 30 Sep 2022 19:40
 Operator : JC/MD
 Sample : N4859-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.954	1744	1746	1749	rVB2	309	149	0.01%	0.001%
38	7.031	1767	1770	1771	rBV	219	97	0.01%	0.001%
39	7.044	1772	1774	1776	rVV	384	169	0.01%	0.001%
40	7.067	1779	1781	1784	rVB	425	181	0.01%	0.001%
41	7.141	1802	1804	1807	rVB	334	181	0.01%	0.001%
42	7.186	1807	1818	1825	rBV7	1794	3536	0.20%	0.028%
43	7.298	1850	1853	1855	rBV2	303	212	0.01%	0.002%
44	7.327	1860	1862	1865	rBV2	289	108	0.01%	0.001%
45	7.350	1865	1869	1872	rBV	279	305	0.02%	0.002%
46	7.433	1891	1895	1898	rBV2	207	165	0.01%	0.001%
47	7.481	1907	1910	1911	rBV	198	102	0.01%	0.001%
48	7.494	1911	1914	1918	rVB2	456	325	0.02%	0.003%
49	7.565	1922	1936	1957	rBV	206542	368697	21.31%	2.893%
50	7.829	2015	2018	2021	rBV2	375	293	0.02%	0.002%
51	7.896	2025	2039	2058	rBV	722498	1227201	70.92%	9.629%
52	8.179	2114	2127	2147	rBV	145540	248369	14.35%	1.949%
53	8.468	2214	2217	2222	rVB2	764	633	0.04%	0.005%
54	8.555	2238	2244	2252	rVB6	1864	2445	0.14%	0.019%
55	8.632	2255	2268	2307	rBV3	496026	1062166	61.38%	8.334%
56	8.944	2363	2365	2367	rBV2	336	188	0.01%	0.001%
57	9.002	2380	2383	2385	rBV	291	212	0.01%	0.002%
58	9.150	2426	2429	2430	rBV	218	129	0.01%	0.001%
59	9.266	2460	2465	2470	rBV2	575	743	0.04%	0.006%
60	9.292	2470	2473	2477	rVV2	288	247	0.01%	0.002%
61	9.359	2492	2494	2496	rBV	89	40	0.00%	0.000%
62	9.417	2498	2512	2531	rBV	706306	1171001	67.67%	9.188%
63	9.655	2584	2586	2587	rBV	235	86	0.00%	0.001%
64	9.854	2645	2648	2651	rBV2	417	251	0.01%	0.002%
65	9.948	2672	2677	2681	rBV2	446	398	0.02%	0.003%
66	9.980	2685	2687	2692	rBV	329	229	0.01%	0.002%
67	10.099	2719	2724	2725	rBV2	552	413	0.02%	0.003%
68	10.337	2796	2798	2799	rBV2	246	115	0.01%	0.001%
69	10.530	2856	2858	2861	rBV	234	126	0.01%	0.001%
70	10.568	2864	2870	2873	rBV2	357	403	0.02%	0.003%
71	10.648	2892	2895	2899	rVB2	425	279	0.02%	0.002%
72	10.671	2899	2902	2904	rBV	333	243	0.01%	0.002%
73	10.755	2915	2928	2954	rBV	603253	969403	56.02%	7.606%
74	11.073	3024	3027	3030	rBV	589	383	0.02%	0.003%
75	11.092	3030	3033	3037	rBV3	303	262	0.02%	0.002%
76	11.337	3107	3109	3113	rVB2	386	252	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051045.D
 Acq On : 30 Sep 2022 19:40
 Operator : JC/MD
 Sample : N4859-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

77	11.809	3243	3256	3283	rBV	551021	877019	50.68%	6.882%
78	12.192	3362	3375	3393	rBV	618434	1014180	58.61%	7.958%
79	12.909	3594	3598	3599	rBV2	495	384	0.02%	0.003%
80	12.960	3611	3614	3618	rBV3	517	465	0.03%	0.004%
81	13.034	3634	3637	3638	rBV2	980	527	0.03%	0.004%
82	13.153	3671	3674	3676	rBV2	638	369	0.02%	0.003%




Sum of corrected areas: 12744498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051045.D
Acq On : 30 Sep 2022 19:40
Operator : JC/MD
Sample : N4859-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10053

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

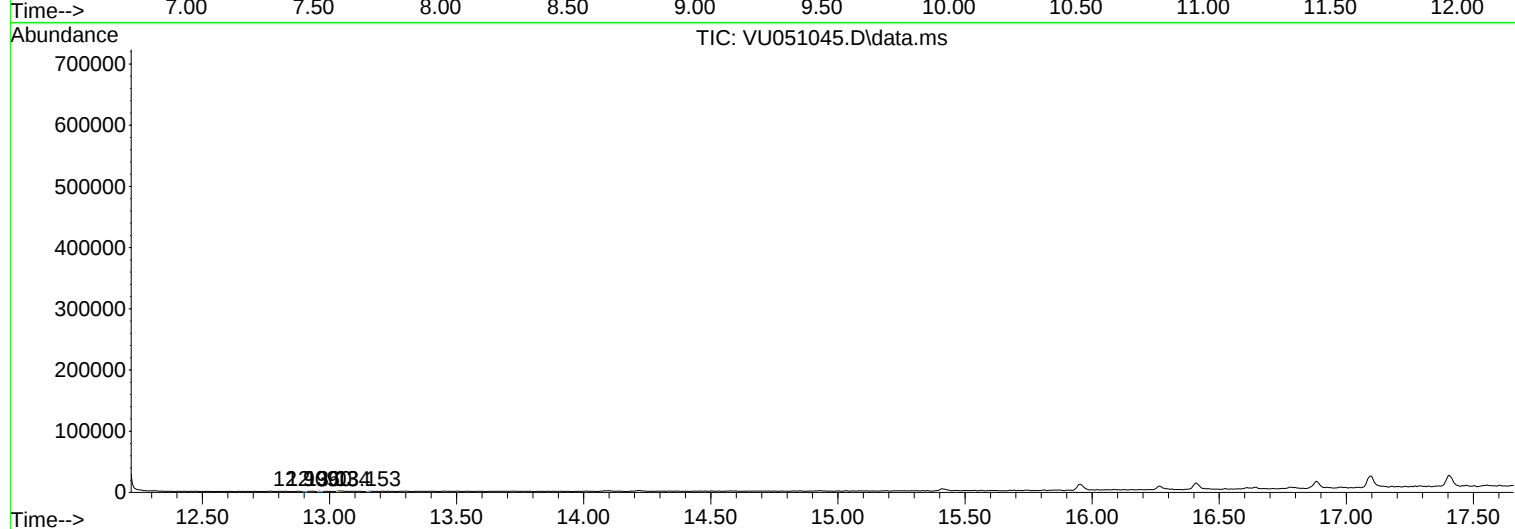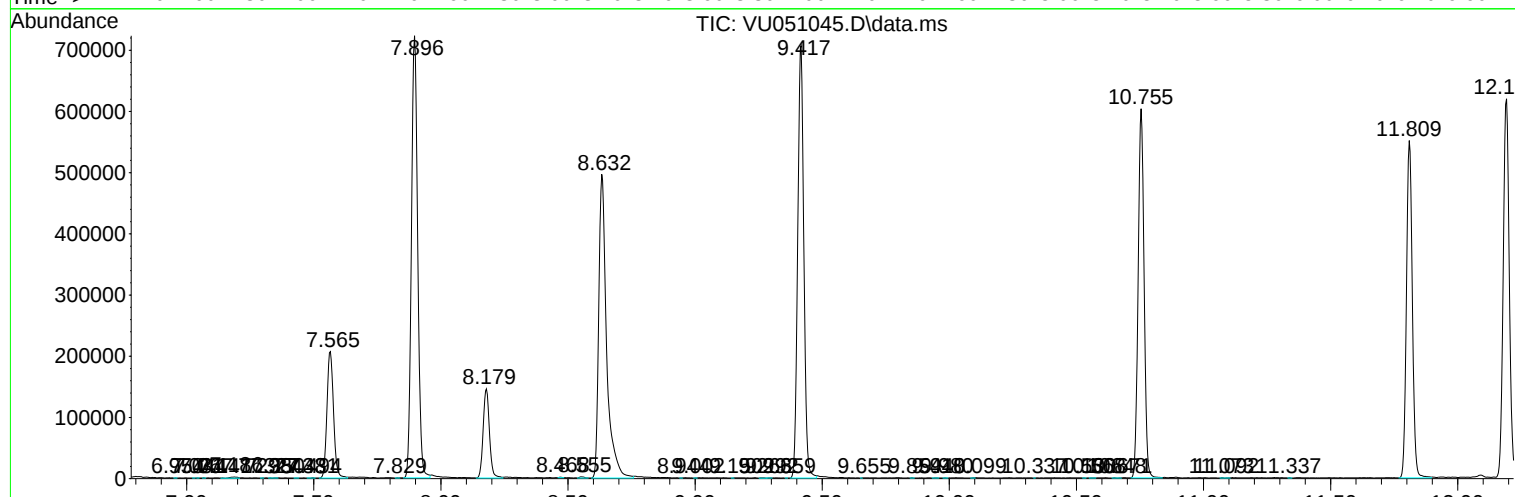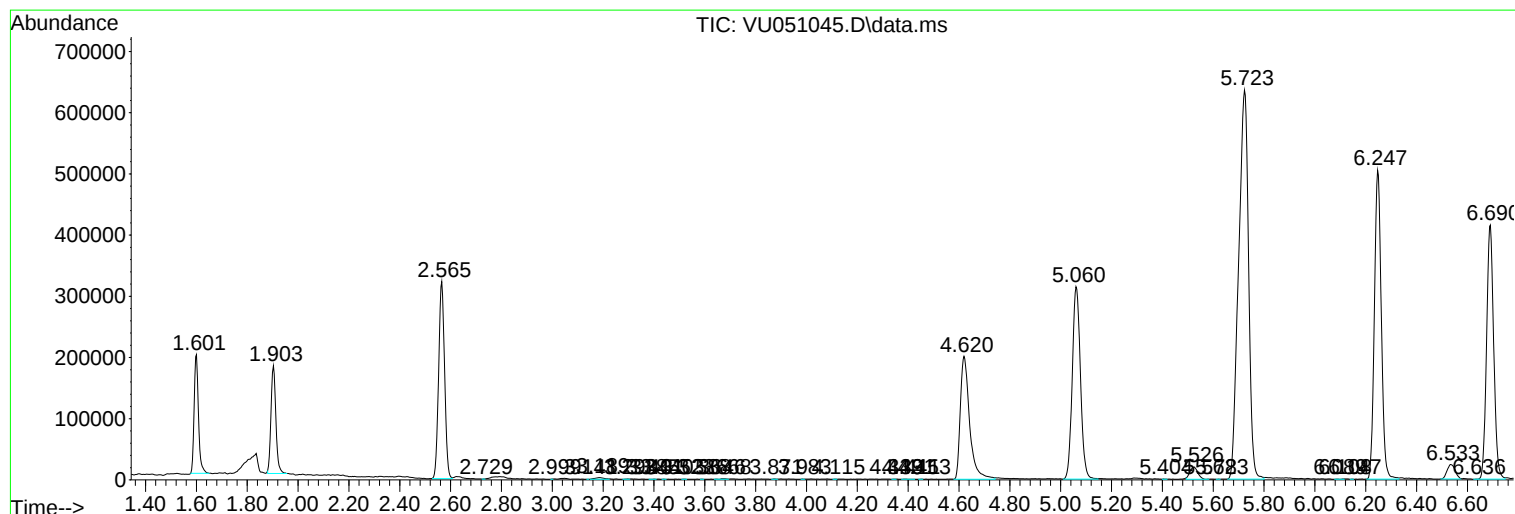

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051045.D
Acq On : 30 Sep 2022 19:40
Operator : JC/MD
Sample : N4859-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10053

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051045.D
Acq On : 30 Sep 2022 19:40
Operator : JC/MD
Sample : N4859-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10053

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc