

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051046.D
 Acq On : 30 Sep 2022 20:04
 Operator : JC/MD
 Sample : N4859-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	41	46	52	rBV2	7151	7461	0.44%	0.058%
2	1.597	72	80	98	rBV	191434	236485	13.83%	1.823%
3	1.900	166	174	191	rVB	174426	238446	13.95%	1.838%
4	2.501	355	361	364	rBV3	652	778	0.05%	0.006%
5	2.565	368	381	393	rVV	315060	508887	29.76%	3.923%
6	2.626	394	400	413	rVB2	10835	18783	1.10%	0.145%
7	2.719	424	429	431	rBV4	446	433	0.03%	0.003%
8	2.771	433	445	447	rBV5	2730	3973	0.23%	0.031%
9	2.893	480	483	486	rBV3	444	419	0.02%	0.003%
10	2.948	494	500	501	rBV5	616	572	0.03%	0.004%
11	3.044	522	530	536	rVB5	1336	2161	0.13%	0.017%
12	3.125	553	555	559	rVB3	529	368	0.02%	0.003%
13	3.186	559	574	579	rBV6	3464	7224	0.42%	0.056%
14	3.337	611	621	624	rBV2	526	924	0.05%	0.007%
15	3.501	667	672	676	rBV2	305	348	0.02%	0.003%
16	3.584	692	698	702	rBV3	432	553	0.03%	0.004%
17	3.658	713	721	726	rBV2	316	460	0.03%	0.004%
18	3.819	767	771	776	rVB2	402	329	0.02%	0.003%
19	3.887	783	792	800	rVB2	349	708	0.04%	0.005%
20	3.925	800	804	808	rVB2	489	329	0.02%	0.003%
21	4.018	831	833	838	rBV3	424	345	0.02%	0.003%
22	4.073	846	850	856	rBV	456	407	0.02%	0.003%
23	4.208	888	892	902	rVB3	520	832	0.05%	0.006%
24	4.253	902	906	914	rBV2	540	700	0.04%	0.005%
25	4.446	960	966	971	rVB4	781	849	0.05%	0.007%
26	4.617	1007	1019	1053	rBV	188553	488837	28.59%	3.768%
27	4.854	1091	1093	1097	rVB3	628	377	0.02%	0.003%
28	5.063	1141	1158	1184	rVV2	338422	890668	52.09%	6.866%
29	5.179	1191	1194	1196	rBV2	602	447	0.03%	0.003%
30	5.379	1250	1256	1262	rBV4	756	922	0.05%	0.007%
31	5.491	1288	1291	1294	rVB2	485	322	0.02%	0.002%
32	5.610	1325	1328	1332	rBV2	345	322	0.02%	0.002%
33	5.723	1340	1363	1386	rBV2	631964	1709781	100.00%	13.180%
34	5.967	1437	1439	1446	rVB6	1054	947	0.06%	0.007%
35	6.150	1493	1496	1501	rBV4	652	512	0.03%	0.004%
36	6.247	1512	1526	1545	rBV	500586	951276	55.64%	7.333%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051046.D
 Acq On : 30 Sep 2022 20:04
 Operator : JC/MD
 Sample : N4859-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.375	1563	1566	1567	rBV2	602	345	0.02%	0.003%
38	6.526	1602	1613	1627	rBV2	17154	32359	1.89%	0.249%
39	6.687	1648	1663	1683	rBV	414858	802171	46.92%	6.184%
40	6.877	1720	1722	1726	rVB2	942	488	0.03%	0.004%
41	6.912	1726	1733	1739	rVB2	623	693	0.04%	0.005%
42	7.108	1782	1794	1804	rBV2	10880	18921	1.11%	0.146%
43	7.182	1809	1817	1829	rBV6	1828	3572	0.21%	0.028%
44	7.488	1907	1912	1914	rBV2	459	402	0.02%	0.003%
45	7.565	1923	1936	1950	rBV	203223	357871	20.93%	2.759%
46	7.790	1996	2006	2022	rVB3	5623	11401	0.67%	0.088%
47	7.896	2022	2039	2058	rBV	716632	1226417	71.73%	9.454%
48	8.176	2114	2126	2145	rBV	142866	245034	14.33%	1.889%
49	8.327	2170	2173	2180	rVB6	458	450	0.03%	0.003%
50	8.555	2238	2244	2250	rBV6	1037	1411	0.08%	0.011%
51	8.632	2256	2268	2299	rBV3	495051	1045992	61.18%	8.063%
52	8.890	2345	2348	2351	rVV3	516	405	0.02%	0.003%
53	8.941	2361	2364	2366	rBV	796	450	0.03%	0.003%
54	9.057	2397	2400	2403	rVB2	485	351	0.02%	0.003%
55	9.118	2415	2419	2421	rBV	470	362	0.02%	0.003%
56	9.173	2433	2436	2440	rBV2	482	431	0.03%	0.003%
57	9.414	2498	2511	2534	rBV	704120	1175257	68.74%	9.060%
58	9.568	2552	2559	2572	rVB	11011	17093	1.00%	0.132%
59	9.690	2587	2597	2611	rBV	23877	38778	2.27%	0.299%
60	9.787	2622	2627	2630	rBV	689	434	0.03%	0.003%
61	10.005	2689	2695	2697	rBV2	456	457	0.03%	0.004%
62	10.057	2705	2711	2714	rBV2	378	362	0.02%	0.003%
63	10.099	2714	2724	2739	rBV3	13410	23580	1.38%	0.182%
64	10.202	2754	2756	2759	rVB2	631	361	0.02%	0.003%
65	10.375	2806	2810	2815	rVB2	481	487	0.03%	0.004%
66	10.652	2893	2896	2901	rVB3	596	480	0.03%	0.004%
67	10.755	2914	2928	2948	rBV	596597	955298	55.87%	7.364%
68	11.124	3038	3043	3047	rVB2	612	605	0.04%	0.005%
69	11.478	3148	3153	3155	rBV2	720	726	0.04%	0.006%
70	11.742	3233	3235	3240	rVB3	618	456	0.03%	0.004%
71	11.809	3240	3256	3278	rBV	555970	892553	52.20%	6.880%
72	12.089	3335	3343	3351	rVB7	2295	4535	0.27%	0.035%
73	12.192	3362	3375	3397	rBV	620009	1012710	59.23%	7.807%
74	12.394	3435	3438	3440	rBV2	486	359	0.02%	0.003%
75	12.410	3441	3443	3446	rVB2	594	365	0.02%	0.003%
76	12.465	3455	3460	3462	rBV2	399	327	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051046.D
 Acq On : 30 Sep 2022 20:04
 Operator : JC/MD
 Sample : N4859-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.488	3463	3467	3470	rVV	456	388	0.02%	0.003%
78	12.681	3522	3527	3532	rVB3	594	721	0.04%	0.006%
79	12.706	3532	3535	3539	rBV3	498	498	0.03%	0.004%
80	12.780	3555	3558	3562	rBV2	559	451	0.03%	0.003%
81	12.902	3593	3596	3599	rBV3	521	402	0.02%	0.003%
82	12.976	3616	3619	3621	rBV	523	346	0.02%	0.003%
83	13.012	3626	3630	3636	rBV4	453	545	0.03%	0.004%
84	13.041	3636	3639	3641	rBV2	834	581	0.03%	0.004%
85	13.102	3654	3658	3661	rBV3	620	678	0.04%	0.005%
86	13.529	3787	3791	3792	rBV	603	367	0.02%	0.003%
87	13.561	3798	3801	3806	rBV3	558	551	0.03%	0.004%
88	13.799	3872	3875	3878	rBV2	384	344	0.02%	0.003%
89	13.896	3902	3905	3910	rBV2	608	436	0.03%	0.003%
90	13.986	3931	3933	3938	rVB2	667	535	0.03%	0.004%
91	14.021	3940	3944	3947	rBV2	522	429	0.03%	0.003%
92	14.098	3966	3968	3971	rVB2	849	327	0.02%	0.003%
93	14.208	3996	4002	4005	rBV3	886	1012	0.06%	0.008%
94	14.317	4034	4036	4041	rBV2	498	409	0.02%	0.003%
95	14.446	4073	4076	4081	rBV4	499	569	0.03%	0.004%
96	14.796	4183	4185	4189	rVB2	767	410	0.02%	0.003%
97	14.957	4233	4235	4237	rBV2	538	329	0.02%	0.003%
98	15.468	4391	4394	4396	rBV4	869	514	0.03%	0.004%
99	16.089	4584	4587	4589	rBV3	1537	963	0.06%	0.007%
100	16.410	4681	4687	4700	rVB8	4900	8474	0.50%	0.065%




Sum of corrected areas: 12972213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051046.D
Acq On : 30 Sep 2022 20:04
Operator : JC/MD
Sample : N4859-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

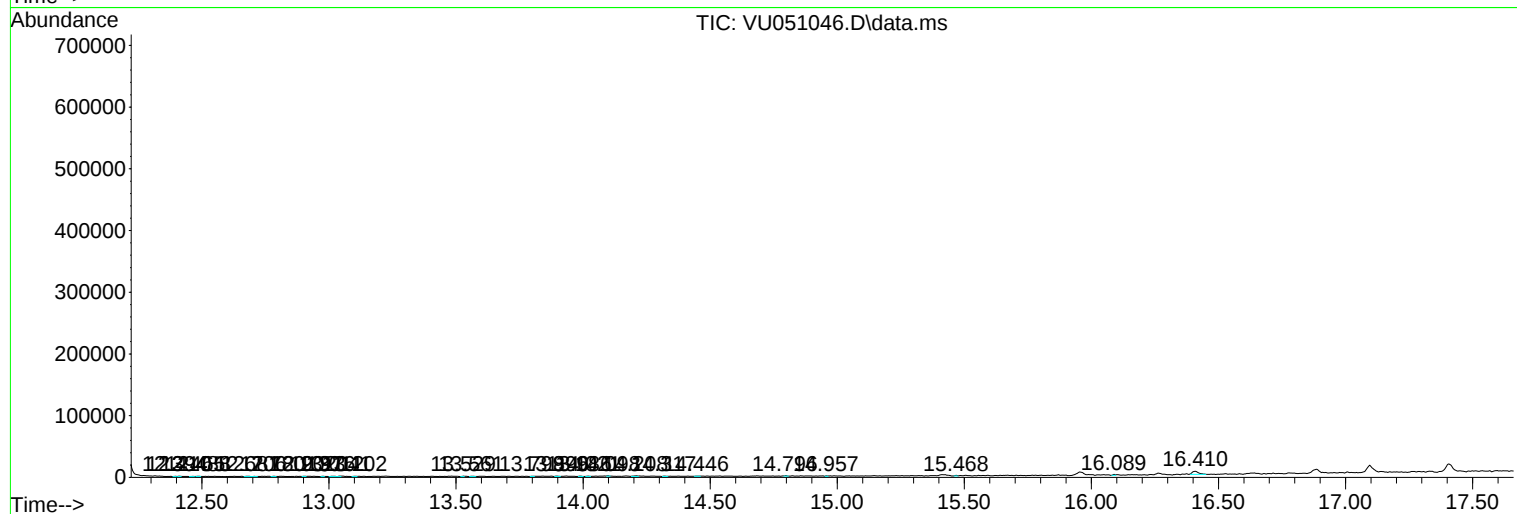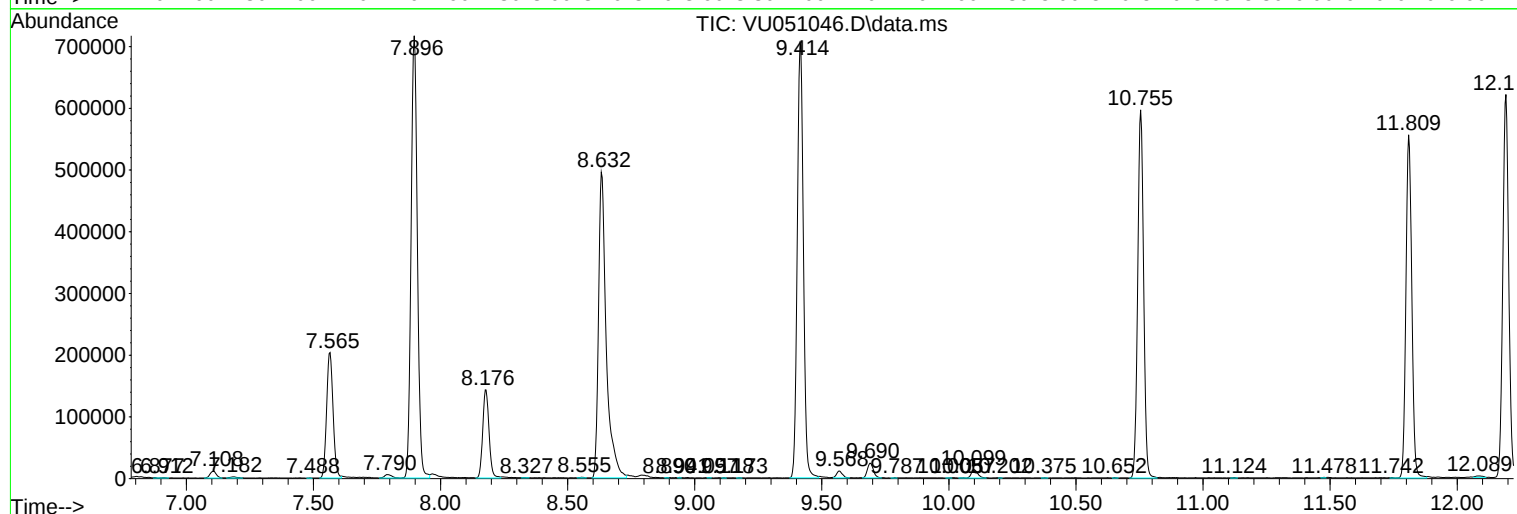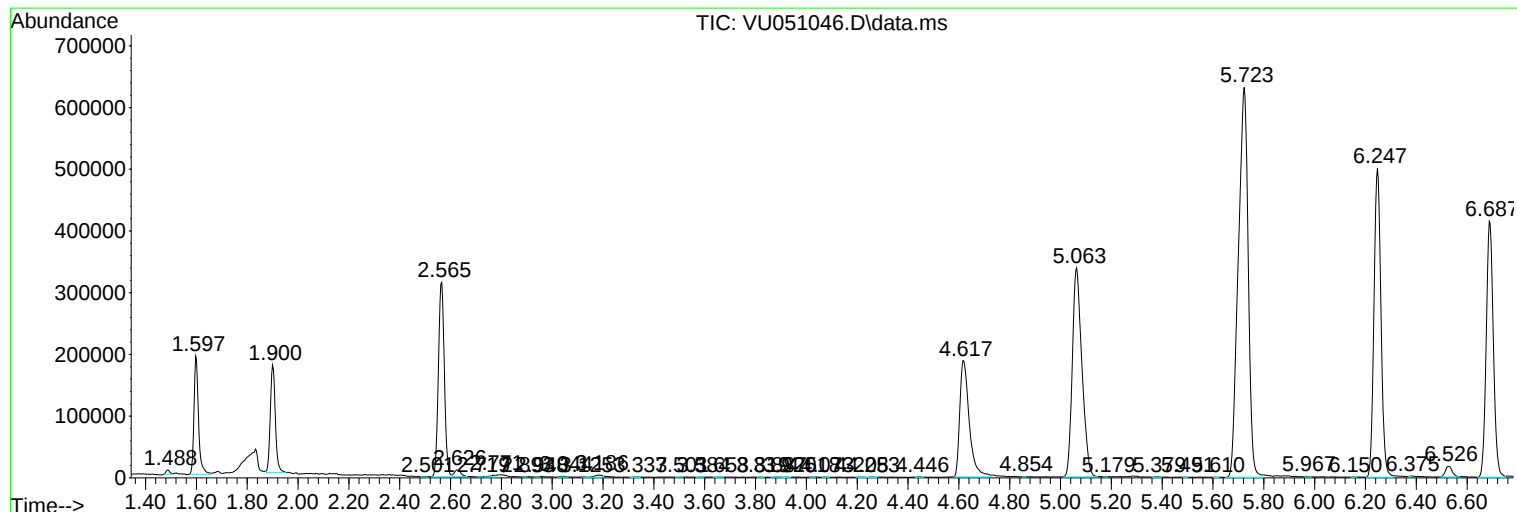

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051046.D
Acq On : 30 Sep 2022 20:04
Operator : JC/MD
Sample : N4859-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051046.D
Acq On : 30 Sep 2022 20:04
Operator : JC/MD
Sample : N4859-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------