

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051054.D
 Acq On : 30 Sep 2022 23:33
 Operator : JC/MD
 Sample : N4869-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	196604	241118	12.64%	1.526%
2	1.912	170	178	196	rBV	200582	272757	14.30%	1.726%
3	2.494	357	359	363	rVB3	802	397	0.02%	0.003%
4	2.565	368	381	400	rBV	336793	551638	28.92%	3.492%
5	2.691	417	420	427	rVB5	966	978	0.05%	0.006%
6	2.787	446	450	463	rVB3	2221	3494	0.18%	0.022%
7	2.861	469	473	475	rBV2	408	311	0.02%	0.002%
8	3.041	520	529	540	rVB3	8042	13995	0.73%	0.089%
9	3.182	559	573	588	rVV	31898	72637	3.81%	0.460%
10	3.266	597	599	602	rVV	653	394	0.02%	0.002%
11	3.282	602	604	609	rVB4	559	401	0.02%	0.003%
12	3.359	620	628	630	rBV7	1627	2312	0.12%	0.015%
13	3.883	786	791	795	rVB2	348	324	0.02%	0.002%
14	4.018	831	833	839	rVB2	403	431	0.02%	0.003%
15	4.051	839	843	845	rBV2	486	409	0.02%	0.003%
16	4.346	931	935	939	rBV2	381	299	0.02%	0.002%
17	4.375	939	944	949	rBV2	336	343	0.02%	0.002%
18	4.642	1008	1027	1030	rBV2	206148	476254	24.97%	3.014%
19	4.964	1123	1127	1129	rBV3	337	298	0.02%	0.002%
20	5.060	1140	1157	1181	rBV	334490	736902	38.63%	4.664%
21	5.372	1244	1254	1256	rBV6	1013	1365	0.07%	0.009%
22	5.420	1267	1269	1275	rVB	504	363	0.02%	0.002%
23	5.594	1318	1323	1329	rBV2	279	329	0.02%	0.002%
24	5.723	1341	1363	1399	rBV2	681368	1846933	96.83%	11.690%
25	5.970	1436	1440	1442	rBV3	1154	1074	0.06%	0.007%
26	6.028	1452	1458	1465	rBV4	581	818	0.04%	0.005%
27	6.182	1504	1506	1509	rVB	641	300	0.02%	0.002%
28	6.247	1509	1526	1554	rBV	559061	1050374	55.07%	6.648%
29	6.539	1603	1617	1632	rBV4	75580	151228	7.93%	0.957%
30	6.690	1648	1664	1681	rBV	441756	861630	45.17%	5.454%
31	6.864	1716	1718	1725	rVB4	687	482	0.03%	0.003%
32	6.896	1725	1728	1730	rVB3	604	317	0.02%	0.002%
33	7.112	1791	1795	1801	rVB4	462	544	0.03%	0.003%
34	7.189	1806	1819	1823	rBV3	1464	2691	0.14%	0.017%
35	7.282	1845	1848	1852	rBV2	352	305	0.02%	0.002%
36	7.359	1870	1872	1879	rVB2	379	347	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051054.D
 Acq On : 30 Sep 2022 23:33
 Operator : JC/MD
 Sample : N4869-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.504	1914	1917	1918	rBV	616	323	0.02%	0.002%
38	7.565	1923	1936	1960	rBV	219817	396477	20.79%	2.510%
39	7.755	1991	1995	1996	rBV2	387	288	0.02%	0.002%
40	7.793	2002	2007	2009	rBV3	1606	1379	0.07%	0.009%
41	7.896	2024	2039	2056	rBV	783622	1353518	70.96%	8.567%
42	8.050	2084	2087	2091	rVB4	791	453	0.02%	0.003%
43	8.179	2114	2127	2149	rBV	152359	269283	14.12%	1.704%
44	8.401	2190	2196	2200	rBV4	861	986	0.05%	0.006%
45	8.443	2204	2209	2212	rBV2	294	324	0.02%	0.002%
46	8.552	2229	2243	2258	rVV	1143648	1907473	100.00%	12.074%
47	8.636	2258	2269	2308	rVB3	508939	1147523	60.16%	7.263%
48	8.832	2328	2330	2332	rBV	465	283	0.01%	0.002%
49	8.922	2352	2358	2363	rBV4	927	991	0.05%	0.006%
50	8.957	2367	2369	2373	rVV2	611	408	0.02%	0.003%
51	9.086	2406	2409	2415	rVB2	529	448	0.02%	0.003%
52	9.157	2429	2431	2435	rVB2	592	314	0.02%	0.002%
53	9.324	2477	2483	2487	rBV3	402	383	0.02%	0.002%
54	9.414	2497	2511	2540	rBV	755441	1275959	66.89%	8.076%
55	9.568	2555	2559	2570	rVB5	2140	2651	0.14%	0.017%
56	9.642	2578	2582	2588	rBV3	525	402	0.02%	0.003%
57	9.693	2592	2598	2605	rVB6	1896	2552	0.13%	0.016%
58	9.838	2640	2643	2648	rVB2	446	373	0.02%	0.002%
59	10.012	2695	2697	2702	rVB2	534	355	0.02%	0.002%
60	10.038	2702	2705	2709	rVB	534	436	0.02%	0.003%
61	10.105	2715	2726	2728	rBV6	1987	2652	0.14%	0.017%
62	10.221	2760	2762	2768	rBV3	463	458	0.02%	0.003%
63	10.475	2838	2841	2842	rBV2	477	307	0.02%	0.002%
64	10.491	2842	2846	2853	rVB3	795	997	0.05%	0.006%
65	10.755	2915	2928	2943	rBV	623465	1015195	53.22%	6.426%
66	11.044	3014	3018	3024	rVV2	410	436	0.02%	0.003%
67	11.076	3024	3028	3029	rVV	609	439	0.02%	0.003%
68	11.092	3029	3033	3036	rVV4	1440	1279	0.07%	0.008%
69	11.121	3036	3042	3045	rVV3	521	541	0.03%	0.003%
70	11.282	3088	3092	3096	rBV2	386	427	0.02%	0.003%
71	11.327	3101	3106	3108	rBV3	610	571	0.03%	0.004%
72	11.472	3144	3151	3158	rBV2	1230	1741	0.09%	0.011%
73	11.745	3226	3236	3244	rBV6	2114	3345	0.18%	0.021%
74	11.809	3244	3256	3278	rBV	595062	962685	50.47%	6.093%
75	12.015	3317	3320	3324	rBV3	488	385	0.02%	0.002%
76	12.086	3336	3342	3346	rBV5	505	602	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051054.D
 Acq On : 30 Sep 2022 23:33
 Operator : JC/MD
 Sample : N4869-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

77	12.192	3357	3375	3394	rBV	664055	1089408	57.11%	6.896%
78	12.758	3546	3551	3554	rBV3	535	442	0.02%	0.003%
79	12.838	3571	3576	3578	rBV2	517	439	0.02%	0.003%
80	12.906	3588	3597	3599	rBV4	561	769	0.04%	0.005%
81	13.076	3647	3650	3653	rVB2	423	301	0.02%	0.002%
82	13.224	3689	3696	3706	rVB7	1969	3100	0.16%	0.020%
83	13.372	3740	3742	3747	rVB3	528	307	0.02%	0.002%
84	13.401	3748	3751	3756	rVV4	442	448	0.02%	0.003%
85	13.516	3783	3787	3789	rBV	458	353	0.02%	0.002%
86	13.671	3831	3835	3840	rBV2	593	452	0.02%	0.003%
87	13.725	3849	3852	3857	rBV3	365	364	0.02%	0.002%
88	13.787	3866	3871	3875	rBV3	711	836	0.04%	0.005%
89	13.844	3881	3889	3898	rBV7	3049	5006	0.26%	0.032%
90	13.880	3898	3900	3903	rVV2	1054	508	0.03%	0.003%
91	13.899	3903	3906	3909	rVB3	681	390	0.02%	0.002%
92	13.963	3923	3926	3931	rBV2	389	395	0.02%	0.003%
93	14.092	3956	3966	3978	rBV2	5685	10782	0.57%	0.068%
94	14.253	4013	4016	4020	rVB3	508	442	0.02%	0.003%
95	14.330	4032	4040	4052	rVB7	3284	6625	0.35%	0.042%
96	14.867	4204	4207	4212	rBV2	791	681	0.04%	0.004%
97	14.973	4238	4240	4246	rBV4	641	697	0.04%	0.004%
98	15.179	4300	4304	4308	rBV5	816	811	0.04%	0.005%
99	16.047	4572	4574	4579	rBV5	1196	942	0.05%	0.006%
100	17.095	4894	4900	4913	rVB4	15077	23887	1.25%	0.151%




Sum of corrected areas: 15798819

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051054.D
Acq On : 30 Sep 2022 23:33
Operator : JC/MD
Sample : N4869-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

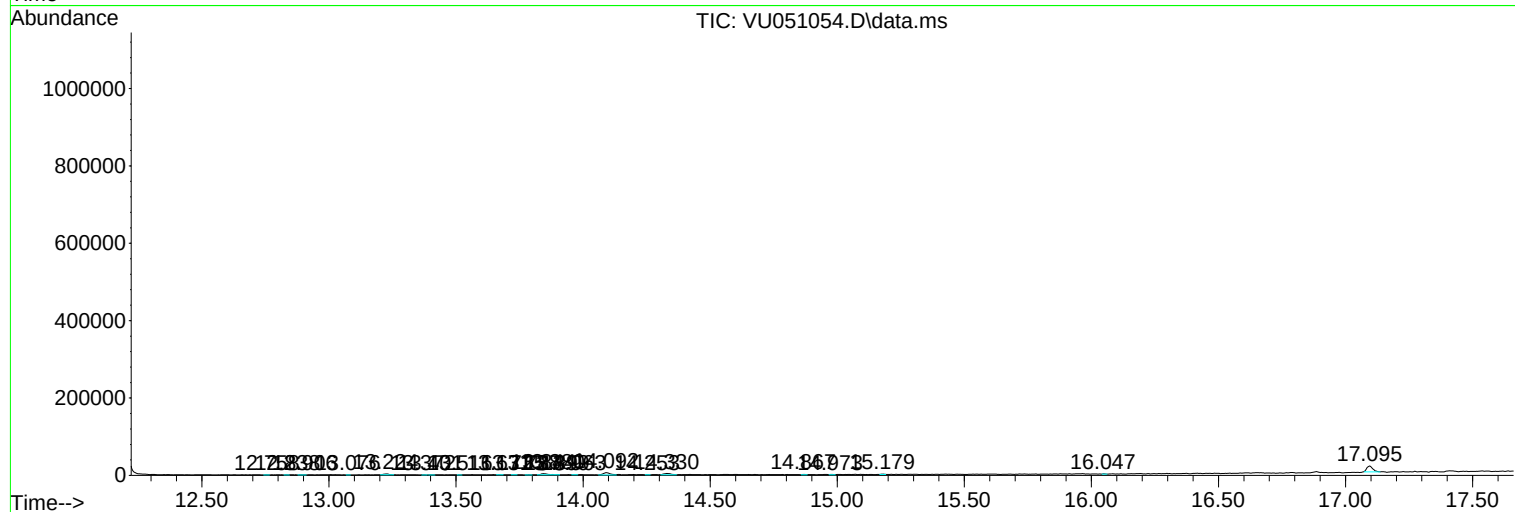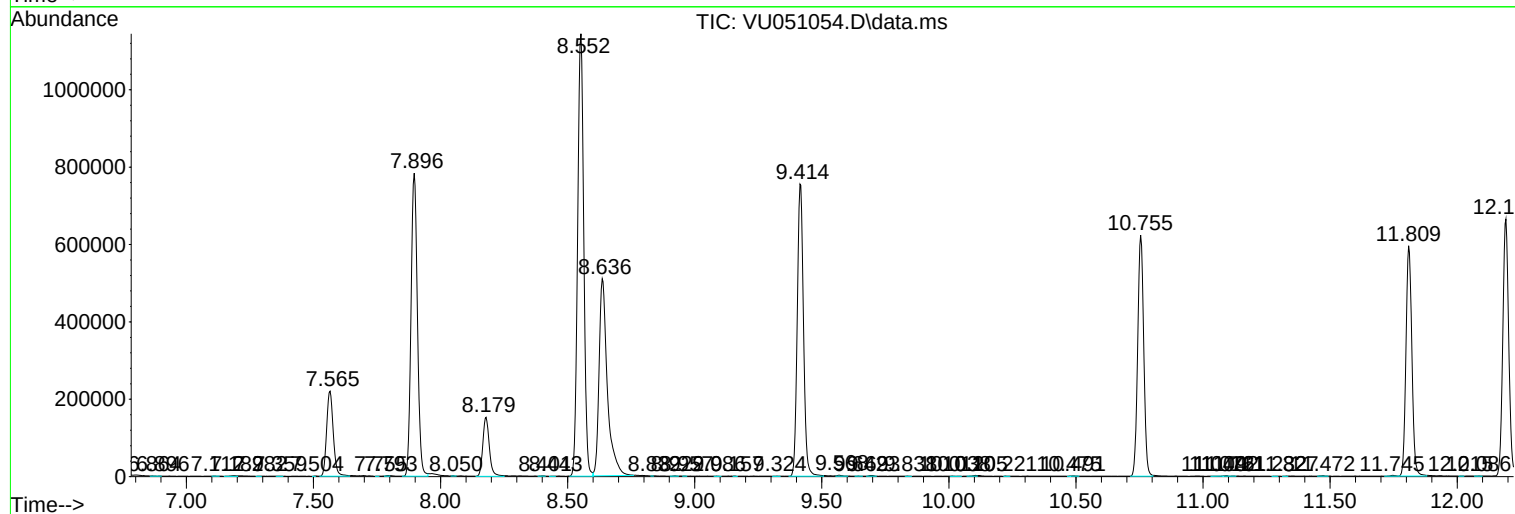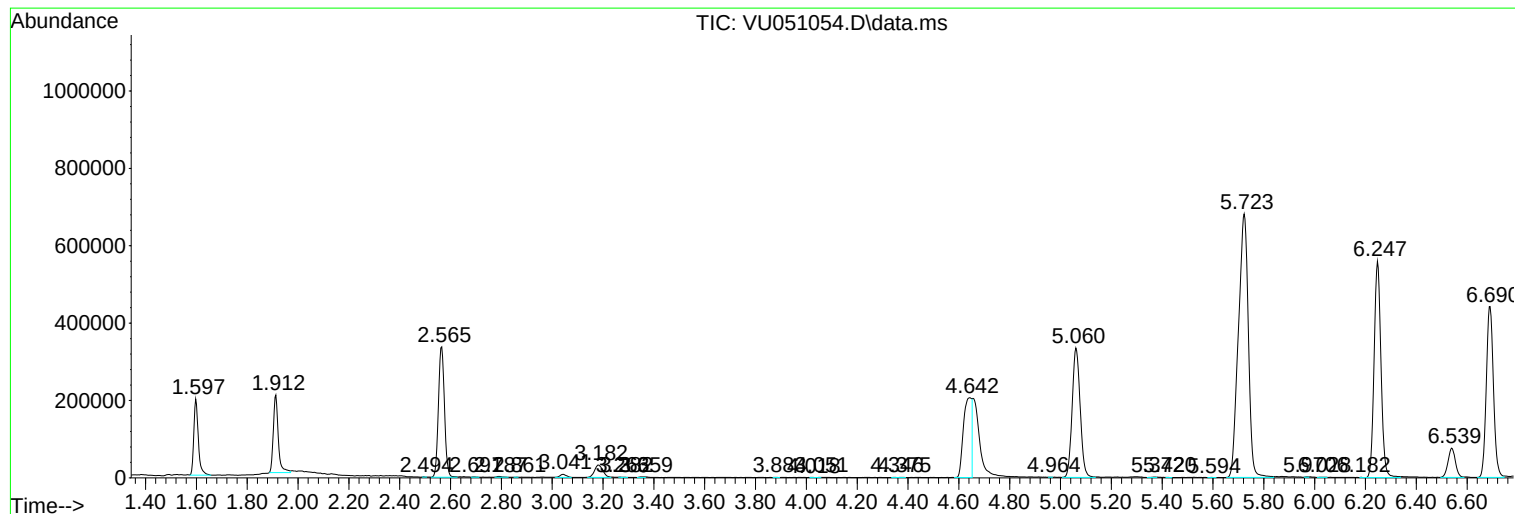

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051054.D
Acq On : 30 Sep 2022 23:33
Operator : JC/MD
Sample : N4869-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051054.D
Acq On : 30 Sep 2022 23:33
Operator : JC/MD
Sample : N4869-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------