

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051055.D
 Acq On : 30 Sep 2022 23:56
 Operator : JC/MD
 Sample : N4869-02DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J02DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	158576	213418	12.77%	1.469%
2	1.877	162	167	192	rVB	176725	255870	15.31%	1.762%
3	2.555	366	378	395	rBV	305475	494574	29.59%	3.405%
4	2.781	437	448	453	rBV5	1983	3057	0.18%	0.021%
5	2.883	477	480	485	rVB2	519	439	0.03%	0.003%
6	2.909	485	488	490	rBV	669	402	0.02%	0.003%
7	3.038	519	528	543	rVV4	5440	9175	0.55%	0.063%
8	3.118	549	553	557	rBV3	414	368	0.02%	0.003%
9	3.179	557	572	587	rBV	43575	102377	6.12%	0.705%
10	3.436	650	652	655	rVV2	476	356	0.02%	0.002%
11	3.459	655	659	662	rVV3	488	420	0.03%	0.003%
12	3.510	673	675	681	rVV	424	344	0.02%	0.002%
13	3.575	692	695	700	rVV2	295	348	0.02%	0.002%
14	3.613	703	707	710	rVV	447	383	0.02%	0.003%
15	3.800	759	765	773	rVB2	343	563	0.03%	0.004%
16	3.848	777	780	784	rVB2	497	368	0.02%	0.003%
17	4.321	920	927	930	rBV2	452	446	0.03%	0.003%
18	4.459	962	970	973	rBV3	343	444	0.03%	0.003%
19	4.539	986	995	1000	rBV2	305	455	0.03%	0.003%
20	4.616	1002	1019	1062	rBV	185747	533405	31.91%	3.672%
21	4.883	1100	1102	1108	rBV4	485	355	0.02%	0.002%
22	5.057	1139	1156	1181	rBV	301066	665636	39.82%	4.583%
23	5.276	1218	1224	1225	rBV3	938	701	0.04%	0.005%
24	5.719	1340	1362	1388	rBV2	618479	1671573	100.00%	11.508%
25	5.964	1431	1438	1450	rVB7	3009	5838	0.35%	0.040%
26	6.115	1480	1485	1488	rBV3	614	615	0.04%	0.004%
27	6.160	1495	1499	1501	rBV2	448	446	0.03%	0.003%
28	6.247	1510	1526	1549	rBV	543366	1027082	61.44%	7.071%
29	6.472	1593	1596	1599	rBV2	414	324	0.02%	0.002%
30	6.526	1603	1613	1626	rBV7	15298	31155	1.86%	0.214%
31	6.597	1631	1635	1640	rVB5	1362	1370	0.08%	0.009%
32	6.687	1647	1663	1690	rBV	399714	783956	46.90%	5.397%
33	6.809	1695	1701	1702	rBV3	762	716	0.04%	0.005%
34	6.864	1713	1718	1722	rBV3	524	612	0.04%	0.004%
35	6.909	1729	1732	1737	rBV4	461	457	0.03%	0.003%
36	7.102	1787	1792	1798	rBV2	459	595	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051055.D
 Acq On : 30 Sep 2022 23:56
 Operator : JC/MD
 Sample : N4869-02DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J02DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.179	1806	1816	1819	rBV5	2554	3626	0.22%	0.025%
38	7.279	1841	1847	1850	rVB3	358	317	0.02%	0.002%
39	7.562	1922	1935	1956	rBV	200242	358287	21.43%	2.467%
40	7.694	1973	1976	1980	rBV3	517	462	0.03%	0.003%
41	7.800	2002	2009	2011	rBV3	1087	928	0.06%	0.006%
42	7.832	2016	2019	2023	rBV2	430	445	0.03%	0.003%
43	7.896	2024	2039	2056	rBV	705914	1220514	73.02%	8.403%
44	8.176	2111	2126	2150	rBV	141618	246597	14.75%	1.698%
45	8.349	2175	2180	2183	rVV4	450	471	0.03%	0.003%
46	8.430	2197	2205	2209	rBV3	631	823	0.05%	0.006%
47	8.452	2209	2212	2217	rBV3	682	732	0.04%	0.005%
48	8.552	2229	2243	2257	rBV	663404	1127388	67.44%	7.761%
49	8.636	2257	2269	2303	rVB3	506038	1105009	66.11%	7.607%
50	8.841	2331	2333	2341	rVB4	707	472	0.03%	0.003%
51	8.890	2345	2348	2351	rVB2	646	425	0.03%	0.003%
52	9.124	2417	2421	2427	rVB	570	575	0.03%	0.004%
53	9.173	2433	2436	2442	rBV2	733	777	0.05%	0.005%
54	9.247	2456	2459	2468	rVB2	535	530	0.03%	0.004%
55	9.292	2471	2473	2476	rBV2	426	332	0.02%	0.002%
56	9.417	2497	2512	2538	rBV	776786	1288454	77.08%	8.870%
57	9.571	2558	2560	2563	rVB3	933	523	0.03%	0.004%
58	9.623	2573	2576	2580	rVB3	502	375	0.02%	0.003%
59	9.652	2580	2585	2588	rBV2	466	382	0.02%	0.003%
60	9.671	2588	2591	2593	rBV2	514	348	0.02%	0.002%
61	9.697	2593	2599	2603	rVB3	735	924	0.06%	0.006%
62	10.018	2695	2699	2704	rBV3	645	666	0.04%	0.005%
63	10.102	2719	2725	2729	rBV6	1066	1233	0.07%	0.008%
64	10.124	2729	2732	2734	rVV3	577	345	0.02%	0.002%
65	10.314	2787	2791	2795	rVB2	371	317	0.02%	0.002%
66	10.343	2795	2800	2805	rBV3	444	466	0.03%	0.003%
67	10.410	2813	2821	2828	rBV2	585	890	0.05%	0.006%
68	10.488	2836	2845	2850	rBV2	764	1098	0.07%	0.008%
69	10.539	2858	2861	2865	rBV	625	507	0.03%	0.003%
70	10.674	2898	2903	2906	rBV2	399	387	0.02%	0.003%
71	10.755	2915	2928	2944	rBV	636308	1033513	61.83%	7.115%
72	10.912	2975	2977	2982	rVB3	433	345	0.02%	0.002%
73	10.941	2982	2986	2990	rVB2	368	326	0.02%	0.002%
74	11.121	3038	3042	3048	rVB5	616	655	0.04%	0.005%
75	11.237	3074	3078	3083	rVB2	559	485	0.03%	0.003%
76	11.285	3090	3093	3096	rBV	399	320	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051055.D
 Acq On : 30 Sep 2022 23:56
 Operator : JC/MD
 Sample : N4869-02DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J02DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.472	3145	3151	3157	rVB4	1179	1543	0.09%	0.011%
78	11.587	3180	3187	3190	rBV2	558	669	0.04%	0.005%
79	11.748	3230	3237	3243	rBV4	1620	2177	0.13%	0.015%
80	11.809	3244	3256	3281	rBV	707336	1132736	67.76%	7.798%
81	12.002	3313	3316	3320	rVB3	803	690	0.04%	0.005%
82	12.098	3341	3346	3350	rBV2	565	701	0.04%	0.005%
83	12.192	3361	3375	3406	rBV	705489	1157118	69.22%	7.966%
84	12.410	3441	3443	3451	rVB	662	515	0.03%	0.004%
85	12.677	3522	3526	3528	rBV	527	435	0.03%	0.003%
86	12.844	3576	3578	3586	rVB3	428	423	0.03%	0.003%
87	12.967	3612	3616	3621	rVB3	535	514	0.03%	0.004%
88	13.224	3691	3696	3700	rBV3	1384	1346	0.08%	0.009%
89	13.330	3722	3729	3730	rBV3	617	743	0.04%	0.005%
90	13.529	3787	3791	3792	rBV2	606	489	0.03%	0.003%
91	13.629	3819	3822	3825	rBV2	378	332	0.02%	0.002%
92	13.851	3885	3891	3899	rVB7	1798	2840	0.17%	0.020%
93	13.896	3902	3905	3908	rBV2	651	411	0.02%	0.003%
94	14.098	3959	3968	3976	rBV2	2971	4629	0.28%	0.032%
95	14.253	4013	4016	4018	rBV	615	385	0.02%	0.003%
96	14.340	4032	4043	4050	rBV8	2528	4564	0.27%	0.031%
97	15.195	4307	4309	4312	rVB4	954	559	0.03%	0.004%
98	15.221	4313	4317	4319	rBV5	678	634	0.04%	0.004%
99	15.385	4365	4368	4371	rBV3	685	619	0.04%	0.004%
100	15.674	4456	4458	4460	rBV2	908	506	0.03%	0.003%




Sum of corrected areas: 14525490

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051055.D
Acq On : 30 Sep 2022 23:56
Operator : JC/MD
Sample : N4869-02DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J02DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

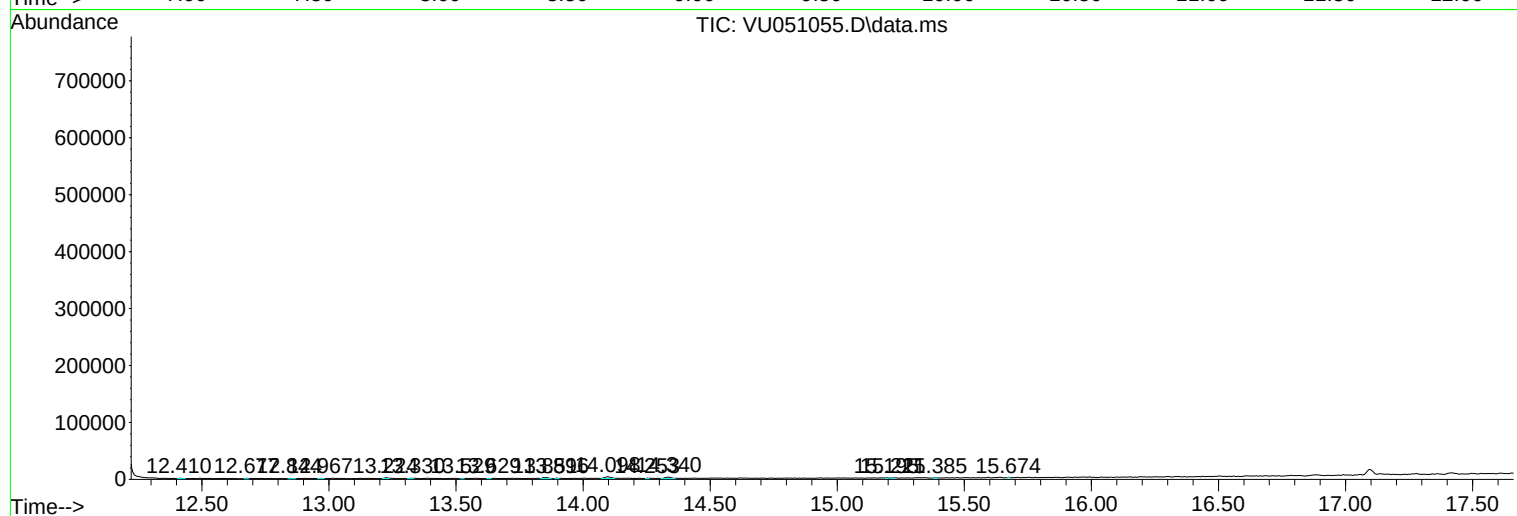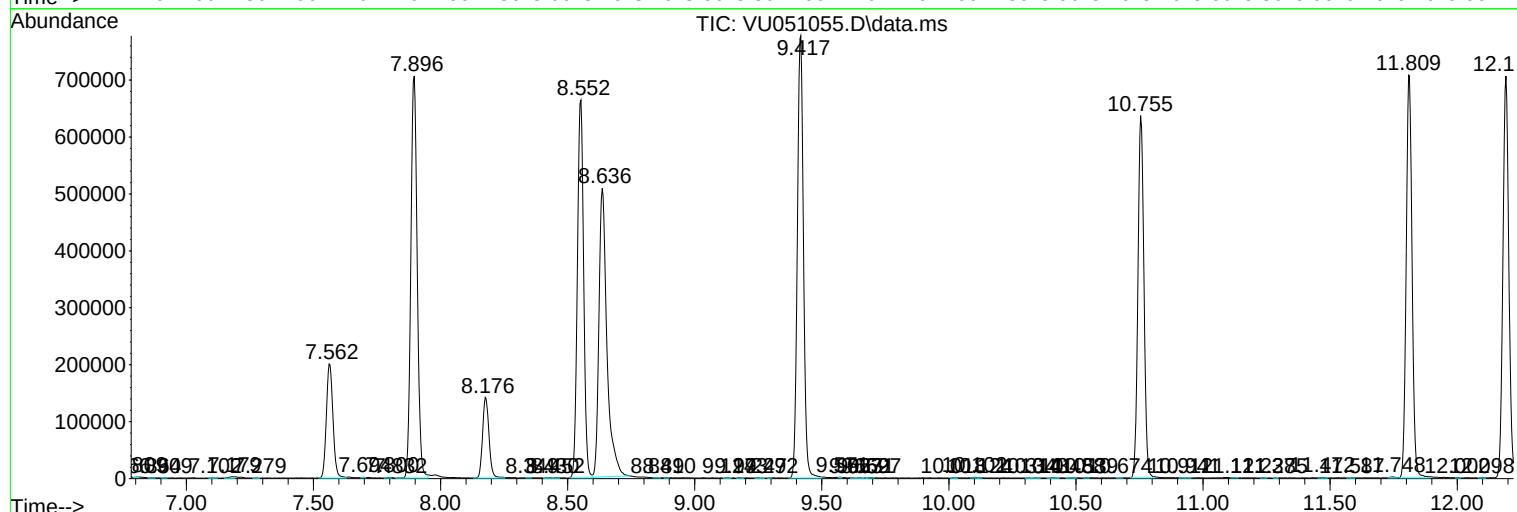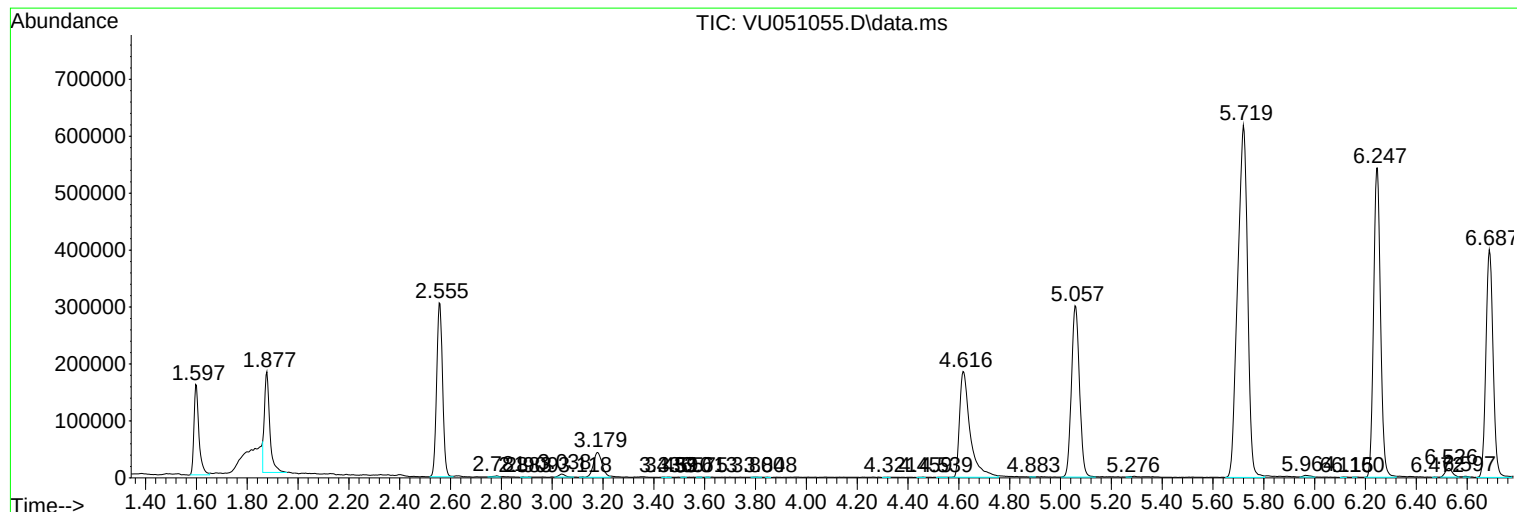

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051055.D
Acq On : 30 Sep 2022 23:56
Operator : JC/MD
Sample : N4869-02DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J02DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051055.D
Acq On : 30 Sep 2022 23:56
Operator : JC/MD
Sample : N4869-02DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J02DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------