

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051056.D
 Acq On : 01 Oct 2022 00:19
 Operator : JC/MD
 Sample : N4869-03DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J05DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	104	rVB	168081	228481	12.80%	1.492%
2	1.900	168	174	201	rVB	202977	377369	21.15%	2.464%
3	2.559	366	379	393	rBV	328673	530944	29.76%	3.467%
4	2.636	400	403	406	rBV2	1238	846	0.05%	0.006%
5	2.748	435	438	442	rBV2	479	346	0.02%	0.002%
6	2.790	442	451	461	rBV4	1587	2846	0.16%	0.019%
7	2.890	474	482	484	rBV3	513	772	0.04%	0.005%
8	2.999	510	516	519	rBV3	410	489	0.03%	0.003%
9	3.044	519	530	541	rVV3	5111	10467	0.59%	0.068%
10	3.182	558	573	590	rBV2	36037	80830	4.53%	0.528%
11	3.427	645	649	655	rVV2	370	384	0.02%	0.003%
12	3.491	665	669	672	rBV	558	367	0.02%	0.002%
13	3.626	706	711	714	rBV	487	376	0.02%	0.002%
14	3.771	752	756	760	rBV2	491	306	0.02%	0.002%
15	3.935	802	807	810	rVV2	423	323	0.02%	0.002%
16	4.028	834	836	847	rVB	571	790	0.04%	0.005%
17	4.076	847	851	854	rBV	570	446	0.02%	0.003%
18	4.198	883	889	891	rBV2	574	576	0.03%	0.004%
19	4.407	951	954	959	rBV2	389	387	0.02%	0.003%
20	4.626	1009	1022	1073	rBV	182287	579495	32.48%	3.784%
21	5.060	1140	1157	1180	rBV	328818	717460	40.21%	4.685%
22	5.343	1242	1245	1248	rBV2	458	335	0.02%	0.002%
23	5.407	1262	1265	1269	rVB2	502	397	0.02%	0.003%
24	5.520	1297	1300	1302	rBV	465	330	0.02%	0.002%
25	5.723	1337	1363	1383	rBV2	660709	1784364	100.00%	11.652%
26	5.964	1433	1438	1439	rBV3	2721	2050	0.11%	0.013%
27	6.115	1480	1485	1488	rBV4	709	721	0.04%	0.005%
28	6.147	1493	1495	1502	rVB4	560	598	0.03%	0.004%
29	6.186	1502	1507	1510	rVB3	443	316	0.02%	0.002%
30	6.247	1512	1526	1552	rBV	562141	1067490	59.82%	6.971%
31	6.526	1602	1613	1627	rVV5	17308	34481	1.93%	0.225%
32	6.591	1627	1633	1635	rBV4	1582	1597	0.09%	0.010%
33	6.687	1649	1663	1685	rBV	423209	839381	47.04%	5.481%
34	6.931	1736	1739	1744	rBV2	347	314	0.02%	0.002%
35	7.083	1781	1786	1789	rBV2	427	478	0.03%	0.003%
36	7.198	1809	1822	1823	rBV3	2879	3912	0.22%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051056.D
 Acq On : 01 Oct 2022 00:19
 Operator : JC/MD
 Sample : N4869-03DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J05DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.314	1853	1858	1859	rBV	446	323	0.02%	0.002%
38	7.362	1865	1873	1876	rBV2	696	538	0.03%	0.004%
39	7.446	1894	1899	1901	rVB2	493	315	0.02%	0.002%
40	7.472	1901	1907	1909	rBV2	438	383	0.02%	0.003%
41	7.565	1923	1936	1961	rBV	215691	382492	21.44%	2.498%
42	7.677	1968	1971	1974	rBV3	702	438	0.02%	0.003%
43	7.787	2001	2005	2007	rBV2	463	406	0.02%	0.003%
44	7.800	2007	2009	2014	rVB2	589	402	0.02%	0.003%
45	7.896	2025	2039	2058	rBV	756292	1300835	72.90%	8.495%
46	8.179	2114	2127	2145	rBV	147149	257551	14.43%	1.682%
47	8.308	2164	2167	2170	rBV2	562	322	0.02%	0.002%
48	8.465	2212	2216	2218	rBV2	360	307	0.02%	0.002%
49	8.552	2229	2243	2258	rBV	816950	1397901	78.34%	9.129%
50	8.642	2258	2271	2302	rVB3	495885	1122584	62.91%	7.331%
51	8.922	2355	2358	2364	rVB4	883	821	0.05%	0.005%
52	8.983	2375	2377	2381	rVB2	675	373	0.02%	0.002%
53	9.038	2392	2394	2399	rVB2	395	309	0.02%	0.002%
54	9.185	2435	2440	2444	rBV2	715	704	0.04%	0.005%
55	9.417	2498	2512	2537	rBV	785968	1320987	74.03%	8.626%
56	9.568	2553	2559	2563	rVB5	1112	1266	0.07%	0.008%
57	9.693	2594	2598	2606	rBV3	880	1273	0.07%	0.008%
58	9.992	2689	2691	2701	rVB2	522	732	0.04%	0.005%
59	10.041	2701	2706	2711	rBV2	407	546	0.03%	0.004%
60	10.099	2717	2724	2730	rVV3	843	949	0.05%	0.006%
61	10.128	2730	2733	2738	rVB2	606	474	0.03%	0.003%
62	10.166	2741	2745	2750	rVB	541	438	0.02%	0.003%
63	10.192	2750	2753	2755	rBV	565	341	0.02%	0.002%
64	10.491	2843	2846	2851	rVB2	477	436	0.02%	0.003%
65	10.591	2871	2877	2879	rBV2	333	319	0.02%	0.002%
66	10.603	2879	2881	2885	rVB2	536	347	0.02%	0.002%
67	10.754	2916	2928	2950	rBV	621483	1034052	57.95%	6.753%
68	10.986	2997	3000	3005	rBV	530	388	0.02%	0.003%
69	11.082	3026	3030	3031	rBV2	756	434	0.02%	0.003%
70	11.111	3037	3039	3047	rVB4	637	654	0.04%	0.004%
71	11.156	3050	3053	3057	rVB2	418	351	0.02%	0.002%
72	11.192	3057	3064	3070	rBV3	403	653	0.04%	0.004%
73	11.410	3128	3132	3135	rBV2	501	447	0.03%	0.003%
74	11.475	3148	3152	3159	rVB2	840	819	0.05%	0.005%
75	11.748	3231	3237	3243	rVB2	1307	1548	0.09%	0.010%
76	11.809	3243	3256	3274	rBV	677315	1069897	59.96%	6.987%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051056.D
 Acq On : 01 Oct 2022 00:19
 Operator : JC/MD
 Sample : N4869-03DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J05DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.944	3294	3298	3304	rVB5	1106	1189	0.07%	0.008%
78	12.082	3337	3341	3344	rBV2	592	393	0.02%	0.003%
79	12.192	3359	3375	3393	rBV	683155	1123273	62.95%	7.335%
80	12.607	3498	3504	3509	rVB3	673	856	0.05%	0.006%
81	12.700	3529	3533	3537	rBV4	652	639	0.04%	0.004%
82	12.761	3548	3552	3557	rVV2	496	430	0.02%	0.003%
83	12.861	3580	3583	3587	rVB3	681	511	0.03%	0.003%
84	12.883	3587	3590	3593	rVB2	657	456	0.03%	0.003%
85	12.902	3593	3596	3598	rBV2	744	533	0.03%	0.003%
86	12.999	3622	3626	3631	rBV2	529	420	0.02%	0.003%
87	13.221	3690	3695	3696	rBV3	1265	1009	0.06%	0.007%
88	13.259	3703	3707	3712	rBV3	503	456	0.03%	0.003%
89	13.333	3727	3730	3735	rVB3	490	396	0.02%	0.003%
90	13.362	3735	3739	3741	rBV2	450	397	0.02%	0.003%
91	13.526	3785	3790	3792	rBV3	616	461	0.03%	0.003%
92	13.783	3866	3870	3873	rBV3	390	401	0.02%	0.003%
93	13.928	3912	3915	3918	rVB	746	433	0.02%	0.003%
94	14.259	4015	4018	4024	rVB3	947	665	0.04%	0.004%
95	14.298	4024	4030	4034	rBV2	776	1126	0.06%	0.007%
96	14.340	4038	4043	4051	rVB6	1246	1695	0.09%	0.011%
97	14.481	4084	4087	4090	rBV3	641	485	0.03%	0.003%
98	14.687	4148	4151	4154	rBV	680	493	0.03%	0.003%
99	15.005	4247	4250	4254	rBV4	618	515	0.03%	0.003%
100	15.182	4303	4305	4309	rVB2	888	543	0.03%	0.004%




Sum of corrected areas: 15313194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051056.D
Acq On : 01 Oct 2022 00:19
Operator : JC/MD
Sample : N4869-03DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J05DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

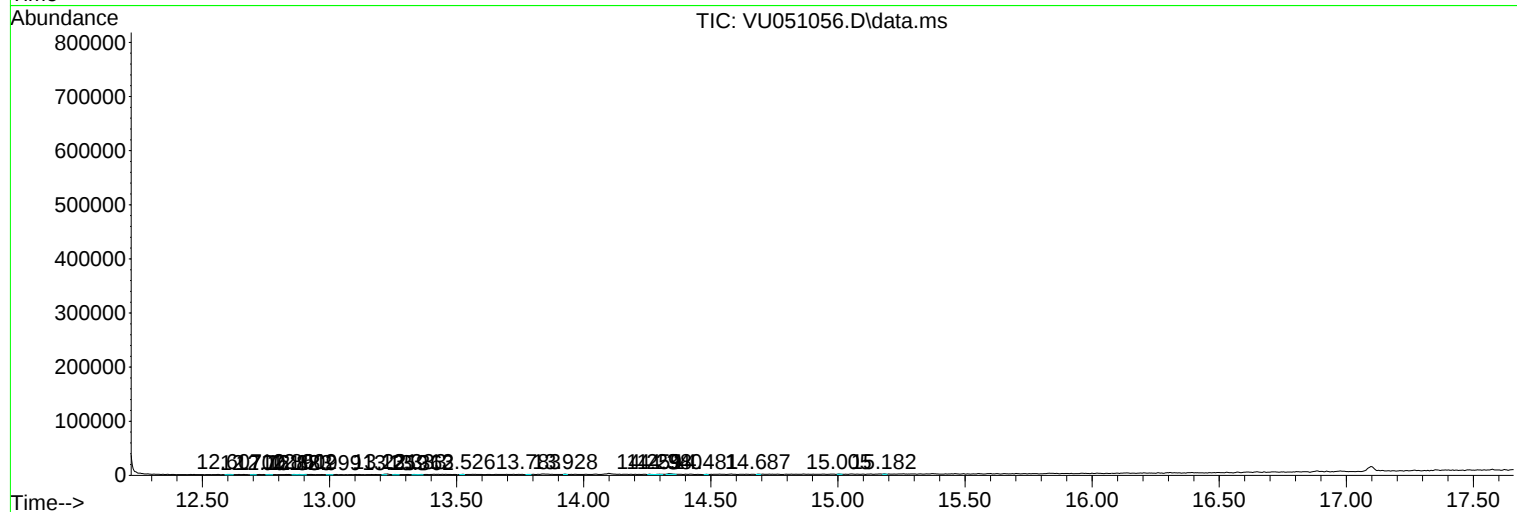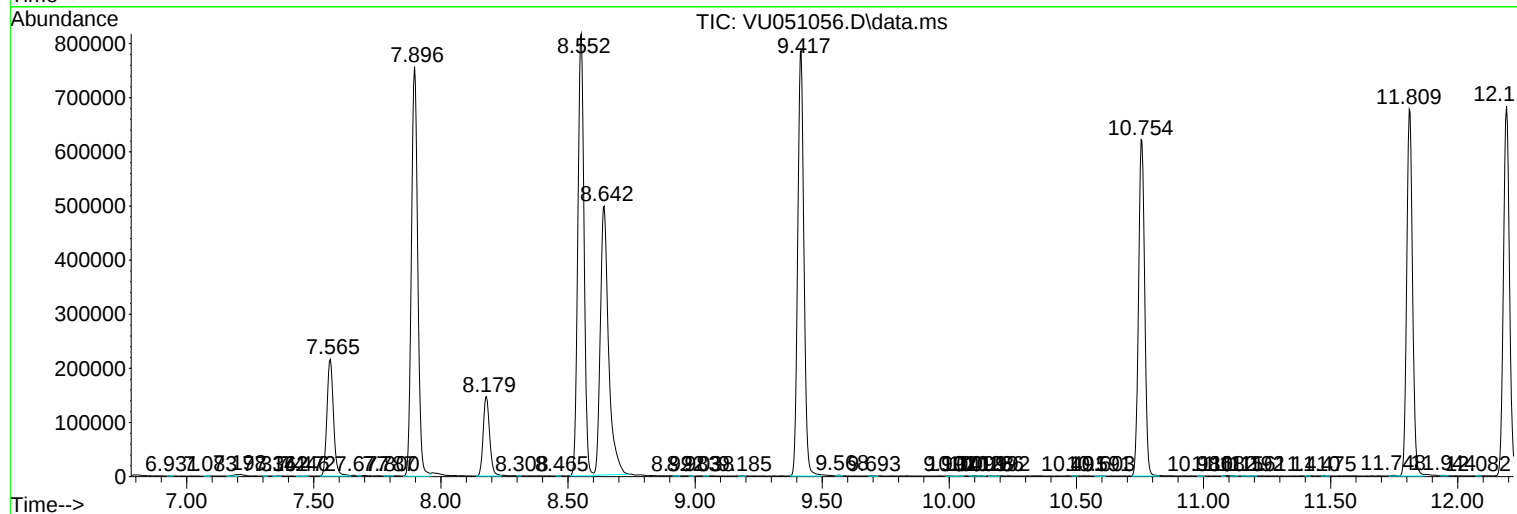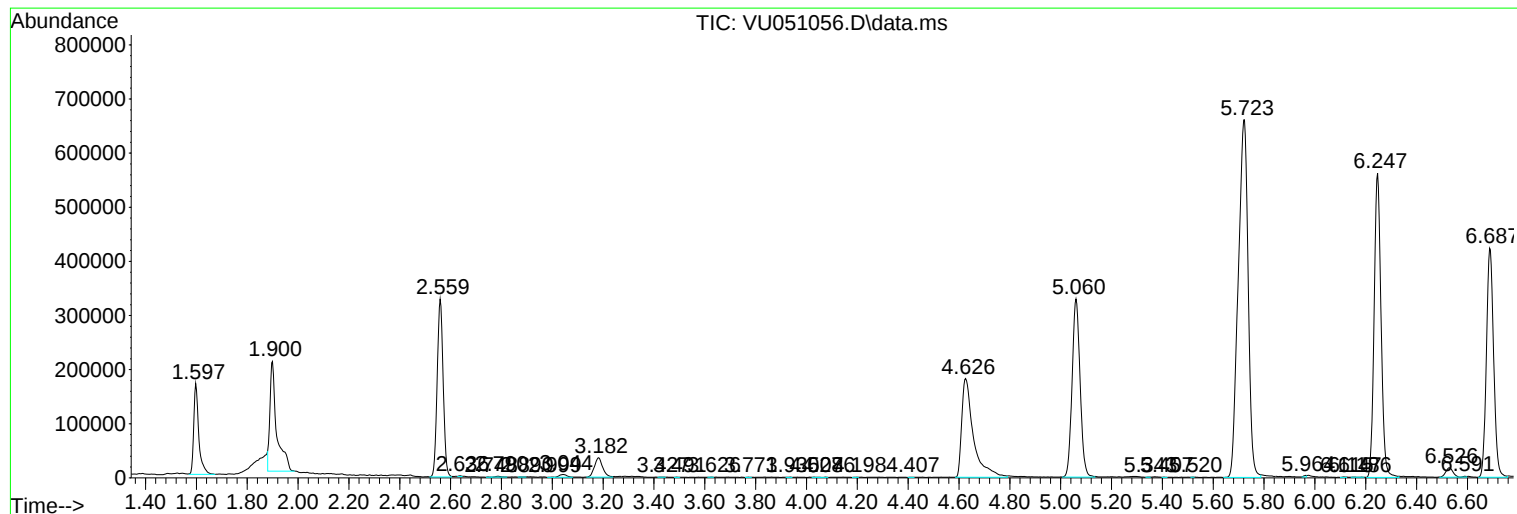

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051056.D
Acq On : 01 Oct 2022 00:19
Operator : JC/MD
Sample : N4869-03DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J05DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051056.D
Acq On : 01 Oct 2022 00:19
Operator : JC/MD
Sample : N4869-03DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J05DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc