

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051059.D
 Acq On : 01 Oct 2022 01:29
 Operator : JC/MD
 Sample : N4869-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	173603	205811	7.46%	1.417%
2	1.903	167	175	194	rVB	159989	216588	7.85%	1.491%
3	2.494	357	359	363	rVB4	1058	522	0.02%	0.004%
4	2.565	368	381	395	rBV	282009	460004	16.67%	3.168%
5	2.678	413	416	419	rBV2	624	441	0.02%	0.003%
6	2.700	420	423	426	rVB2	841	548	0.02%	0.004%
7	2.719	426	429	431	rBV	596	396	0.01%	0.003%
8	2.758	437	441	444	rBV3	518	538	0.02%	0.004%
9	3.009	512	519	522	rBV3	427	546	0.02%	0.004%
10	3.041	522	529	531	rBV4	1141	1044	0.04%	0.007%
11	3.128	551	556	558	rVV2	520	420	0.02%	0.003%
12	3.186	562	574	588	rVV2	6907	15664	0.57%	0.108%
13	3.237	588	590	596	rVB2	796	521	0.02%	0.004%
14	3.308	610	612	616	rVB2	502	352	0.01%	0.002%
15	3.337	616	621	624	rBV2	397	385	0.01%	0.003%
16	3.468	655	662	667	rBV2	554	773	0.03%	0.005%
17	3.530	676	681	683	rBV2	425	356	0.01%	0.002%
18	3.623	707	710	715	rVB2	303	282	0.01%	0.002%
19	3.700	729	734	737	rBV2	382	284	0.01%	0.002%
20	3.742	744	747	753	rVB2	454	408	0.01%	0.003%
21	3.986	817	823	826	rBV2	466	327	0.01%	0.002%
22	4.067	844	848	850	rBV2	513	375	0.01%	0.003%
23	4.144	866	872	874	rBV2	453	414	0.02%	0.003%
24	4.520	986	989	994	rBV	384	273	0.01%	0.002%
25	4.549	994	998	1002	rVB	363	275	0.01%	0.002%
26	4.620	1002	1020	1057	rBV	172428	467028	16.92%	3.216%
27	4.980	1130	1132	1137	rVB3	630	462	0.02%	0.003%
28	5.060	1141	1157	1178	rBV	288036	640912	23.22%	4.413%
29	5.375	1252	1255	1260	rVB4	660	652	0.02%	0.004%
30	5.504	1289	1295	1298	rBV	380	362	0.01%	0.002%
31	5.552	1306	1310	1313	rBV2	381	306	0.01%	0.002%
32	5.600	1319	1325	1328	rBV2	402	531	0.02%	0.004%
33	5.722	1341	1363	1390	rBV2	577552	1569599	56.88%	10.809%
34	6.044	1460	1463	1467	rVB2	662	452	0.02%	0.003%
35	6.247	1512	1526	1545	rBV	494624	928987	33.66%	6.397%
36	6.529	1603	1614	1628	rVB5	15990	35433	1.28%	0.244%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051059.D
 Acq On : 01 Oct 2022 01:29
 Operator : JC/MD
 Sample : N4869-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.603	1632	1637	1642	rVB4	810	910	0.03%	0.006%
38	6.690	1648	1664	1681	rBV	378154	739063	26.78%	5.089%
39	7.057	1772	1778	1780	rBV	510	344	0.01%	0.002%
40	7.105	1784	1793	1800	rBV3	975	1766	0.06%	0.012%
41	7.182	1814	1817	1826	rVB5	1390	1668	0.06%	0.011%
42	7.311	1852	1857	1859	rBV2	347	293	0.01%	0.002%
43	7.330	1860	1863	1866	rBV	431	359	0.01%	0.002%
44	7.481	1907	1910	1915	rBV2	386	353	0.01%	0.002%
45	7.565	1922	1936	1951	rBV	183620	321532	11.65%	2.214%
46	7.697	1974	1977	1990	rVB6	1248	1582	0.06%	0.011%
47	7.896	2025	2039	2057	rBV	645068	1101298	39.91%	7.584%
48	8.179	2114	2127	2141	rBV	128443	219298	7.95%	1.510%
49	8.320	2169	2171	2174	rBV2	465	308	0.01%	0.002%
50	8.459	2210	2214	2218	rBV4	555	488	0.02%	0.003%
51	8.552	2229	2243	2257	rBV	1636870	2759712	100.00%	19.004%
52	8.632	2258	2268	2297	rVB4	449816	958372	34.73%	6.600%
53	8.902	2350	2352	2356	rVB3	427	291	0.01%	0.002%
54	9.060	2395	2401	2402	rBV	757	668	0.02%	0.005%
55	9.417	2498	2512	2533	rBV	696808	1157836	41.95%	7.973%
56	9.613	2571	2573	2577	rVB3	493	289	0.01%	0.002%
57	9.697	2597	2599	2605	rVB3	777	600	0.02%	0.004%
58	9.851	2645	2647	2651	rVB	539	290	0.01%	0.002%
59	9.889	2656	2659	2664	rVB2	388	335	0.01%	0.002%
60	9.918	2664	2668	2672	rVB	464	372	0.01%	0.003%
61	9.944	2672	2676	2679	rBV3	498	335	0.01%	0.002%
62	10.044	2705	2707	2712	rVB2	471	381	0.01%	0.003%
63	10.098	2719	2724	2726	rBV3	565	561	0.02%	0.004%
64	10.221	2759	2762	2766	rVB3	400	328	0.01%	0.002%
65	10.407	2818	2820	2825	rVB3	553	393	0.01%	0.003%
66	10.439	2826	2830	2834	rBV2	380	327	0.01%	0.002%
67	10.574	2869	2872	2874	rBV2	432	284	0.01%	0.002%
68	10.632	2887	2890	2894	rVB2	317	273	0.01%	0.002%
69	10.661	2894	2899	2903	rVB2	441	442	0.02%	0.003%
70	10.687	2903	2907	2914	rVB	439	515	0.02%	0.004%
71	10.754	2914	2928	2949	rBV	548326	884161	32.04%	6.089%
72	10.857	2957	2960	2966	rVV3	597	546	0.02%	0.004%
73	10.886	2967	2969	2972	rVB2	584	283	0.01%	0.002%
74	11.166	3054	3056	3063	rVB2	504	525	0.02%	0.004%
75	11.266	3083	3087	3088	rBV3	437	299	0.01%	0.002%
76	11.307	3096	3100	3103	rBV2	371	371	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051059.D
 Acq On : 01 Oct 2022 01:29
 Operator : JC/MD
 Sample : N4869-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.484	3153	3155	3162	rVB	411	319	0.01%	0.002%
78	11.520	3162	3166	3168	rBV2	415	281	0.01%	0.002%
79	11.568	3179	3181	3186	rBV2	415	302	0.01%	0.002%
80	11.616	3193	3196	3199	rBV	512	296	0.01%	0.002%
81	11.751	3234	3238	3244	rBV4	570	481	0.02%	0.003%
82	11.809	3244	3256	3281	rBV	547680	876153	31.75%	6.033%
83	12.121	3349	3353	3355	rBV3	426	326	0.01%	0.002%
84	12.192	3362	3375	3394	rBV	569446	924870	33.51%	6.369%
85	12.645	3513	3516	3523	rVB3	593	659	0.02%	0.005%
86	12.709	3533	3536	3541	rVB3	566	527	0.02%	0.004%
87	12.738	3541	3545	3547	rBV2	319	300	0.01%	0.002%
88	13.005	3626	3628	3630	rBV	472	277	0.01%	0.002%
89	13.095	3654	3656	3659	rBV	482	299	0.01%	0.002%
90	13.130	3664	3667	3671	rVB2	918	665	0.02%	0.005%
91	13.169	3672	3679	3686	rBV3	832	1234	0.04%	0.008%
92	13.237	3693	3700	3704	rBV5	781	930	0.03%	0.006%
93	13.375	3740	3743	3745	rBV3	529	293	0.01%	0.002%
94	13.600	3810	3813	3817	rBV	619	455	0.02%	0.003%
95	13.709	3844	3847	3853	rBV3	406	428	0.02%	0.003%
96	13.790	3869	3872	3876	rBV3	500	384	0.01%	0.003%
97	14.147	3979	3983	3985	rVB4	511	347	0.01%	0.002%
98	14.301	4028	4031	4035	rVB2	735	488	0.02%	0.003%
99	15.021	4252	4255	4257	rBV2	661	414	0.02%	0.003%
100	15.191	4304	4308	4311	rVB3	967	743	0.03%	0.005%




Sum of corrected areas: 14521793

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051059.D
Acq On : 01 Oct 2022 01:29
Operator : JC/MD
Sample : N4869-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

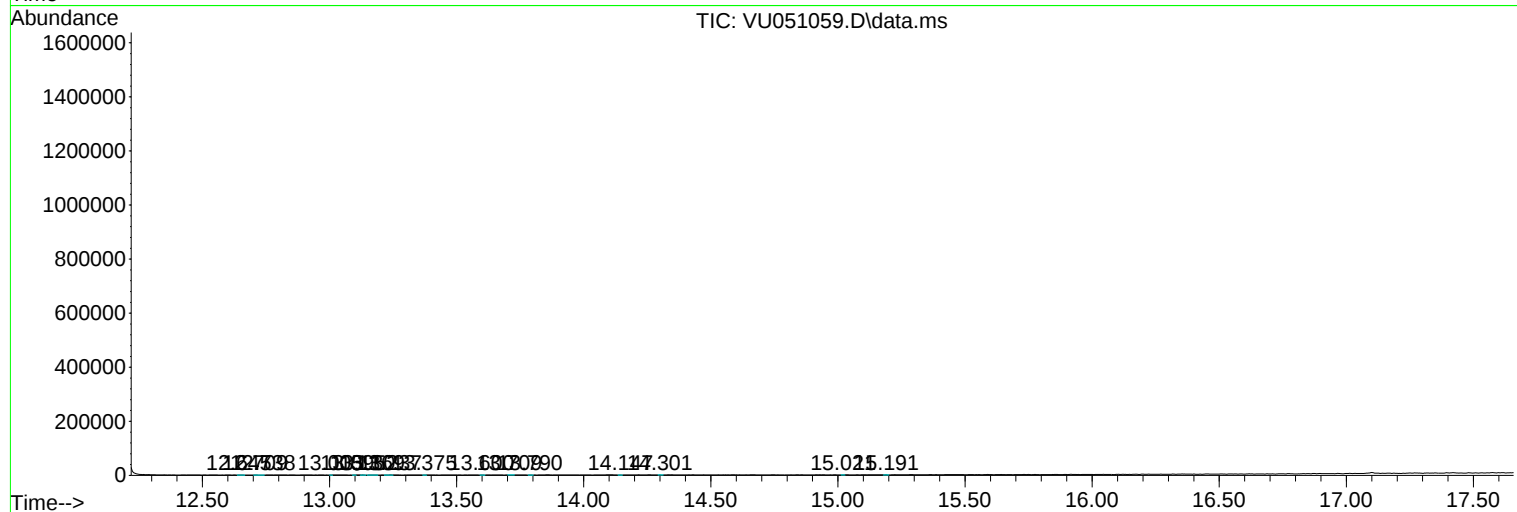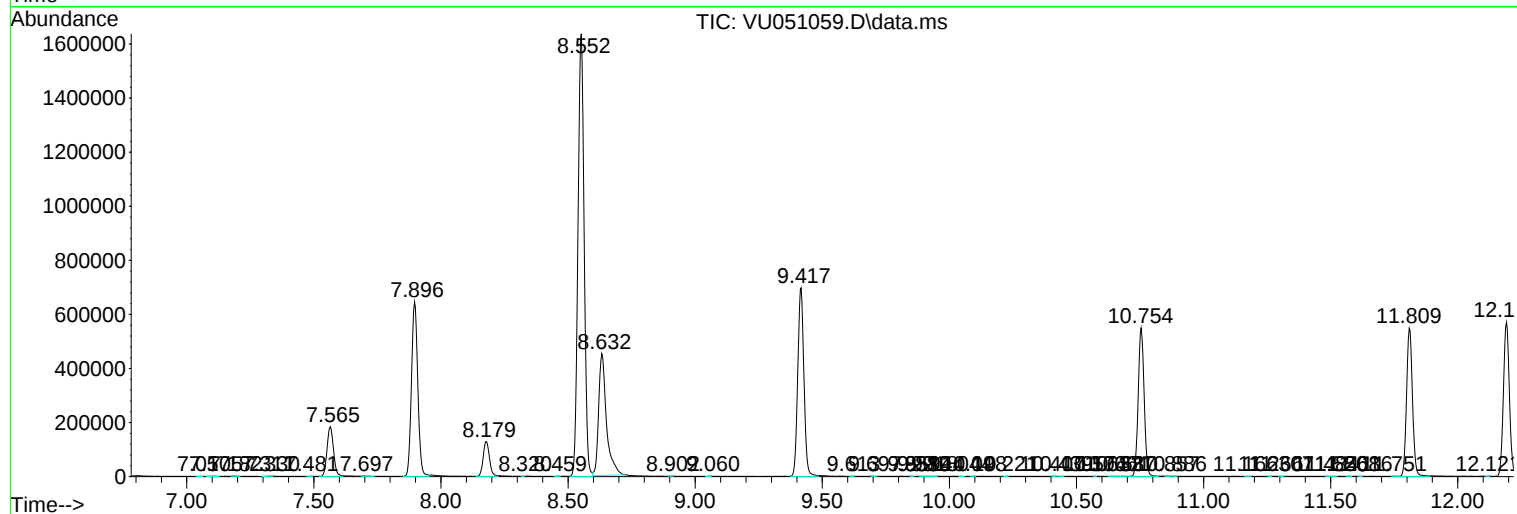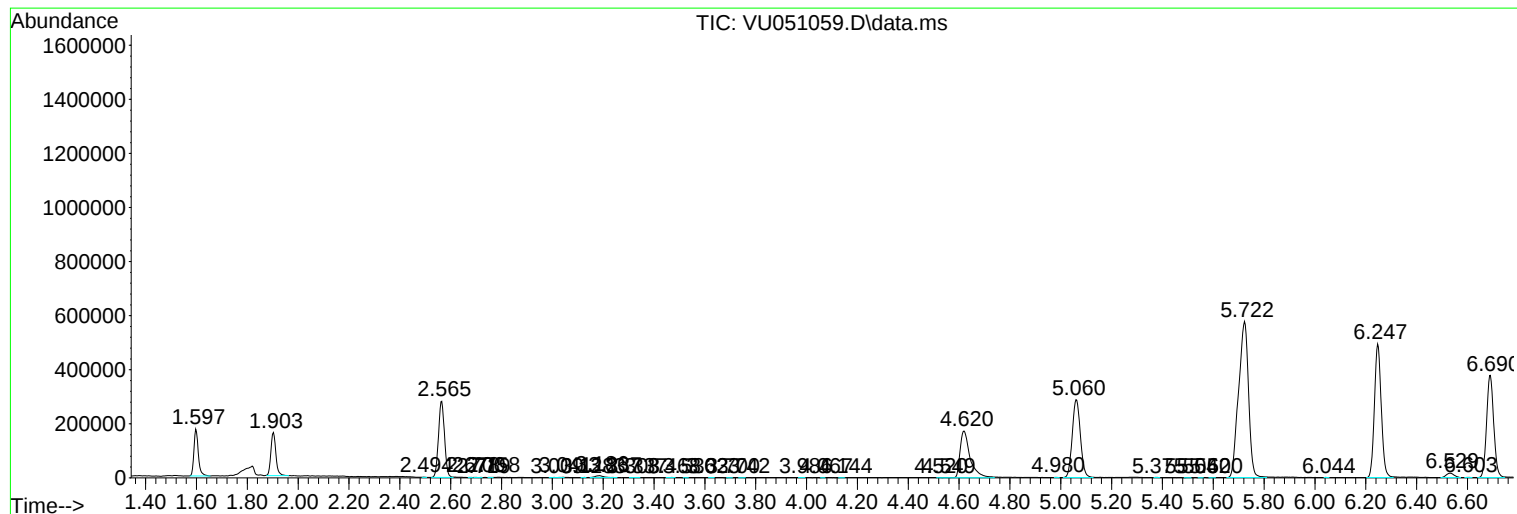

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051059.D
Acq On : 01 Oct 2022 01:29
Operator : JC/MD
Sample : N4869-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051059.D
Acq On : 01 Oct 2022 01:29
Operator : JC/MD
Sample : N4869-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------