

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051060.D
 Acq On : 01 Oct 2022 01:52
 Operator : JC/MD
 Sample : N4869-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	174593	200096	13.00%	1.640%
2	1.900	166	174	199	rVB	155084	219179	14.24%	1.796%
3	2.562	367	380	396	rBV	279767	454590	29.54%	3.725%
4	2.877	475	478	482	rBV3	355	300	0.02%	0.002%
5	2.941	496	498	501	rBV2	466	278	0.02%	0.002%
6	3.038	522	528	539	rBV6	1508	2526	0.16%	0.021%
7	3.179	561	572	588	rBV	8776	19963	1.30%	0.164%
8	3.362	619	629	641	rVB3	2637	4978	0.32%	0.041%
9	3.459	657	659	663	rVB	432	269	0.02%	0.002%
10	3.742	745	747	752	rVV	333	252	0.02%	0.002%
11	3.803	763	766	774	rVB2	381	426	0.03%	0.003%
12	4.044	833	841	848	rBV	483	583	0.04%	0.005%
13	4.105	857	860	865	rVB2	378	299	0.02%	0.002%
14	4.141	865	871	873	rBV2	333	335	0.02%	0.003%
15	4.353	931	937	941	rBV2	241	287	0.02%	0.002%
16	4.401	949	952	960	rVB2	362	419	0.03%	0.003%
17	4.520	987	989	993	rBV2	423	327	0.02%	0.003%
18	4.552	996	999	1005	rVB2	387	334	0.02%	0.003%
19	4.616	1006	1019	1050	rBV	175705	444333	28.87%	3.641%
20	4.893	1101	1105	1107	rBV3	346	262	0.02%	0.002%
21	5.060	1141	1157	1179	rVB	285893	623308	40.50%	5.108%
22	5.214	1202	1205	1210	rBV5	687	577	0.04%	0.005%
23	5.327	1236	1240	1241	rBV3	493	327	0.02%	0.003%
24	5.369	1249	1253	1254	rBV3	426	291	0.02%	0.002%
25	5.407	1263	1265	1270	rVB2	385	278	0.02%	0.002%
26	5.440	1270	1275	1278	rVB2	461	360	0.02%	0.003%
27	5.604	1319	1326	1334	rVB3	345	703	0.05%	0.006%
28	5.723	1341	1363	1377	rBV2	564750	1538900	100.00%	12.611%
29	5.986	1443	1445	1451	rVB3	1014	626	0.04%	0.005%
30	6.115	1479	1485	1488	rBV3	422	429	0.03%	0.004%
31	6.247	1512	1526	1548	rBV	482938	912545	59.30%	7.478%
32	6.456	1588	1591	1596	rVB2	790	647	0.04%	0.005%
33	6.536	1603	1616	1630	rBV6	18664	40829	2.65%	0.335%
34	6.591	1630	1633	1644	rVB4	708	1087	0.07%	0.009%
35	6.690	1647	1664	1685	rBV	373686	730677	47.48%	5.988%
36	6.944	1741	1743	1749	rVV3	458	394	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051060.D
 Acq On : 01 Oct 2022 01:52
 Operator : JC/MD
 Sample : N4869-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.047	1770	1775	1778	rBV2	328	276	0.02%	0.002%
38	7.169	1810	1813	1814	rBV	688	311	0.02%	0.003%
39	7.185	1815	1818	1820	rVV4	651	494	0.03%	0.004%
40	7.375	1869	1877	1881	rBV2	366	435	0.03%	0.004%
41	7.436	1892	1896	1900	rVV2	237	283	0.02%	0.002%
42	7.565	1923	1936	1954	rBV2	181410	319509	20.76%	2.618%
43	7.693	1971	1976	1985	rBV6	1205	1894	0.12%	0.016%
44	7.787	1997	2005	2006	rBV3	561	552	0.04%	0.005%
45	7.896	2026	2039	2061	rBV	637582	1090112	70.84%	8.933%
46	8.105	2100	2104	2107	rBV3	367	344	0.02%	0.003%
47	8.176	2114	2126	2142	rBV	128274	215108	13.98%	1.763%
48	8.359	2180	2183	2188	rBV2	400	322	0.02%	0.003%
49	8.552	2230	2243	2256	rBV	340912	577929	37.55%	4.736%
50	8.632	2257	2268	2301	rVV4	431361	927270	60.26%	7.599%
51	8.828	2325	2329	2331	rBV3	568	411	0.03%	0.003%
52	8.915	2348	2356	2361	rBV5	800	1006	0.07%	0.008%
53	8.951	2361	2367	2368	rBV	379	286	0.02%	0.002%
54	8.964	2368	2371	2378	rVB3	440	411	0.03%	0.003%
55	9.156	2428	2431	2438	rVB3	287	358	0.02%	0.003%
56	9.234	2450	2455	2458	rBV2	310	260	0.02%	0.002%
57	9.282	2465	2470	2475	rBV4	451	636	0.04%	0.005%
58	9.327	2481	2484	2486	rBV2	344	255	0.02%	0.002%
59	9.414	2498	2511	2538	rBV	688727	1154405	75.01%	9.460%
60	9.629	2575	2578	2582	rBV3	296	325	0.02%	0.003%
61	9.674	2585	2592	2594	rBV2	906	1142	0.07%	0.009%
62	9.780	2622	2625	2629	rVB2	365	262	0.02%	0.002%
63	9.918	2665	2668	2670	rBV	464	294	0.02%	0.002%
64	9.973	2681	2685	2689	rBV2	295	335	0.02%	0.003%
65	10.031	2699	2703	2708	rBV	327	290	0.02%	0.002%
66	10.481	2838	2843	2846	rBV3	561	352	0.02%	0.003%
67	10.500	2846	2849	2851	rBV2	550	346	0.02%	0.003%
68	10.706	2910	2913	2914	rBV	567	317	0.02%	0.003%
69	10.754	2915	2928	2948	rVV	555060	893258	58.05%	7.320%
70	10.947	2984	2988	2994	rBV2	490	433	0.03%	0.004%
71	11.066	3022	3025	3030	rBV2	301	342	0.02%	0.003%
72	11.365	3115	3118	3120	rBV	480	341	0.02%	0.003%
73	11.465	3145	3149	3152	rBV2	473	416	0.03%	0.003%
74	11.481	3152	3154	3161	rVB2	693	566	0.04%	0.005%
75	11.520	3161	3166	3167	rBV	407	304	0.02%	0.002%
76	11.745	3231	3236	3241	rBV3	744	946	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051060.D
 Acq On : 01 Oct 2022 01:52
 Operator : JC/MD
 Sample : N4869-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.809	3243	3256	3279	rBV	545343	874386	56.82%	7.165%
78	11.983	3306	3310	3313	rBV2	816	568	0.04%	0.005%
79	12.047	3326	3330	3333	rBV2	405	404	0.03%	0.003%
80	12.092	3341	3344	3345	rBV2	564	297	0.02%	0.002%
81	12.192	3359	3375	3398	rBV	555118	923085	59.98%	7.564%
82	12.365	3425	3429	3433	rBV4	830	616	0.04%	0.005%
83	12.455	3454	3457	3461	rBV	486	338	0.02%	0.003%
84	12.713	3533	3537	3540	rBV2	458	293	0.02%	0.002%
85	12.803	3560	3565	3572	rBV3	716	936	0.06%	0.008%
86	12.838	3572	3576	3579	rBV2	470	451	0.03%	0.004%
87	12.873	3584	3587	3588	rBV2	455	287	0.02%	0.002%
88	12.941	3606	3608	3613	rBV3	346	296	0.02%	0.002%
89	12.986	3619	3622	3625	rVB2	616	465	0.03%	0.004%
90	13.420	3753	3757	3758	rBV2	388	310	0.02%	0.003%
91	13.497	3779	3781	3785	rVB2	514	301	0.02%	0.002%
92	13.523	3785	3789	3793	rBV3	497	466	0.03%	0.004%
93	13.767	3859	3865	3868	rBV3	518	701	0.05%	0.006%
94	13.857	3891	3893	3899	rVB4	729	446	0.03%	0.004%
95	14.256	4014	4017	4018	rBV	838	437	0.03%	0.004%
96	14.732	4162	4165	4167	rBV2	707	477	0.03%	0.004%
97	14.783	4178	4181	4186	rBV2	691	657	0.04%	0.005%
98	15.182	4303	4305	4308	rBV2	475	309	0.02%	0.003%
99	15.555	4419	4421	4426	rVB3	754	458	0.03%	0.004%
100	16.314	4654	4657	4661	rBV4	1475	1114	0.07%	0.009%




Sum of corrected areas: 12203248

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051060.D
Acq On : 01 Oct 2022 01:52
Operator : JC/MD
Sample : N4869-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

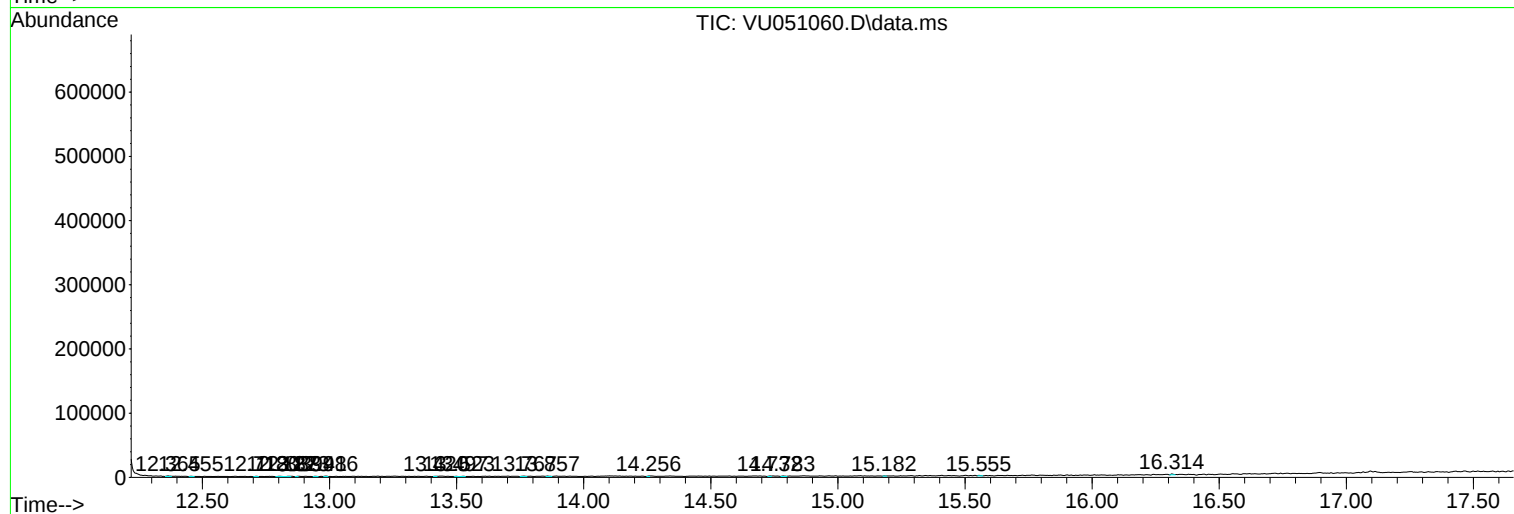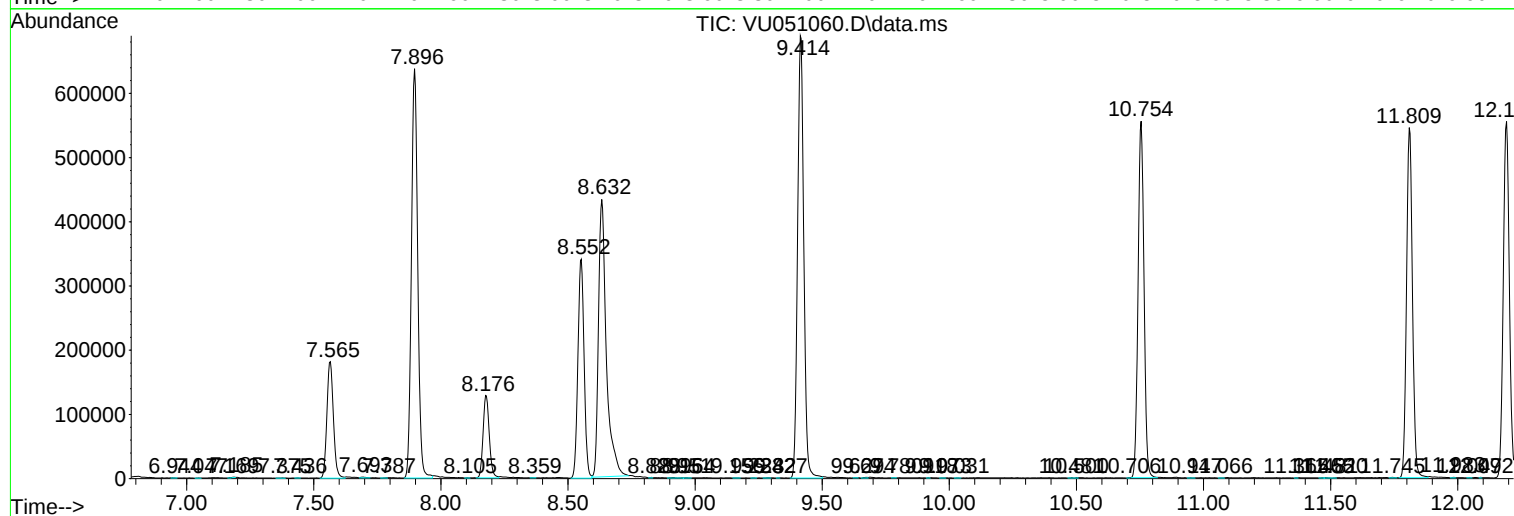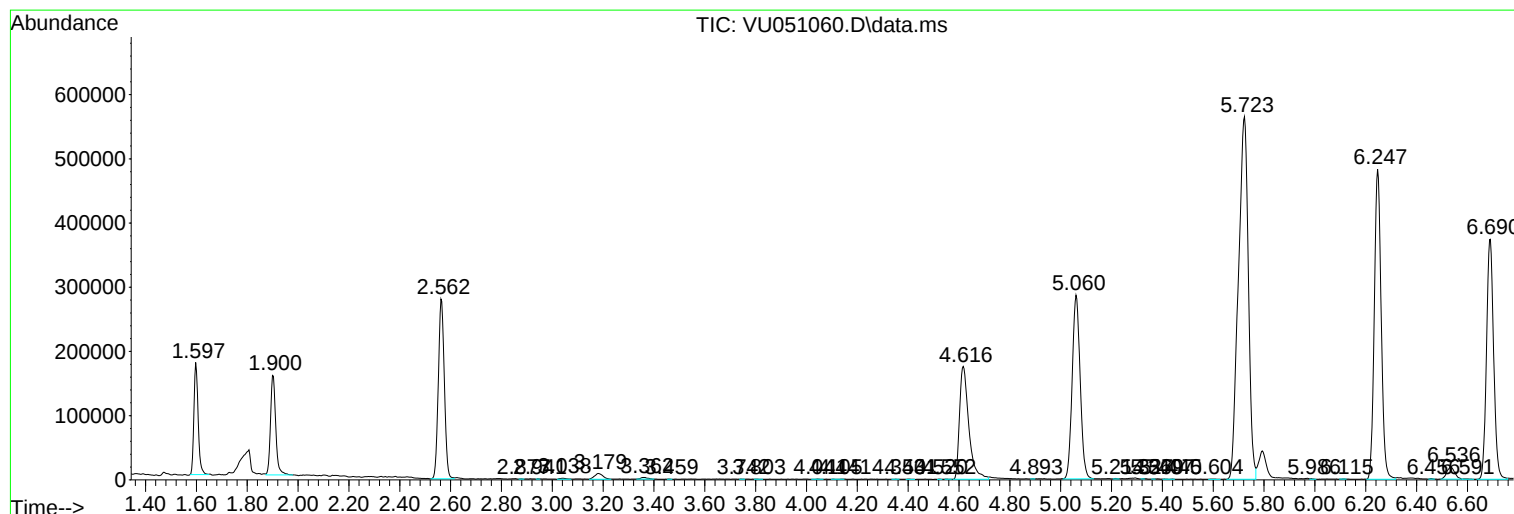

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051060.D
Acq On : 01 Oct 2022 01:52
Operator : JC/MD
Sample : N4869-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051060.D
Acq On : 01 Oct 2022 01:52
Operator : JC/MD
Sample : N4869-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------