

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051061.D
 Acq On : 01 Oct 2022 02:16
 Operator : JC/MD
 Sample : N4869-08DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J30DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	172938	202634	13.10%	1.552%
2	1.900	167	174	187	rVB	156276	203370	13.15%	1.558%
3	2.562	369	380	395	rBV	277891	448275	28.99%	3.434%
4	2.748	432	438	439	rBV3	597	589	0.04%	0.005%
5	3.044	518	530	540	rVB3	5075	8701	0.56%	0.067%
6	3.086	540	543	545	rBV	254	178	0.01%	0.001%
7	3.112	549	551	554	rVB2	325	167	0.01%	0.001%
8	3.182	558	573	598	rBV2	30328	73191	4.73%	0.561%
9	3.295	606	608	611	rBV	375	212	0.01%	0.002%
10	3.363	622	629	640	rVB6	3046	5882	0.38%	0.045%
11	3.488	665	668	673	rVV2	345	272	0.02%	0.002%
12	3.517	674	677	681	rVB2	456	337	0.02%	0.003%
13	3.571	691	694	696	rBV	315	188	0.01%	0.001%
14	3.658	718	721	723	rBV	318	150	0.01%	0.001%
15	3.774	753	757	760	rBV2	264	218	0.01%	0.002%
16	3.790	760	762	766	rVB2	308	168	0.01%	0.001%
17	3.916	798	801	803	rBV	202	147	0.01%	0.001%
18	4.034	832	838	839	rBV	264	288	0.02%	0.002%
19	4.096	851	857	862	rBV3	486	483	0.03%	0.004%
20	4.205	887	891	893	rBV2	489	363	0.02%	0.003%
21	4.260	905	908	912	rBB2	217	143	0.01%	0.001%
22	4.279	912	914	919	rVB2	400	249	0.02%	0.002%
23	4.308	919	923	927	rVB2	255	240	0.02%	0.002%
24	4.379	938	945	948	rBV2	373	501	0.03%	0.004%
25	4.514	983	987	996	rVB2	294	326	0.02%	0.002%
26	4.565	998	1003	1004	rBV	173	159	0.01%	0.001%
27	4.620	1007	1020	1049	rBV	182821	468282	30.28%	3.587%
28	5.060	1141	1157	1183	rVV	284123	629253	40.69%	4.820%
29	5.417	1265	1268	1271	rBV2	415	259	0.02%	0.002%
30	5.555	1308	1311	1314	rBV2	214	157	0.01%	0.001%
31	5.623	1330	1332	1339	rVB2	314	292	0.02%	0.002%
32	5.723	1341	1363	1384	rBV2	569732	1546307	100.00%	11.844%
33	6.038	1458	1461	1464	rBV2	458	412	0.03%	0.003%
34	6.102	1479	1481	1488	rBV4	432	543	0.04%	0.004%
35	6.176	1500	1504	1507	rVB2	309	237	0.02%	0.002%
36	6.195	1507	1510	1512	rBV2	354	261	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051061.D
 Acq On : 01 Oct 2022 02:16
 Operator : JC/MD
 Sample : N4869-08DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J30DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.247	1512	1526	1552	rBV	500240	944003	61.05%	7.231%
38	6.526	1603	1613	1631	rVV5	14902	32406	2.10%	0.248%
39	6.600	1631	1636	1642	rVB3	895	950	0.06%	0.007%
40	6.687	1649	1663	1685	rBV	374598	729125	47.15%	5.585%
41	6.886	1723	1725	1729	rVB2	539	346	0.02%	0.003%
42	6.906	1729	1731	1733	rBV2	445	260	0.02%	0.002%
43	6.938	1738	1741	1743	rBV2	244	169	0.01%	0.001%
44	6.954	1743	1746	1749	rVB	492	299	0.02%	0.002%
45	6.977	1749	1753	1755	rBV	452	324	0.02%	0.002%
46	6.989	1755	1757	1761	rBV2	481	350	0.02%	0.003%
47	7.034	1768	1771	1773	rBV2	241	161	0.01%	0.001%
48	7.112	1789	1795	1799	rVB3	408	441	0.03%	0.003%
49	7.240	1831	1835	1838	rBV2	333	288	0.02%	0.002%
50	7.330	1859	1863	1866	rBV2	258	228	0.01%	0.002%
51	7.385	1874	1880	1883	rBV2	345	436	0.03%	0.003%
52	7.407	1886	1887	1890	rBV	198	144	0.01%	0.001%
53	7.565	1922	1936	1952	rBV	180910	315630	20.41%	2.418%
54	7.796	2002	2008	2014	rBV3	656	797	0.05%	0.006%
55	7.896	2025	2039	2058	rBV	636051	1095880	70.87%	8.394%
56	8.179	2114	2127	2142	rBV	126516	216218	13.98%	1.656%
57	8.472	2216	2218	2221	rBV2	432	260	0.02%	0.002%
58	8.552	2228	2243	2257	rBV	778629	1310165	84.73%	10.035%
59	8.632	2258	2268	2304	rVB4	440370	948306	61.33%	7.264%
60	8.915	2350	2356	2360	rVB3	978	992	0.06%	0.008%
61	8.947	2360	2366	2369	rBV4	906	667	0.04%	0.005%
62	8.996	2378	2381	2383	rBV2	378	232	0.02%	0.002%
63	9.012	2384	2386	2390	rBV2	355	254	0.02%	0.002%
64	9.050	2395	2398	2400	rBV	336	180	0.01%	0.001%
65	9.118	2415	2419	2424	rBV2	284	252	0.02%	0.002%
66	9.166	2428	2434	2436	rBV2	443	407	0.03%	0.003%
67	9.266	2458	2465	2468	rBV3	506	513	0.03%	0.004%
68	9.337	2485	2487	2494	rBV2	352	352	0.02%	0.003%
69	9.414	2498	2511	2537	rBV	704536	1174600	75.96%	8.997%
70	9.568	2556	2559	2562	rBV5	401	350	0.02%	0.003%
71	9.661	2583	2588	2591	rBV2	330	375	0.02%	0.003%
72	9.825	2635	2639	2645	rVB2	487	519	0.03%	0.004%
73	9.857	2645	2649	2651	rBV2	329	278	0.02%	0.002%
74	9.899	2659	2662	2665	rBV	443	280	0.02%	0.002%
75	10.025	2698	2701	2704	rBV2	292	234	0.02%	0.002%
76	10.066	2710	2714	2718	rBV2	547	490	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051061.D
 Acq On : 01 Oct 2022 02:16
 Operator : JC/MD
 Sample : N4869-08DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J30DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.089	2718	2721	2723	rVV2	200	150	0.01%	0.001%
78	10.115	2727	2729	2734	rVB2	404	254	0.02%	0.002%
79	10.189	2749	2752	2756	rVB3	228	180	0.01%	0.001%
80	10.237	2764	2767	2769	rBV2	218	147	0.01%	0.001%
81	10.320	2790	2793	2796	rVV2	370	239	0.02%	0.002%
82	10.349	2796	2802	2804	rBV3	339	274	0.02%	0.002%
83	10.449	2829	2833	2836	rBV	332	321	0.02%	0.002%
84	10.523	2853	2856	2862	rVB3	439	475	0.03%	0.004%
85	10.552	2862	2865	2867	rBV	304	212	0.01%	0.002%
86	10.697	2908	2910	2912	rBV	269	162	0.01%	0.001%
87	10.754	2915	2928	2950	rVV	543987	881471	57.00%	6.752%
88	10.996	3000	3003	3006	rVB2	456	274	0.02%	0.002%
89	11.015	3006	3009	3011	rBV2	284	215	0.01%	0.002%
90	11.057	3020	3022	3024	rBV2	354	161	0.01%	0.001%
91	11.192	3057	3064	3067	rBV2	572	718	0.05%	0.005%
92	11.346	3109	3112	3114	rBV	400	259	0.02%	0.002%
93	11.484	3153	3155	3158	rBV	258	166	0.01%	0.001%
94	11.809	3244	3256	3271	rBV	560387	883323	57.12%	6.766%
95	12.127	3353	3355	3357	rBV	335	175	0.01%	0.001%
96	12.192	3363	3375	3396	rBV	569143	912594	59.02%	6.990%
97	12.346	3419	3423	3426	rBV2	956	914	0.06%	0.007%
98	13.012	3626	3630	3632	rBV3	470	395	0.03%	0.003%
99	13.060	3642	3645	3648	rBV2	437	345	0.02%	0.003%
100	14.542	4104	4106	4109	rBV2	889	603	0.04%	0.005%




Sum of corrected areas: 13055622

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051061.D
Acq On : 01 Oct 2022 02:16
Operator : JC/MD
Sample : N4869-08DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

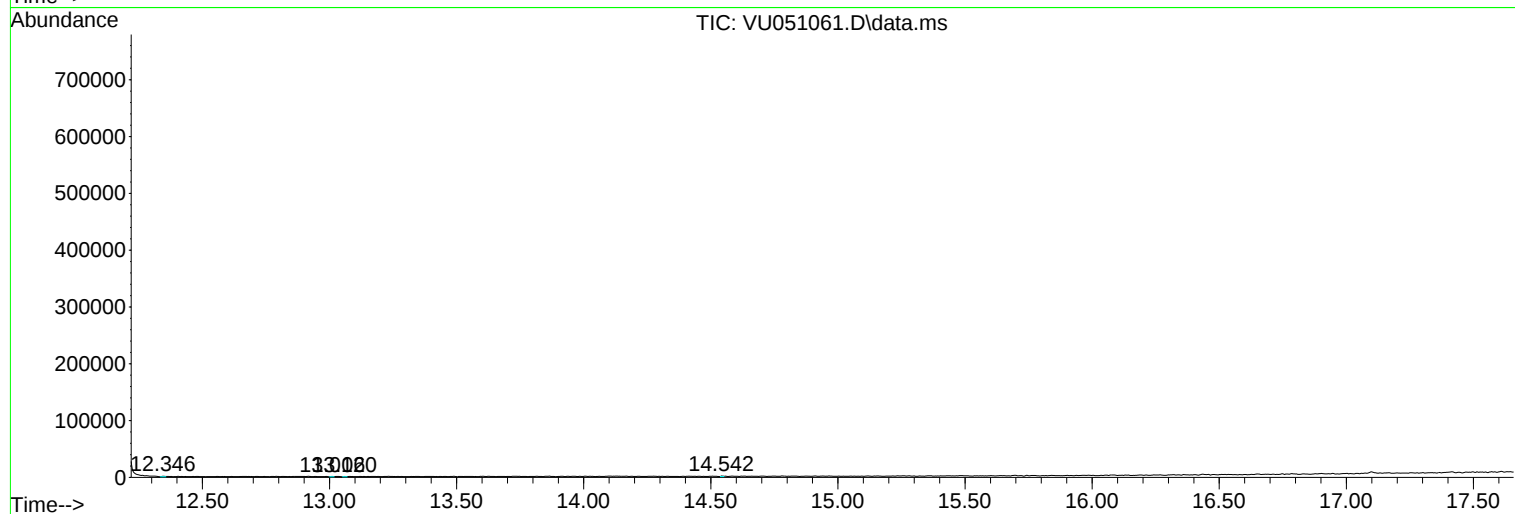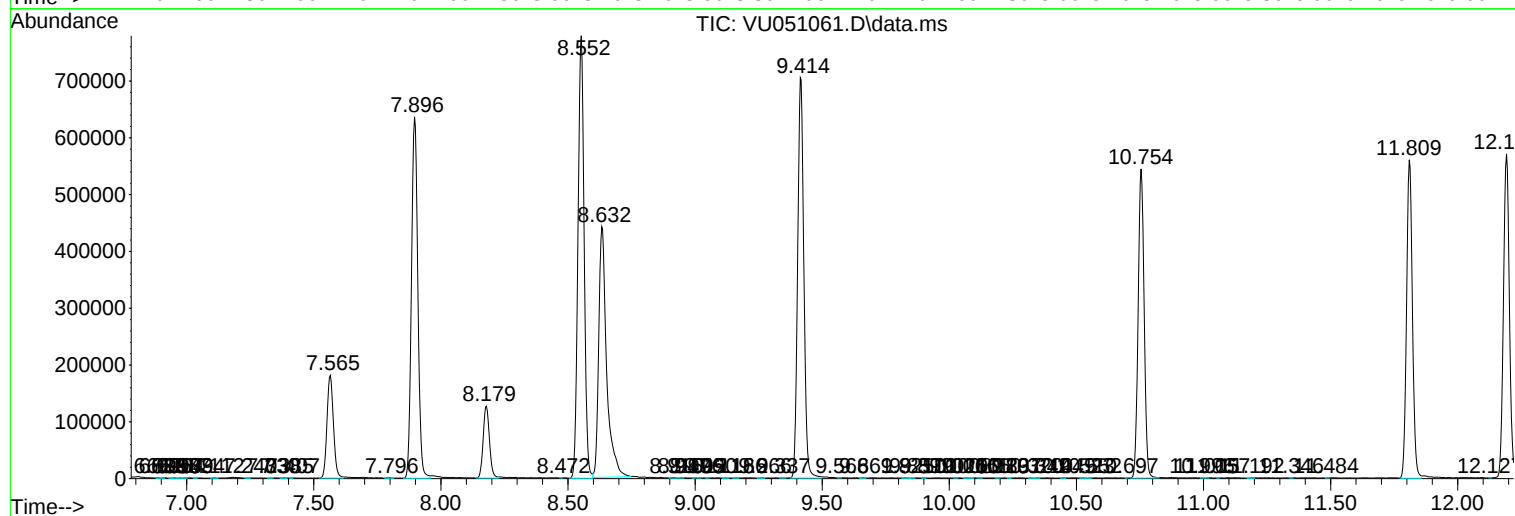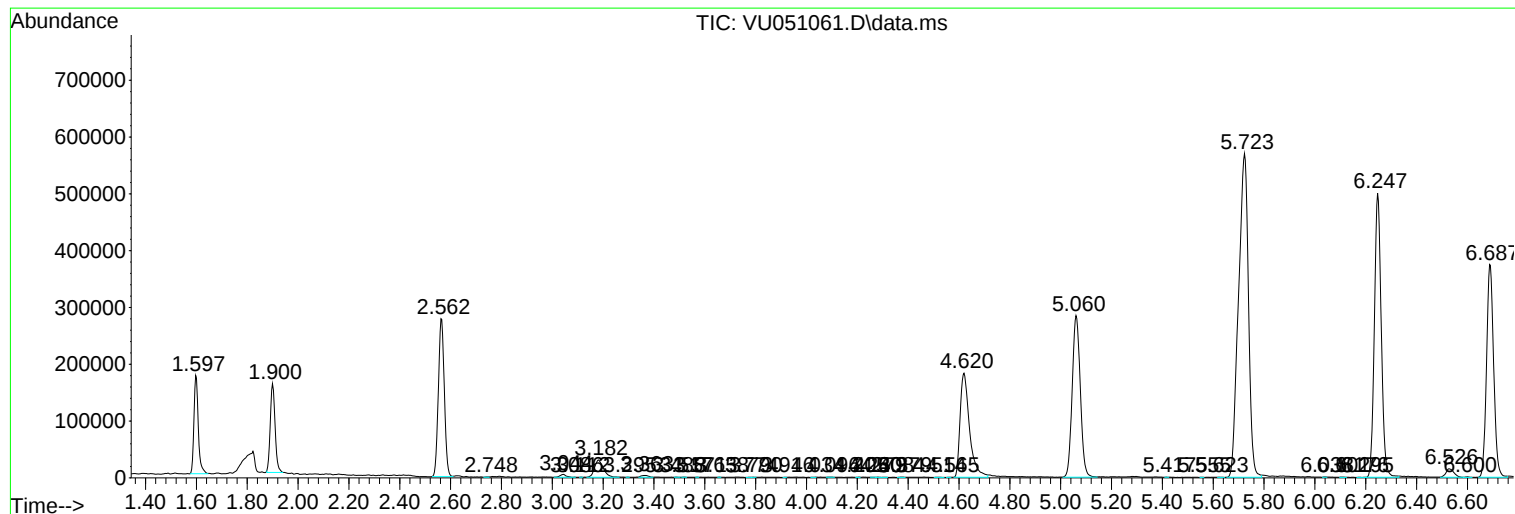

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051061.D
Acq On : 01 Oct 2022 02:16
Operator : JC/MD
Sample : N4869-08DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051061.D
Acq On : 01 Oct 2022 02:16
Operator : JC/MD
Sample : N4869-08DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc