

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051063.D
 Acq On : 01 Oct 2022 03:02
 Operator : JC/MD
 Sample : N4869-10DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J32DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	166481	193584	12.67%	1.556%
2	1.813	125	147	153	rBV3	36497	104589	6.85%	0.841%
3	1.900	165	174	187	rBV	153732	206310	13.51%	1.658%
4	2.562	368	380	395	rBV	259613	417039	27.31%	3.352%
5	2.871	472	476	478	rBV	372	277	0.02%	0.002%
6	2.957	499	503	509	rVB3	456	479	0.03%	0.004%
7	3.041	520	529	540	rBV4	6050	11212	0.73%	0.090%
8	3.182	558	573	590	rVV2	36272	84693	5.55%	0.681%
9	3.356	616	627	642	rVB7	4426	9096	0.60%	0.073%
10	3.787	755	761	764	rBV2	267	297	0.02%	0.002%
11	3.973	814	819	824	rVB3	318	328	0.02%	0.003%
12	4.308	919	923	925	rBV2	431	302	0.02%	0.002%
13	4.539	989	995	999	rBV2	355	389	0.03%	0.003%
14	4.562	999	1002	1007	rBV3	252	296	0.02%	0.002%
15	4.616	1007	1019	1051	rBV	197277	507659	33.24%	4.081%
16	4.915	1109	1112	1113	rBV	531	269	0.02%	0.002%
17	4.951	1120	1123	1126	rBV4	657	401	0.03%	0.003%
18	5.060	1140	1157	1184	rBV	290655	631666	41.36%	5.078%
19	5.369	1248	1253	1254	rBV3	538	421	0.03%	0.003%
20	5.407	1263	1265	1270	rVB2	584	462	0.03%	0.004%
21	5.433	1270	1273	1277	rBV2	496	413	0.03%	0.003%
22	5.530	1300	1303	1308	rVV2	451	337	0.02%	0.003%
23	5.639	1334	1337	1339	rBV	403	275	0.02%	0.002%
24	5.723	1342	1363	1390	rBV2	547374	1527309	100.00%	12.277%
25	5.977	1438	1442	1446	rVB4	720	589	0.04%	0.005%
26	6.070	1467	1471	1474	rBV3	353	329	0.02%	0.003%
27	6.118	1483	1486	1488	rBV2	490	304	0.02%	0.002%
28	6.157	1493	1498	1500	rBV2	597	505	0.03%	0.004%
29	6.247	1512	1526	1547	rBV	457367	859774	56.29%	6.911%
30	6.430	1581	1583	1586	rVB2	830	411	0.03%	0.003%
31	6.530	1602	1614	1628	rBV6	12882	27545	1.80%	0.221%
32	6.587	1628	1632	1637	rBV3	479	461	0.03%	0.004%
33	6.687	1648	1663	1684	rBV	377410	736753	48.24%	5.922%
34	6.980	1749	1754	1760	rBV	307	502	0.03%	0.004%
35	7.083	1779	1786	1789	rBV3	494	471	0.03%	0.004%
36	7.157	1803	1809	1811	rBV2	433	395	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051063.D
 Acq On : 01 Oct 2022 03:02
 Operator : JC/MD
 Sample : N4869-10DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J32DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.179	1811	1816	1817	rBV3	1001	687	0.04%	0.006%
38	7.359	1865	1872	1878	rBV2	400	554	0.04%	0.004%
39	7.388	1878	1881	1886	rVB2	372	319	0.02%	0.003%
40	7.423	1886	1892	1895	rBV	344	412	0.03%	0.003%
41	7.459	1901	1903	1908	rVB	429	289	0.02%	0.002%
42	7.565	1919	1936	1952	rBV	180418	314309	20.58%	2.527%
43	7.694	1971	1976	1977	rBV3	476	381	0.02%	0.003%
44	7.739	1987	1990	1993	rVB2	428	302	0.02%	0.002%
45	7.800	1999	2009	2012	rBV4	927	1252	0.08%	0.010%
46	7.896	2022	2039	2057	rBV	586513	998791	65.40%	8.029%
47	8.118	2106	2108	2111	rVB	480	277	0.02%	0.002%
48	8.137	2111	2114	2115	rBV	543	277	0.02%	0.002%
49	8.179	2115	2127	2148	rVV	132794	223863	14.66%	1.800%
50	8.439	2206	2208	2212	rVB2	498	319	0.02%	0.003%
51	8.462	2212	2215	2219	rBV2	803	654	0.04%	0.005%
52	8.552	2228	2243	2257	rBV	552063	933951	61.15%	7.508%
53	8.632	2257	2268	2304	rVB3	468288	997902	65.34%	8.022%
54	8.886	2342	2347	2349	rBV4	715	640	0.04%	0.005%
55	8.925	2356	2359	2365	rVB3	556	485	0.03%	0.004%
56	9.150	2425	2429	2434	rVB3	404	476	0.03%	0.004%
57	9.292	2469	2473	2476	rVB2	562	464	0.03%	0.004%
58	9.417	2495	2512	2537	rBV	637690	1070315	70.08%	8.604%
59	9.574	2558	2561	2565	rBV4	514	428	0.03%	0.003%
60	9.684	2592	2595	2597	rBV3	566	329	0.02%	0.003%
61	10.099	2721	2724	2726	rBV2	445	304	0.02%	0.002%
62	10.153	2738	2741	2744	rBV	472	290	0.02%	0.002%
63	10.218	2758	2761	2765	rBV2	629	506	0.03%	0.004%
64	10.343	2795	2800	2803	rBV2	355	420	0.03%	0.003%
65	10.362	2803	2806	2813	rVB	505	505	0.03%	0.004%
66	10.439	2826	2830	2834	rBV2	673	669	0.04%	0.005%
67	10.754	2914	2928	2949	rBV	575372	934964	61.22%	7.516%
68	10.851	2953	2958	2964	rVV4	768	761	0.05%	0.006%
69	10.902	2971	2974	2977	rVB2	479	303	0.02%	0.002%
70	10.967	2992	2994	2999	rVB3	409	375	0.02%	0.003%
71	11.147	3045	3050	3054	rBV3	521	537	0.04%	0.004%
72	11.587	3184	3187	3190	rBV2	509	323	0.02%	0.003%
73	11.729	3229	3231	3235	rVB	513	317	0.02%	0.003%
74	11.754	3237	3239	3242	rVB2	579	286	0.02%	0.002%
75	11.809	3242	3256	3272	rBV	478182	763577	49.99%	6.138%
76	12.050	3326	3331	3336	rBV2	579	732	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051063.D
 Acq On : 01 Oct 2022 03:02
 Operator : JC/MD
 Sample : N4869-10DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J32DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.192	3361	3375	3392	rBV	519068	849463	55.62%	6.828%
78	12.369	3424	3430	3432	rVB3	658	635	0.04%	0.005%
79	12.388	3432	3436	3442	rBV4	894	1019	0.07%	0.008%
80	12.478	3460	3464	3466	rBV3	558	396	0.03%	0.003%
81	12.645	3514	3516	3523	rVB3	607	557	0.04%	0.004%
82	12.873	3583	3587	3590	rBV3	344	376	0.02%	0.003%
83	12.951	3608	3611	3613	rBV	484	294	0.02%	0.002%
84	13.034	3631	3637	3641	rBV2	838	832	0.05%	0.007%
85	13.224	3693	3696	3698	rBV	541	272	0.02%	0.002%
86	13.262	3706	3708	3712	rVB4	488	363	0.02%	0.003%
87	13.285	3713	3715	3725	rVB4	479	696	0.05%	0.006%
88	13.340	3728	3732	3734	rBV2	646	488	0.03%	0.004%
89	13.372	3739	3742	3745	rBV2	469	401	0.03%	0.003%
90	13.468	3767	3772	3779	rBV3	640	927	0.06%	0.007%
91	13.909	3904	3909	3912	rBV	447	438	0.03%	0.004%
92	14.034	3944	3948	3950	rBV2	346	293	0.02%	0.002%
93	14.111	3969	3972	3974	rBV2	480	378	0.02%	0.003%
94	14.179	3990	3993	3996	rBV3	417	300	0.02%	0.002%
95	14.340	4040	4043	4049	rVB5	637	554	0.04%	0.004%
96	14.542	4103	4106	4109	rBV2	415	296	0.02%	0.002%
97	14.822	4191	4193	4196	rVB2	558	294	0.02%	0.002%
98	14.841	4196	4199	4202	rBV3	638	470	0.03%	0.004%
99	15.298	4338	4341	4343	rBV2	725	498	0.03%	0.004%
100	15.783	4488	4492	4494	rBV4	1183	1040	0.07%	0.008%




Sum of corrected areas: 12439967

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051063.D
Acq On : 01 Oct 2022 03:02
Operator : JC/MD
Sample : N4869-10DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

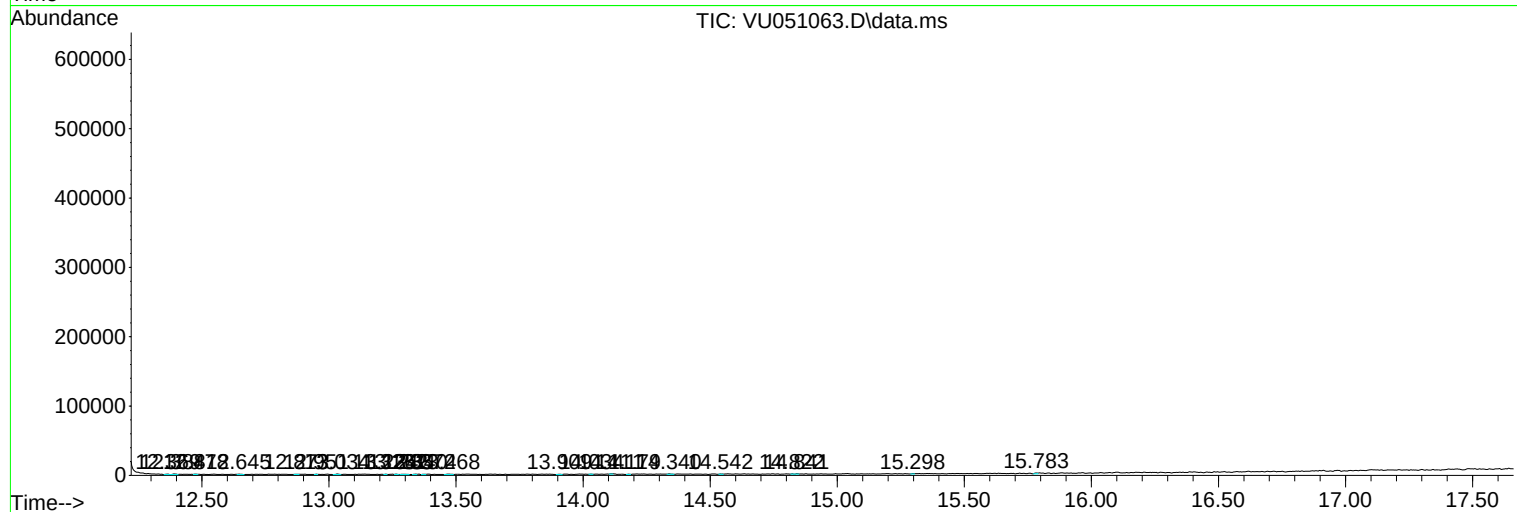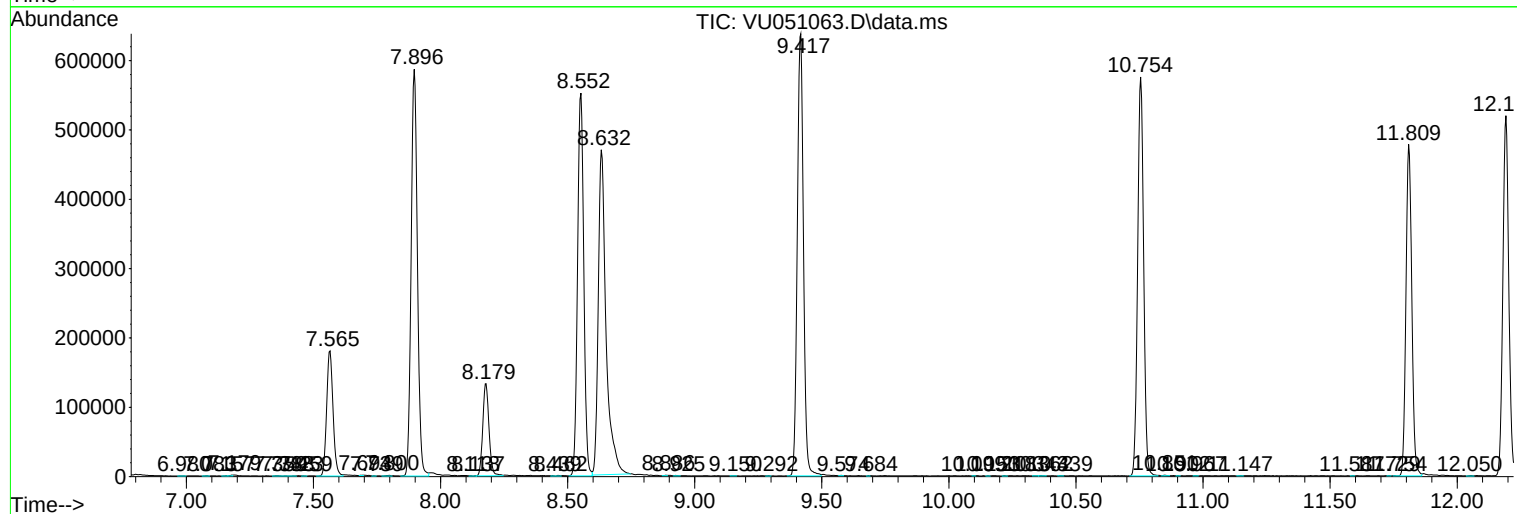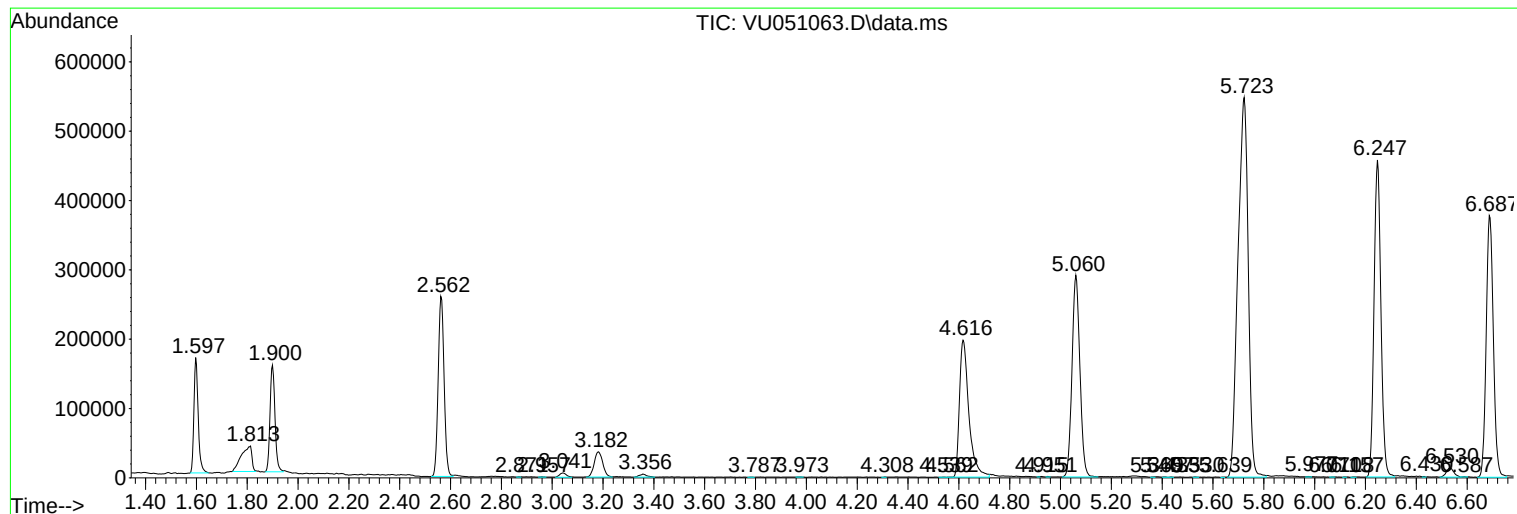

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051063.D
Acq On : 01 Oct 2022 03:02
Operator : JC/MD
Sample : N4869-10DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051063.D
Acq On : 01 Oct 2022 03:02
Operator : JC/MD
Sample : N4869-10DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------