

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051064.D
 Acq On : 01 Oct 2022 03:26
 Operator : JC/MD
 Sample : N4869-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rBV	278025	324478	16.49%	2.213%
2	1.900	166	174	198	rVB	215698	298994	15.20%	2.039%
3	2.565	368	381	394	rBV	391631	639865	32.52%	4.364%
4	2.681	410	417	426	rVB4	2983	5000	0.25%	0.034%
5	2.774	443	446	447	rBV2	596	359	0.02%	0.002%
6	2.822	458	461	466	rBV2	494	530	0.03%	0.004%
7	2.928	491	494	496	rBV3	435	305	0.02%	0.002%
8	3.112	548	551	555	rVB2	730	597	0.03%	0.004%
9	3.137	555	559	560	rBV2	546	366	0.02%	0.002%
10	3.179	560	572	591	rVB	7615	17852	0.91%	0.122%
11	3.353	612	626	643	rBV2	70835	142441	7.24%	0.971%
12	3.469	659	662	665	rBV2	422	370	0.02%	0.003%
13	3.485	665	667	672	rVB3	564	317	0.02%	0.002%
14	3.517	672	677	680	rBV2	479	457	0.02%	0.003%
15	3.719	736	740	744	rVB3	388	326	0.02%	0.002%
16	3.848	772	780	792	rBV4	2306	5248	0.27%	0.036%
17	3.951	806	812	814	rBV2	279	312	0.02%	0.002%
18	4.009	828	830	835	rVB2	596	376	0.02%	0.003%
19	4.099	854	858	862	rVB2	336	349	0.02%	0.002%
20	4.308	920	923	930	rVB2	334	408	0.02%	0.003%
21	4.414	951	956	959	rVB2	585	466	0.02%	0.003%
22	4.433	959	962	965	rBV	416	309	0.02%	0.002%
23	4.555	990	1000	1003	rBV3	601	754	0.04%	0.005%
24	4.617	1003	1019	1052	rBV	205438	592476	30.12%	4.041%
25	4.854	1090	1093	1096	rBV2	564	493	0.03%	0.003%
26	5.060	1138	1157	1178	rBV	364430	790571	40.18%	5.392%
27	5.247	1211	1215	1219	rBV4	672	715	0.04%	0.005%
28	5.379	1250	1256	1260	rBV4	592	509	0.03%	0.003%
29	5.411	1264	1266	1269	rBV	535	392	0.02%	0.003%
30	5.723	1339	1363	1386	rBV2	727802	1967366	100.00%	13.417%
31	6.031	1456	1459	1463	rBV2	600	399	0.02%	0.003%
32	6.060	1466	1468	1474	rVB3	601	497	0.03%	0.003%
33	6.089	1474	1477	1479	rBV2	393	306	0.02%	0.002%
34	6.115	1479	1485	1489	rVV4	740	842	0.04%	0.006%
35	6.247	1511	1526	1549	rVV	478843	906306	46.07%	6.181%
36	6.436	1582	1585	1590	rVB3	863	503	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051064.D
 Acq On : 01 Oct 2022 03:26
 Operator : JC/MD
 Sample : N4869-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.526	1603	1613	1629	rVB7	12309	25909	1.32%	0.177%
38	6.620	1639	1642	1648	rVB3	500	387	0.02%	0.003%
39	6.687	1648	1663	1685	rBV	475397	921372	46.83%	6.284%
40	7.157	1806	1809	1810	rBV	802	360	0.02%	0.002%
41	7.240	1831	1835	1840	rBV2	303	337	0.02%	0.002%
42	7.433	1892	1895	1900	rBV2	440	391	0.02%	0.003%
43	7.565	1922	1936	1955	rBV	226021	397282	20.19%	2.709%
44	7.694	1973	1976	1978	rBV3	640	380	0.02%	0.003%
45	7.793	2004	2007	2011	rBV	623	603	0.03%	0.004%
46	7.896	2024	2039	2057	rBV	826795	1420702	72.21%	9.689%
47	8.176	2114	2126	2145	rBV	165072	279520	14.21%	1.906%
48	8.552	2230	2243	2256	rBV	257304	432096	21.96%	2.947%
49	8.632	2256	2268	2303	rVV3	529614	1137976	57.84%	7.761%
50	8.919	2354	2357	2364	rVV4	685	669	0.03%	0.005%
51	9.047	2393	2397	2401	rBV2	317	306	0.02%	0.002%
52	9.169	2433	2435	2445	rVB4	719	900	0.05%	0.006%
53	9.414	2496	2511	2532	rBV	707831	1156494	58.78%	7.887%
54	9.555	2553	2555	2559	rBV4	804	579	0.03%	0.004%
55	9.684	2592	2595	2599	rBV4	455	403	0.02%	0.003%
56	9.771	2614	2622	2633	rBV3	6331	9210	0.47%	0.063%
57	9.899	2658	2662	2667	rBV3	442	461	0.02%	0.003%
58	10.021	2694	2700	2704	rVB3	380	457	0.02%	0.003%
59	10.378	2807	2811	2817	rBV2	349	503	0.03%	0.003%
60	10.420	2818	2824	2827	rVV2	399	419	0.02%	0.003%
61	10.529	2849	2858	2872	rVB2	4915	9344	0.47%	0.064%
62	10.642	2888	2893	2895	rBV2	604	469	0.02%	0.003%
63	10.665	2895	2900	2905	rBV2	292	331	0.02%	0.002%
64	10.687	2905	2907	2910	rVB2	526	312	0.02%	0.002%
65	10.755	2915	2928	2950	rBV	680058	1090743	55.44%	7.439%
66	11.025	3009	3012	3016	rVV2	359	352	0.02%	0.002%
67	11.086	3027	3031	3033	rBV2	522	387	0.02%	0.003%
68	11.169	3051	3057	3059	rBV2	349	355	0.02%	0.002%
69	11.224	3070	3074	3079	rVB3	524	449	0.02%	0.003%
70	11.253	3079	3083	3087	rBV	540	538	0.03%	0.004%
71	11.533	3166	3170	3175	rVB3	408	449	0.02%	0.003%
72	11.809	3244	3256	3279	rBV	550219	875268	44.49%	5.969%
73	12.037	3324	3327	3331	rVB3	417	388	0.02%	0.003%
74	12.095	3341	3345	3348	rBV2	432	337	0.02%	0.002%
75	12.115	3348	3351	3355	rVB2	529	366	0.02%	0.002%
76	12.192	3361	3375	3394	rBV	722662	1178924	59.92%	8.040%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051064.D
 Acq On : 01 Oct 2022 03:26
 Operator : JC/MD
 Sample : N4869-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.401	3437	3440	3443	rVB2	1001	597	0.03%	0.004%
78	12.420	3443	3446	3448	rBV2	397	308	0.02%	0.002%
79	12.523	3472	3478	3484	rVB2	380	589	0.03%	0.004%
80	13.176	3679	3681	3687	rVB3	630	460	0.02%	0.003%
81	13.208	3687	3691	3693	rBV2	582	500	0.03%	0.003%
82	13.272	3708	3711	3714	rBV2	569	454	0.02%	0.003%
83	13.352	3733	3736	3739	rBV	471	389	0.02%	0.003%
84	13.478	3772	3775	3778	rBV2	650	482	0.02%	0.003%
85	13.545	3791	3796	3799	rBV2	523	526	0.03%	0.004%
86	13.610	3812	3816	3818	rBV3	611	421	0.02%	0.003%
87	13.938	3913	3918	3922	rBV4	547	627	0.03%	0.004%
88	14.012	3939	3941	3945	rBV2	430	387	0.02%	0.003%
89	14.272	4020	4022	4025	rBV2	459	317	0.02%	0.002%
90	14.751	4168	4171	4177	rBV2	674	676	0.03%	0.005%
91	14.812	4186	4190	4195	rBV4	844	852	0.04%	0.006%
92	15.008	4249	4251	4255	rVB	700	466	0.02%	0.003%
93	15.073	4268	4271	4274	rBV	588	445	0.02%	0.003%
94	15.114	4280	4284	4287	rBV3	692	694	0.04%	0.005%
95	15.288	4336	4338	4341	rBV4	520	312	0.02%	0.002%
96	15.407	4373	4375	4379	rVB4	1156	601	0.03%	0.004%
97	15.623	4438	4442	4447	rBV4	1099	1286	0.07%	0.009%
98	15.725	4471	4474	4475	rBV3	890	504	0.03%	0.003%
99	15.893	4523	4526	4529	rBV3	1205	986	0.05%	0.007%
100	16.073	4579	4582	4588	rVB6	1387	1319	0.07%	0.009%




Sum of corrected areas: 14662780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051064.D
Acq On : 01 Oct 2022 03:26
Operator : JC/MD
Sample : N4869-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

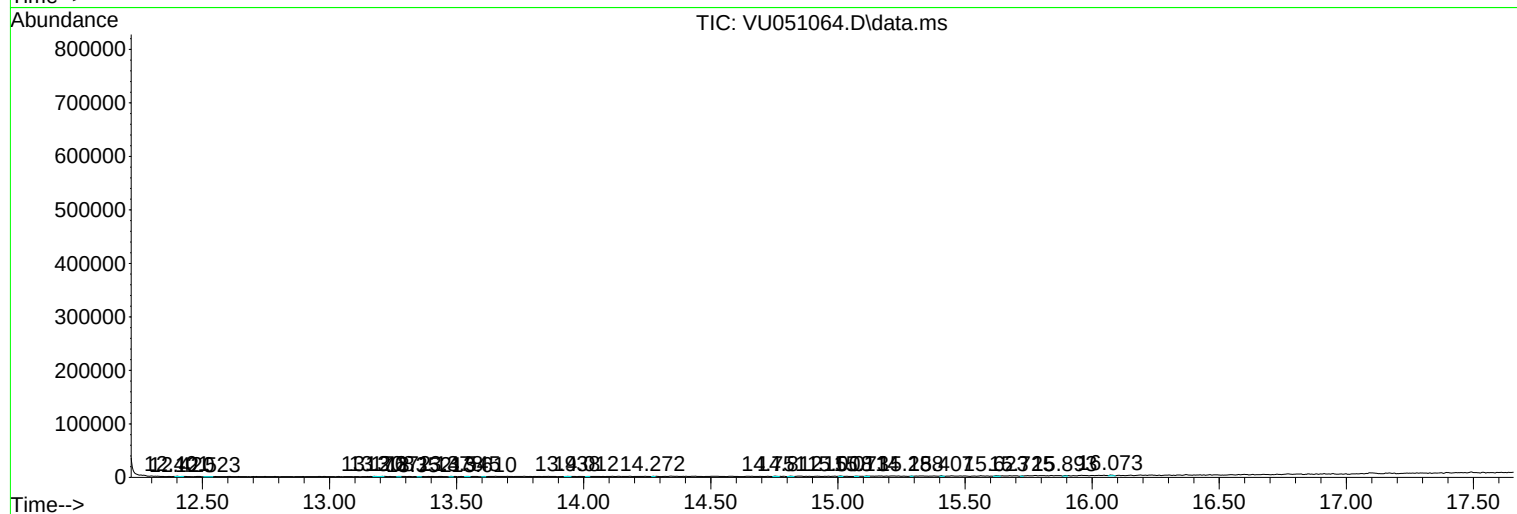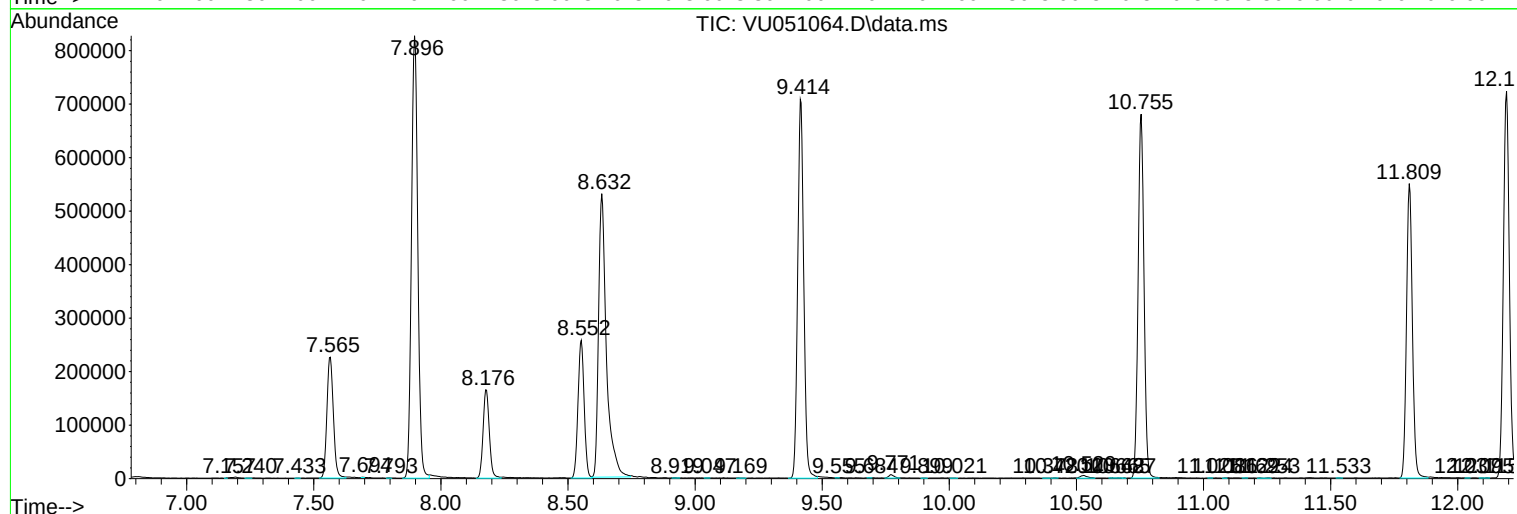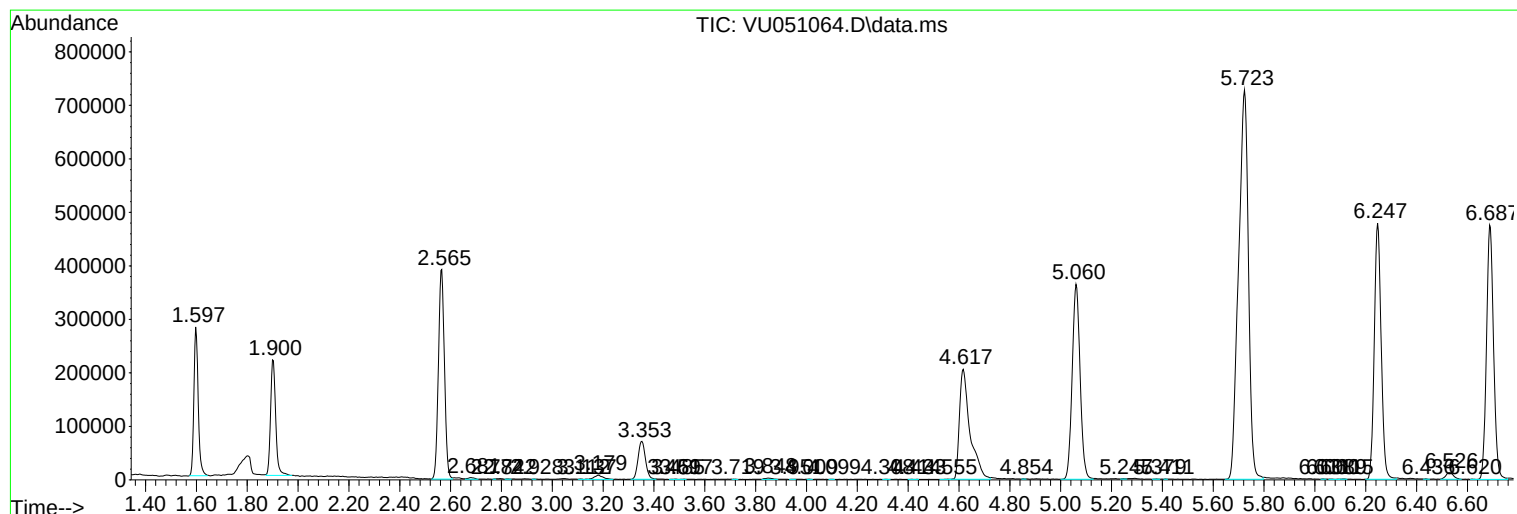

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051064.D
Acq On : 01 Oct 2022 03:26
Operator : JC/MD
Sample : N4869-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051064.D
Acq On : 01 Oct 2022 03:26
Operator : JC/MD
Sample : N4869-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc