

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051066.D
 Acq On : 01 Oct 2022 04:12
 Operator : JC/MD
 Sample : N4880-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051066.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.356	3	5	15	rVB	17054	14991	0.74%	0.105%
2	1.597	72	80	95	rBV	286794	335192	16.63%	2.338%
3	1.900	165	174	198	rVB	223224	310192	15.39%	2.164%
4	2.562	365	380	394	rBV	403353	655410	32.51%	4.571%
5	2.858	460	472	478	rBV6	2342	4071	0.20%	0.028%
6	2.970	505	507	511	rVB2	442	265	0.01%	0.002%
7	2.996	513	515	519	rVB3	587	347	0.02%	0.002%
8	3.018	519	522	524	rBV	548	350	0.02%	0.002%
9	3.131	555	557	560	rBV2	491	343	0.02%	0.002%
10	3.182	562	573	588	rVB	4582	9828	0.49%	0.069%
11	3.408	638	643	647	rBV2	359	313	0.02%	0.002%
12	3.453	654	657	661	rBV2	443	305	0.02%	0.002%
13	3.565	689	692	694	rBV3	832	462	0.02%	0.003%
14	3.584	694	698	704	rVB7	1299	1317	0.07%	0.009%
15	3.694	724	732	733	rBV	399	427	0.02%	0.003%
16	3.864	781	785	795	rVB3	429	740	0.04%	0.005%
17	3.916	795	801	806	rBV2	509	602	0.03%	0.004%
18	3.989	821	824	827	rBV	410	289	0.01%	0.002%
19	4.356	935	938	942	rVB2	475	376	0.02%	0.003%
20	4.465	965	972	973	rBV3	334	325	0.02%	0.002%
21	4.530	988	992	995	rBV2	405	330	0.02%	0.002%
22	4.616	1006	1019	1062	rBV	204592	512460	25.42%	3.574%
23	4.797	1073	1075	1079	rVB3	695	482	0.02%	0.003%
24	4.954	1121	1124	1128	rVB3	439	354	0.02%	0.002%
25	5.060	1140	1157	1181	rBV	369483	818859	40.62%	5.711%
26	5.205	1199	1202	1203	rBV2	592	332	0.02%	0.002%
27	5.333	1240	1242	1246	rBV	558	306	0.02%	0.002%
28	5.366	1249	1252	1255	rBV2	536	325	0.02%	0.002%
29	5.504	1290	1295	1299	rBV2	476	485	0.02%	0.003%
30	5.723	1339	1363	1390	rBV2	746980	2015766	100.00%	14.059%
31	6.160	1496	1499	1502	rBV2	331	281	0.01%	0.002%
32	6.247	1511	1526	1553	rBV	488199	925425	45.91%	6.455%
33	6.526	1602	1613	1627	rVB4	12203	24801	1.23%	0.173%
34	6.587	1627	1632	1633	rBV2	523	449	0.02%	0.003%
35	6.687	1648	1663	1684	rBV	482693	939056	46.59%	6.550%
36	6.996	1755	1759	1761	rVV2	363	333	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051066.D
 Acq On : 01 Oct 2022 04:12
 Operator : JC/MD
 Sample : N4880-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.022	1764	1767	1771	rBV3	390	270	0.01%	0.002%
38	7.189	1810	1819	1828	rVV6	1501	3117	0.15%	0.022%
39	7.330	1860	1863	1866	rBV2	401	308	0.02%	0.002%
40	7.430	1891	1894	1901	rVB2	446	424	0.02%	0.003%
41	7.565	1922	1936	1954	rBV	227945	406634	20.17%	2.836%
42	7.800	2005	2009	2012	rBV4	716	555	0.03%	0.004%
43	7.896	2025	2039	2058	rBV	857375	1447886	71.83%	10.099%
44	8.176	2115	2126	2142	rBV	162909	276035	13.69%	1.925%
45	8.459	2209	2214	2216	rBV2	812	683	0.03%	0.005%
46	8.552	2232	2243	2255	rVB2	54326	89364	4.43%	0.623%
47	8.632	2255	2268	2309	rBV3	534898	1145545	56.83%	7.990%
48	8.957	2366	2369	2371	rBV2	419	285	0.01%	0.002%
49	9.012	2378	2386	2387	rBV3	439	448	0.02%	0.003%
50	9.137	2422	2425	2430	rVV2	340	319	0.02%	0.002%
51	9.163	2430	2433	2437	rVB	387	290	0.01%	0.002%
52	9.205	2442	2446	2449	rVB2	394	319	0.02%	0.002%
53	9.414	2498	2511	2540	rBV	696309	1162460	57.67%	8.108%
54	9.648	2579	2584	2587	rVB2	620	572	0.03%	0.004%
55	9.697	2592	2599	2607	rBV4	765	1135	0.06%	0.008%
56	9.848	2641	2646	2651	rBV3	850	1158	0.06%	0.008%
57	9.912	2662	2666	2670	rVB3	615	561	0.03%	0.004%
58	9.935	2670	2673	2679	rVB2	427	421	0.02%	0.003%
59	9.989	2685	2690	2695	rBV3	515	630	0.03%	0.004%
60	10.012	2695	2697	2703	rVB2	369	288	0.01%	0.002%
61	10.044	2703	2707	2710	rVB2	348	275	0.01%	0.002%
62	10.108	2721	2727	2734	rBV4	612	921	0.05%	0.006%
63	10.298	2782	2786	2789	rBV2	330	261	0.01%	0.002%
64	10.343	2795	2800	2801	rBV2	848	617	0.03%	0.004%
65	10.398	2813	2817	2823	rBV2	432	533	0.03%	0.004%
66	10.481	2839	2843	2844	rBV	525	352	0.02%	0.002%
67	10.558	2864	2867	2871	rBV	532	480	0.02%	0.003%
68	10.655	2894	2897	2898	rBV2	591	308	0.02%	0.002%
69	10.754	2915	2928	2945	rBV	688046	1108367	54.98%	7.731%
70	10.880	2964	2967	2975	rVB3	807	971	0.05%	0.007%
71	10.980	2993	2998	3001	rBV2	407	395	0.02%	0.003%
72	11.047	3017	3019	3023	rVB	536	294	0.01%	0.002%
73	11.111	3034	3039	3042	rVB2	511	454	0.02%	0.003%
74	11.401	3127	3129	3132	rVV2	416	313	0.02%	0.002%
75	11.426	3135	3137	3143	rVB	402	307	0.02%	0.002%
76	11.594	3187	3189	3194	rVB2	417	327	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051066.D
 Acq On : 01 Oct 2022 04:12
 Operator : JC/MD
 Sample : N4880-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.632	3194	3201	3211	rBV3	841	1375	0.07%	0.010%
78	11.687	3211	3218	3225	rBV5	2247	3292	0.16%	0.023%
79	11.738	3231	3234	3237	rBV2	437	329	0.02%	0.002%
80	11.809	3244	3256	3273	rBV	557969	889728	44.14%	6.206%
81	12.021	3320	3322	3326	rBV2	576	351	0.02%	0.002%
82	12.050	3327	3331	3332	rBV2	1048	554	0.03%	0.004%
83	12.076	3333	3339	3349	rVB8	2752	5051	0.25%	0.035%
84	12.192	3362	3375	3397	rBV	745129	1194889	59.28%	8.334%
85	12.324	3413	3416	3423	rVB5	746	672	0.03%	0.005%
86	12.391	3433	3437	3440	rBV3	656	446	0.02%	0.003%
87	12.491	3462	3468	3473	rBV3	464	569	0.03%	0.004%
88	12.787	3557	3560	3566	rVB2	574	603	0.03%	0.004%
89	12.893	3587	3593	3600	rBV6	2396	2869	0.14%	0.020%
90	13.005	3623	3628	3629	rBV2	582	457	0.02%	0.003%
91	13.188	3679	3685	3687	rBV4	580	528	0.03%	0.004%
92	13.243	3699	3702	3705	rBV2	341	271	0.01%	0.002%
93	13.385	3743	3746	3752	rVB3	757	739	0.04%	0.005%
94	13.491	3775	3779	3783	rBV2	497	465	0.02%	0.003%
95	13.809	3871	3878	3884	rBV	638	1009	0.05%	0.007%
96	14.028	3943	3946	3949	rBV3	689	359	0.02%	0.003%
97	14.095	3963	3967	3972	rBV5	1039	926	0.05%	0.006%
98	14.278	4021	4024	4027	rBV3	468	262	0.01%	0.002%
99	14.333	4039	4041	4046	rVB4	621	353	0.02%	0.002%
100	14.844	4197	4200	4201	rBV	493	306	0.02%	0.002%




Sum of corrected areas: 14337474

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051066.D
Acq On : 01 Oct 2022 04:12
Operator : JC/MD
Sample : N4880-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

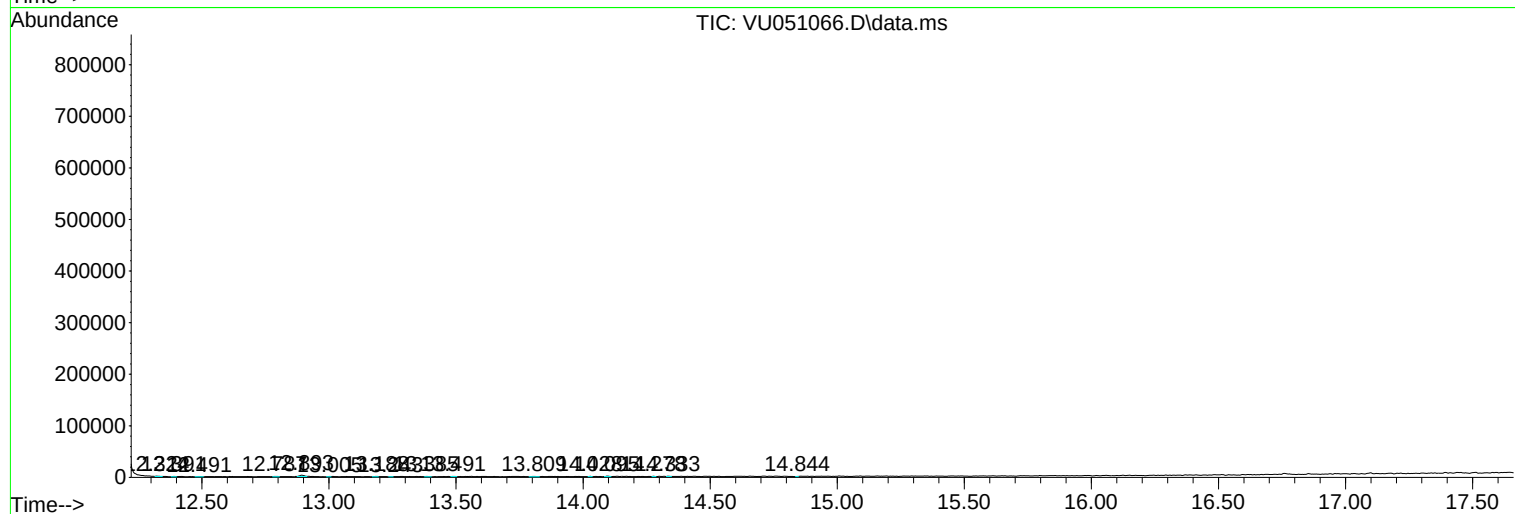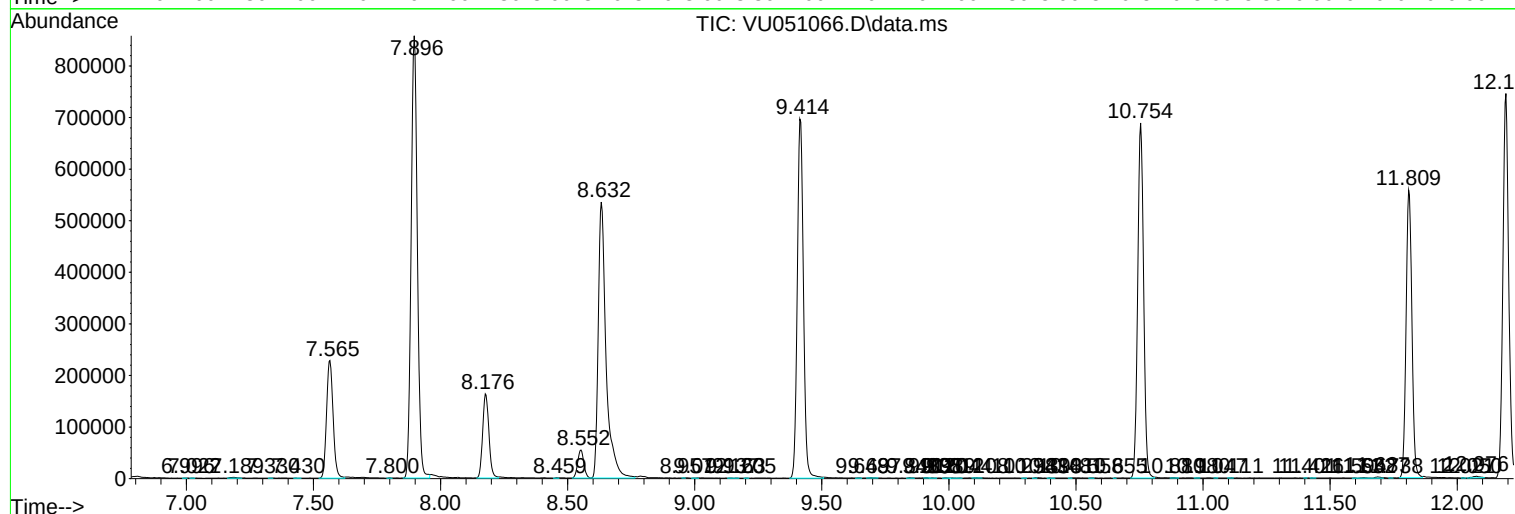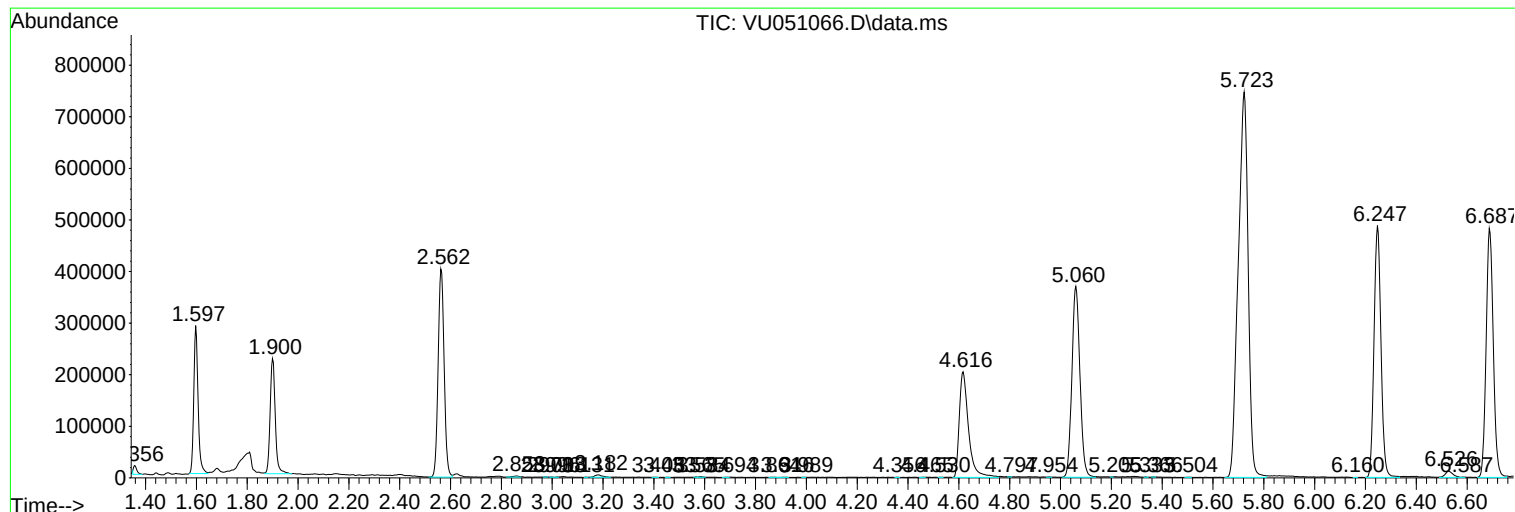

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051066.D
Acq On : 01 Oct 2022 04:12
Operator : JC/MD
Sample : N4880-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051066.D
Acq On : 01 Oct 2022 04:12
Operator : JC/MD
Sample : N4880-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc