

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051067.D
 Acq On : 01 Oct 2022 04:36
 Operator : JC/MD
 Sample : N4880-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rBV	273307	320403	16.17%	2.283%
2	1.903	166	175	187	rBV	215764	290020	14.63%	2.066%
3	2.565	368	381	396	rBV	388239	641149	32.35%	4.568%
4	2.719	425	429	432	rBV3	487	328	0.02%	0.002%
5	2.758	438	441	443	rBV3	692	494	0.02%	0.004%
6	2.848	466	469	472	rBV3	521	431	0.02%	0.003%
7	2.935	493	496	499	rVB	543	339	0.02%	0.002%
8	3.002	515	517	524	rVB4	322	298	0.02%	0.002%
9	3.041	524	529	536	rBV3	1330	1560	0.08%	0.011%
10	3.092	541	545	549	rBV	389	385	0.02%	0.003%
11	3.179	559	572	591	rVB3	7827	18970	0.96%	0.135%
12	3.292	603	607	610	rVB3	836	700	0.04%	0.005%
13	3.440	647	653	655	rBV3	481	513	0.03%	0.004%
14	3.452	655	657	662	rVB2	541	354	0.02%	0.003%
15	3.594	696	701	705	rBV2	459	549	0.03%	0.004%
16	3.710	732	737	740	rBV2	522	474	0.02%	0.003%
17	3.787	757	761	764	rBV2	348	306	0.02%	0.002%
18	3.819	765	771	776	rVB2	411	575	0.03%	0.004%
19	4.340	925	933	936	rVB	280	339	0.02%	0.002%
20	4.417	951	957	960	rBV	281	306	0.02%	0.002%
21	4.536	988	994	997	rBV2	340	364	0.02%	0.003%
22	4.616	1005	1019	1056	rBV	204153	508739	25.67%	3.625%
23	4.941	1117	1120	1125	rVB3	463	393	0.02%	0.003%
24	5.060	1139	1157	1181	rBV	357602	789613	39.84%	5.626%
25	5.282	1221	1226	1236	rVB6	1547	2572	0.13%	0.018%
26	5.324	1236	1239	1244	rBV3	416	329	0.02%	0.002%
27	5.420	1266	1269	1273	rBV2	500	422	0.02%	0.003%
28	5.517	1292	1299	1303	rVB3	550	667	0.03%	0.005%
29	5.722	1338	1363	1392	rBV2	730618	1981817	100.00%	14.120%
30	5.973	1438	1441	1444	rBV5	732	381	0.02%	0.003%
31	6.063	1467	1469	1475	rVB2	452	344	0.02%	0.002%
32	6.246	1511	1526	1544	rBV	481818	906502	45.74%	6.459%
33	6.529	1603	1614	1628	rBV4	14715	28359	1.43%	0.202%
34	6.687	1649	1663	1686	rBV	468180	925675	46.71%	6.595%
35	6.967	1743	1750	1752	rBV2	583	522	0.03%	0.004%
36	7.140	1800	1804	1807	rVB2	482	381	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051067.D
 Acq On : 01 Oct 2022 04:36
 Operator : JC/MD
 Sample : N4880-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.182	1807	1817	1819	rBV3	1372	1953	0.10%	0.014%
38	7.256	1834	1840	1844	rBV2	465	564	0.03%	0.004%
39	7.275	1844	1846	1850	rVB	487	308	0.02%	0.002%
40	7.343	1859	1867	1873	rBV2	340	516	0.03%	0.004%
41	7.565	1922	1936	1954	rBV	222737	394537	19.91%	2.811%
42	7.681	1970	1972	1975	rBV3	480	309	0.02%	0.002%
43	7.754	1991	1995	2001	rVB3	508	588	0.03%	0.004%
44	7.790	2001	2006	2011	rBV4	545	655	0.03%	0.005%
45	7.896	2024	2039	2070	rBV	821249	1428255	72.07%	10.176%
46	8.176	2115	2126	2151	rBV	160655	274713	13.86%	1.957%
47	8.262	2151	2153	2155	rVV3	630	312	0.02%	0.002%
48	8.320	2169	2171	2176	rBV3	425	318	0.02%	0.002%
49	8.484	2219	2222	2228	rVB3	902	744	0.04%	0.005%
50	8.552	2232	2243	2256	rBV2	76188	129937	6.56%	0.926%
51	8.632	2256	2268	2304	rBV2	518260	1120952	56.56%	7.987%
52	9.024	2386	2390	2395	rBV3	437	389	0.02%	0.003%
53	9.050	2395	2398	2405	rVB2	427	408	0.02%	0.003%
54	9.131	2417	2423	2429	rVB4	555	716	0.04%	0.005%
55	9.259	2457	2463	2466	rVB	385	319	0.02%	0.002%
56	9.295	2469	2474	2480	rVB3	379	433	0.02%	0.003%
57	9.414	2498	2511	2541	rBV	691385	1152707	58.16%	8.213%
58	9.658	2582	2587	2593	rVB3	527	665	0.03%	0.005%
59	9.687	2593	2596	2599	rBV3	606	567	0.03%	0.004%
60	9.796	2624	2630	2633	rBV	418	381	0.02%	0.003%
61	10.224	2758	2763	2768	rVB2	567	500	0.03%	0.004%
62	10.346	2792	2801	2806	rBV3	571	709	0.04%	0.005%
63	10.426	2821	2826	2829	rBV	432	386	0.02%	0.003%
64	10.549	2860	2864	2868	rVB2	421	344	0.02%	0.002%
65	10.754	2915	2928	2945	rBV	666104	1074672	54.23%	7.657%
66	10.889	2967	2970	2977	rVB3	531	594	0.03%	0.004%
67	10.995	2998	3003	3004	rBV	402	339	0.02%	0.002%
68	11.031	3011	3014	3021	rBV3	355	309	0.02%	0.002%
69	11.060	3021	3023	3027	rVB2	608	336	0.02%	0.002%
70	11.082	3027	3030	3033	rBV2	571	361	0.02%	0.003%
71	11.121	3037	3042	3048	rVB3	563	591	0.03%	0.004%
72	11.166	3052	3056	3061	rVB3	437	447	0.02%	0.003%
73	11.221	3070	3073	3076	rBV	542	337	0.02%	0.002%
74	11.256	3076	3084	3085	rBV	279	306	0.02%	0.002%
75	11.372	3115	3120	3124	rVB3	585	564	0.03%	0.004%
76	11.417	3129	3134	3136	rBV2	749	463	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051067.D
 Acq On : 01 Oct 2022 04:36
 Operator : JC/MD
 Sample : N4880-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.632	3196	3201	3204	rBV2	549	438	0.02%	0.003%
78	11.693	3209	3220	3227	rBV8	1754	2706	0.14%	0.019%
79	11.745	3229	3236	3238	rBV3	826	721	0.04%	0.005%
80	11.809	3244	3256	3276	rBV	527887	851967	42.99%	6.070%
81	12.069	3328	3337	3344	rBV7	3877	6961	0.35%	0.050%
82	12.140	3356	3359	3361	rVB3	693	386	0.02%	0.003%
83	12.192	3361	3375	3397	rBV	702353	1143382	57.69%	8.146%
84	12.368	3428	3430	3433	rVB2	517	296	0.01%	0.002%
85	12.442	3450	3453	3454	rBV	596	309	0.02%	0.002%
86	12.532	3478	3481	3487	rBV	508	505	0.03%	0.004%
87	12.680	3524	3527	3531	rBV2	542	488	0.02%	0.003%
88	12.735	3539	3544	3547	rBV2	451	463	0.02%	0.003%
89	12.754	3547	3550	3553	rVV2	572	498	0.03%	0.004%
90	12.777	3555	3557	3561	rVB2	442	324	0.02%	0.002%
91	12.893	3587	3593	3602	rBV5	2527	3388	0.17%	0.024%
92	13.159	3673	3676	3684	rVB3	513	513	0.03%	0.004%
93	13.269	3707	3710	3715	rVB2	441	369	0.02%	0.003%
94	13.433	3756	3761	3763	rBV3	474	384	0.02%	0.003%
95	13.532	3788	3792	3798	rVB3	531	475	0.02%	0.003%
96	13.571	3798	3804	3806	rBV2	660	689	0.03%	0.005%
97	13.629	3820	3822	3829	rVB2	702	596	0.03%	0.004%
98	14.716	4157	4160	4165	rBV3	650	611	0.03%	0.004%
99	15.018	4252	4254	4258	rBV2	702	405	0.02%	0.003%
100	15.436	4382	4384	4388	rBV4	851	470	0.02%	0.003%




Sum of corrected areas: 14035421

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051067.D
Acq On : 01 Oct 2022 04:36
Operator : JC/MD
Sample : N4880-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

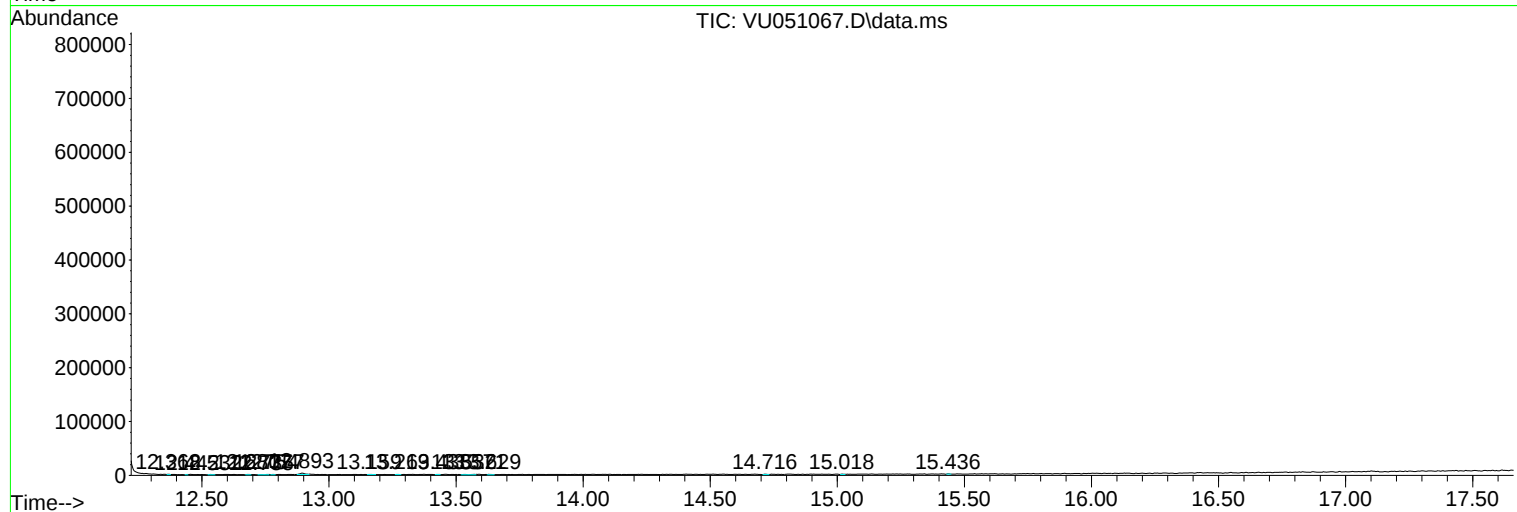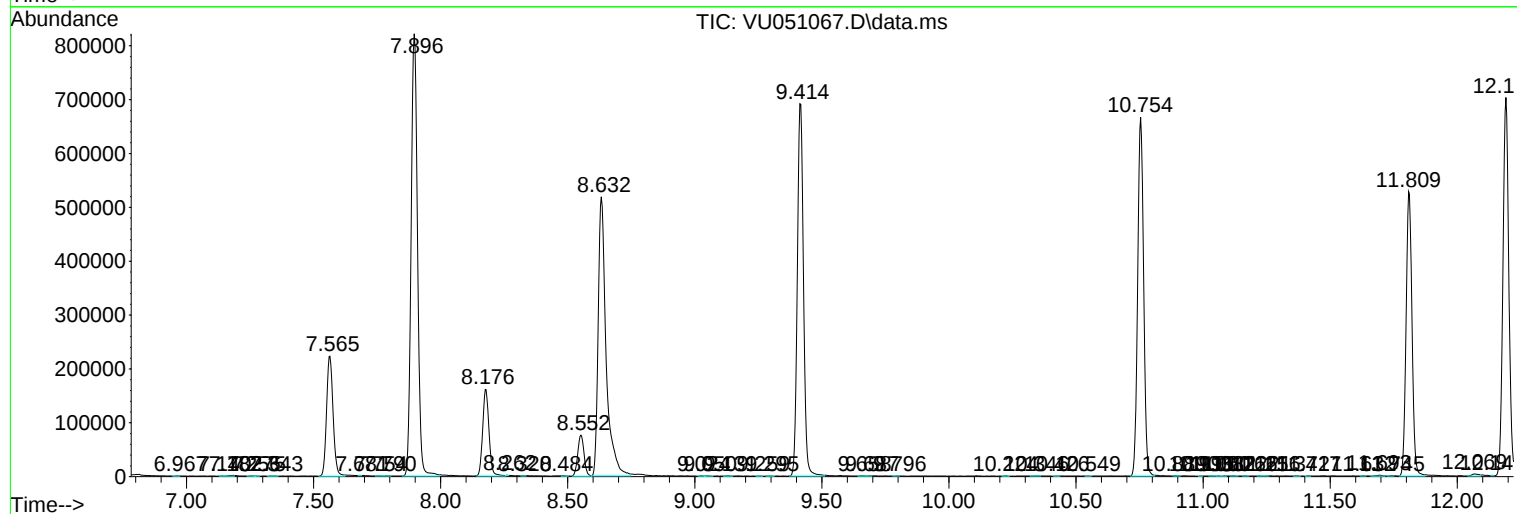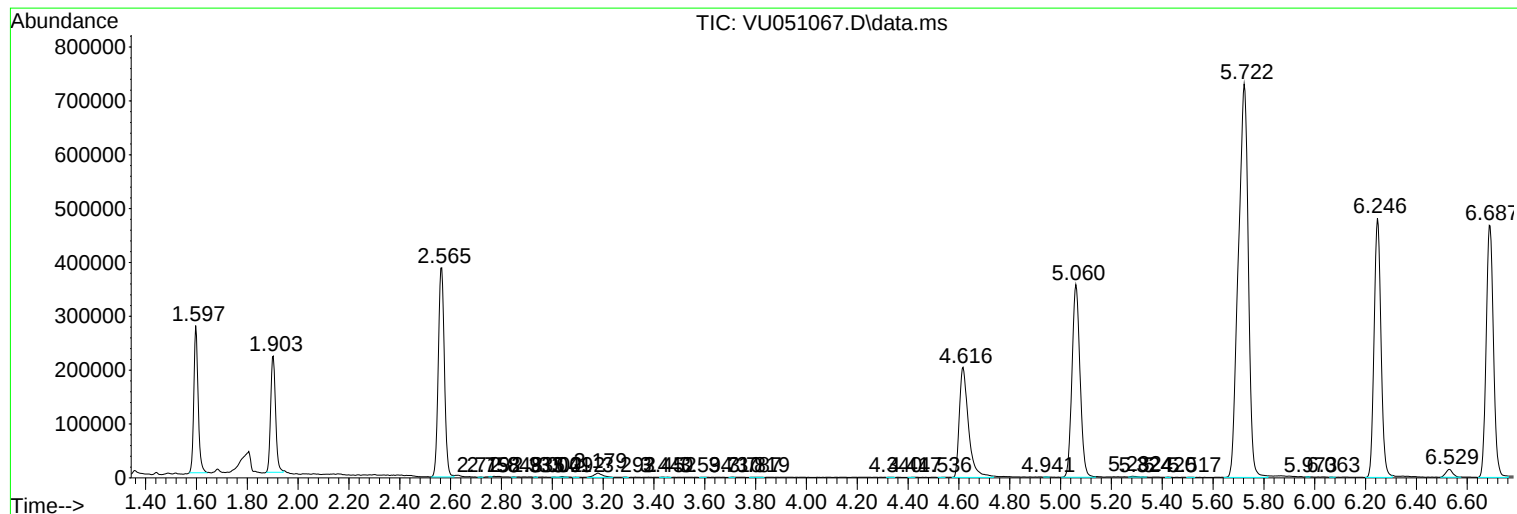

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051067.D
Acq On : 01 Oct 2022 04:36
Operator : JC/MD
Sample : N4880-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051067.D
Acq On : 01 Oct 2022 04:36
Operator : JC/MD
Sample : N4880-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------