

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051070.D
 Acq On : 01 Oct 2022 05:45
 Operator : JC/MD
 Sample : N4880-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	96	rVB	281752	334955	16.72%	2.366%
2	1.900	167	174	195	rVB	218669	297603	14.85%	2.103%
3	2.562	367	380	393	rBV	401510	653267	32.61%	4.615%
4	2.948	498	500	506	rVB3	757	680	0.03%	0.005%
5	2.977	506	509	512	rBV	466	382	0.02%	0.003%
6	3.080	539	541	542	rBV	178	59	0.00%	0.000%
7	3.093	542	545	549	rVB3	669	552	0.03%	0.004%
8	3.122	549	554	558	rBV4	719	810	0.04%	0.006%
9	3.180	562	572	589	rVB6	2681	6530	0.33%	0.046%
10	3.247	589	593	597	rBV3	505	394	0.02%	0.003%
11	3.328	616	618	620	rBV	480	228	0.01%	0.002%
12	3.437	650	652	654	rBV	218	112	0.01%	0.001%
13	3.585	689	698	711	rVB8	1868	4161	0.21%	0.029%
14	3.681	725	728	729	rBV	360	198	0.01%	0.001%
15	3.742	744	747	753	rVB2	400	342	0.02%	0.002%
16	3.819	768	771	773	rBV	296	212	0.01%	0.001%
17	3.964	813	816	819	rVB3	335	195	0.01%	0.001%
18	3.983	819	822	823	rBV	182	108	0.01%	0.001%
19	4.099	854	858	859	rBV	156	123	0.01%	0.001%
20	4.160	875	877	883	rVB2	439	348	0.02%	0.002%
21	4.196	883	888	892	rBV3	412	434	0.02%	0.003%
22	4.215	892	894	898	rVB2	547	341	0.02%	0.002%
23	4.237	898	901	903	rBV	112	77	0.00%	0.001%
24	4.247	903	904	907	rBV	126	41	0.00%	0.000%
25	4.276	911	913	916	rBV	253	186	0.01%	0.001%
26	4.430	958	961	962	rBV2	419	221	0.01%	0.002%
27	4.569	1002	1004	1006	rBV	320	123	0.01%	0.001%
28	4.617	1006	1019	1044	rBV	199391	503060	25.11%	3.554%
29	5.061	1140	1157	1183	rBV	365416	806971	40.28%	5.701%
30	5.414	1262	1267	1270	rBV3	387	374	0.02%	0.003%
31	5.459	1278	1281	1284	rBV2	213	222	0.01%	0.002%
32	5.623	1329	1332	1335	rBV	298	250	0.01%	0.002%
33	5.639	1335	1337	1338	rBV	216	74	0.00%	0.001%
34	5.723	1341	1363	1391	rBV2	733378	2003527	100.00%	14.155%
35	6.192	1507	1509	1512	rVB2	290	134	0.01%	0.001%
36	6.247	1512	1526	1546	rBV	474666	907337	45.29%	6.410%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051070.D
 Acq On : 01 Oct 2022 05:45
 Operator : JC/MD
 Sample : N4880-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.530	1603	1614	1628	rVB8	12052	26105	1.30%	0.184%
38	6.588	1628	1632	1636	rBV4	768	727	0.04%	0.005%
39	6.630	1641	1645	1648	rBV2	801	581	0.03%	0.004%
40	6.688	1648	1663	1684	rBV	471777	928702	46.35%	6.561%
41	6.942	1740	1742	1743	rBV	495	267	0.01%	0.002%
42	7.138	1800	1803	1805	rBV	234	148	0.01%	0.001%
43	7.179	1811	1816	1817	rBV2	858	695	0.03%	0.005%
44	7.331	1860	1863	1865	rBV2	335	250	0.01%	0.002%
45	7.446	1893	1899	1903	rBV2	398	524	0.03%	0.004%
46	7.482	1907	1910	1915	rBV2	462	396	0.02%	0.003%
47	7.507	1915	1918	1923	rBV2	326	319	0.02%	0.002%
48	7.562	1923	1935	1954	rBV	221298	391951	19.56%	2.769%
49	7.896	2025	2039	2055	rBV	826310	1423146	71.03%	10.055%
50	8.176	2114	2126	2144	rBV	158262	273314	13.64%	1.931%
51	8.443	2207	2209	2210	rBV	470	172	0.01%	0.001%
52	8.552	2232	2243	2255	rBV2	80205	134058	6.69%	0.947%
53	8.633	2256	2268	2308	rBV3	516650	1121238	55.96%	7.922%
54	8.954	2364	2368	2369	rBV	510	298	0.01%	0.002%
55	9.257	2460	2462	2468	rVB2	335	251	0.01%	0.002%
56	9.282	2468	2470	2473	rBV2	487	306	0.02%	0.002%
57	9.414	2498	2511	2544	rBV	699168	1156287	57.71%	8.169%
58	9.568	2555	2559	2562	rBV4	1097	1007	0.05%	0.007%
59	9.681	2591	2594	2595	rBV2	876	466	0.02%	0.003%
60	9.922	2667	2669	2671	rBV	313	169	0.01%	0.001%
61	10.279	2777	2780	2782	rBV	250	178	0.01%	0.001%
62	10.353	2796	2803	2808	rBV5	1155	1596	0.08%	0.011%
63	10.472	2835	2840	2844	rBV4	707	742	0.04%	0.005%
64	10.520	2852	2855	2862	rBV2	459	536	0.03%	0.004%
65	10.623	2883	2887	2891	rBV2	450	394	0.02%	0.003%
66	10.755	2915	2928	2953	rBV	701075	1120080	55.91%	7.913%
67	11.086	3027	3031	3034	rBV2	385	441	0.02%	0.003%
68	11.266	3084	3087	3089	rBV2	373	182	0.01%	0.001%
69	11.279	3089	3091	3093	rBV	268	130	0.01%	0.001%
70	11.809	3243	3256	3275	rBV	539295	859370	42.89%	6.072%
71	12.070	3327	3337	3353	rBV9	6560	13895	0.69%	0.098%
72	12.192	3361	3375	3401	rBV	718766	1167232	58.26%	8.247%
73	12.411	3438	3443	3448	rBV5	777	795	0.04%	0.006%
74	12.893	3589	3593	3597	rBV3	1688	1734	0.09%	0.012%
75	12.980	3617	3620	3624	rBV3	750	747	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051070.D
Acq On : 01 Oct 2022 05:45
Operator : JC/MD
Sample : N4880-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Title : VOC Analysis




Sum of corrected areas: 14154060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051070.D
Acq On : 01 Oct 2022 05:45
Operator : JC/MD
Sample : N4880-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

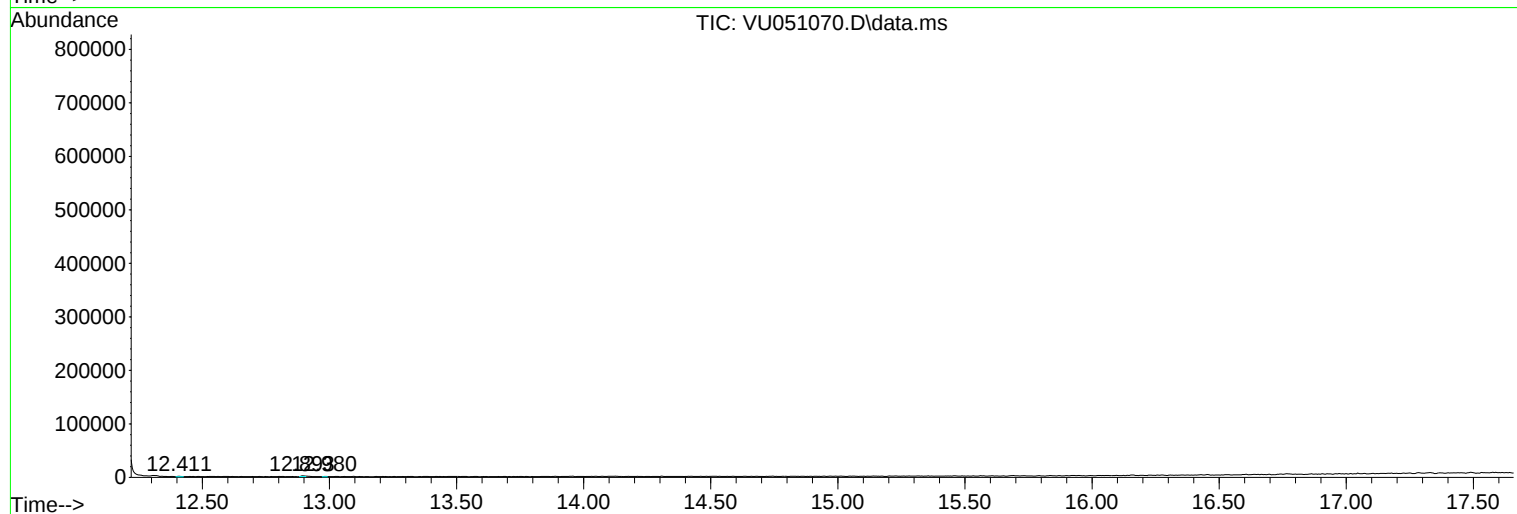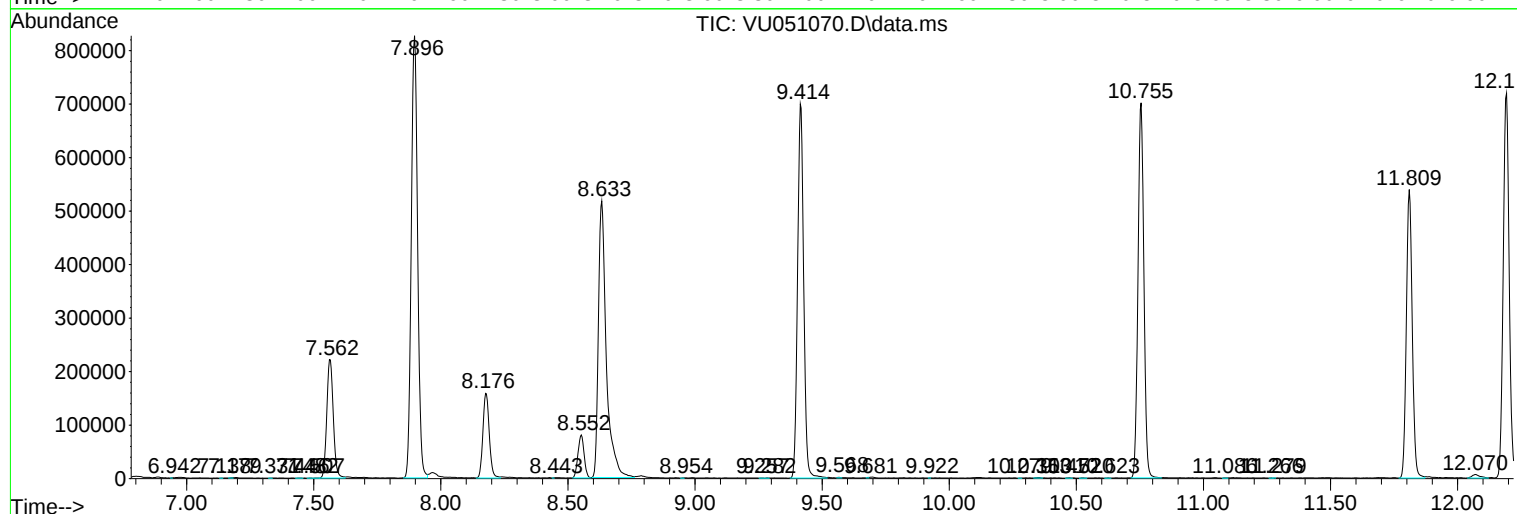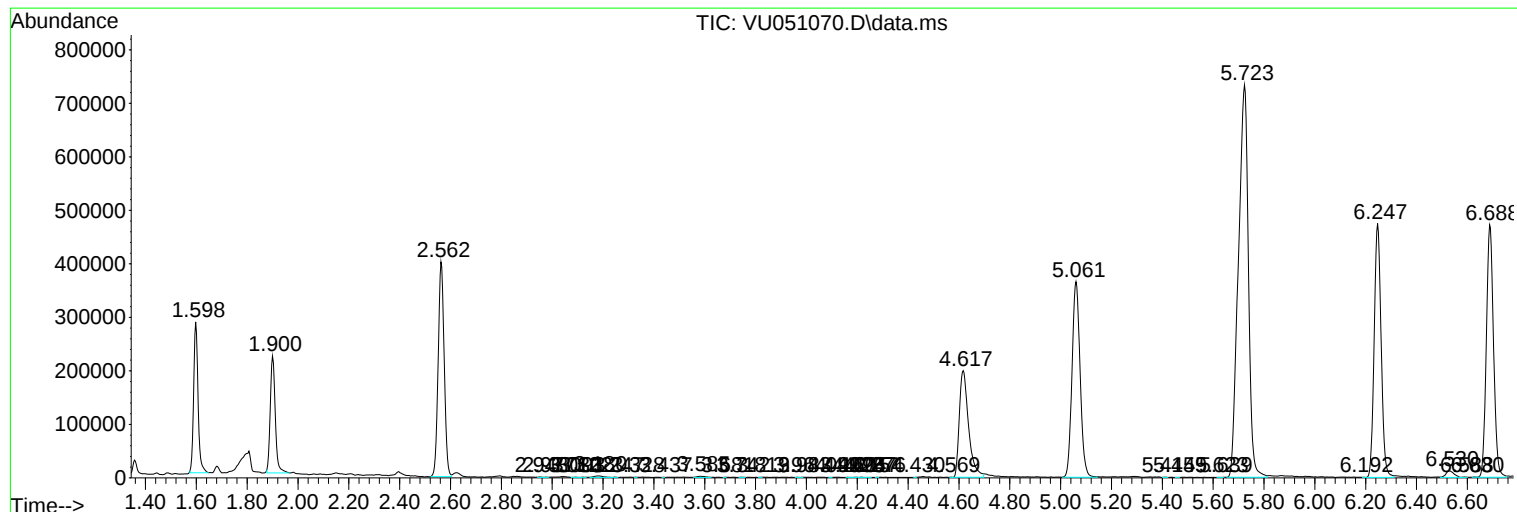

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051070.D
Acq On : 01 Oct 2022 05:45
Operator : JC/MD
Sample : N4880-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051070.D
Acq On : 01 Oct 2022 05:45
Operator : JC/MD
Sample : N4880-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc