

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051072.D
 Acq On : 01 Oct 2022 06:32
 Operator : JC/MD
 Sample : N4880-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.356	3	5	18	rVB4	10912	10828	0.54%	0.075%
2	1.597	71	80	100	rBV	281941	334853	16.63%	2.331%
3	1.900	165	174	194	rBV	223847	306307	15.21%	2.132%
4	2.472	350	352	359	rVB3	795	803	0.04%	0.006%
5	2.504	359	362	366	rBV3	847	868	0.04%	0.006%
6	2.562	368	380	394	rBV	401350	653164	32.44%	4.547%
7	2.723	426	430	434	rBV2	392	378	0.02%	0.003%
8	2.755	434	440	442	rBV3	853	958	0.05%	0.007%
9	3.038	522	528	532	rBV4	1133	1466	0.07%	0.010%
10	3.118	549	553	558	rVB3	499	527	0.03%	0.004%
11	3.179	558	572	585	rBV4	3496	8051	0.40%	0.056%
12	3.276	597	602	608	rVB2	556	651	0.03%	0.005%
13	3.433	646	651	656	rVB2	554	485	0.02%	0.003%
14	3.469	656	662	665	rBV2	438	341	0.02%	0.002%
15	3.539	680	684	688	rBV2	503	437	0.02%	0.003%
16	3.816	768	770	775	rVB2	393	329	0.02%	0.002%
17	3.999	823	827	837	rVB2	546	658	0.03%	0.005%
18	4.121	858	865	867	rBV2	318	356	0.02%	0.002%
19	4.205	885	891	894	rVV2	333	328	0.02%	0.002%
20	4.240	897	902	905	rVB2	309	324	0.02%	0.002%
21	4.266	905	910	917	rVB2	335	386	0.02%	0.003%
22	4.314	922	925	928	rBV2	378	304	0.02%	0.002%
23	4.478	971	976	980	rVB2	438	418	0.02%	0.003%
24	4.617	1004	1019	1059	rBV	202702	516892	25.67%	3.598%
25	4.809	1077	1079	1082	rBV3	528	400	0.02%	0.003%
26	4.858	1088	1094	1099	rVB3	569	694	0.03%	0.005%
27	5.060	1140	1157	1179	rBV	369784	812715	40.36%	5.658%
28	5.215	1202	1205	1207	rBV3	477	338	0.02%	0.002%
29	5.366	1249	1252	1255	rBV3	676	501	0.02%	0.003%
30	5.526	1298	1302	1304	rBV2	503	328	0.02%	0.002%
31	5.723	1341	1363	1385	rBV2	743745	2013583	100.00%	14.018%
32	6.038	1459	1461	1465	rVV3	526	361	0.02%	0.003%
33	6.105	1480	1482	1485	rBV	585	299	0.01%	0.002%
34	6.247	1511	1526	1558	rBV	482767	917575	45.57%	6.388%
35	6.465	1591	1594	1597	rVB3	690	336	0.02%	0.002%
36	6.478	1597	1598	1602	rVB2	671	313	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051072.D
 Acq On : 01 Oct 2022 06:32
 Operator : JC/MD
 Sample : N4880-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.530	1602	1614	1628	rBV4	11674	24952	1.24%	0.174%
38	6.607	1636	1638	1642	rVB2	603	390	0.02%	0.003%
39	6.687	1647	1663	1688	rBV	482087	937537	46.56%	6.527%
40	6.925	1735	1737	1743	rVB2	505	357	0.02%	0.002%
41	7.051	1771	1776	1780	rVB2	493	495	0.02%	0.003%
42	7.182	1805	1817	1818	rBV4	1424	1601	0.08%	0.011%
43	7.497	1911	1915	1920	rBV2	309	332	0.02%	0.002%
44	7.565	1920	1936	1962	rBV	224569	398520	19.79%	2.774%
45	7.806	2006	2011	2015	rBV2	379	370	0.02%	0.003%
46	7.896	2021	2039	2059	rBV	841319	1444188	71.72%	10.054%
47	8.176	2115	2126	2143	rBV	162515	274454	13.63%	1.911%
48	8.552	2231	2243	2255	rVV2	110531	185769	9.23%	1.293%
49	8.632	2255	2268	2310	rVV3	532710	1147293	56.98%	7.987%
50	8.890	2345	2348	2351	rVV3	714	674	0.03%	0.005%
51	8.919	2354	2357	2364	rVB2	629	455	0.02%	0.003%
52	8.954	2364	2368	2372	rVB2	526	474	0.02%	0.003%
53	8.980	2372	2376	2381	rBV3	765	818	0.04%	0.006%
54	9.108	2410	2416	2419	rBV2	394	405	0.02%	0.003%
55	9.253	2455	2461	2464	rBV3	402	389	0.02%	0.003%
56	9.414	2499	2511	2547	rBV	697509	1167344	57.97%	8.126%
57	9.594	2563	2567	2572	rVB4	547	481	0.02%	0.003%
58	9.681	2590	2594	2595	rBV	448	303	0.02%	0.002%
59	9.874	2651	2654	2657	rBV	554	389	0.02%	0.003%
60	9.928	2667	2671	2673	rBV2	636	429	0.02%	0.003%
61	10.163	2742	2744	2747	rVB	520	293	0.01%	0.002%
62	10.189	2747	2752	2755	rBV2	471	389	0.02%	0.003%
63	10.308	2785	2789	2792	rBV	398	305	0.02%	0.002%
64	10.542	2855	2862	2866	rVB2	328	441	0.02%	0.003%
65	10.565	2866	2869	2873	rBV	595	433	0.02%	0.003%
66	10.755	2912	2928	2950	rBV	687933	1117082	55.48%	7.777%
67	10.925	2978	2981	2985	rVB2	546	360	0.02%	0.003%
68	10.957	2985	2991	2998	rVB3	451	594	0.03%	0.004%
69	11.115	3038	3040	3044	rVB2	626	333	0.02%	0.002%
70	11.173	3054	3058	3062	rBV2	572	601	0.03%	0.004%
71	11.343	3108	3111	3114	rVV3	483	352	0.02%	0.002%
72	11.407	3127	3131	3135	rVB4	605	551	0.03%	0.004%
73	11.558	3174	3178	3181	rBV	507	403	0.02%	0.003%
74	11.632	3198	3201	3206	rVB2	441	345	0.02%	0.002%
75	11.661	3206	3210	3215	rBV2	496	331	0.02%	0.002%
76	11.710	3222	3225	3231	rVB2	624	484	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051072.D
 Acq On : 01 Oct 2022 06:32
 Operator : JC/MD
 Sample : N4880-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.751	3231	3238	3241	rVB4	667	810	0.04%	0.006%
78	11.809	3244	3256	3277	rBV	533305	860963	42.76%	5.994%
79	12.070	3329	3337	3345	rBV5	3665	6173	0.31%	0.043%
80	12.192	3363	3375	3397	rBV	738212	1186903	58.94%	8.263%
81	12.391	3433	3437	3442	rVB4	906	818	0.04%	0.006%
82	12.430	3443	3449	3456	rVB6	584	865	0.04%	0.006%
83	12.462	3456	3459	3461	rBV2	585	340	0.02%	0.002%
84	12.619	3504	3508	3511	rBV3	485	466	0.02%	0.003%
85	12.754	3544	3550	3552	rBV2	699	608	0.03%	0.004%
86	12.793	3559	3562	3568	rBV3	433	409	0.02%	0.003%
87	12.880	3584	3589	3590	rBV3	1287	1032	0.05%	0.007%
88	12.935	3604	3606	3610	rBV2	508	372	0.02%	0.003%
89	13.102	3654	3658	3662	rBV3	473	528	0.03%	0.004%
90	13.253	3702	3705	3709	rBV4	701	620	0.03%	0.004%
91	13.298	3716	3719	3721	rVB2	512	341	0.02%	0.002%
92	13.597	3809	3812	3814	rBV2	557	441	0.02%	0.003%
93	13.664	3830	3833	3835	rBV2	477	312	0.02%	0.002%
94	13.761	3859	3863	3865	rBV2	498	367	0.02%	0.003%
95	14.105	3964	3970	3974	rBV4	827	1022	0.05%	0.007%
96	14.452	4075	4078	4081	rBV2	491	429	0.02%	0.003%
97	14.513	4094	4097	4099	rBV	442	318	0.02%	0.002%
98	14.674	4145	4147	4152	rVB2	639	300	0.01%	0.002%
99	15.163	4297	4299	4302	rBV	882	528	0.03%	0.004%
100	15.420	4377	4379	4385	rBV5	692	536	0.03%	0.004%




Sum of corrected areas: 14364772

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051072.D
Acq On : 01 Oct 2022 06:32
Operator : JC/MD
Sample : N4880-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

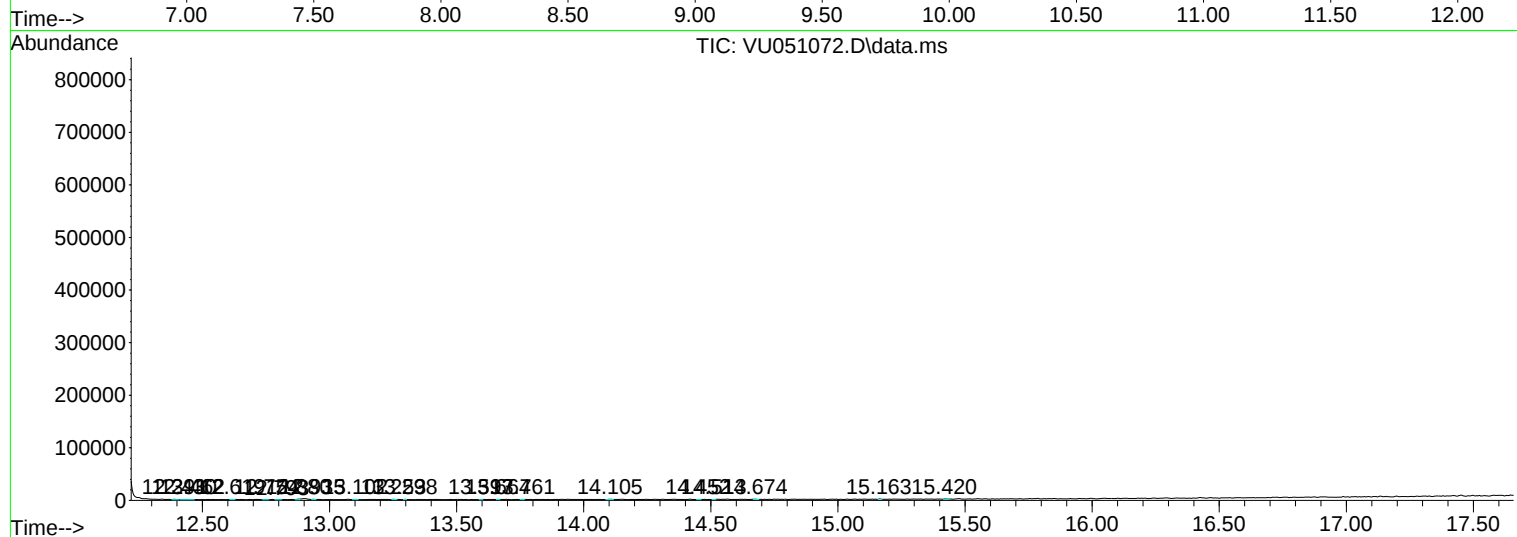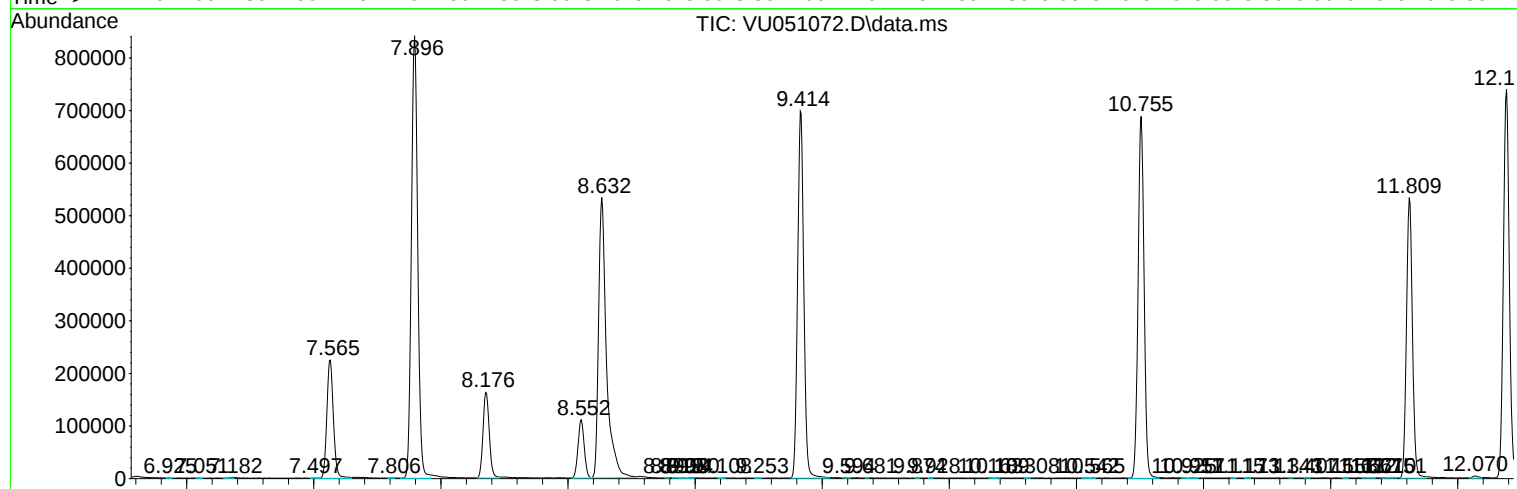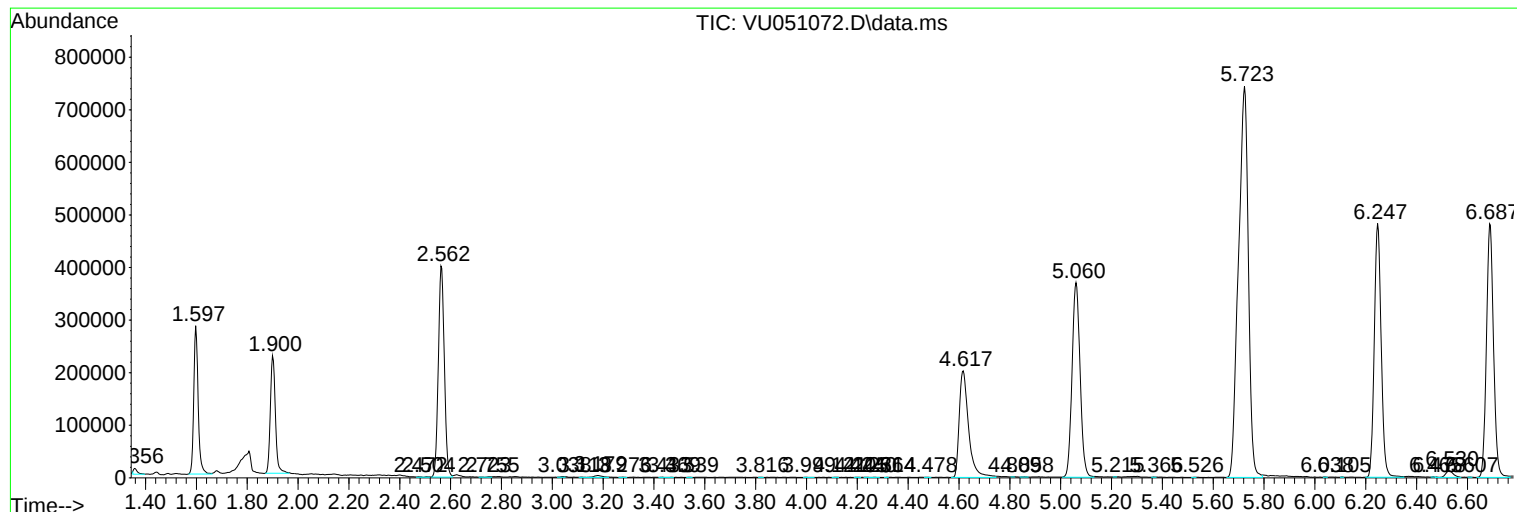

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051072.D
Acq On : 01 Oct 2022 06:32
Operator : JC/MD
Sample : N4880-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051072.D
Acq On : 01 Oct 2022 06:32
Operator : JC/MD
Sample : N4880-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc