

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051073.D
 Acq On : 01 Oct 2022 06:55
 Operator : JC/MD
 Sample : N4880-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051073.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	277815	325858	16.44%	2.265%
2	1.903	167	175	194	rVB	216332	294592	14.86%	2.048%
3	2.562	369	380	395	rBV	390781	635162	32.05%	4.416%
4	3.176	562	571	573	rBV2	2506	3239	0.16%	0.023%
5	3.363	618	629	630	rBV4	2938	4080	0.21%	0.028%
6	3.446	652	655	656	rBV	409	251	0.01%	0.002%
7	3.517	673	677	680	rBV2	505	461	0.02%	0.003%
8	3.572	690	694	696	rBV3	544	419	0.02%	0.003%
9	3.674	724	726	729	rVB	207	81	0.00%	0.001%
10	3.690	729	731	735	rBV2	196	126	0.01%	0.001%
11	3.729	740	743	745	rBV	289	195	0.01%	0.001%
12	3.832	770	775	777	rBV2	386	354	0.02%	0.002%
13	3.845	777	779	782	rVB	413	151	0.01%	0.001%
14	3.858	782	783	785	rBV2	267	129	0.01%	0.001%
15	4.015	829	832	835	rBV2	293	184	0.01%	0.001%
16	4.108	858	861	865	rBV2	326	253	0.01%	0.002%
17	4.144	870	872	874	rVV2	323	154	0.01%	0.001%
18	4.160	874	877	881	rVB2	415	286	0.01%	0.002%
19	4.186	881	885	888	rBV	278	181	0.01%	0.001%
20	4.282	912	915	922	rBV3	357	355	0.02%	0.002%
21	4.337	926	932	937	rBV2	232	254	0.01%	0.002%
22	4.417	951	957	960	rBV2	256	307	0.02%	0.002%
23	4.469	969	973	975	rBV3	740	579	0.03%	0.004%
24	4.546	994	997	999	rVB2	207	107	0.01%	0.001%
25	4.616	1005	1019	1048	rBV	198868	504739	25.47%	3.509%
26	5.060	1142	1157	1181	rBV	360787	789863	39.85%	5.491%
27	5.417	1266	1268	1270	rBV	291	120	0.01%	0.001%
28	5.507	1293	1296	1299	rVB	307	177	0.01%	0.001%
29	5.526	1299	1302	1305	rBV2	273	160	0.01%	0.001%
30	5.604	1323	1326	1333	rBV	273	260	0.01%	0.002%
31	5.645	1336	1339	1341	rVB2	293	147	0.01%	0.001%
32	5.723	1341	1363	1394	rBV2	722827	1981975	100.00%	13.779%
33	6.131	1487	1490	1492	rBV2	374	212	0.01%	0.001%
34	6.173	1501	1503	1507	rBV2	195	136	0.01%	0.001%
35	6.247	1511	1526	1546	rBV	483707	914167	46.12%	6.355%
36	6.542	1603	1618	1629	rBV4	32049	66344	3.35%	0.461%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051073.D
 Acq On : 01 Oct 2022 06:55
 Operator : JC/MD
 Sample : N4880-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.687	1649	1663	1686	rBV	473844	921412	46.49%	6.406%
38	6.989	1754	1757	1758	rBV	359	149	0.01%	0.001%
39	7.115	1791	1796	1798	rBV	328	290	0.01%	0.002%
40	7.179	1812	1816	1818	rBV3	1066	779	0.04%	0.005%
41	7.269	1841	1844	1846	rBV2	270	180	0.01%	0.001%
42	7.346	1865	1868	1871	rBV	188	109	0.01%	0.001%
43	7.362	1871	1873	1874	rBV	265	139	0.01%	0.001%
44	7.401	1883	1885	1887	rBV	230	147	0.01%	0.001%
45	7.417	1887	1890	1893	rVV2	303	177	0.01%	0.001%
46	7.478	1906	1909	1912	rBV	319	219	0.01%	0.002%
47	7.565	1923	1936	1957	rBV	222701	391816	19.77%	2.724%
48	7.896	2025	2039	2057	rBV	811951	1407296	71.00%	9.784%
49	8.179	2116	2127	2146	rBV	158215	264600	13.35%	1.840%
50	8.552	2230	2243	2256	rBV	247567	419316	21.16%	2.915%
51	8.632	2257	2268	2309	rVV2	519900	1116787	56.35%	7.764%
52	9.002	2378	2383	2386	rVB4	569	541	0.03%	0.004%
53	9.034	2391	2393	2396	rVB2	345	166	0.01%	0.001%
54	9.063	2397	2402	2406	rBV3	381	423	0.02%	0.003%
55	9.124	2418	2421	2424	rVB3	327	192	0.01%	0.001%
56	9.153	2427	2430	2432	rBV	497	251	0.01%	0.002%
57	9.263	2461	2464	2467	rVB2	553	317	0.02%	0.002%
58	9.337	2484	2487	2492	rBV2	566	360	0.02%	0.003%
59	9.417	2497	2512	2539	rBV	707361	1172243	59.15%	8.150%
60	9.645	2580	2583	2586	rBV2	508	327	0.02%	0.002%
61	9.738	2608	2612	2613	rBV	342	209	0.01%	0.001%
62	9.787	2624	2627	2631	rBV	659	408	0.02%	0.003%
63	9.812	2631	2635	2636	rBV	271	181	0.01%	0.001%
64	9.883	2652	2657	2666	rBV3	647	969	0.05%	0.007%
65	9.931	2669	2672	2673	rBV	318	175	0.01%	0.001%
66	9.992	2688	2691	2696	rBV2	407	348	0.02%	0.002%
67	10.083	2714	2719	2720	rBV	468	384	0.02%	0.003%
68	10.140	2734	2737	2740	rBV2	710	469	0.02%	0.003%
69	10.285	2779	2782	2785	rBV	281	187	0.01%	0.001%
70	10.526	2852	2857	2859	rBV2	310	277	0.01%	0.002%
71	10.587	2873	2876	2878	rBV2	253	175	0.01%	0.001%
72	10.648	2892	2895	2897	rBV	409	225	0.01%	0.002%
73	10.755	2915	2928	2949	rBV	694159	1112738	56.14%	7.736%
74	11.037	3013	3016	3020	rBV3	390	390	0.02%	0.003%
75	11.121	3040	3042	3047	rBV3	465	332	0.02%	0.002%
76	11.263	3083	3086	3088	rBV	369	248	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051073.D
 Acq On : 01 Oct 2022 06:55
 Operator : JC/MD
 Sample : N4880-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.285	3091	3093	3096	rBV2	534	301	0.02%	0.002%
78	11.809	3243	3256	3276	rBV	540607	863961	43.59%	6.006%
79	12.192	3361	3375	3402	rBV	706454	1167864	58.92%	8.119%
80	12.674	3521	3525	3529	rBV2	512	518	0.03%	0.004%
81	12.774	3553	3556	3558	rBV2	510	277	0.01%	0.002%
82	12.896	3588	3594	3607	rVB7	4050	6258	0.32%	0.044%
83	13.211	3687	3692	3694	rBV4	699	582	0.03%	0.004%
84	13.336	3726	3731	3735	rBV2	790	816	0.04%	0.006%
85	13.516	3784	3787	3793	rVB3	718	750	0.04%	0.005%
86	13.561	3796	3801	3802	rBV3	715	621	0.03%	0.004%




Sum of corrected areas: 14383957

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051073.D
Acq On : 01 Oct 2022 06:55
Operator : JC/MD
Sample : N4880-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

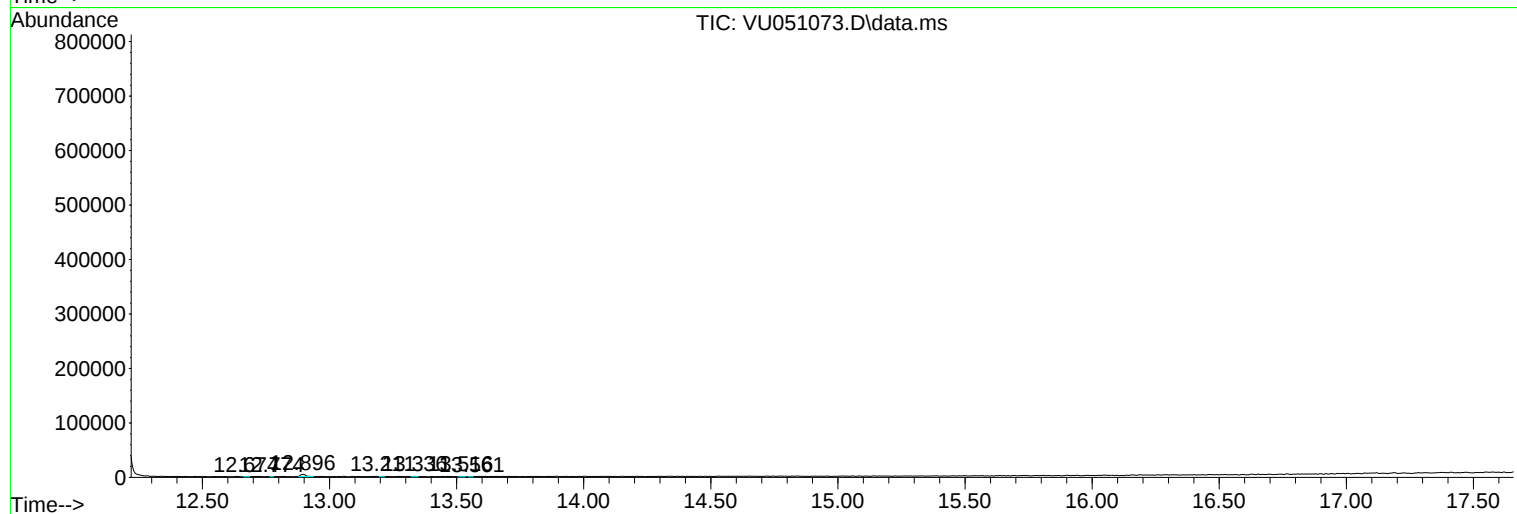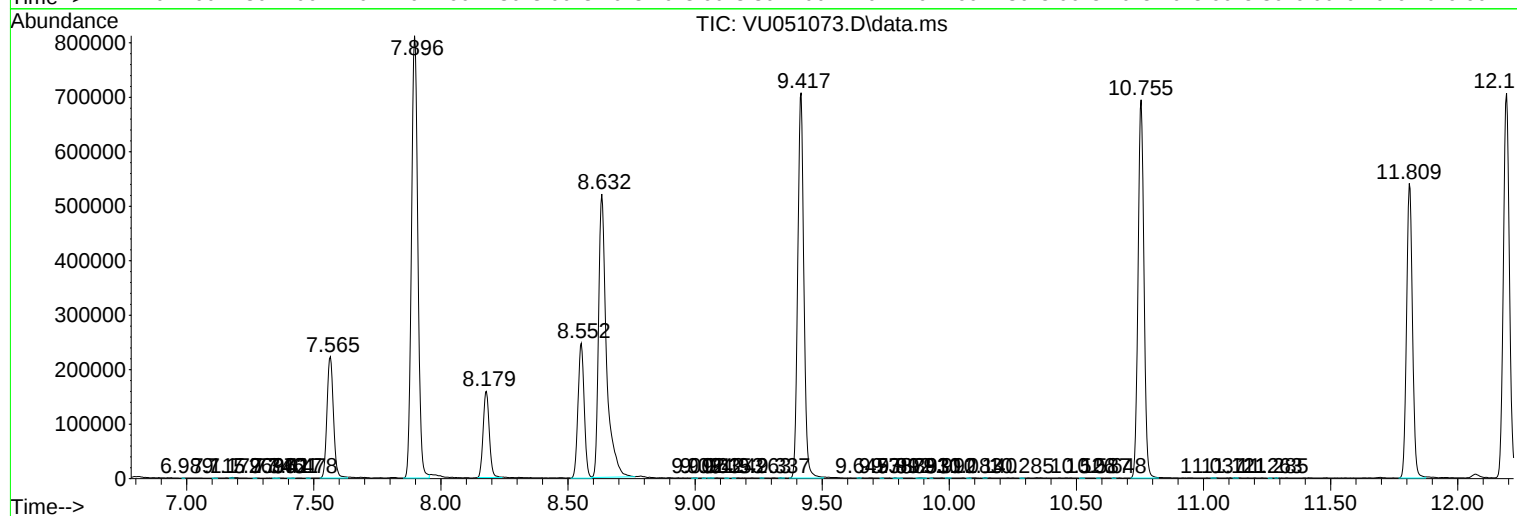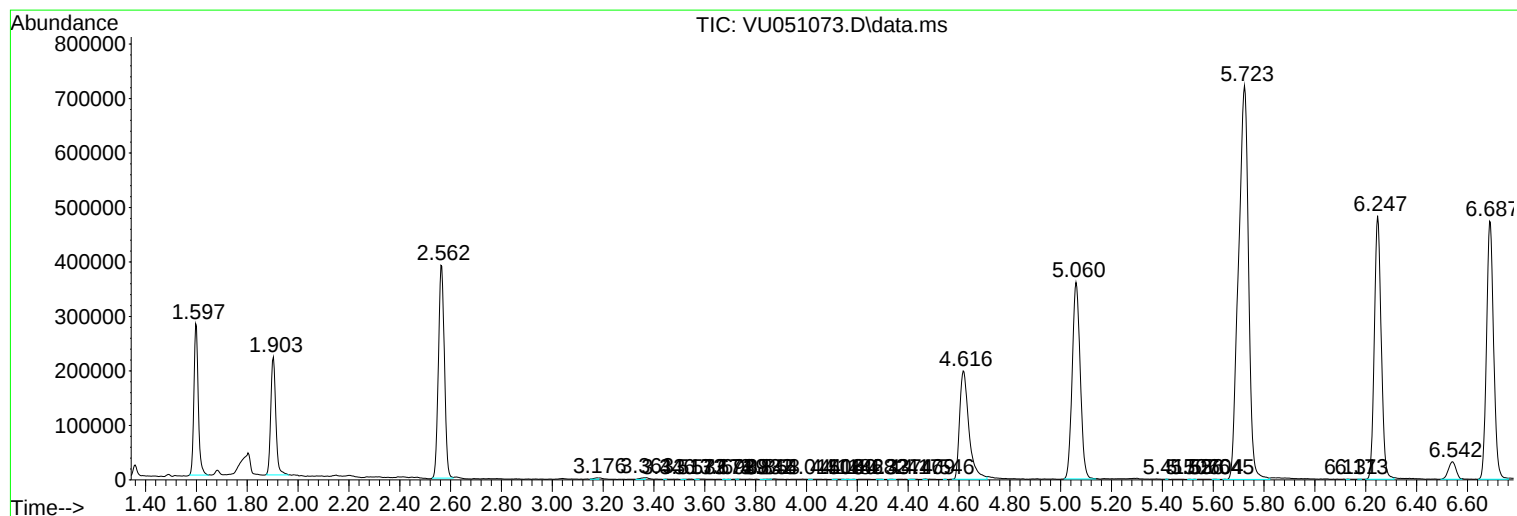

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051073.D
Acq On : 01 Oct 2022 06:55
Operator : JC/MD
Sample : N4880-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051073.D
Acq On : 01 Oct 2022 06:55
Operator : JC/MD
Sample : N4880-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------