

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051074.D
 Acq On : 01 Oct 2022 07:18
 Operator : JC/MD
 Sample : N4880-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	287825	332656	16.27%	2.283%
2	1.900	166	174	197	rVB	228757	315474	15.43%	2.165%
3	2.565	368	381	394	rBV	410000	673306	32.93%	4.620%
4	2.761	434	442	446	rBV5	1518	2295	0.11%	0.016%
5	2.887	479	481	483	rVV3	659	361	0.02%	0.002%
6	3.041	519	529	538	rVV5	1145	2325	0.11%	0.016%
7	3.080	538	541	543	rVB2	532	289	0.01%	0.002%
8	3.105	543	549	553	rBV2	412	476	0.02%	0.003%
9	3.183	561	573	589	rVB3	5081	11458	0.56%	0.079%
10	3.408	639	643	645	rBV2	448	294	0.01%	0.002%
11	3.507	668	674	680	rVB2	404	416	0.02%	0.003%
12	3.565	690	692	697	rVV	299	303	0.01%	0.002%
13	4.115	859	863	870	rBV2	444	480	0.02%	0.003%
14	4.273	907	912	918	rVB2	437	471	0.02%	0.003%
15	4.617	1006	1019	1056	rVV	210379	527836	25.82%	3.622%
16	5.060	1140	1157	1179	rBV	372821	819323	40.08%	5.622%
17	5.221	1204	1207	1210	rBV2	724	405	0.02%	0.003%
18	5.359	1247	1250	1252	rBV2	437	314	0.02%	0.002%
19	5.408	1260	1265	1268	rBV2	674	736	0.04%	0.005%
20	5.462	1279	1282	1287	rBV2	312	383	0.02%	0.003%
21	5.723	1341	1363	1400	rBV2	753802	2044370	100.00%	14.029%
22	5.925	1422	1426	1430	rBV4	886	694	0.03%	0.005%
23	6.182	1502	1506	1509	rBV2	408	357	0.02%	0.002%
24	6.247	1512	1526	1551	rBV	482442	928995	45.44%	6.375%
25	6.530	1604	1614	1625	rBV5	6386	12679	0.62%	0.087%
26	6.607	1635	1638	1640	rBV3	749	442	0.02%	0.003%
27	6.687	1646	1663	1689	rBV	490648	956670	46.80%	6.565%
28	6.951	1740	1745	1747	rBV	345	304	0.01%	0.002%
29	7.057	1773	1778	1781	rBV2	450	410	0.02%	0.003%
30	7.086	1783	1787	1789	rBV2	443	383	0.02%	0.003%
31	7.179	1809	1816	1820	rBV5	1336	1797	0.09%	0.012%
32	7.224	1827	1830	1834	rBV3	462	347	0.02%	0.002%
33	7.263	1838	1842	1847	rBV2	437	314	0.02%	0.002%
34	7.504	1914	1917	1920	rBV	468	338	0.02%	0.002%
35	7.565	1920	1936	1956	rBV	226521	400665	19.60%	2.749%
36	7.758	1990	1996	1997	rBV2	410	348	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051074.D
 Acq On : 01 Oct 2022 07:18
 Operator : JC/MD
 Sample : N4880-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.813	2010	2013	2019	rVB2	317	310	0.02%	0.002%
38	7.841	2019	2022	2025	rBV2	367	276	0.01%	0.002%
39	7.896	2025	2039	2068	rBV	859513	1484157	72.60%	10.184%
40	8.176	2114	2126	2148	rBV	162091	279964	13.69%	1.921%
41	8.552	2233	2243	2254	rBV7	3742	6547	0.32%	0.045%
42	8.632	2255	2268	2307	rBV3	550605	1210451	59.21%	8.306%
43	8.784	2312	2315	2326	rVV7	6357	10921	0.53%	0.075%
44	8.838	2330	2332	2334	rVV2	1146	539	0.03%	0.004%
45	8.854	2335	2337	2339	rVV3	582	326	0.02%	0.002%
46	8.874	2341	2343	2347	rVB	797	429	0.02%	0.003%
47	8.912	2351	2355	2359	rBV2	790	638	0.03%	0.004%
48	8.935	2359	2362	2365	rBV3	827	499	0.02%	0.003%
49	9.005	2380	2384	2387	rBV2	509	464	0.02%	0.003%
50	9.221	2448	2451	2455	rVB2	446	327	0.02%	0.002%
51	9.263	2458	2464	2466	rBV2	455	412	0.02%	0.003%
52	9.282	2467	2470	2472	rVV	459	279	0.01%	0.002%
53	9.356	2488	2493	2496	rBV2	392	339	0.02%	0.002%
54	9.414	2497	2511	2534	rBV	709380	1179981	57.72%	8.097%
55	9.555	2553	2555	2559	rVB4	718	404	0.02%	0.003%
56	9.767	2617	2621	2624	rBV3	466	443	0.02%	0.003%
57	10.073	2710	2716	2718	rBV2	287	289	0.01%	0.002%
58	10.346	2794	2801	2810	rBV6	3423	4537	0.22%	0.031%
59	10.385	2810	2813	2820	rVB2	574	569	0.03%	0.004%
60	10.529	2852	2858	2863	rVB2	307	372	0.02%	0.003%
61	10.555	2863	2866	2873	rBV	399	427	0.02%	0.003%
62	10.591	2873	2877	2880	rBV2	500	403	0.02%	0.003%
63	10.755	2914	2928	2946	rBV	715363	1166753	57.07%	8.006%
64	10.864	2959	2962	2965	rBV3	458	327	0.02%	0.002%
65	10.893	2969	2971	2976	rVB4	710	583	0.03%	0.004%
66	10.986	2996	3000	3005	rVB2	398	358	0.02%	0.002%
67	11.083	3027	3030	3035	rVB3	582	488	0.02%	0.003%
68	11.169	3054	3057	3062	rBV2	386	317	0.02%	0.002%
69	11.256	3081	3084	3087	rBV2	479	378	0.02%	0.003%
70	11.308	3097	3100	3104	rBV2	406	318	0.02%	0.002%
71	11.414	3131	3133	3139	rVB3	650	530	0.03%	0.004%
72	11.446	3139	3143	3150	rBV2	453	467	0.02%	0.003%
73	11.475	3150	3152	3155	rBV2	481	345	0.02%	0.002%
74	11.636	3197	3202	3204	rBV2	307	323	0.02%	0.002%
75	11.690	3211	3219	3229	rBV6	10128	15563	0.76%	0.107%
76	11.809	3241	3256	3279	rBV	561546	900712	44.06%	6.181%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051074.D
 Acq On : 01 Oct 2022 07:18
 Operator : JC/MD
 Sample : N4880-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.070	3329	3337	3351	rBV7	3658	7515	0.37%	0.052%
78	12.192	3361	3375	3396	rBV	755858	1223430	59.84%	8.395%
79	12.356	3422	3426	3427	rBV2	896	616	0.03%	0.004%
80	12.369	3428	3430	3431	rVV2	678	287	0.01%	0.002%
81	12.404	3439	3441	3445	rVB3	441	314	0.02%	0.002%
82	12.430	3445	3449	3451	rBV2	356	286	0.01%	0.002%
83	12.545	3482	3485	3491	rVB4	595	606	0.03%	0.004%
84	12.774	3552	3556	3558	rBV	432	320	0.02%	0.002%
85	12.838	3572	3576	3577	rBV2	385	302	0.01%	0.002%
86	12.890	3583	3592	3610	rBV7	11610	21396	1.05%	0.147%
87	12.957	3610	3613	3616	rBV2	853	622	0.03%	0.004%
88	13.301	3715	3720	3724	rBV2	651	635	0.03%	0.004%
89	13.475	3771	3774	3780	rBV3	578	629	0.03%	0.004%
90	13.536	3790	3793	3795	rBV2	570	407	0.02%	0.003%
91	13.639	3821	3825	3829	rBV	479	527	0.03%	0.004%
92	13.684	3836	3839	3847	rVB3	637	720	0.04%	0.005%
93	13.999	3934	3937	3941	rBV3	512	423	0.02%	0.003%
94	14.111	3970	3972	3979	rVB4	651	529	0.03%	0.004%
95	14.227	4006	4008	4013	rBV3	362	321	0.02%	0.002%
96	14.253	4013	4016	4021	rVB2	586	433	0.02%	0.003%
97	14.687	4146	4151	4153	rBV3	622	583	0.03%	0.004%
98	15.076	4270	4272	4275	rBV	579	394	0.02%	0.003%
99	15.397	4370	4372	4374	rBV	700	383	0.02%	0.003%
100	15.770	4486	4488	4493	rVB3	988	736	0.04%	0.005%




Sum of corrected areas: 14572893

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051074.D
Acq On : 01 Oct 2022 07:18
Operator : JC/MD
Sample : N4880-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

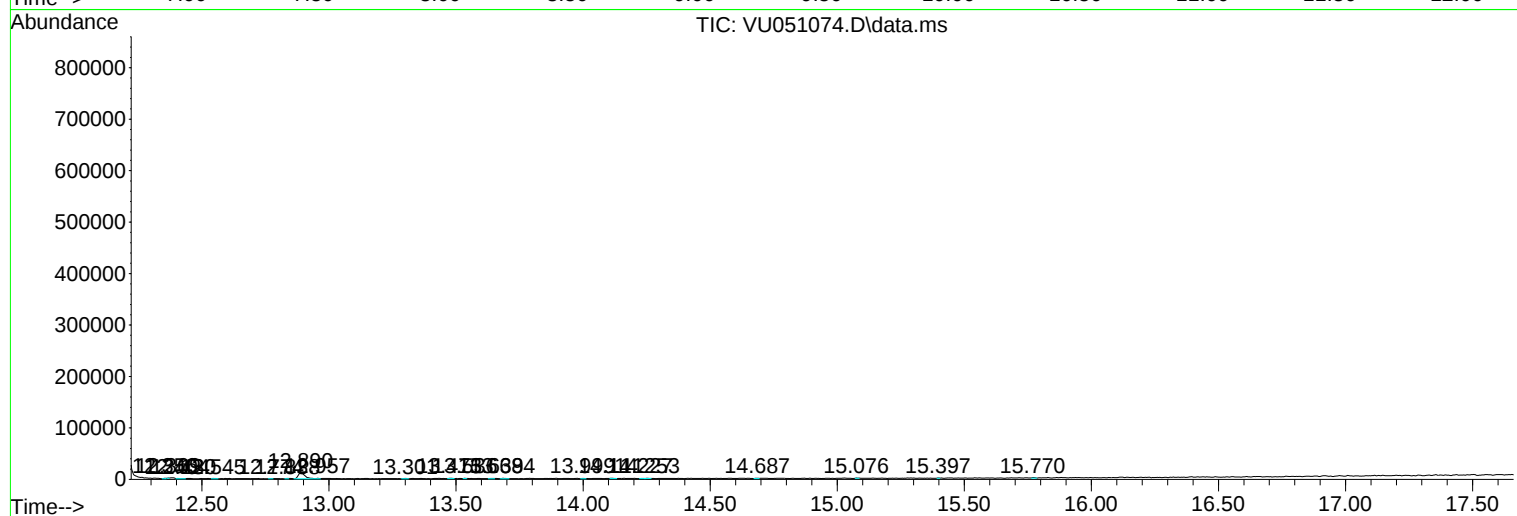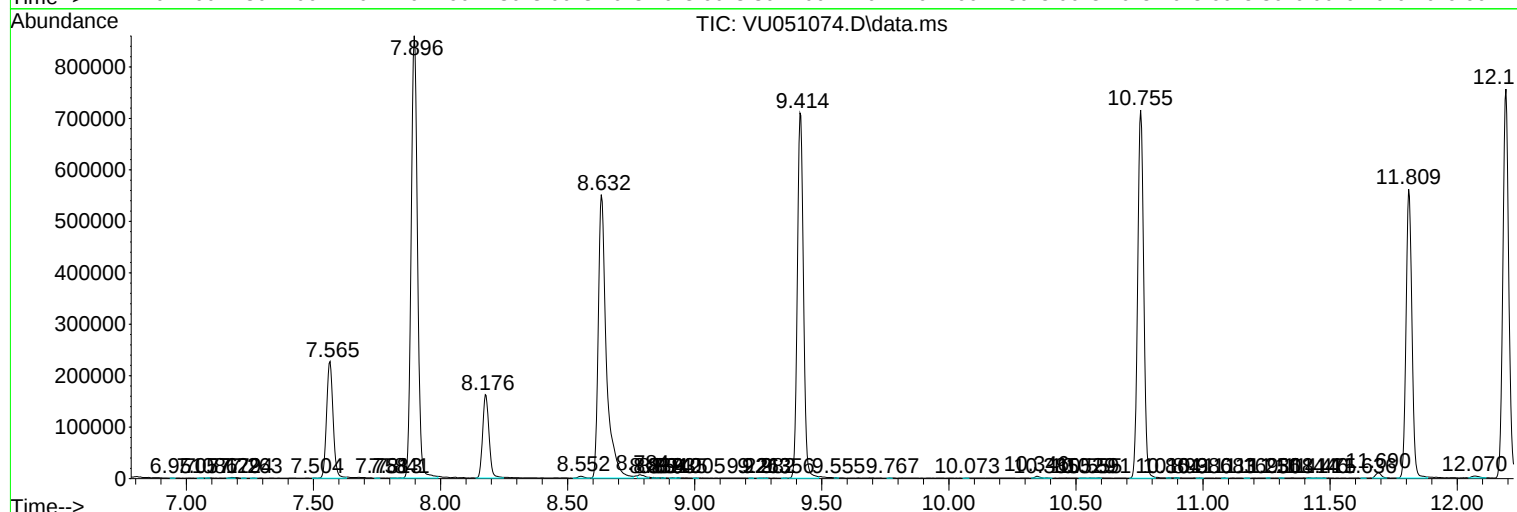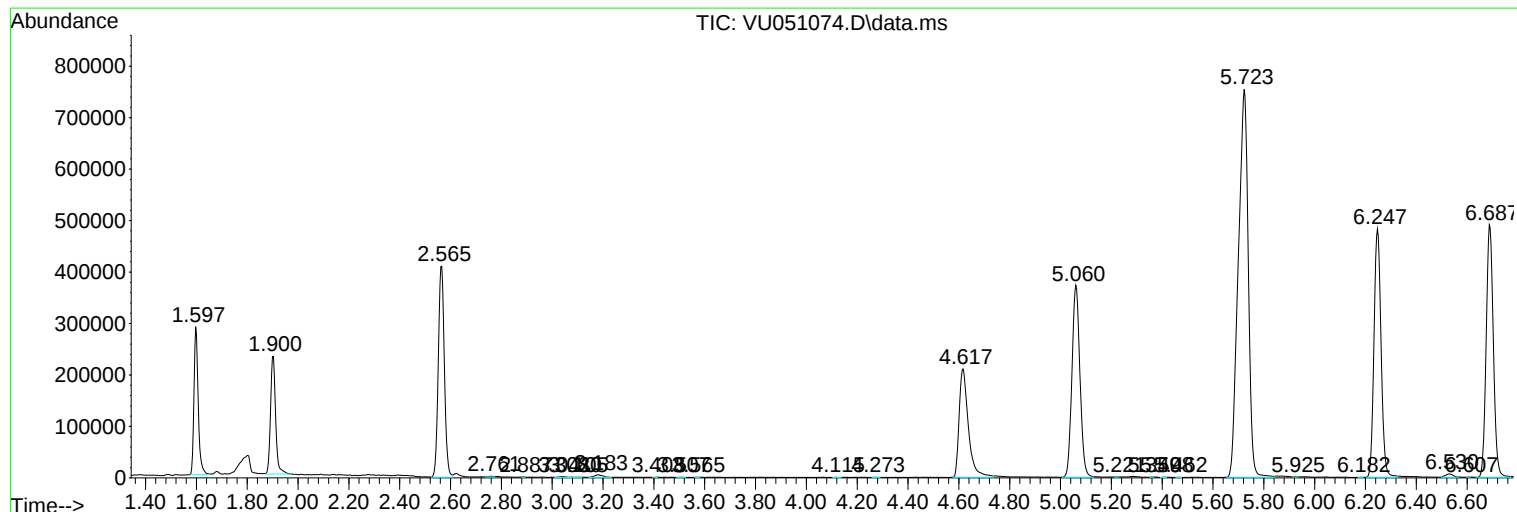

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051074.D
Acq On : 01 Oct 2022 07:18
Operator : JC/MD
Sample : N4880-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051074.D
Acq On : 01 Oct 2022 07:18
Operator : JC/MD
Sample : N4880-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc