

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051075.D
 Acq On : 01 Oct 2022 07:42
 Operator : JC/MD
 Sample : N4880-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.356	3	5	15	rVB2	11423	9979	0.50%	0.070%
2	1.440	28	31	38	rVB2	2686	2691	0.14%	0.019%
3	1.597	72	80	99	rVB	281388	328069	16.47%	2.318%
4	1.681	101	106	114	rVB	12180	14636	0.73%	0.103%
5	1.900	166	174	195	rVB	216518	301705	15.14%	2.131%
6	2.562	368	380	394	rBV	397543	647240	32.49%	4.572%
7	2.729	430	432	435	rBV	532	427	0.02%	0.003%
8	2.855	466	471	477	rVV4	1490	1817	0.09%	0.013%
9	3.028	520	525	526	rBV3	438	319	0.02%	0.002%
10	3.044	527	530	539	rVB4	1351	1727	0.09%	0.012%
11	3.176	563	571	573	rBV2	3662	4555	0.23%	0.032%
12	3.237	586	590	594	rBV2	338	319	0.02%	0.002%
13	3.308	609	612	620	rVB3	550	651	0.03%	0.005%
14	3.343	620	623	628	rBV3	357	381	0.02%	0.003%
15	3.414	641	645	648	rVV3	515	339	0.02%	0.002%
16	3.498	667	671	673	rBV	384	295	0.01%	0.002%
17	3.584	696	698	706	rVB5	635	744	0.04%	0.005%
18	3.732	741	744	749	rVB3	387	294	0.01%	0.002%
19	3.810	765	768	773	rBV2	363	377	0.02%	0.003%
20	3.980	815	821	823	rBV	302	297	0.01%	0.002%
21	4.253	900	906	907	rBV	436	398	0.02%	0.003%
22	4.388	943	948	955	rBV3	390	528	0.03%	0.004%
23	4.437	956	963	964	rBV	348	396	0.02%	0.003%
24	4.478	971	976	981	rVV3	422	434	0.02%	0.003%
25	4.617	1004	1019	1053	rBV	201451	508355	25.52%	3.591%
26	4.973	1126	1130	1136	rVB3	745	833	0.04%	0.006%
27	5.060	1139	1157	1179	rBV	365269	813521	40.83%	5.747%
28	5.256	1216	1218	1221	rBV3	443	294	0.01%	0.002%
29	5.282	1221	1226	1227	rBV3	912	824	0.04%	0.006%
30	5.375	1252	1255	1256	rBV	654	343	0.02%	0.002%
31	5.488	1284	1290	1294	rBV2	424	380	0.02%	0.003%
32	5.723	1340	1363	1388	rBV2	735465	1992228	100.00%	14.074%
33	5.970	1436	1440	1446	rVB5	1278	1203	0.06%	0.008%
34	5.996	1446	1448	1450	rVB3	689	312	0.02%	0.002%
35	6.247	1510	1526	1548	rBV	486888	925868	46.47%	6.541%
36	6.530	1601	1614	1627	rBV6	7008	13539	0.68%	0.096%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051075.D
 Acq On : 01 Oct 2022 07:42
 Operator : JC/MD
 Sample : N4880-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.581	1627	1630	1632	rBV	572	353	0.02%	0.002%
38	6.687	1649	1663	1681	rBV	476383	924772	46.42%	6.533%
39	6.964	1743	1749	1754	rBV4	341	385	0.02%	0.003%
40	7.044	1770	1774	1778	rVB3	374	295	0.01%	0.002%
41	7.186	1806	1818	1822	rBV4	1353	2306	0.12%	0.016%
42	7.205	1822	1824	1828	rVV	870	539	0.03%	0.004%
43	7.272	1841	1845	1851	rVB2	410	385	0.02%	0.003%
44	7.311	1851	1857	1864	rVB2	390	468	0.02%	0.003%
45	7.343	1864	1867	1870	rBV2	394	289	0.01%	0.002%
46	7.417	1883	1890	1894	rVB3	589	701	0.04%	0.005%
47	7.446	1894	1899	1905	rBV2	325	435	0.02%	0.003%
48	7.562	1922	1935	1964	rBV	214603	390903	19.62%	2.761%
49	7.896	2025	2039	2060	rBV	827148	1421146	71.33%	10.039%
50	8.176	2114	2126	2141	rBV	162672	271818	13.64%	1.920%
51	8.398	2191	2195	2200	rBV2	455	374	0.02%	0.003%
52	8.552	2232	2243	2254	rVB2	19911	33344	1.67%	0.236%
53	8.632	2256	2268	2306	rBV2	516307	1125596	56.50%	7.952%
54	8.890	2345	2348	2352	rVB2	594	362	0.02%	0.003%
55	9.050	2394	2398	2406	rBV3	663	657	0.03%	0.005%
56	9.414	2498	2511	2543	rBV	698127	1182287	59.34%	8.352%
57	9.796	2625	2630	2634	rBV2	595	672	0.03%	0.005%
58	10.041	2701	2706	2711	rVB3	287	292	0.01%	0.002%
59	10.073	2711	2716	2719	rBV2	294	298	0.01%	0.002%
60	10.124	2729	2732	2734	rBV	528	358	0.02%	0.003%
61	10.198	2751	2755	2760	rBV	397	351	0.02%	0.002%
62	10.311	2783	2790	2795	rBV2	671	681	0.03%	0.005%
63	10.346	2795	2801	2812	rBV3	1630	2332	0.12%	0.016%
64	10.427	2823	2826	2831	rBV2	388	381	0.02%	0.003%
65	10.658	2895	2898	2904	rVB3	335	296	0.01%	0.002%
66	10.755	2915	2928	2947	rBV	702135	1130297	56.74%	7.985%
67	11.121	3036	3042	3044	rBV2	506	437	0.02%	0.003%
68	11.240	3075	3079	3082	rBV	293	291	0.01%	0.002%
69	11.282	3087	3092	3093	rBV2	453	376	0.02%	0.003%
70	11.411	3130	3132	3137	rVB4	617	484	0.02%	0.003%
71	11.629	3194	3200	3209	rBV4	718	1037	0.05%	0.007%
72	11.690	3210	3219	3229	rVB7	2793	4459	0.22%	0.032%
73	11.809	3244	3256	3275	rBV	556347	879964	44.17%	6.216%
74	11.925	3290	3292	3294	rVB2	730	332	0.02%	0.002%
75	11.960	3300	3303	3306	rBV2	514	428	0.02%	0.003%
76	12.031	3321	3325	3327	rBV2	567	360	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051075.D
 Acq On : 01 Oct 2022 07:42
 Operator : JC/MD
 Sample : N4880-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.070	3327	3337	3351	rBV7	6150	13343	0.67%	0.094%
78	12.192	3361	3375	3398	rBV	721927	1164540	58.45%	8.227%
79	12.362	3426	3428	3431	rVB3	636	345	0.02%	0.002%
80	12.404	3439	3441	3445	rBV2	426	302	0.02%	0.002%
81	12.603	3498	3503	3508	rBV2	499	529	0.03%	0.004%
82	12.648	3512	3517	3523	rVB2	573	506	0.03%	0.004%
83	12.690	3525	3530	3533	rBV3	605	526	0.03%	0.004%
84	12.890	3585	3592	3602	rBV8	5970	10012	0.50%	0.071%
85	13.118	3659	3663	3665	rBV	400	317	0.02%	0.002%
86	13.137	3666	3669	3675	rVB2	566	585	0.03%	0.004%
87	13.234	3695	3699	3703	rVB2	536	533	0.03%	0.004%
88	13.266	3706	3709	3712	rBV2	529	455	0.02%	0.003%
89	13.333	3725	3730	3735	rBV2	559	686	0.03%	0.005%
90	13.472	3771	3773	3777	rVB3	564	352	0.02%	0.002%
91	13.504	3778	3783	3790	rBV3	558	659	0.03%	0.005%
92	13.549	3793	3797	3798	rBV2	474	336	0.02%	0.002%
93	13.989	3931	3934	3936	rBV2	510	329	0.02%	0.002%
94	14.060	3950	3956	3958	rBV2	713	704	0.04%	0.005%
95	14.336	4040	4042	4046	rBV3	586	521	0.03%	0.004%
96	14.761	4172	4174	4176	rBV2	545	303	0.02%	0.002%
97	15.044	4260	4262	4265	rBV2	600	339	0.02%	0.002%
98	15.105	4278	4281	4284	rVB2	585	312	0.02%	0.002%
99	15.484	4395	4399	4400	rBV	516	420	0.02%	0.003%
100	15.632	4441	4445	4448	rBV4	866	738	0.04%	0.005%




Sum of corrected areas: 14155551

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051075.D
Acq On : 01 Oct 2022 07:42
Operator : JC/MD
Sample : N4880-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

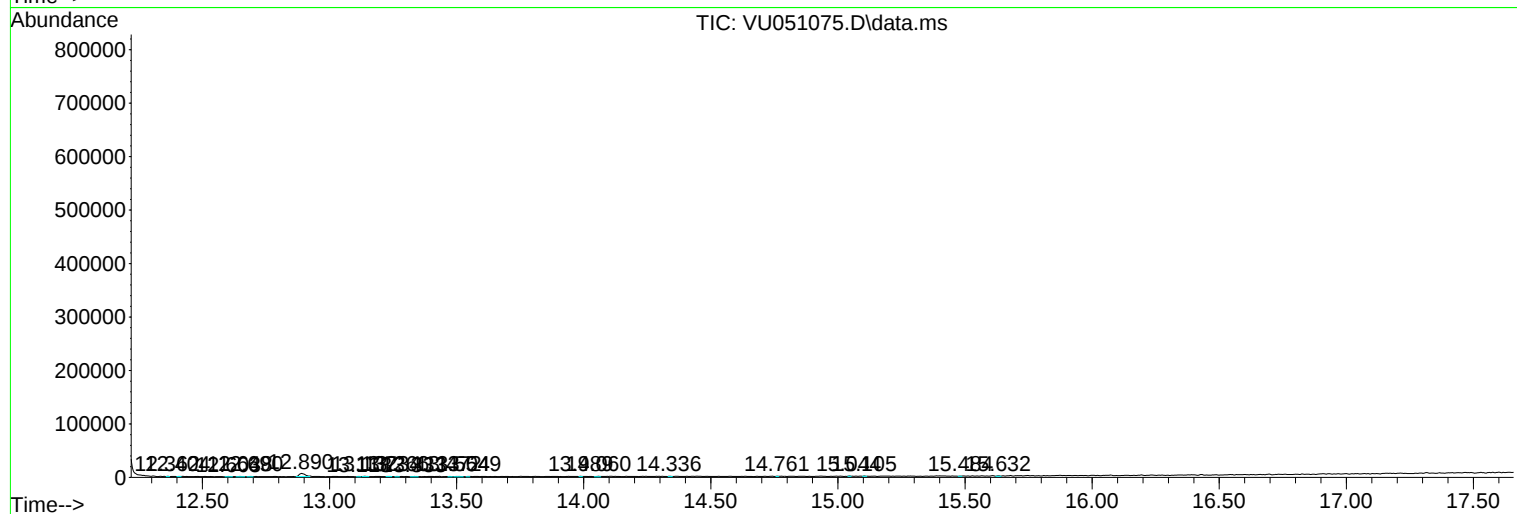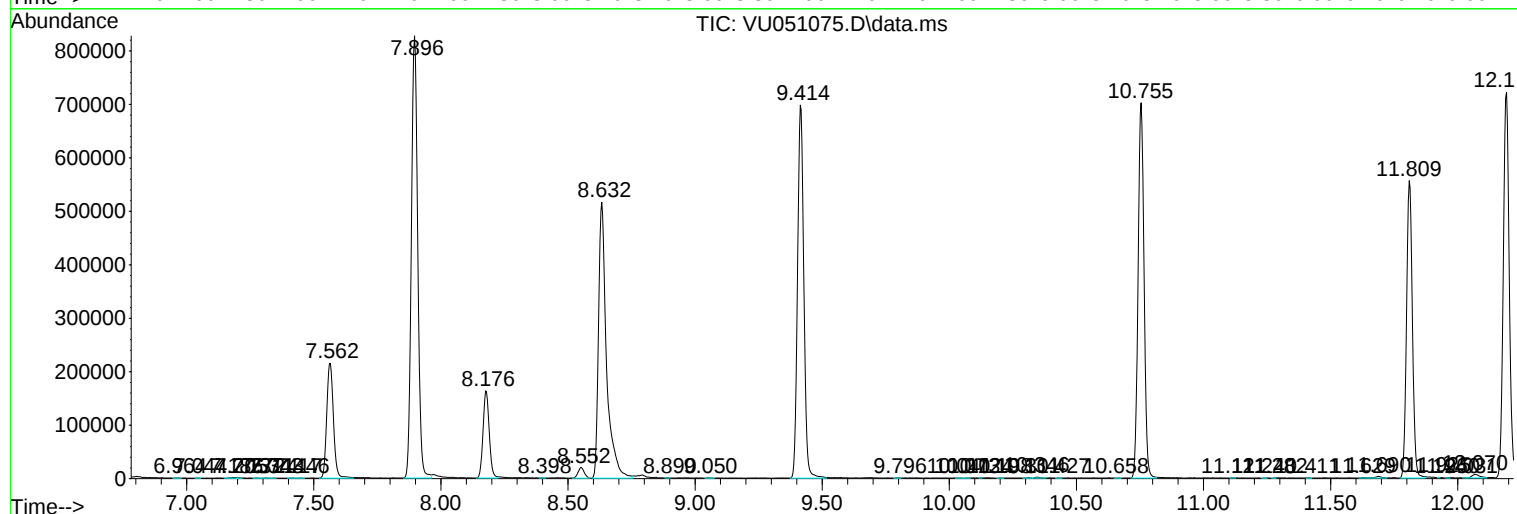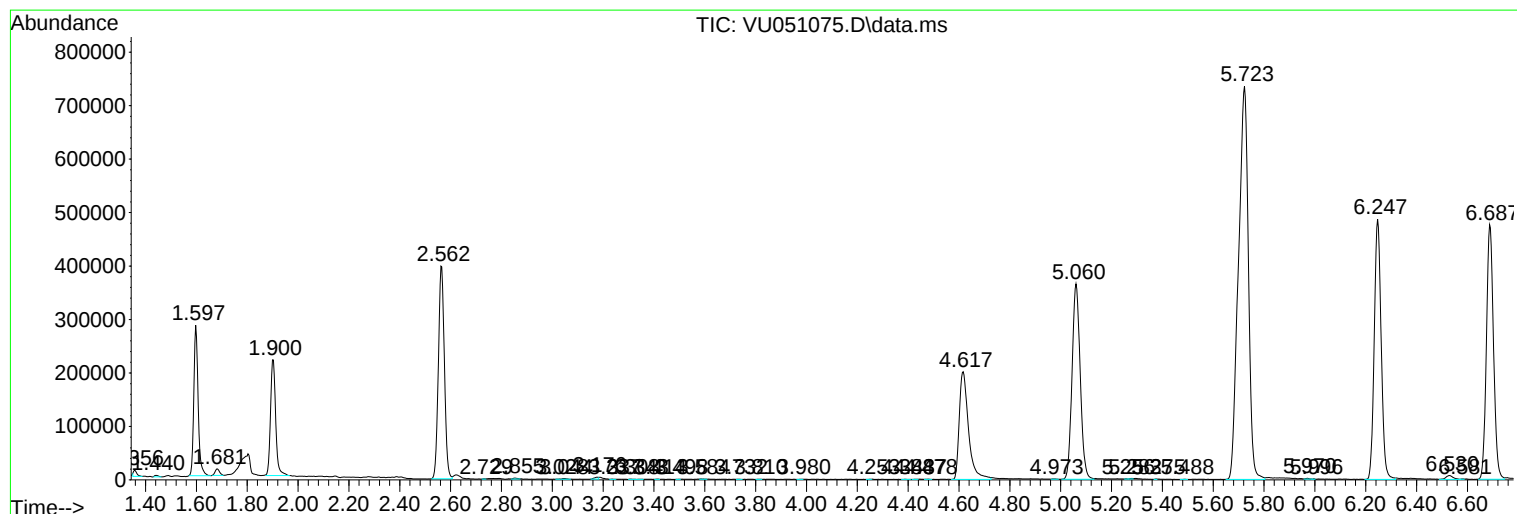

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051075.D
Acq On : 01 Oct 2022 07:42
Operator : JC/MD
Sample : N4880-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
Data File : VU051075.D
Acq On : 01 Oct 2022 07:42
Operator : JC/MD
Sample : N4880-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc