


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU093022\
 Data File : VU051025.D
 Acq On : 30 Sep 2022 11:10
 Operator : JC/MD
 Sample : BFB134
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB134

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 01 03:04:59 2022

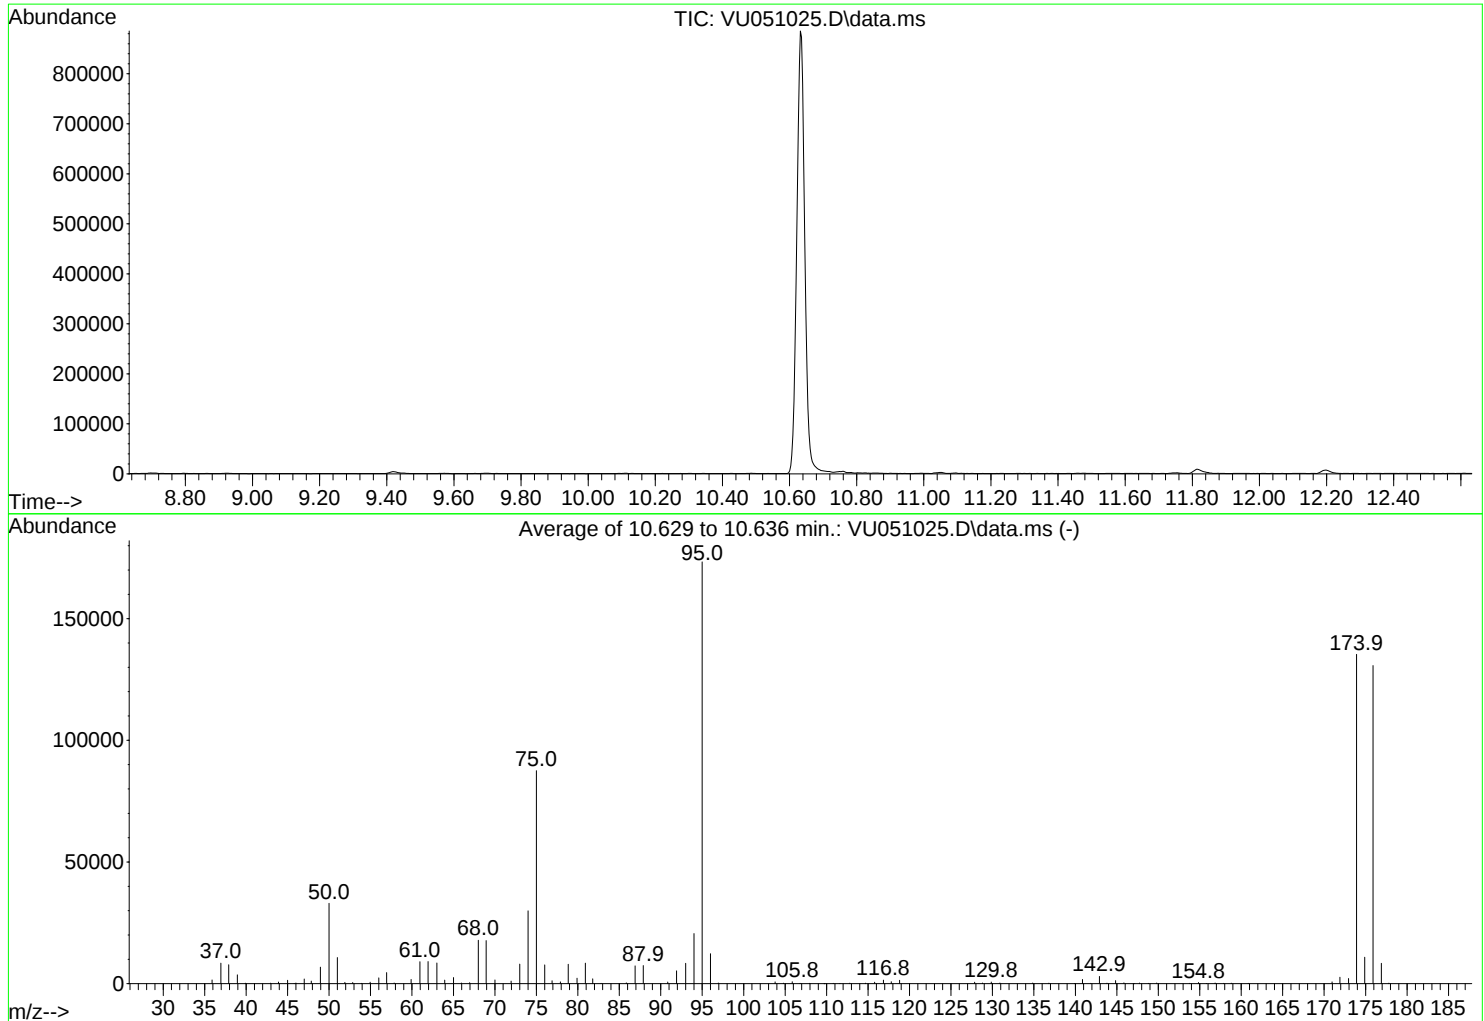

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	33008	PASS
75	95	30	80	50.5	87512	PASS
95	95	100	100	100.0	173355	PASS
96	95	5	9	7.1	12286	PASS
173	174	0.00	2	1.6	2134	PASS
174	95	50	120	78.1	135315	PASS
175	174	5	9	8.0	10857	PASS
176	174	95	101	96.6	130712	PASS
177	176	5	9	6.4	8375	PASS

Scan 2876 (10.587 min): VU051025.D\data.ms
BFB134

m/z	Abundance
39.80	160.0
43.90	575.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

m/z	Abundance
35.90	1591.0
36.90	8381.0
37.90	7425.0
39.00	3433.0
39.90	335.0
41.00	155.0
43.00	224.0
43.90	1181.0
45.00	1221.0
45.80	310.0
47.00	1818.0
47.90	1100.0
49.00	6656.0
50.00	32000.0
51.00	10548.0
51.90	587.0
52.80	441.0
53.90	158.0
55.00	594.0
56.00	2361.0
57.00	4386.0
57.80	239.0
59.90	1790.0
60.90	8907.0
61.90	9106.0
63.00	8383.0
64.00	1458.0
65.00	2422.0
66.00	263.0
67.00	413.0
68.00	16984.0
68.90	17120.0
70.00	1495.0
71.90	1074.0
73.00	7714.0
74.00	29160.0
75.00	84160.0
76.00	7411.0
76.90	1057.0
77.90	639.0
78.90	7577.0
79.90	2172.0
80.90	8147.0
81.80	1946.0
82.80	128.0
85.80	219.0
86.90	6996.0
87.90	7363.0
90.90	662.0
91.90	5208.0
93.00	8233.0
94.00	19520.0
95.00	164032.0
96.00	11945.0
97.00	304.0
103.80	703.0
104.80	192.0
105.90	700.0
106.80	121.0
107.90	108.0
110.80	144.0
112.80	151.0
114.70	121.0
115.80	644.0
116.80	1350.0
117.80	851.0
118.80	1319.0
127.80	597.0
128.80	218.0
129.90	611.0
130.90	265.0
134.80	248.0
136.80	202.0
139.90	111.0
140.80	1502.0
141.90	160.0
142.90	2941.0
143.80	184.0
144.80	1134.0
145.80	373.0
147.00	113.0
147.70	238.0
148.80	114.0
149.80	280.0
153.80	135.0
154.80	401.0
156.80	292.0
157.90	114.0
158.80	191.0
160.80	202.0
170.90	643.0
171.90	2595.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

172.90	2032.0
173.90	127736.0
174.90	10127.0
175.90	121480.0
176.90	7755.0
177.80	207.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

m/z	Abundance
35.90	1560.0
37.00	8728.0
37.90	8007.0
39.00	3756.0
40.00	342.0
41.00	118.0
43.00	238.0
43.90	1207.0
45.00	1427.0
46.00	397.0
47.00	2008.0
47.90	1075.0
49.00	6922.0
50.00	34040.0
51.00	11071.0
51.90	514.0
52.90	442.0
53.90	151.0
55.00	626.0
56.00	2359.0
56.90	4670.0
57.90	246.0
59.90	1747.0
61.00	9228.0
61.90	9421.0
63.00	8746.0
64.00	1465.0
65.00	2587.0
66.00	292.0
67.00	405.0
68.00	18424.0
69.00	18200.0
70.00	1601.0
71.90	1112.0
73.00	8173.0
74.00	30992.0
75.00	90392.0
76.00	7935.0
76.90	1258.0
77.90	789.0
78.90	8214.0
79.90	2242.0
80.90	8708.0
81.80	2038.0
82.80	161.0
85.90	298.0
86.90	7485.0
87.90	7682.0
90.80	661.0
91.90	5458.0
93.00	8574.0
94.00	21160.0
95.00	178752.0
96.00	12749.0
97.00	310.0
103.80	740.0
104.90	187.0
105.80	812.0
106.80	129.0
108.00	111.0
110.80	158.0
111.60	108.0
112.80	210.0
114.70	194.0
115.80	635.0
116.90	1486.0
117.80	816.0
118.80	1419.0
127.90	625.0
128.80	276.0
129.80	722.0
130.90	292.0
134.90	269.0
136.80	223.0
140.80	1766.0
141.90	173.0
142.90	3065.0
143.80	165.0
144.90	1241.0
145.90	349.0
147.80	283.0
148.80	133.0
149.80	288.0
153.80	143.0
154.90	441.0
155.80	128.0
156.80	264.0
157.90	182.0
158.80	207.0
160.90	164.0
170.90	796.0
171.90	2702.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

173.00	2171.0
173.90	139328.0
174.90	11322.0
175.90	134720.0
176.90	8583.0
177.80	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

m/z	Abundance
35.90	1383.0
37.00	8167.0
37.90	7875.0
38.90	3633.0
40.00	339.0
42.90	196.0
43.90	1291.0
45.00	1557.0
46.00	425.0
47.00	1868.0
47.80	925.0
48.90	6737.0
50.00	32984.0
51.00	10584.0
51.90	402.0
52.90	443.0
53.90	122.0
54.90	587.0
56.00	2466.0
56.90	4558.0
57.90	255.0
59.90	1658.0
61.00	8937.0
62.00	8749.0
63.00	8248.0
63.90	1426.0
65.00	2479.0
65.90	249.0
66.90	361.0
68.00	18080.0
69.00	17680.0
70.00	1558.0
72.00	1073.0
73.00	8168.0
74.00	29616.0
75.00	87984.0
76.00	7770.0
76.90	1322.0
77.90	833.0
78.80	8157.0
79.90	2224.0
80.90	8507.0
81.80	1902.0
82.80	165.0
85.90	394.0
86.90	7368.0
87.90	7240.0
90.80	659.0
91.90	5138.0
93.00	8302.0
94.00	21152.0
95.00	177280.0
96.00	12164.0
96.90	272.0
103.80	712.0
104.70	192.0
105.80	817.0
106.80	141.0
108.00	112.0
109.70	113.0
110.80	164.0
111.60	131.0
112.80	166.0
114.70	214.0
115.80	541.0
116.80	1613.0
117.80	664.0
118.80	1363.0
127.90	653.0
128.80	275.0
129.80	680.0
130.90	299.0
134.90	252.0
136.80	244.0
139.90	103.0
140.90	1849.0
141.80	159.0
142.90	2919.0
143.80	176.0
144.90	1344.0
145.90	337.0
147.80	354.0
148.80	110.0
149.80	233.0
153.80	144.0
154.90	469.0
155.80	155.0
156.90	261.0
157.90	179.0
158.80	209.0
171.00	808.0
171.90	2590.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

173.00	2199.0
173.90	138880.0
174.90	11121.0
175.90	135936.0
176.90	8786.0
177.80	244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134