

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
 Data File : VU051087.D
 Acq On : 03 Oct 2022 17:06
 Operator : JC/MD
 Sample : N4869-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J60

Quant Time: Oct 03 23:33:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 01 03:04:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.246	114	368152	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	375718	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	132249	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	150206	40.259	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.520%
7) Chloroethane-d5	1.906	69	154126	44.470	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.940%
11) 1,1-Dichloroethene-d2	2.565	63	186374	33.817	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.640%
21) 2-Butanone-d5	4.623	46	223580	92.393	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.390%
24) Chloroform-d	5.060	84	281347	46.804	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.600%
26) 1,2-Dichloroethane-d4	5.700	65	182060	48.932	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.860%
32) Benzene-d6	5.726	84	556235	50.556	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.120%
36) 1,2-Dichloropropane-d6	6.690	67	191820	53.728	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.460%
41) Toluene-d8	7.896	98	448181	44.089	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.180%
43) trans-1,3-Dichloroprop...	8.179	79	73471	43.145	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.300%
47) 2-Hexanone-d5	8.632	63	107013	74.233	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	74.230%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	284860	45.654	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.300%
66) 1,2-Dichlorobenzene-d4	12.192	152	147460	52.194	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.380%
Target Compounds						
13) Acetone	2.632	43	7877	4.076	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100322\
Data File : VU051087.D
Acq On : 03 Oct 2022 17:06
Operator : JC/MD
Sample : N4869-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J60

Quant Time: Oct 03 23:33:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 01 03:04:59 2022
Response via : Initial Calibration

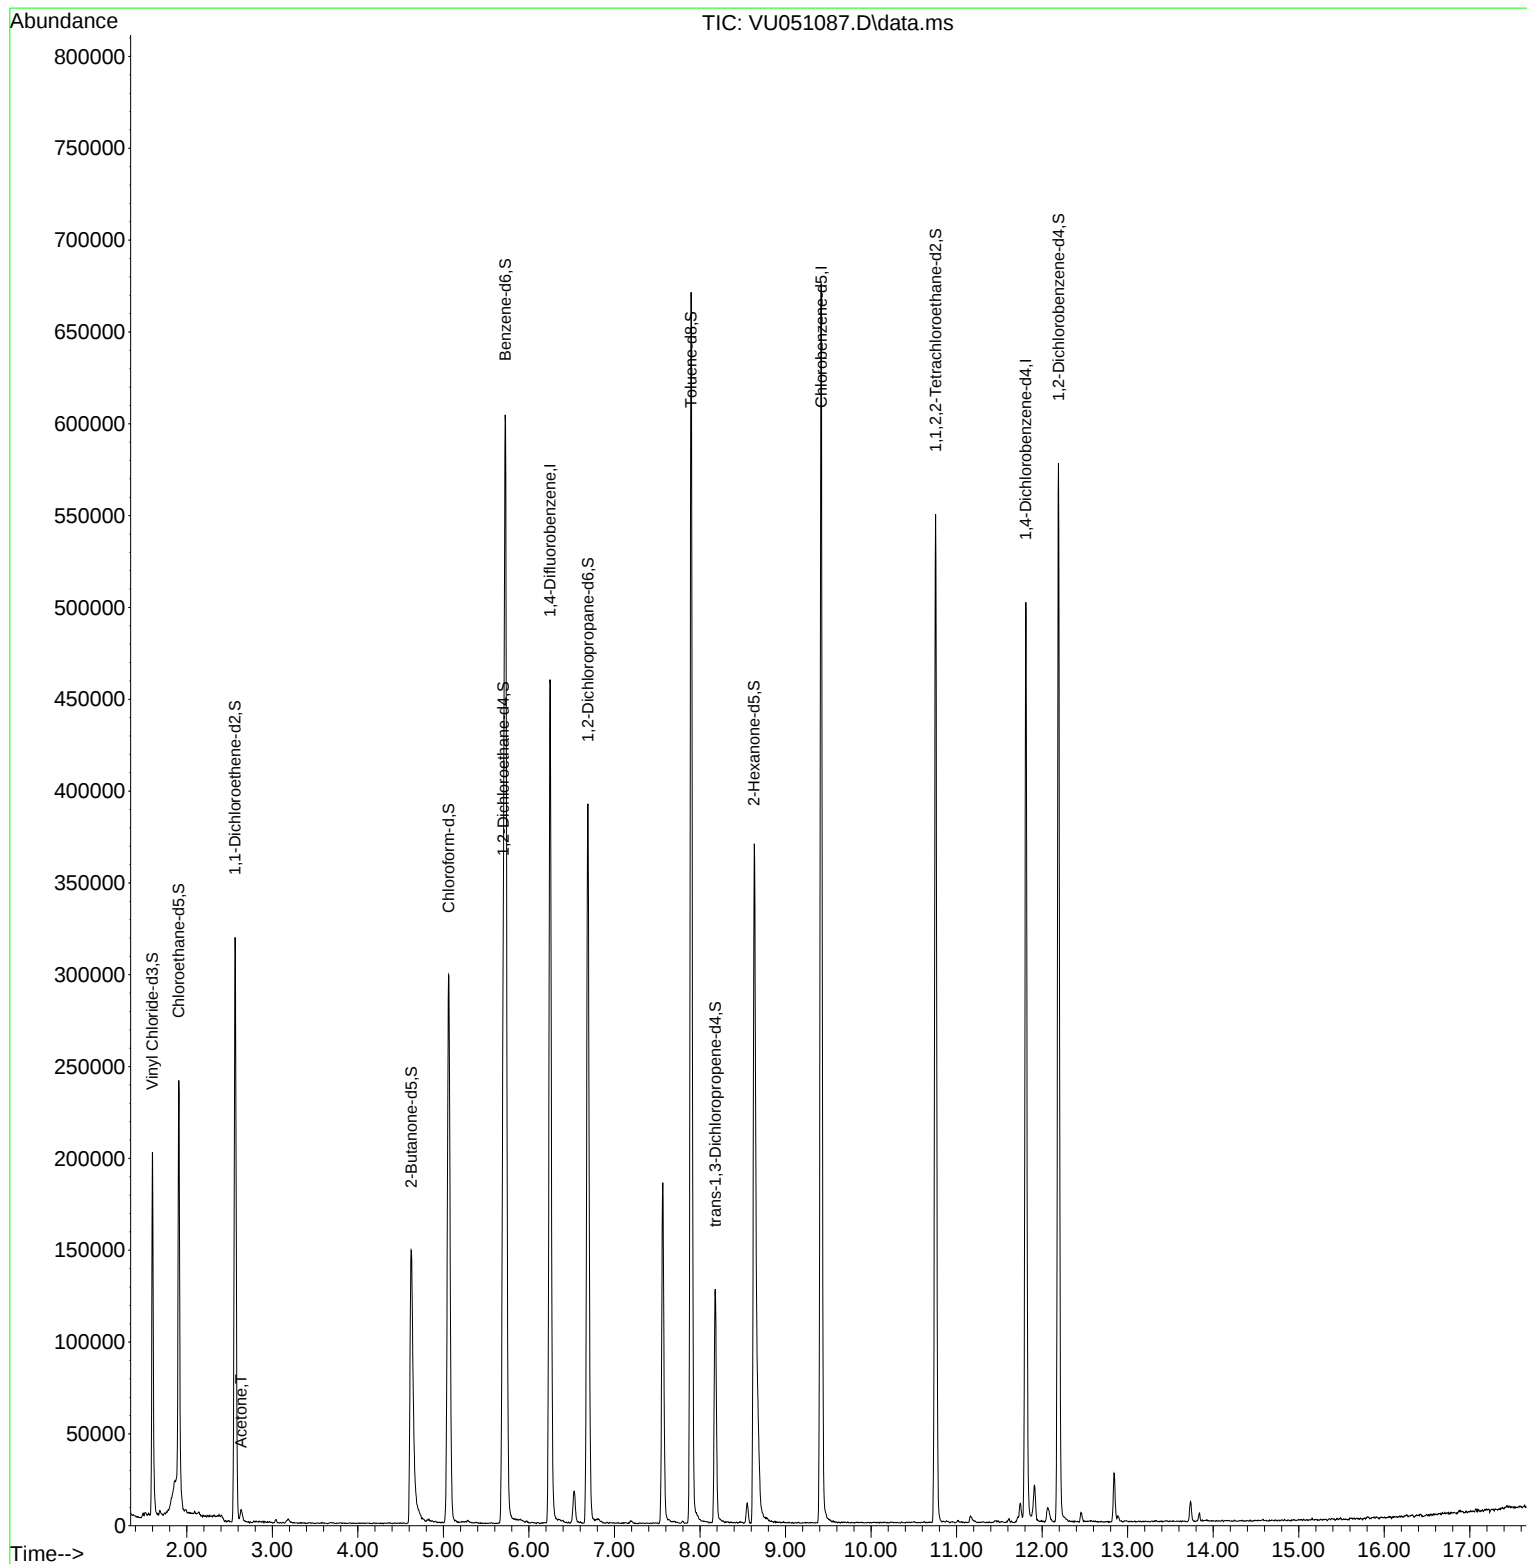

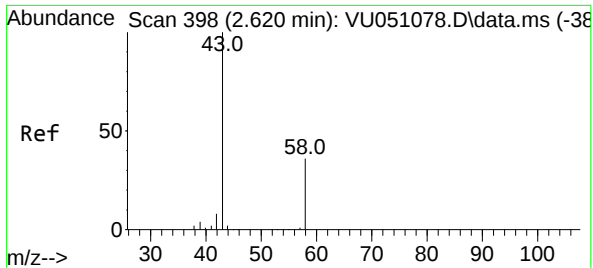

#13
 Acetone
 Concen: 4.076 ug/L
 RT: 2.632 min Scan# 40
 Delta R.T. -0.007 min
 Lab File: VU051087.D
 Acq: 03 Oct 2022 17:06

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J60

Tgt Ion: 43 Resp: 7877
 Ion Ratio Lower Upper
 43 100
 58 32.6 0.0 73.6

